

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042623\
 Data File : BM039691.D
 Acq On : 26 Apr 2023 22:45
 Operator : CG/JU
 Sample : 02488-09
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BHE64

Quant Time: Apr 27 01:23:12 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 27 01:14:42 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.817	152	3889	0.400	ng/ul	-0.04
4) Naphthalene-d8	10.622	136	13833	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.464	164	7510	0.400	ng/ul	#-0.01
13) Phenanthrene-d10	17.221	188	12475	0.400	ng/ul	-0.03
17) Chrysene-d12	21.440	240	8051	0.400	ng/ul	# 0.00
23) Perylene-d12	0.000	264	0	0.000	ng/ul	-23.81
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.210	96	26625	3.698	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.234	152	5510	0.344	ng/ul	0.00
18) Fluoranthene-d10	19.257	212	8958	0.357	ng/ul	-0.02
Target Compounds						
					Qvalue	
12) Fluorene	15.459	166	1865	0.082	ng/ul#	19
20) Pyrene	19.615	202	1514	0.040	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042623\
Data File : BM039691.D
Acq On : 26 Apr 2023 22:45
Operator : CG/JU
Sample : 02488-09
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHE64

Quant Time: Apr 27 01:23:12 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 27 01:14:42 2023
Response via : Initial Calibration

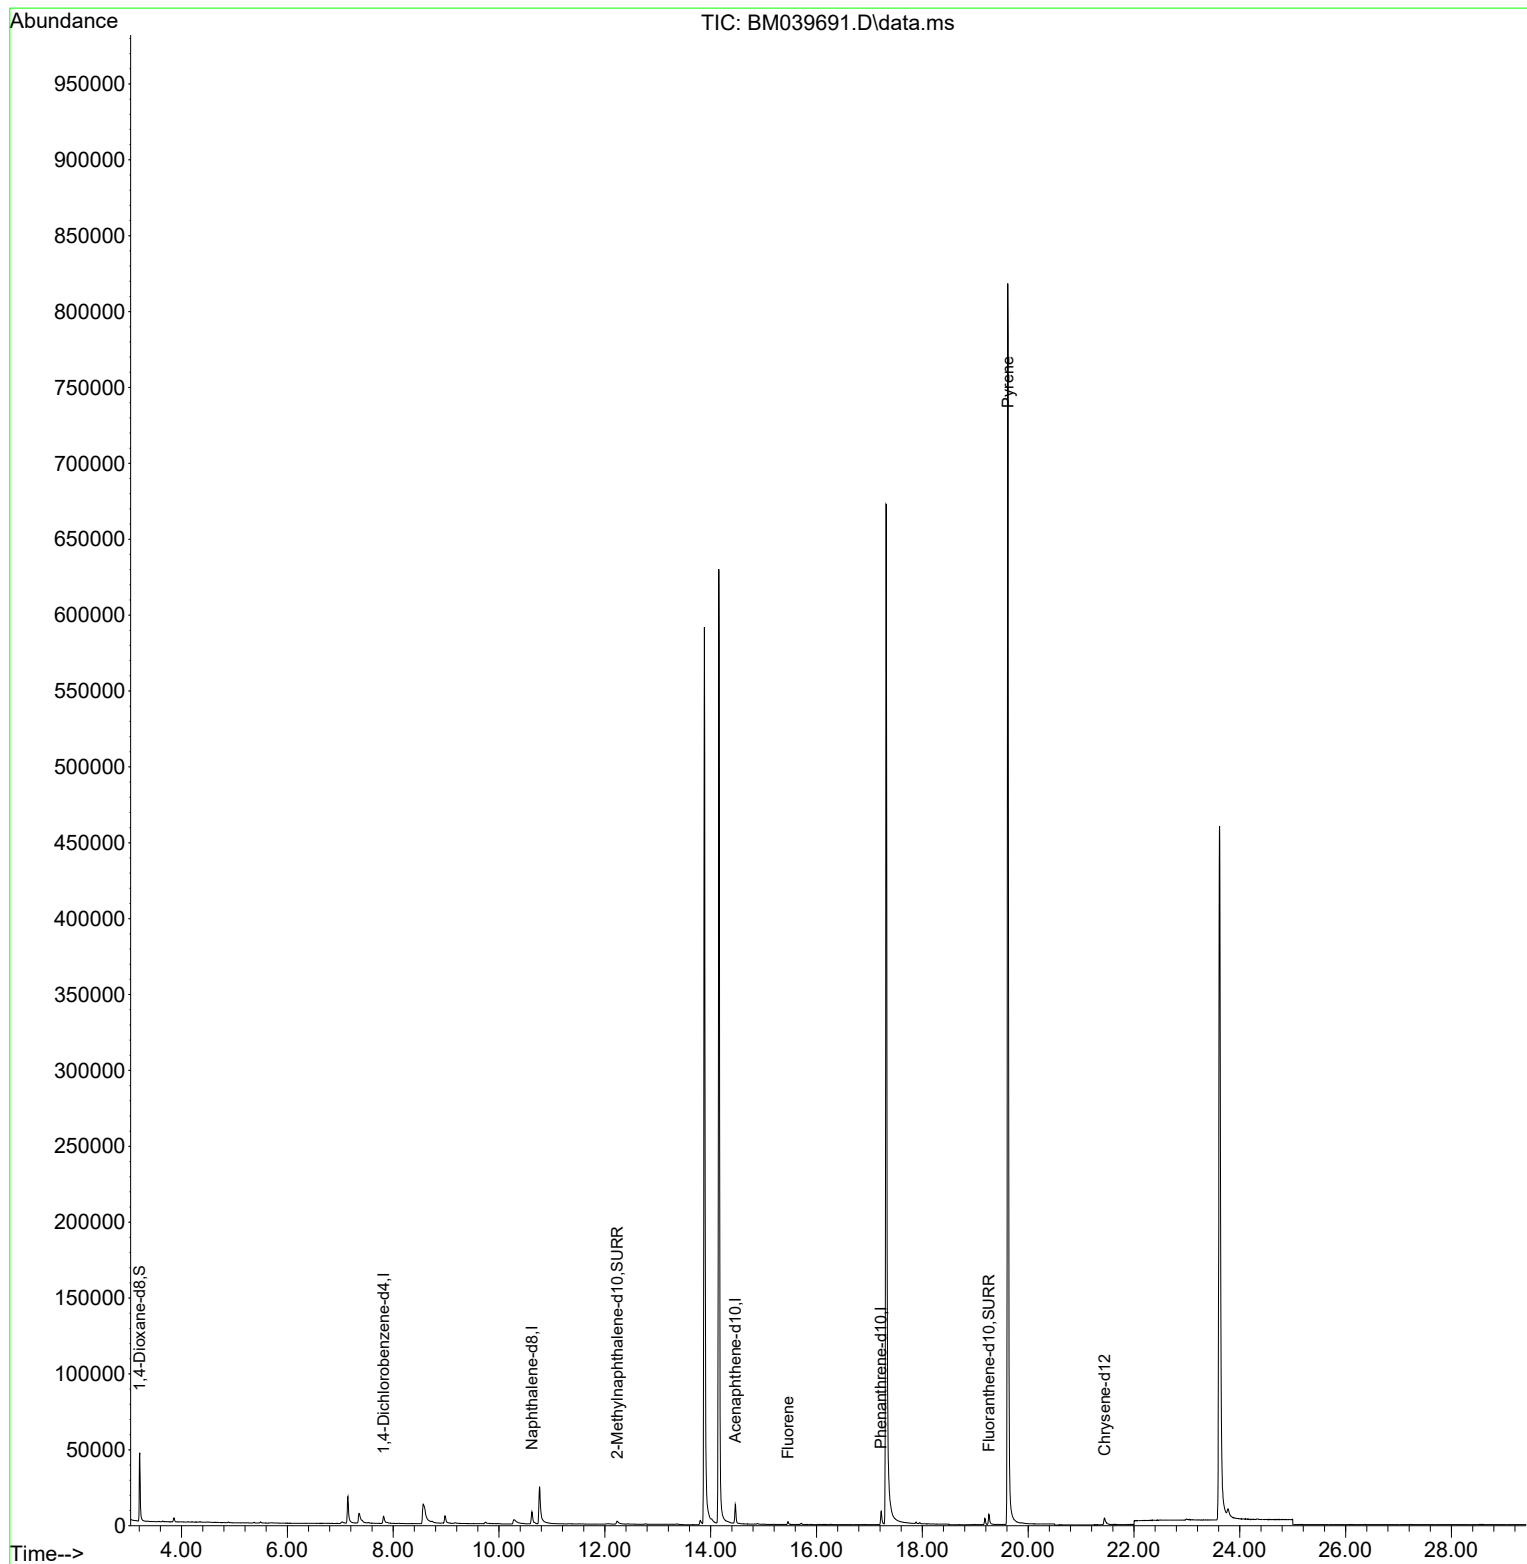

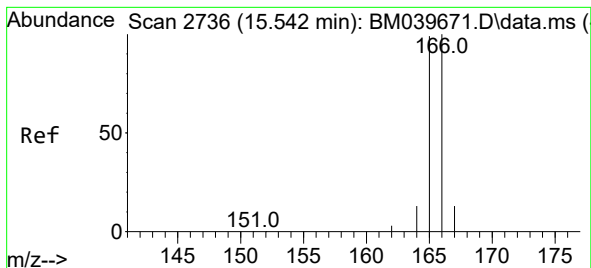

#12

Fluorene

Concen: 0.082 ng/ul

RT: 15.459 min Scan# 21

Delta R.T. -0.083 min

Lab File: BM039691.D

Acq: 26 Apr 2023 22:45

Instrument :

BNA_M

ClientSampleId :

BHE64





Tgt Ion:166 Resp: 1865

Ion Ratio Lower Upper

166 100

165 11.1 77.8 116.8#

167 31.8 11.8 17.6#

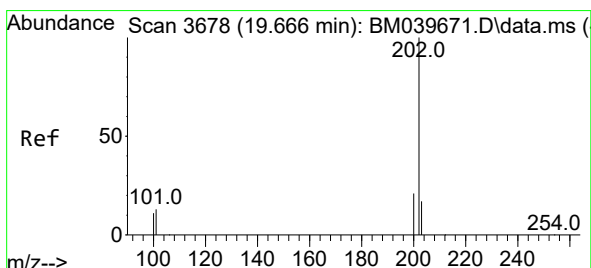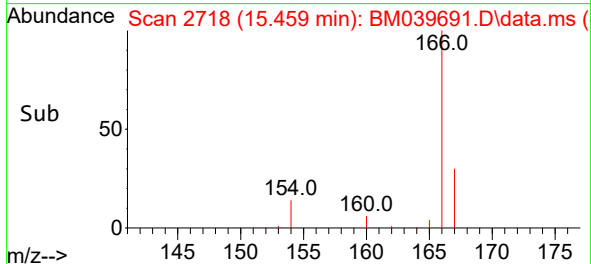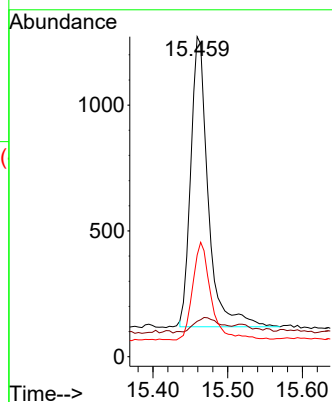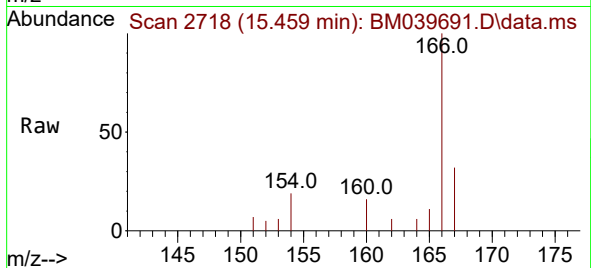

#20

Pyrene

Concen: 0.040 ng/ul

RT: 19.615 min Scan# 3667

Delta R.T. -0.051 min

Lab File: BM039691.D

Acq: 26 Apr 2023 22:45

Tgt Ion:202 Resp: 1514

Ion Ratio Lower Upper

202 100

101 164.2 11.1 16.7#

100 1239.7 8.8 13.2#

