




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042623\
 Data File : BM039686.D
 Acq On : 26 Apr 2023 19:45
 Operator : CG/JU
 Sample : 02488-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BHE58

Manual IntegrationsAPPROVED

Quant Time: Apr 27 01:22:38 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 27 01:14:42 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/27/2023
 Supervised By :Jagrut Upadhyay 04/27/2023

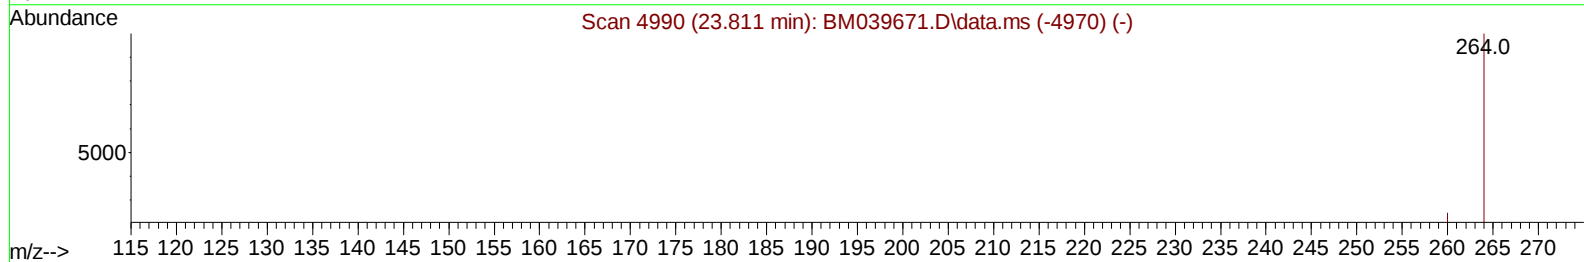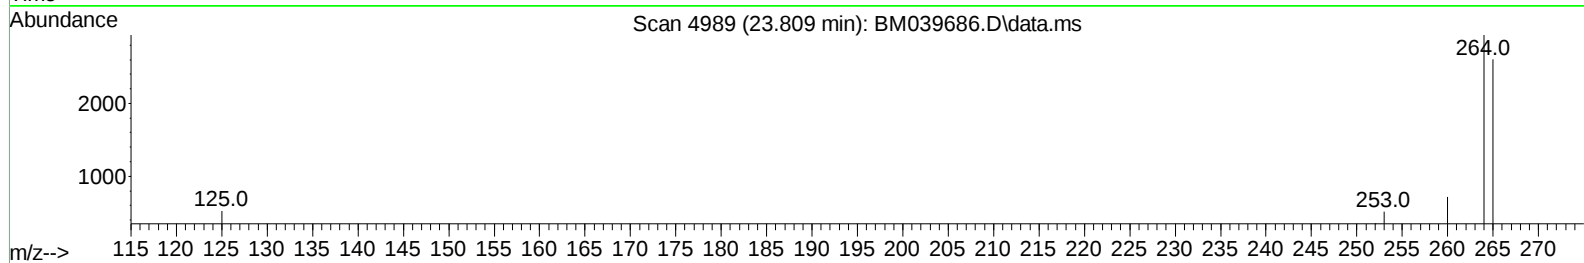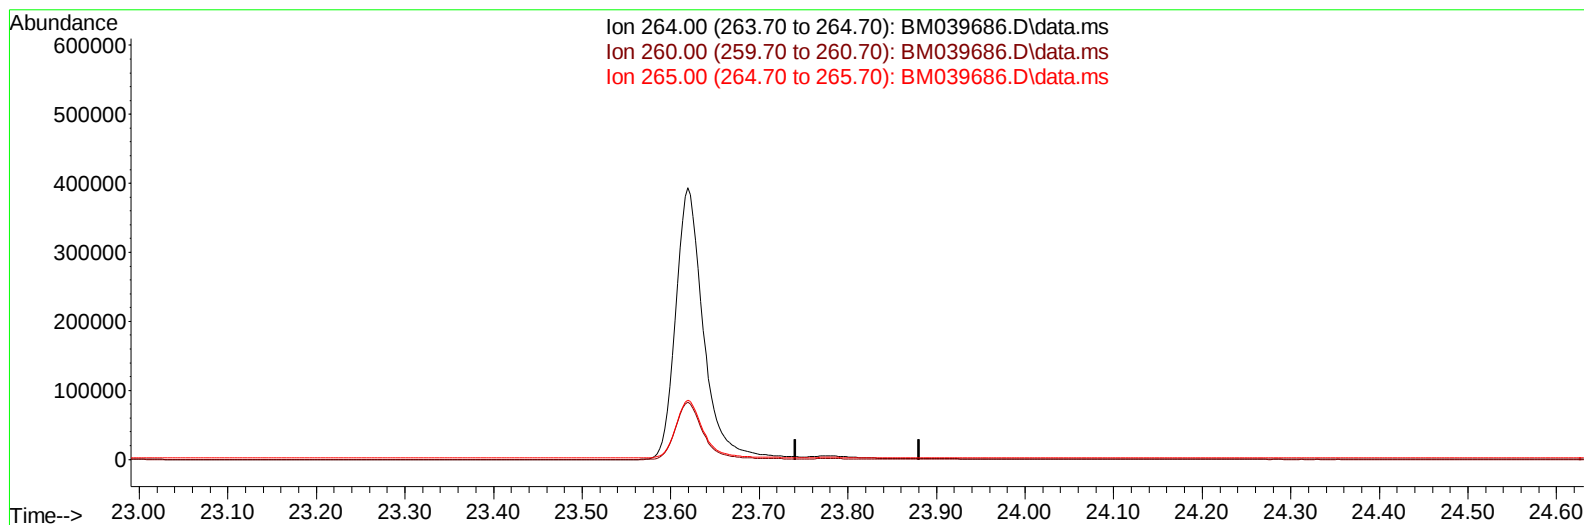

TIC: BM039686.D\data.ms

(23) Perylene-d12 (I)

23.811min (-23.811) 0.00 ng/ul

response 0

Ion	Exp%	Act%
264.00	100.00	0.00
260.00	27.00	0.00#
265.00	147.40	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042623\
 Data File : BM039686.D
 Acq On : 26 Apr 2023 19:45
 Operator : CG/JU
 Sample : 02488-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BHE58

Manual IntegrationsAPPROVED

Quant Time: Apr 27 01:22:38 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 27 01:14:42 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/27/2023
 Supervised By :Jagrut Upadhyay 04/27/2023

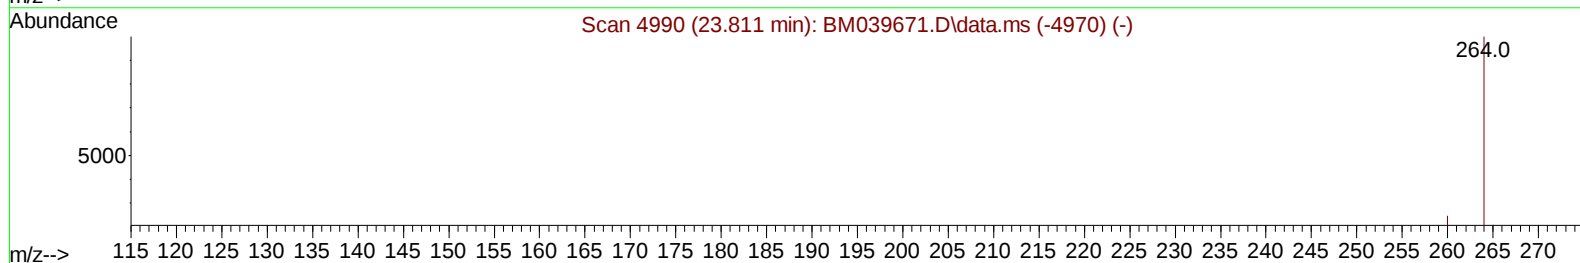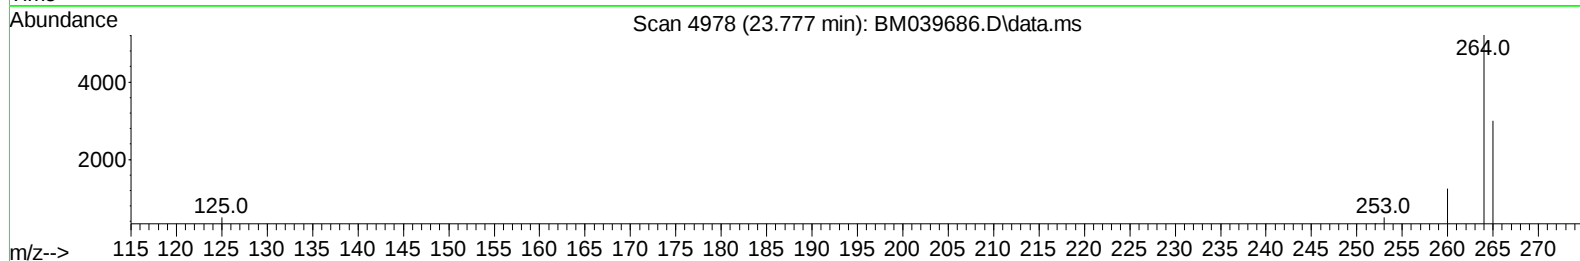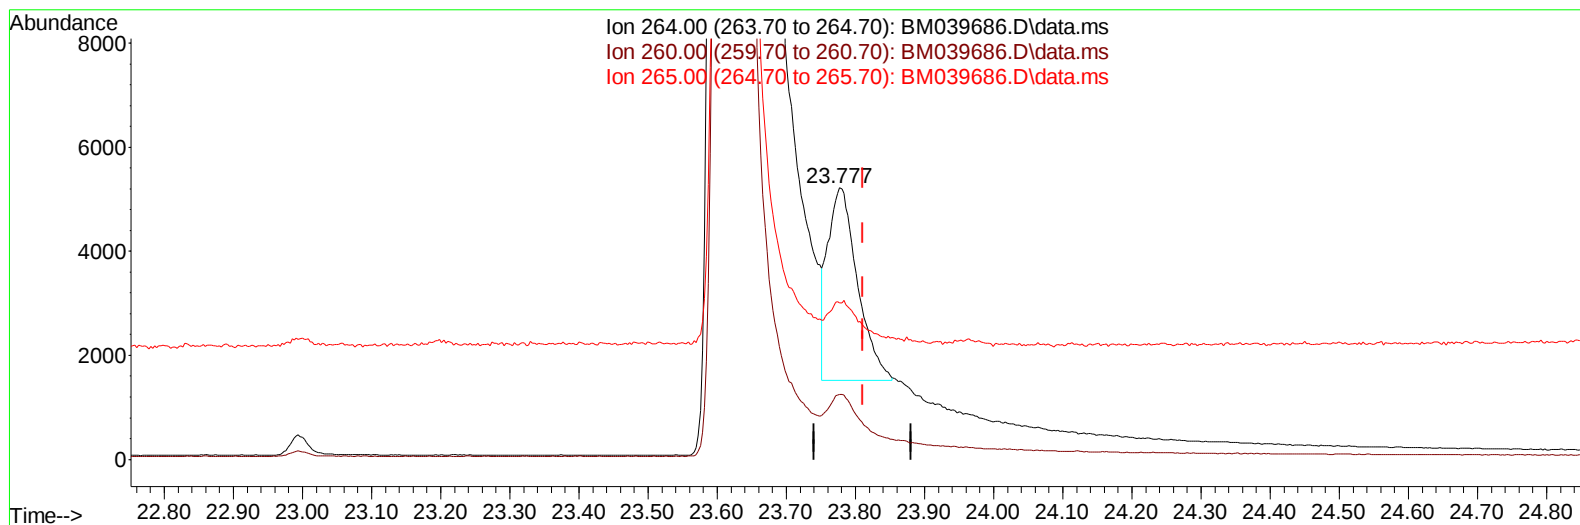

TIC: BM039686.D\data.ms

(23) Perylene-d12 (I)

23.777min (-0.033) 0.40 ng/ul m

response 11095

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	27.00	23.92
265.00	147.40	57.66#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042623\
 Data File : BM039686.D
 Acq On : 26 Apr 2023 19:45
 Operator : CG/JU
 Sample : 02488-02
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BHE58

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 04/27/2023
 Supervised By :Jagrut Upadhyay 04/27/2023

Quant Time: Apr 27 01:22:38 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 27 01:14:42 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.817	152		3491	0.400	ng/ul	-0.04
4) Naphthalene-d8	10.617	136		13341	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.464	164		7623	0.400	ng/ul	#-0.01
13) Phenanthrene-d10	17.221	188		15281	0.400	ng/ul	-0.03
17) Chrysene-d12	21.439	240		9569	0.400	ng/ul	# 0.00
23) Perylene-d12	23.777	264		11095m	0.400	ng/ul	-0.03
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.209	96		25804	3.993	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.234	152		6148	0.399	ng/ul	0.00
18) Fluoranthene-d10	19.257	212		13976	0.469	ng/ul	-0.02

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042623\
Data File : BM039686.D
Acq On : 26 Apr 2023 19:45
Operator : CG/JU
Sample : 02488-02
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHE58

Manual IntegrationsAPPROVED

Quant Time: Apr 27 01:22:38 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 27 01:14:42 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 04/27/2023
Supervised By :Jagrut Upadhyay 04/27/2023

