

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042623\
 Data File : BM039674.D
 Acq On : 26 Apr 2023 12:32
 Operator : CG/JU
 Sample : 02433-13
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BHE48

Quant Time: Apr 27 01:16:35 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 27 01:14:42 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.817	152	3987	0.400	ng/ul	-0.04
4) Naphthalene-d8	10.617	136	13945	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.469	164	7426	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.221	188	14000	0.400	ng/ul	-0.03
17) Chrysene-d12	21.432	240	10917	0.400	ng/ul	# 0.00
23) Perylene-d12	23.787	264	11680	0.400	ng/ul	#-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.210	96	21967	2.976	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.223	152	5095	0.316	ng/ul	-0.02
18) Fluoranthene-d10	19.257	212	9637	0.283	ng/ul	-0.02
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.248	88	977	0.124	ng/ul#	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042623\
Data File : BM039674.D
Acq On : 26 Apr 2023 12:32
Operator : CG/JU
Sample : 02433-13
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHE48


Quant Time: Apr 27 01:16:35 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 27 01:14:42 2023
Response via : Initial Calibration

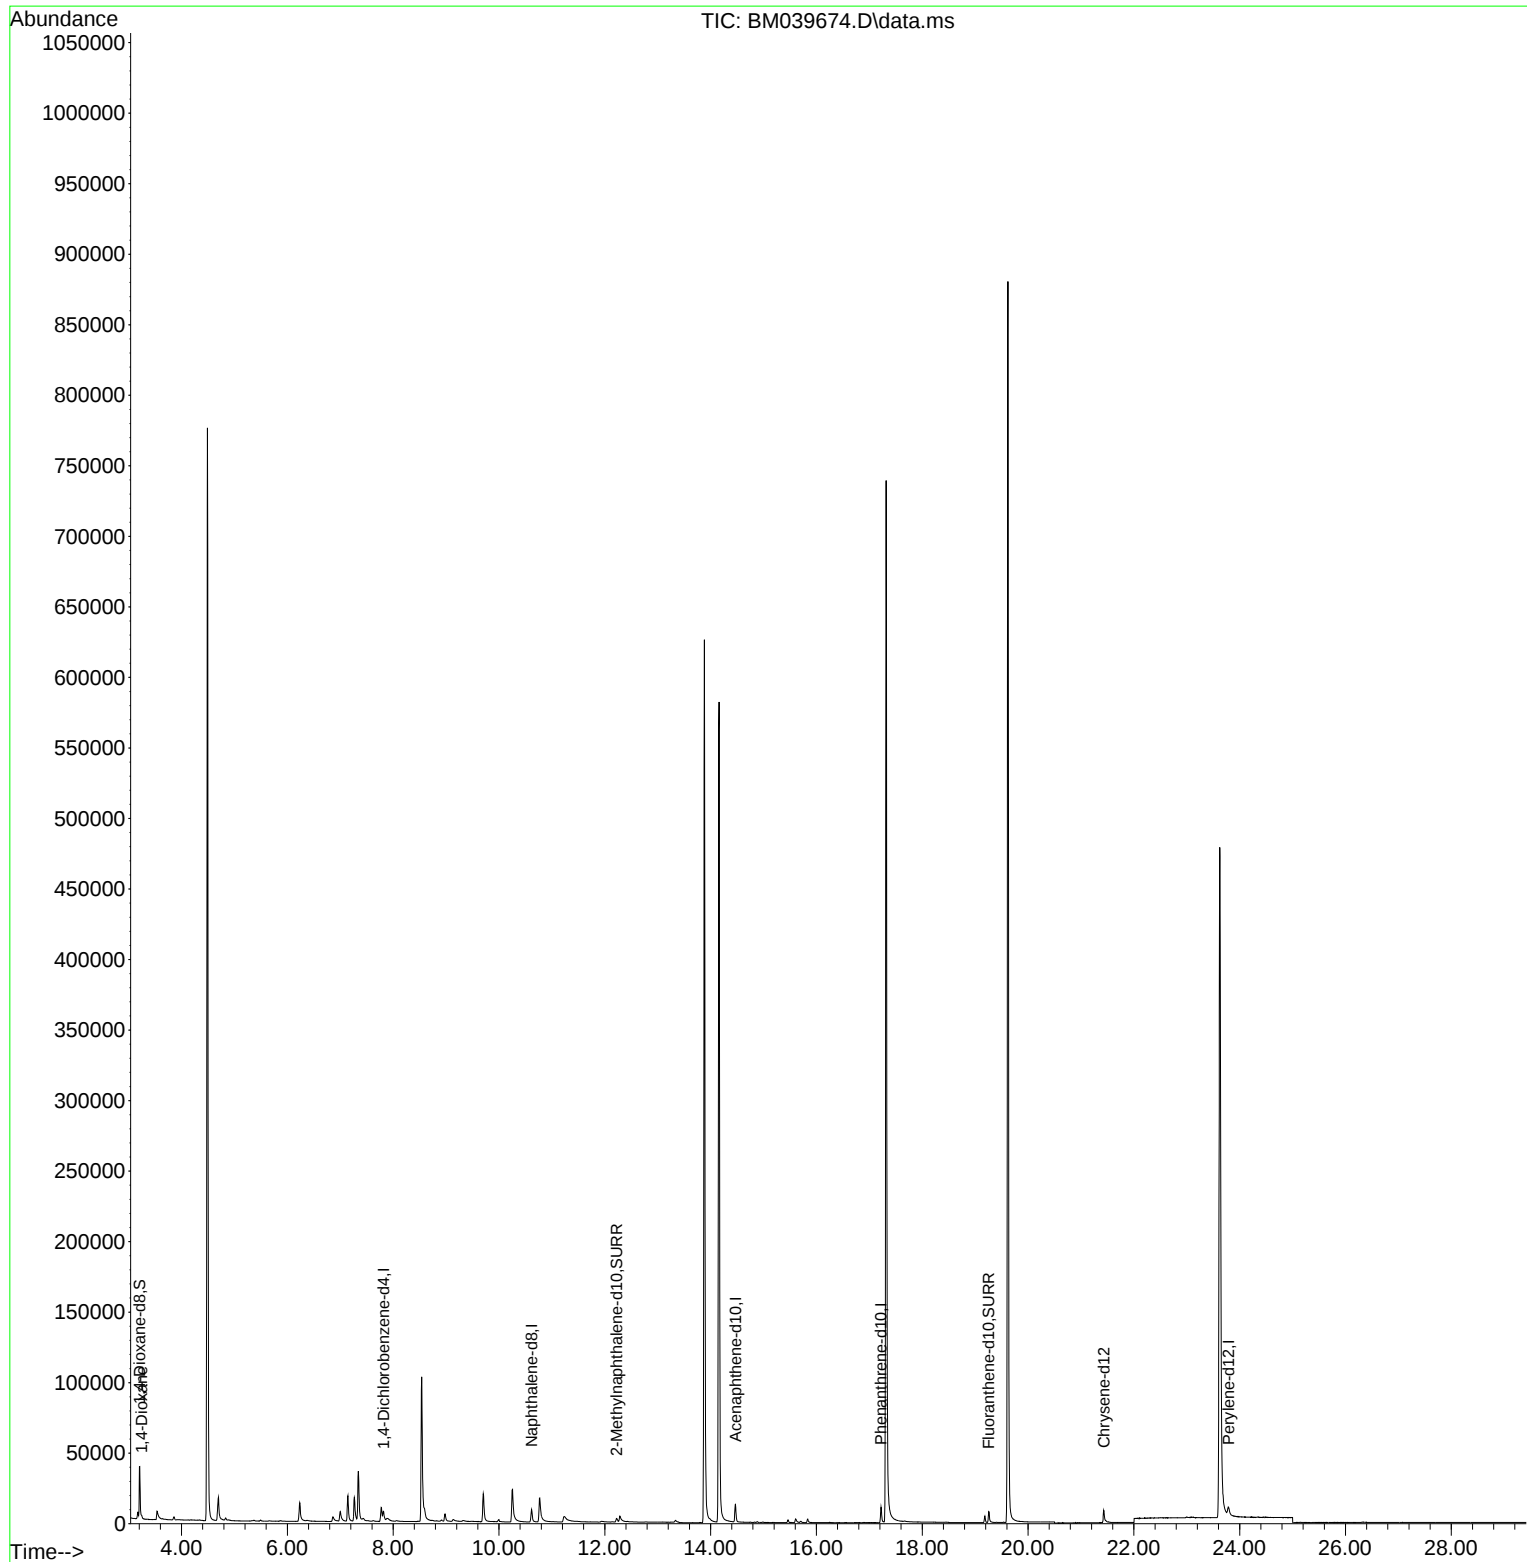

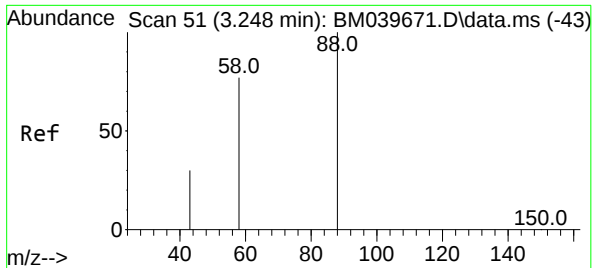

#2
 1,4-Dioxane
 Concen: 0.124 ng/ul
 RT: 3.248 min Scan# 51
 Delta R.T. 0.000 min
 Lab File: BM039674.D
 Acq: 26 Apr 2023 12:32

Instrument :
 BNA_M
 ClientSampleId :
 BHE48

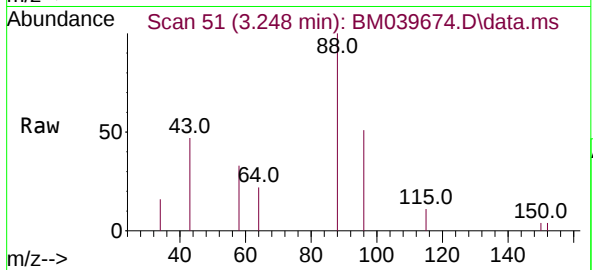

Tgt Ion:	88	Resp:	977
Ion	Ratio	Lower	Upper
88	100		
43	46.9	30.6	45.8#
58	33.4	34.1	51.1#

