

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042623\
 Data File : BM039689.D
 Acq On : 26 Apr 2023 21:33
 Operator : CG/JU
 Sample : 02488-06
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BHE62

Quant Time: Apr 27 01:22:58 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 27 01:14:42 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.817	152	3744	0.400	ng/ul	-0.04
4) Naphthalene-d8	10.617	136	14097	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.464	164	7795	0.400	ng/ul	#-0.01
13) Phenanthrene-d10	17.217	188	16118	0.400	ng/ul	-0.03
17) Chrysene-d12	21.430	240	9623	0.400	ng/ul	#-0.01
23) Perylene-d12	23.777	264	10605	0.400	ng/ul	#-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.210	96	24427	3.524	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.234	152	6349	0.390	ng/ul	0.00
18) Fluoranthene-d10	19.257	212	14961	0.499	ng/ul	-0.02
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.247	88	1125	0.152	ng/ul#	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM042623\
Data File : BM039689.D
Acq On : 26 Apr 2023 21:33
Operator : CG/JU
Sample : 02488-06
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BHE62

Quant Time: Apr 27 01:22:58 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM040623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 27 01:14:42 2023
Response via : Initial Calibration

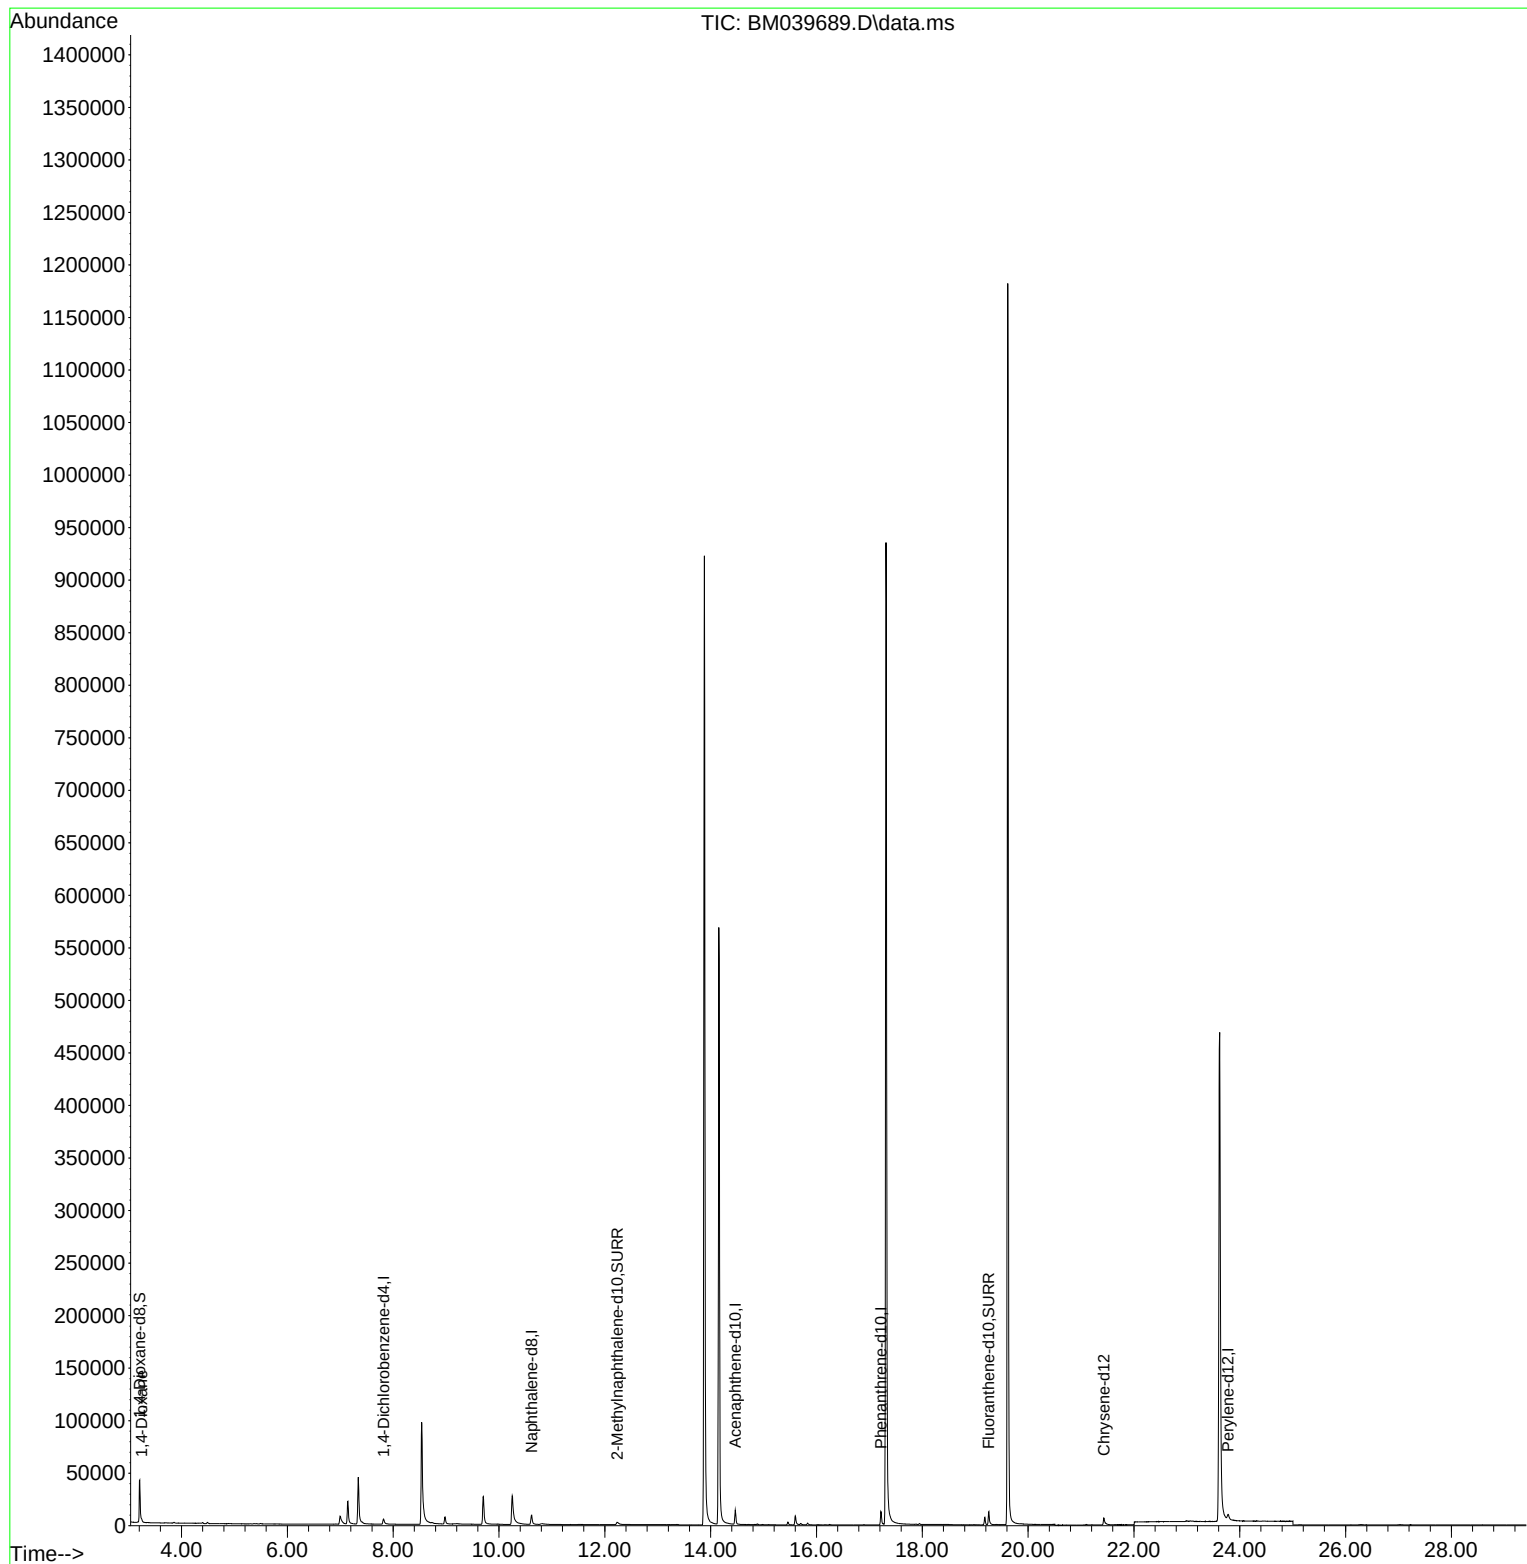

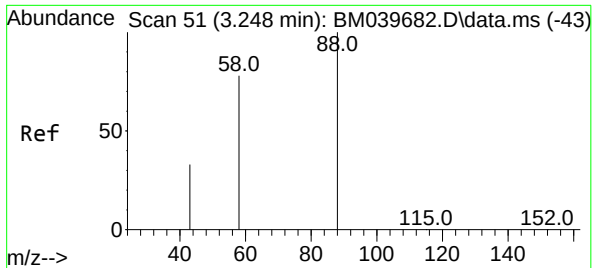

#2
 1,4-Dioxane
 Concen: 0.152 ng/ul
 RT: 3.247 min Scan# 51
 Delta R.T. -0.000 min
 Lab File: BM039689.D
 Acq: 26 Apr 2023 21:33

Instrument :
 BNA_M
 ClientSampleId :
 BHE62

Tgt Ion: 88 Resp: 1125

Ion	Ratio	Lower	Upper
88	100		
43	47.6	30.6	45.8#
58	34.7	34.1	51.1

