

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050123\
 Data File : BM039775.D
 Acq On : 01 May 2023 13:43
 Operator : CG/JU
 Sample : 02374-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB9D6

Quant Time: May 02 01:25:26 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM042723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Apr 29 04:28:45 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.796	152	3240	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.595	136	12722	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.446	164	7330	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.200	188	16724	0.400	ng/ul	0.00
17) Chrysene-d12	21.392	240	11880	0.400	ng/ul	# 0.00
23) Perylene-d12	23.742	264	10253	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.184	96	16381	3.431	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.195	152	4264	0.261	ng/ul	0.00
18) Fluoranthene-d10	19.234	212	10851	0.339	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.231	88	185	0.037	ng/ul#	42
5) Naphthalene	10.639	128	3860	0.121	ng/ul#	94
7) 2-Methylnaphthalene	12.272	142	1684	0.091	ng/ul	95
8) 1-Methylnaphthalene	12.487	142	1385	0.070	ng/ul	100
10) Acenaphthylene	14.168	152	6918	0.244	ng/ul	96
11) Acenaphthene	14.506	153	8723	0.391	ng/ul	98
12) Fluorene	15.501	166	7940	0.321	ng/ul	99
15) Phenanthrene	17.238	178	228628	5.189	ng/ul	98
16) Anthracene	17.331	178	34197	0.904	ng/ul	98
19) Fluoranthene	19.262	202	576830	13.610	ng/ul	99
20) Pyrene	19.624	202	492652	10.764	ng/ul	98
21) Benzo(a)anthracene	21.378	228	260716	7.633	ng/ul	99
22) Chrysene	21.430	228	277740	7.185	ng/ul	98
24) Benzo(b)fluoranthene	23.029	252	351321	9.757	ng/ul	92
26) Benzo(a)pyrene	23.634	252	194806	6.026	ng/ul#	85
27) Indeno(1,2,3-cd)pyrene	26.162	276	134920	3.300	ng/ul#	92
28) Dibenzo(a,h)anthracene	26.169	278	32527	1.025	ng/ul	99
29) Benzo(g,h,i)perylene	26.917	276	107758	3.025	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050123\
Data File : BM039775.D
Acq On : 01 May 2023 13:43
Operator : CG/JU
Sample : 02374-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB9D6

Quant Time: May 02 01:25:26 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 29 04:28:45 2023
Response via : Initial Calibration




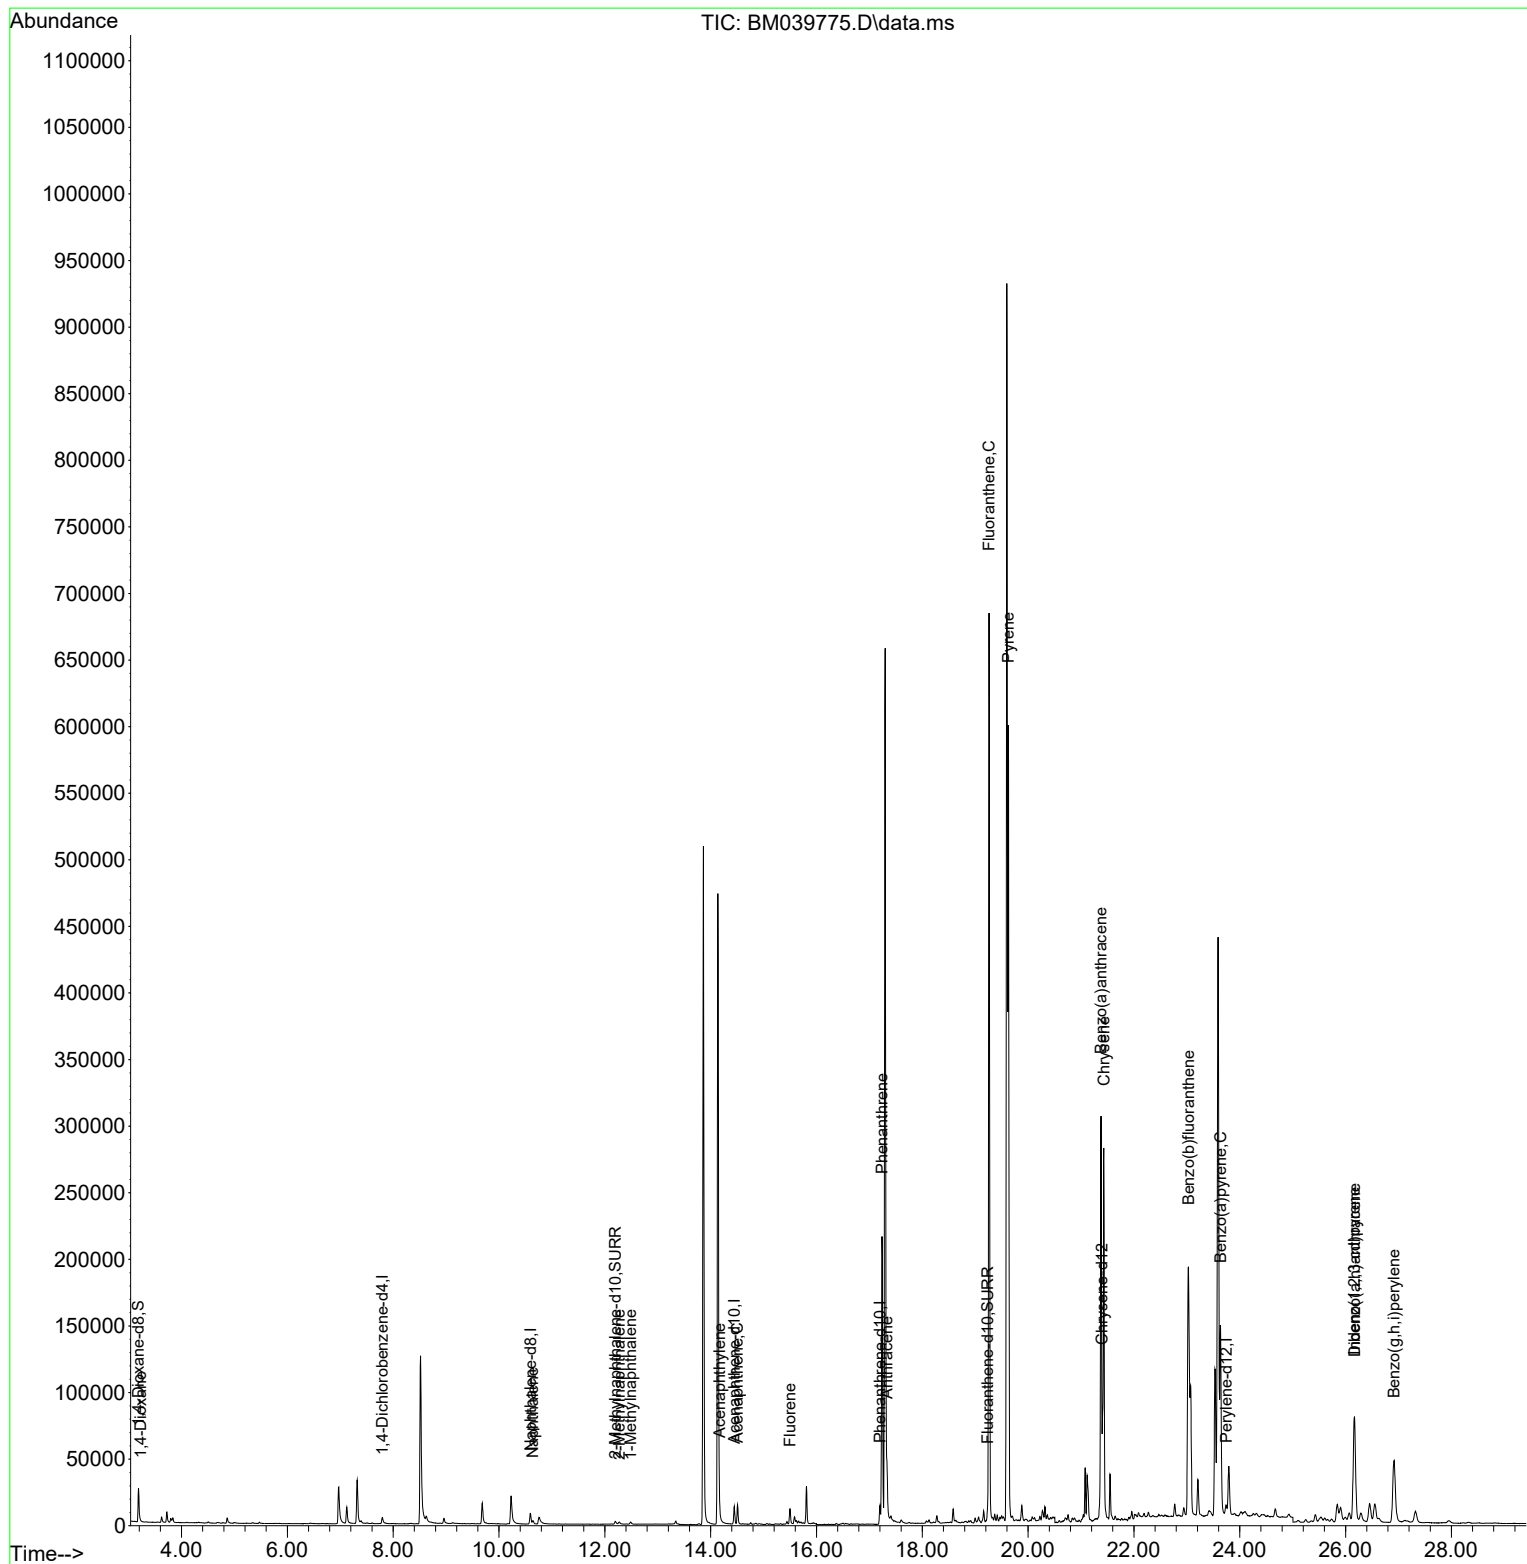




#2
1,4-Dioxane
Concen: 0.037 ng/ul
RT: 3.231 min Scan# 41
Delta R.T. 0.004 min
Lab File: BM039775.D
Acq: 01 May 2023 13:43




Instrument :
BNA_M
ClientSampleId :
CB9D6


Tgt Ion: 88 Resp: 185
Ion Ratio Lower Upper
88 100
43 58.7 102.6 153.8#
58 13.3 40.6 61.0#

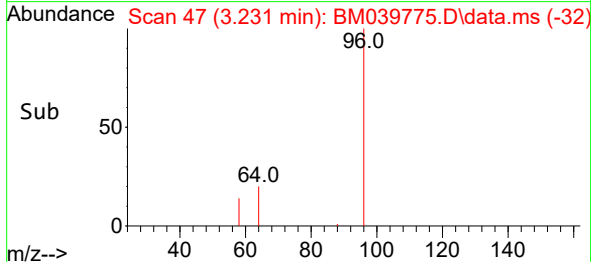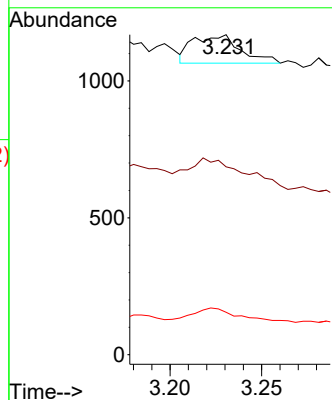

#5
Naphthalene
Concen: 0.121 ng/ul
RT: 10.639 min Scan# 1771
Delta R.T. -0.016 min
Lab File: BM039775.D
Acq: 01 May 2023 13:43

Tgt Ion: 128 Resp: 3860
Ion Ratio Lower Upper
128 100
129 15.9 9.8 14.6#
127 15.2 11.1 16.7


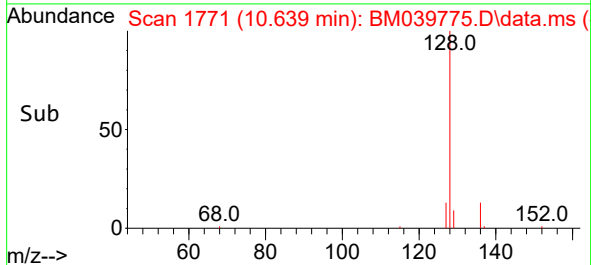
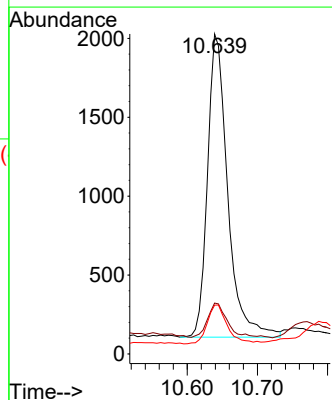
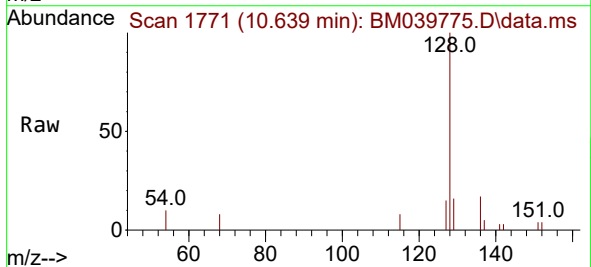




#7
2-Methylnaphthalene
Concen: 0.091 ng/ul
RT: 12.272 min Scan# 2070
Delta R.T. -0.005 min
Lab File: BM039775.D
Acq: 01 May 2023 13:43




Instrument :
BNA_M
ClientSampleId :
CB9D6


Tgt Ion:142 Resp: 1684
Ion Ratio Lower Upper
142 100
141 86.5 73.2 109.8

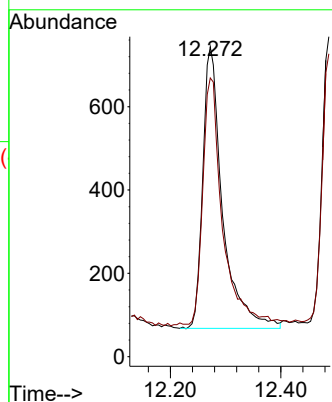

#8
1-Methylnaphthalene
Concen: 0.070 ng/ul
RT: 12.487 min Scan# 2107
Delta R.T. -0.005 min
Lab File: BM039775.D
Acq: 01 May 2023 13:43

Tgt Ion:142 Resp: 1385
Ion Ratio Lower Upper
142 100
141 92.2 73.4 110.2


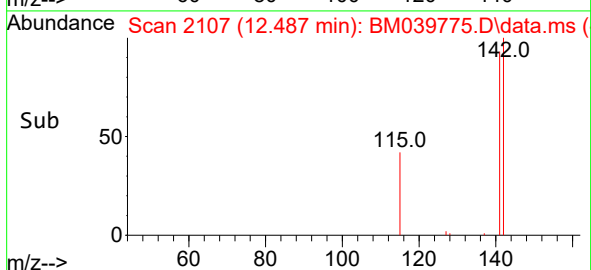
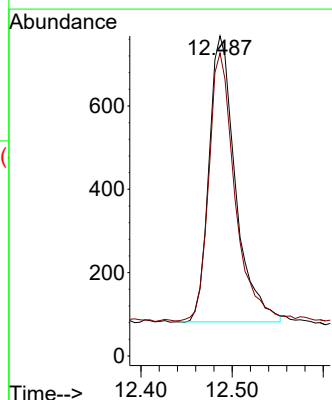





#10
Acenaphthylene
Concen: 0.244 ng/ul
RT: 14.168 min Scan# 2440
Delta R.T. -0.005 min
Lab File: BM039775.D
Acq: 01 May 2023 13:43




Instrument :
BNA_M
ClientSampleId :
CB9D6


Tgt Ion:152 Resp: 6918
Ion Ratio Lower Upper
152 100
151 21.6 16.0 24.0
153 16.1 11.2 16.8

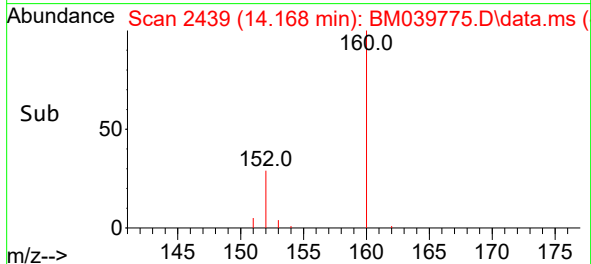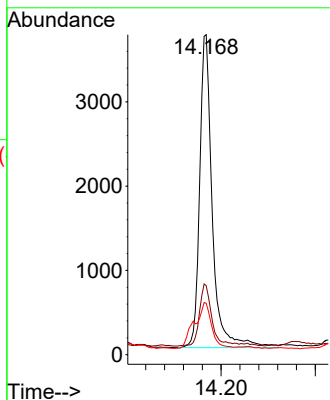

#11
Acenaphthene
Concen: 0.391 ng/ul
RT: 14.506 min Scan# 2512
Delta R.T. -0.005 min
Lab File: BM039775.D
Acq: 01 May 2023 13:43

Tgt Ion:153 Resp: 8723
Ion Ratio Lower Upper
153 100
152 50.5 40.6 61.0
154 87.3 71.9 107.9


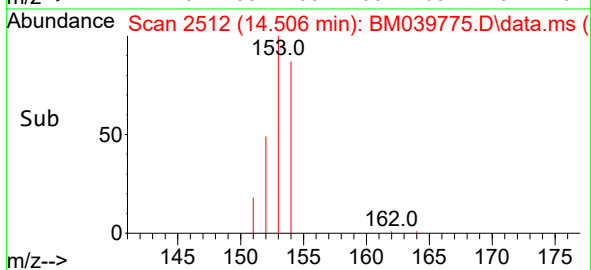
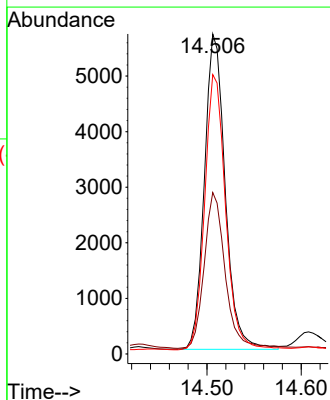
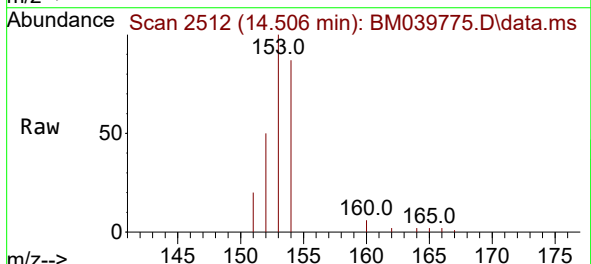




#12
Fluorene
Concen: 0.321 ng/ul
RT: 15.501 min Scan# 21
Delta R.T. -0.009 min
Lab File: BM039775.D
Acq: 01 May 2023 13:43




Instrument :
BNA_M
ClientSampleId :
CB9D6


Tgt Ion:166 Resp: 7940
Ion Ratio Lower Upper
166 100
165 98.0 79.0 118.6
167 16.6 11.8 17.6

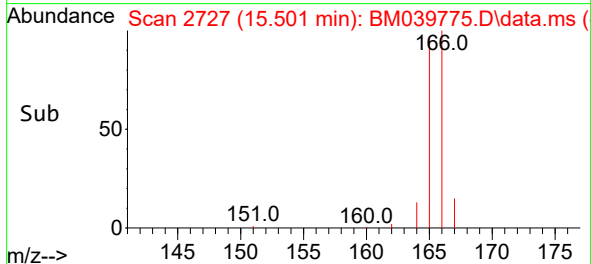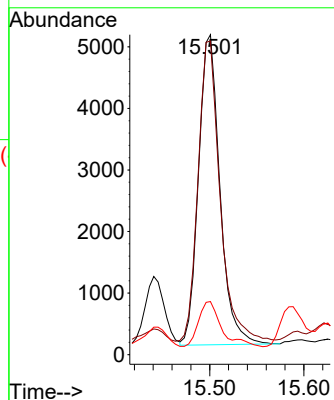

#15
Phenanthrene
Concen: 5.189 ng/ul
RT: 17.238 min Scan# 3128
Delta R.T. -0.008 min
Lab File: BM039775.D
Acq: 01 May 2023 13:43

Tgt Ion:178 Resp: 228628
Ion Ratio Lower Upper
178 100
179 15.4 13.0 19.6
176 19.1 15.8 23.8

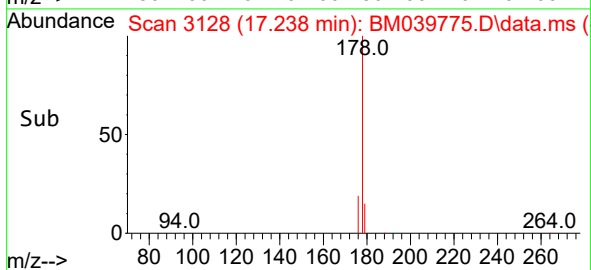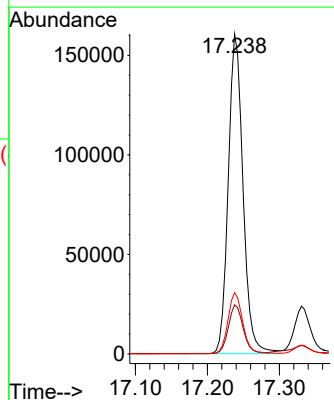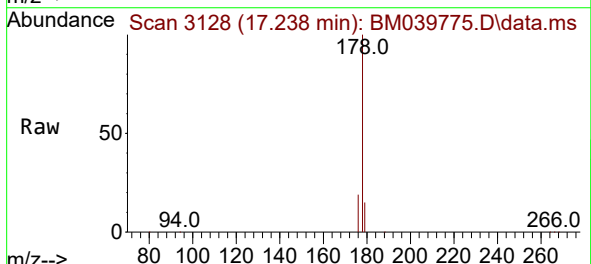



#16

Anthracene

Concen: 0.904 ng/ul

RT: 17.331 min Scan# 3154

Delta R.T. -0.013 min

Lab File: BM039775.D

Acq: 01 May 2023 13:43

Instrument :

BNA_M

ClientSampleId :

CB9D6





Tgt Ion:178 Resp: 34197

Ion Ratio Lower Upper

178 100

179 17.6 13.8 20.6

176 18.8 15.8 23.8

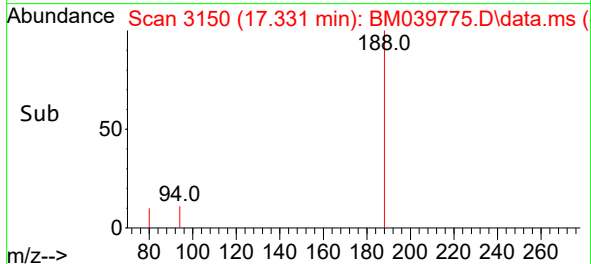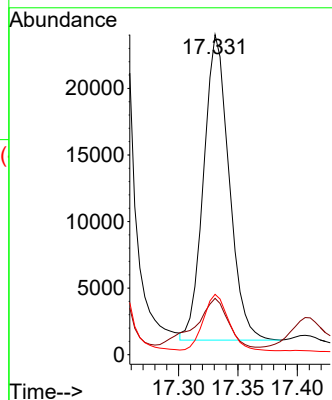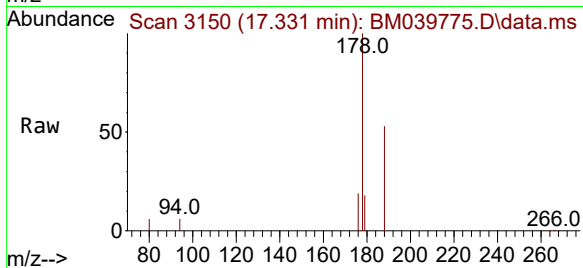

#19

Fluoranthene

Concen: 13.610 ng/ul

RT: 19.262 min Scan# 3591

Delta R.T. -0.005 min

Lab File: BM039775.D

Acq: 01 May 2023 13:43




Tgt Ion:202 Resp: 576830


Ion Ratio Lower Upper

202 100

101 11.6 9.8 14.8

100 8.7 7.3 10.9


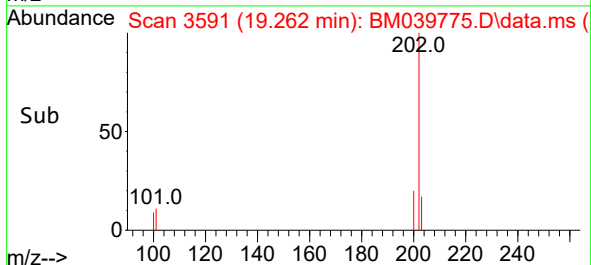
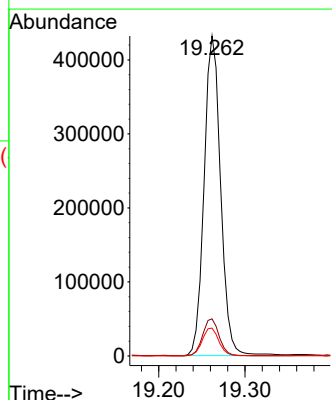
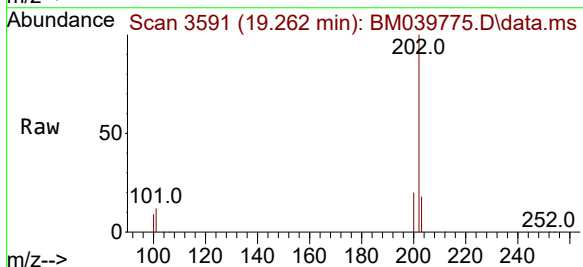




#20
Pyrene
Concen: 10.764 ng/ul
RT: 19.624 min Scan# 30
Delta R.T. -0.009 min
Lab File: BM039775.D
Acq: 01 May 2023 13:43




Instrument :
BNA_M
ClientSampleId :
CB9D6


Tgt Ion:202 Resp: 492652
Ion Ratio Lower Upper
202 100
101 14.2 10.9 16.3
100 11.6 8.9 13.3

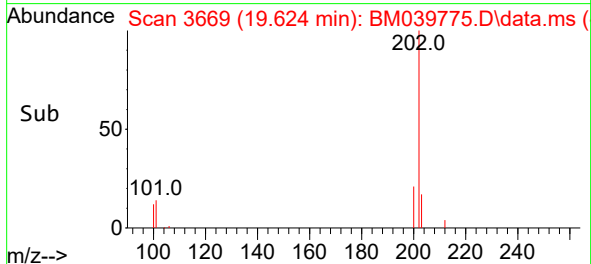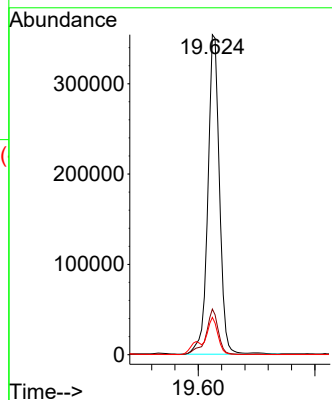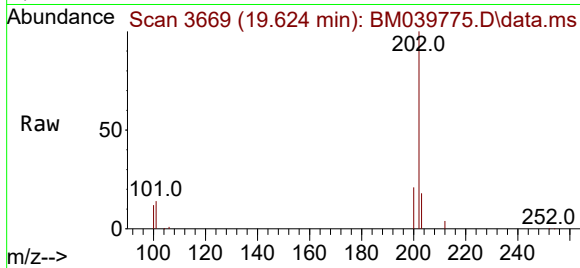

#21
Benzo(a)anthracene
Concen: 7.633 ng/ul
RT: 21.378 min Scan# 4157
Delta R.T. -0.006 min
Lab File: BM039775.D
Acq: 01 May 2023 13:43


Tgt Ion:228 Resp: 260716
Ion Ratio Lower Upper
228 100
229 20.7 16.2 24.2
226 27.3 21.6 32.4

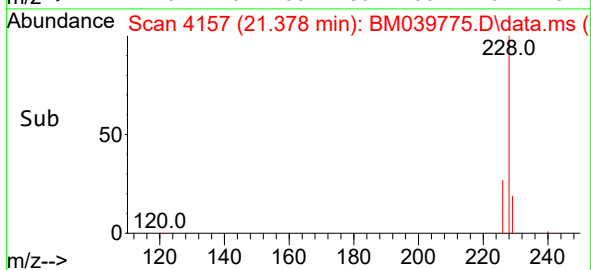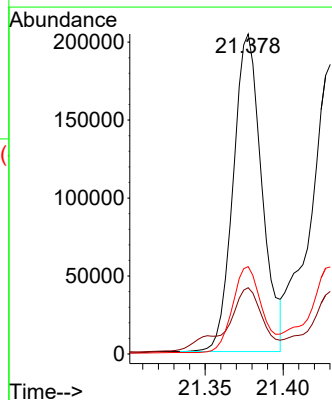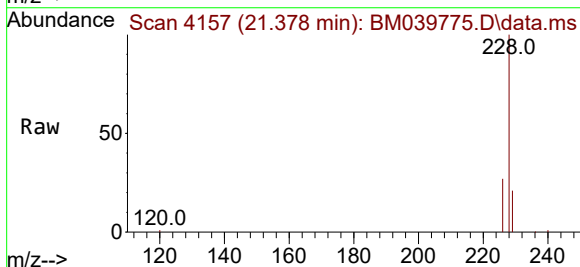






#22
Chrysene
Concen: 7.185 ng/ul
RT: 21.430 min Scan# 4179
Delta R.T. -0.006 min
Lab File: BM039775.D
Acq: 01 May 2023 13:43

Instrument :
BNA_M
ClientSampleId :
CB9D6







Tgt Ion:228 Resp: 277740
Ion Ratio Lower Upper
228 100
226 30.1 24.3 36.5
229 21.6 15.9 23.9

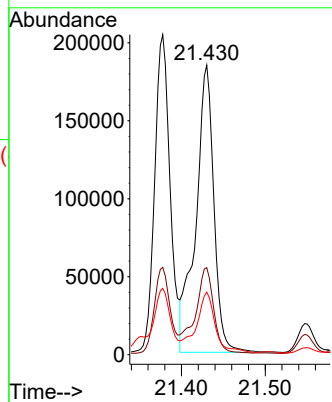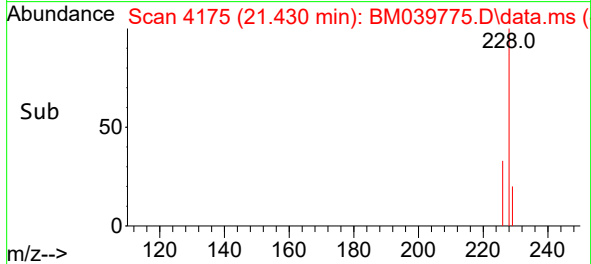

#24
Benzo(b)fluoranthene
Concen: 9.757 ng/ul
RT: 23.029 min Scan# 4722
Delta R.T. -0.003 min
Lab File: BM039775.D
Acq: 01 May 2023 13:43

Tgt Ion:252 Resp: 351321
Ion Ratio Lower Upper
252 100
253 22.8 0.0 52.8
125 12.2 0.0 31.6

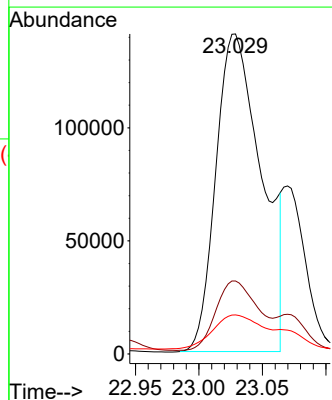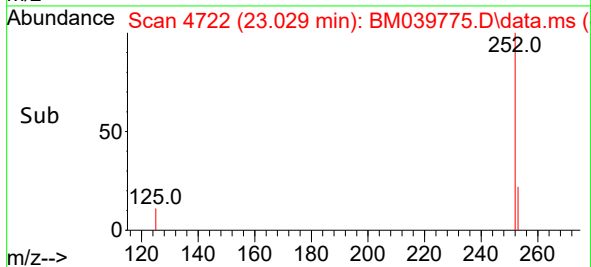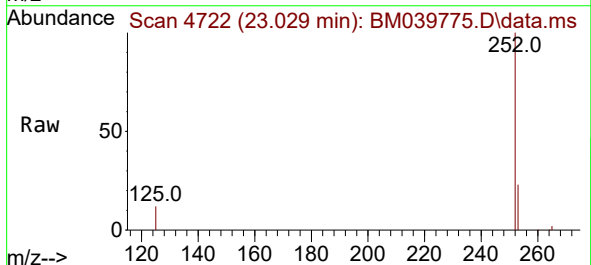



#26

Benzo(a)pyrene

Concen: 6.026 ng/ul

RT: 23.634 min Scan# 4935

Delta R.T. -0.009 min

Lab File: BM039775.D

Acq: 01 May 2023 13:43

Instrument :

BNA_M

ClientSampleId :

CB9D6





Tgt Ion:252 Resp: 194806

Ion Ratio Lower Upper

252 100

253 23.2 24.7 37.1#

125 12.8 16.5 24.7#

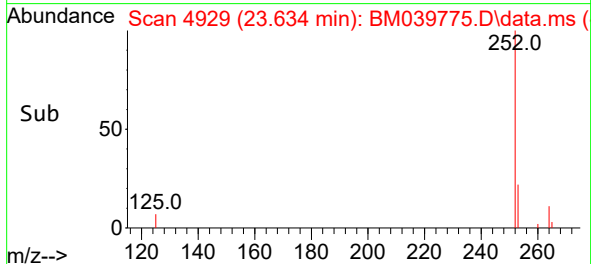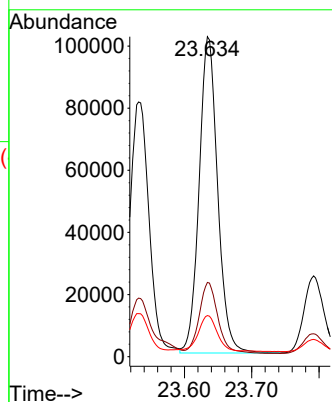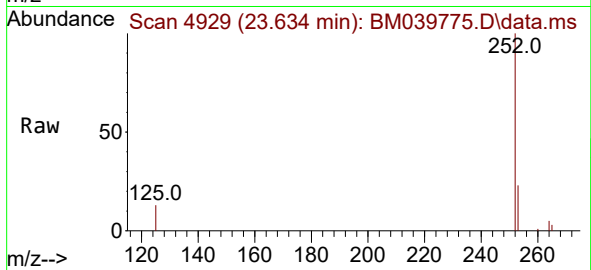

#27

Indeno(1,2,3-cd)pyrene

Concen: 3.300 ng/ul

RT: 26.162 min Scan# 5743

Delta R.T. -0.017 min

Lab File: BM039775.D

Acq: 01 May 2023 13:43




Tgt Ion:276 Resp: 134920


Ion Ratio Lower Upper

276 100

138 22.1 21.1 31.7

227 0.2 0.1 0.1#


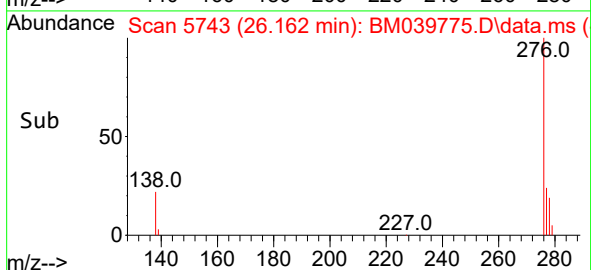
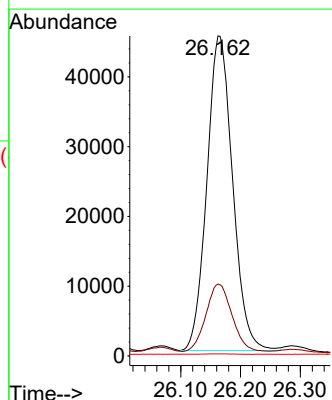





#28
Dibenzo(a,h)anthracene
Concen: 1.025 ng/ul
RT: 26.169 min Scan# 51
Delta R.T. -0.020 min
Lab File: BM039775.D
Acq: 01 May 2023 13:43

Instrument :
BNA_M
ClientSampleId :
CB9D6

Tgt Ion:278 Resp: 32527
Ion Ratio Lower Upper
278 100
139 22.3 17.0 25.6
279 29.3 23.4 35.2

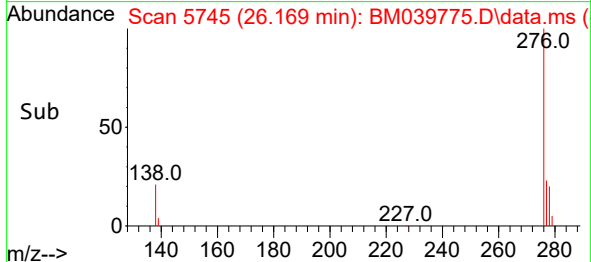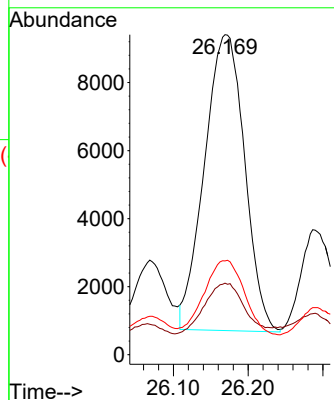

#29
Benzo(g,h,i)perylene
Concen: 3.025 ng/ul
RT: 26.917 min Scan# 5968
Delta R.T. -0.003 min
Lab File: BM039775.D
Acq: 01 May 2023 13:43

Tgt Ion:276 Resp: 107758
Ion Ratio Lower Upper
276 100
138 23.3 20.1 30.1
277 24.6 20.1 30.1

