

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050123\
 Data File : BM039780.D
 Acq On : 01 May 2023 16:48
 Operator : CG/JU
 Sample : PB152375BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK375

Quant Time: May 02 01:26:20 2023
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM042723.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Apr 29 04:28:45 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.796	152	3941	0.400	ng/ul	-0.02
4) Naphthalene-d8	10.589	136	14906	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.446	164	8170	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.200	188	17660	0.400	ng/ul	0.00
17) Chrysene-d12	21.407	240	11534	0.400	ng/ul	0.00
23) Perylene-d12	23.751	264	10831	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.184	96	30327	5.221	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.217	152	5900	0.309	ng/ul	0.02
18) Fluoranthene-d10	19.239	212	12494	0.403	ng/ul	0.00
Target Compounds						
					Qvalue	
20) Pyrene	19.596	202	1867	0.042	ng/ul#	1
26) Benzo(a)pyrene	23.590	252	2950	0.086	ng/ul#	48


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM050123\
Data File : BM039780.D
Acq On : 01 May 2023 16:48
Operator : CG/JU
Sample : PB152375BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK375

Quant Time: May 02 01:26:20 2023
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM042723.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Apr 29 04:28:45 2023
Response via : Initial Calibration

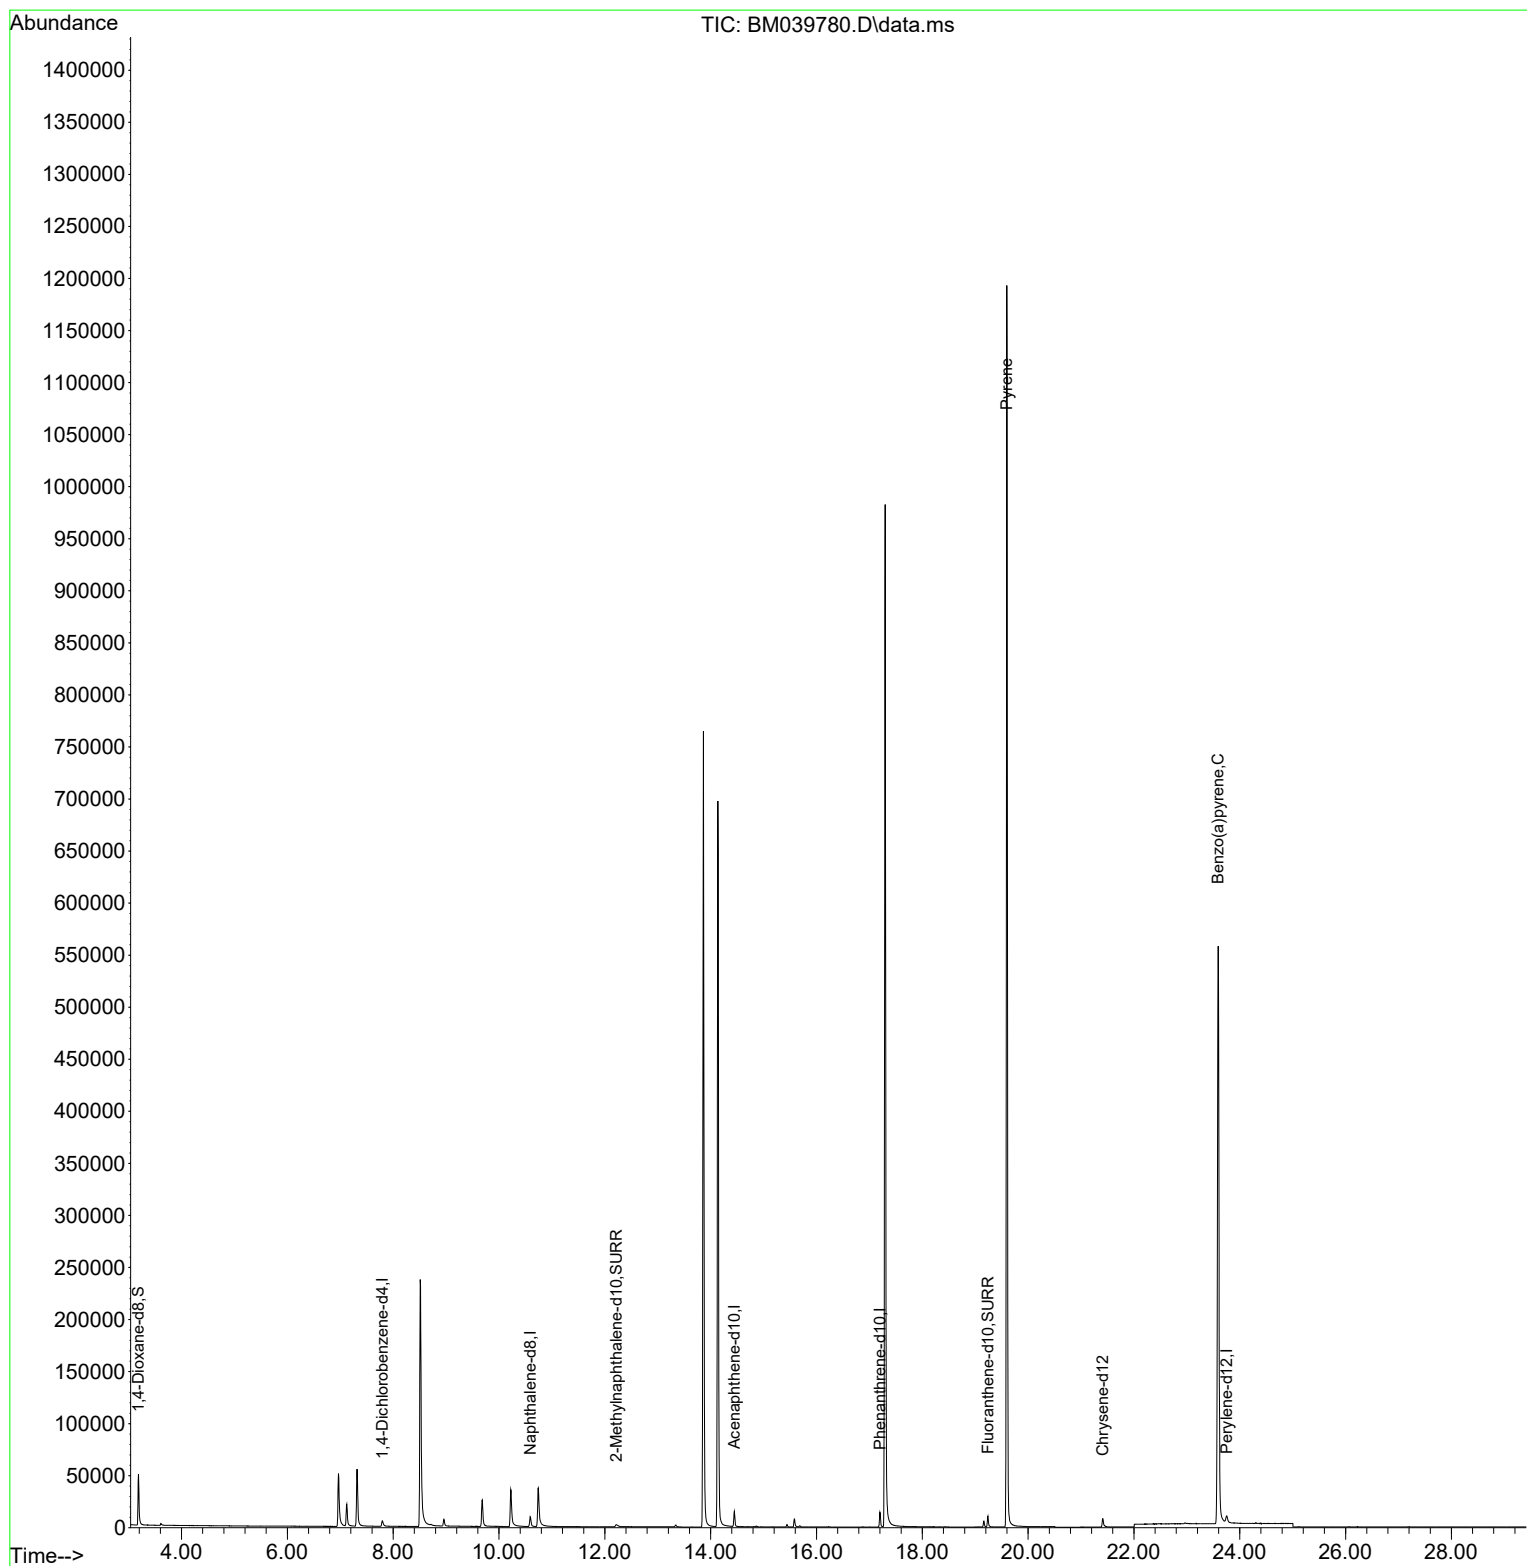

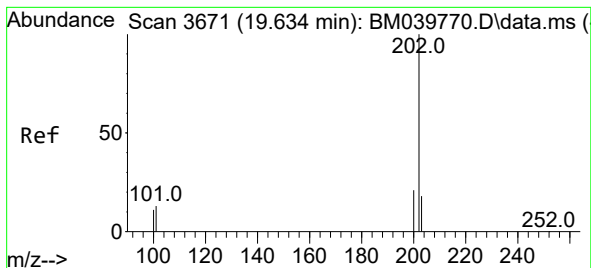

#20

Pyrene

Concen: 0.042 ng/ul

RT: 19.596 min Scan# 3

Delta R.T. -0.037 min

Lab File: BM039780.D

Acq: 01 May 2023 16:48

Instrument :

BNA_M

ClientSampleId :

SBLK375





Tgt Ion:202 Resp: 1867

Ion Ratio Lower Upper

202 100

101 172.7 10.9 16.3#

100 1322.6 8.9 13.3#

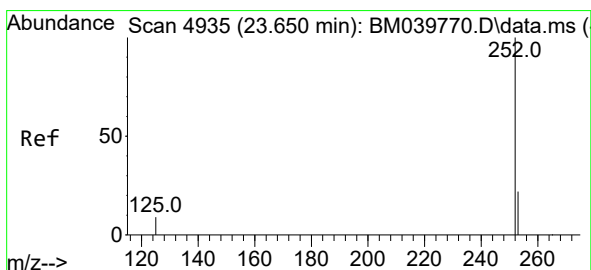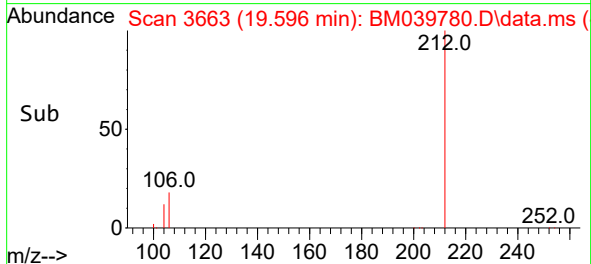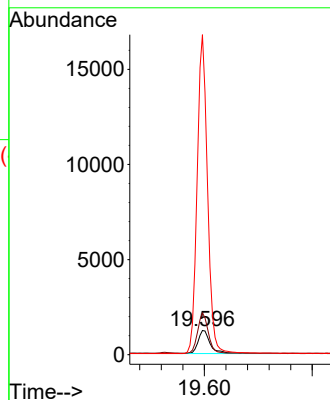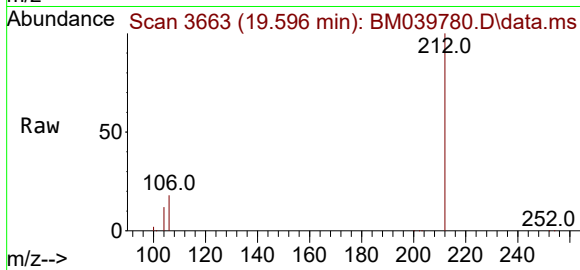

#26

Benzo(a)pyrene

Concen: 0.086 ng/ul

RT: 23.590 min Scan# 4914

Delta R.T. -0.053 min

Lab File: BM039780.D

Acq: 01 May 2023 16:48

Tgt Ion:252 Resp: 2950

Ion Ratio Lower Upper

252 100

253 53.2 24.7 37.1#

125 52.4 16.5 24.7#

