

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051822\
 Data File : BM035135.D
 Acq On : 18 May 2022 09:43
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD020125

Quant Time: May 19 00:48:55 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM051722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 17 16:13:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.904	152	173967	20.000	ng/u1	0.00
20) Naphthalene-d8	10.704	136	676643	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.539	164	403356	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.286	188	804358	20.000	ng/u1	0.00
79) Chrysene-d12	21.468	240	788778	20.000	ng/u1	0.00
88) Perylene-d12	23.850	264	800384	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.369	96	34290	8.144	ng/uL	0.00
4) Pyridine-d5	3.781	84	222634	20.498	ng/u1	0.00
7) Phenol-d5	7.069	99	259314	20.226	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.234	67	169620	20.969	ng/u1	0.00
11) 2-Chlorophenol-d4	7.440	132	233534	20.547	ng/u1	0.00
15) 4-Methylphenol-d8	8.616	113	217452	20.190	ng/u1	0.00
21) Nitrobenzene-d5	9.063	128	108499	20.452	ng/u1	0.00
24) 2-Nitrophenol-d4	9.787	143	118837	20.006	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.328	165	211802	20.047	ng/u1	0.00
31) 4-Chloroaniline-d4	10.839	131	292258	20.061	ng/u1	0.00
46) Dimethylphthalate-d6	13.951	166	613760	20.886	ng/u1	0.00
49) Acenaphthylene-d8	14.233	160	737049	20.985	ng/u1	0.00
54) 4-Nitrophenol-d4	14.733	143	105376	20.226	ng/u1	0.00
60) Fluorene-d10	15.533	176	518239	20.845	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.651	200	99242	19.107	ng/u1	0.00
73) Anthracene-d10	17.380	188	770292	20.574	ng/u1	0.00
81) Pyrene-d10	19.674	212	859237	20.453	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.697	264	837592	20.649	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.399	88	36113	8.254	ng/uL	98
5) Pyridine	3.799	79	235321	20.905	ng/u1	94
6) Benzaldehyde	7.046	77	160712	25.262	ng/u1	98
8) Phenol	7.098	94	276587	20.512	ng/u1	94
10) Bis(2-Chloroethyl)ether	7.328	93	220829	21.128	ng/u1	98
12) 2-Chlorophenol	7.469	128	243747	20.992	ng/u1	99
13) 2-Methylphenol	8.351	108	204974	20.252	ng/u1	99
14) 2,2'-oxybis(1-Chloropr...	8.440	45	321195	21.633	ng/u1	99
16) Acetophenone	8.728	105	342419	20.526	ng/u1	99
17) N-Nitroso-di-n-propyla...	8.716	70	166900	21.102	ng/u1	95
18) 4-Methylphenol	8.675	108	224470	20.754	ng/u1	97
19) Hexachloroethane	8.987	117	104619	20.727	ng/u1	97
22) Nitrobenzene	9.104	77	262138	20.664	ng/u1	98
23) Isophorone	9.634	82	463062	20.683	ng/u1	98
25) 2-Nitrophenol	9.816	139	130460	20.516	ng/u1	91
26) 2,4-Dimethylphenol	9.881	107	258257	20.605	ng/u1	100
27) Bis(2-Chloroethoxy)met...	10.116	93	280529	20.816	ng/u1	100
29) 2,4-Dichlorophenol	10.351	162	214184	20.105	ng/u1	97
30) Naphthalene	10.757	128	719300	20.552	ng/u1	100
32) 4-Chloroaniline	10.863	127	293339	20.135	ng/u1	99
33) Hexachlorobutadiene	11.051	225	153052	19.757	ng/u1	99
34) Caprolactam	11.628	113	60994	19.871	ng/u1	92
35) 4-Chloro-3-methylphenol	11.992	107	220505	20.618	ng/u1	97
36) 2-Methylnaphthalene	12.369	142	486554	20.753	ng/u1	99

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051822\
 Data File : BM035135.D
 Acq On : 18 May 2022 09:43
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD020125

Quant Time: May 19 00:48:55 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM051722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 17 16:13:52 2022
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.586	142	487627	20.751	ng/ul	98
39) 1,2,4,5-Tetrachloroben...	12.739	216	262050	20.204	ng/ul	98
40) Hexachlorocyclopentadiene	12.722	237	172792	18.683	ng/ul	99
41) 2,4,6-Trichlorophenol	12.975	196	169559	20.470	ng/ul	96
42) 2,4,5-Trichlorophenol	13.045	196	179404	20.406	ng/ul	99
43) 1,1'-Biphenyl	13.375	154	652713	20.901	ng/ul	98
44) 2-Chloronaphthalene	13.416	162	500135	20.654	ng/ul	97
45) 2-Nitroaniline	13.616	65	141539	20.801	ng/ul	96
47) Dimethylphthalate	13.998	163	617352	20.982	ng/ul	99
48) 2,6-Dinitrotoluene	14.116	165	122377	20.882	ng/ul	92
50) Acenaphthylene	14.263	152	795219	21.068	ng/ul	99
51) 3-Nitroaniline	14.439	138	118024	21.001	ng/ul	91
52) Acenaphthene	14.604	153	520152	20.692	ng/ul	99
53) 2,4-Dinitrophenol	14.645	184	69177	18.018	ng/ul	93
55) 4-Nitrophenol	14.745	109	96933	19.833	ng/ul	92
56) Dibenzofuran	14.939	168	731962	20.820	ng/ul	96
57) 2,4-Dinitrotoluene	14.904	165	173185	21.045	ng/ul	94
58) 2,3,4,6-Tetrachlorophenol	15.169	232	145860	20.479	ng/ul	96
59) Diethylphthalate	15.363	149	624938	20.975	ng/ul	99
61) Fluorene	15.586	166	597773	20.898	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.580	204	298257	20.539	ng/ul	98
63) 4-Nitroaniline	15.598	138	114624	22.512	ng/ul	86
66) 4,6-Dinitro-2-methylph...	15.669	198	100934	19.388	ng/ul#	95
67) N-Nitrosodiphenylamine	15.792	169	504298	20.725	ng/ul	99
68) 4-Bromophenyl-phenylether	16.474	248	172311	20.227	ng/ul	95
69) Hexachlorobenzene	16.598	284	197007	20.251	ng/ul	99
70) Atrazine	16.751	200	184769	19.461	ng/ul	99
71) Pentachlorophenol	16.933	266	121755	18.729	ng/ul	100
72) Phenanthrene	17.327	178	896428	20.582	ng/ul	99
74) Anthracene	17.415	178	926349	20.872	ng/ul	100
75) 1,2,3,4-Tetrachloroben...	13.339	216	271324	19.364	ng/uL	99
76) Pentachlorobenzene	14.863	250	244516	20.314	ng/uL	99
77) Carbazole	17.686	167	811911	20.671	ng/ul	100
78) Di-n-butylphthalate	18.257	149	1024650	18.229	ng/ul	98
80) Fluoranthene	19.339	202	1028251	20.376	ng/ul	99
82) Pyrene	19.704	202	1066109	20.525	ng/ul	99
83) Butylbenzylphthalate	20.603	149	449763	20.214	ng/ul	96
84) 3,3'-Dichlorobenzidine	21.386	252	338273	20.861	ng/ul	98
85) Benzo(a)anthracene	21.450	228	1043918	20.716	ng/ul	99
86) Bis(2-ethylhexyl)phtha...	21.386	149	690334	20.634	ng/ul	99
87) Chrysene	21.503	228	1023634	20.834	ng/ul	99
89) Di-n-octyl phthalate	22.309	149	1144898	19.950	ng/ul	100
90) Benzo(b)fluoranthene	23.127	252	1088583	20.913	ng/ul	99
91) Benzo(k)fluoranthene	23.174	252	1012359	20.472	ng/ul	100
93) Benzo(a)pyrene	23.744	252	1055234	20.807	ng/ul#	97
94) Indeno(1,2,3-cd)pyrene	26.321	276	1208990	20.745	ng/ul	96
95) Dibenzo(a,h)anthracene	26.333	278	1034021	20.656	ng/ul#	96
96) Benzo(g,h,i)perylene	27.080	276	1007631	20.785	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051822\
 Data File : BM035135.D
 Acq On : 18 May 2022 09:43
 Operator : CG/JU
 Sample : SSTDCCC020
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD020125

Quant Time: May 19 00:48:55 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM051722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 17 16:13:52 2022
 Response via : Initial Calibration




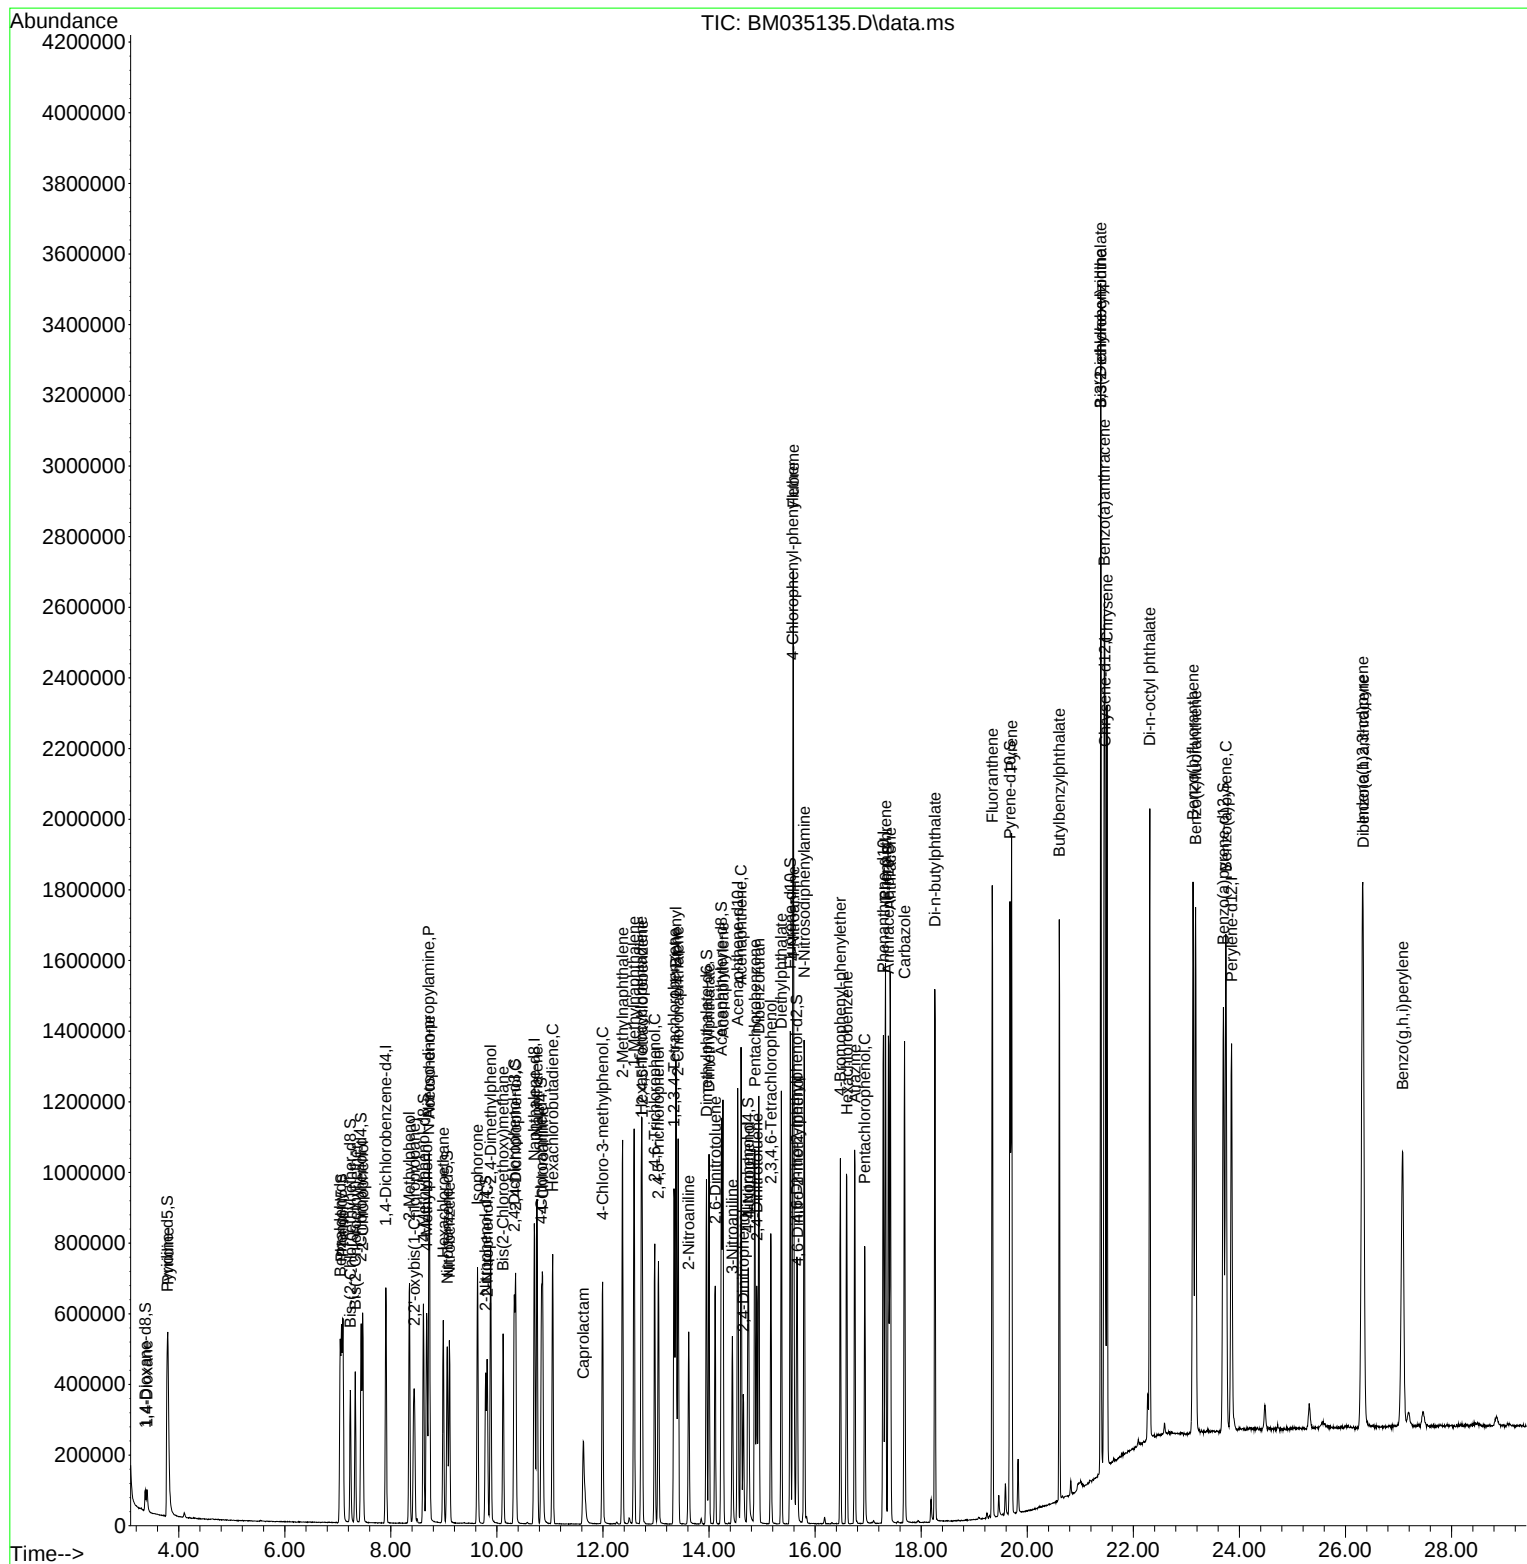




#2
1,4-Dioxane
Concen: 8.254 ng/uL
RT: 3.399 min Scan# 51
Delta R.T. -0.000 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43




Instrument :
BNA_M
ClientSampleId :
SSTD020125


Tgt Ion: 88 Resp: 36113
Ion Ratio Lower Upper
88 100
43 37.8 27.6 41.4
58 73.7 59.5 89.3



#5
Pyridine
Concen: 20.905 ng/uL
RT: 3.799 min Scan# 121
Delta R.T. 0.000 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43

Tgt Ion: 79 Resp: 235321
Ion Ratio Lower Upper
79 100
52 85.5 64.3 96.5
51 44.3 32.4 48.6









#6
Benzaldehyde
Concen: 25.262 ng/ul
RT: 7.046 min Scan# 673
Delta R.T. 0.000 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43




Instrument :
BNA_M
ClientSampleId :
SSTD020125


Tgt Ion: 77 Resp: 160712
Ion Ratio Lower Upper
77 100
105 98.9 77.4 116.0
106 91.1 73.4 110.2



#8
Phenol
Concen: 20.512 ng/ul
RT: 7.098 min Scan# 682
Delta R.T. 0.000 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43

Tgt Ion: 94 Resp: 276587
Ion Ratio Lower Upper
94 100
65 32.9 23.8 35.6
66 42.7 31.3 46.9









#10
Bis(2-Chloroethyl)ether
Concen: 21.128 ng/ul
RT: 7.328 min Scan# 721
Delta R.T. -0.006 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43




Instrument :
BNA_M
ClientSampleId :
SSTD020125


Tgt Ion: 93 Resp: 220829
Ion Ratio Lower Upper
93 100
63 79.9 62.5 93.7
95 30.9 25.8 38.8



#12
2-Chlorophenol
Concen: 20.992 ng/ul
RT: 7.469 min Scan# 745
Delta R.T. 0.000 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43

Tgt Ion:128 Resp: 243747
Ion Ratio Lower Upper
128 100
64 46.0 37.1 55.7
130 31.4 26.2 39.4





#13

2-Methylphenol

Concen: 20.252 ng/ul

RT: 8.351 min Scan# 895

Delta R.T. 0.000 min

Lab File: BM035135.D

Acq: 18 May 2022 09:43

Instrument :

BNA_M

ClientSampleId :





SSTD020125

Tgt Ion:108 Resp: 204974

Ion Ratio Lower Upper

108 100

107 89.5 70.8 106.2

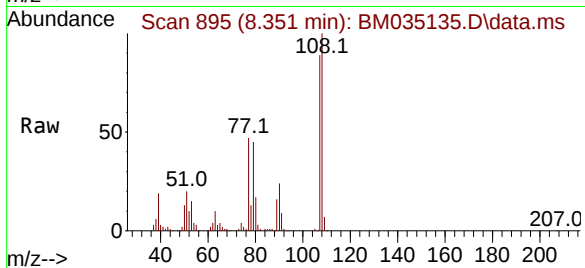

#14

2,2'-oxybis(1-Chloropropane)

Concen: 21.633 ng/ul

RT: 8.440 min Scan# 910

Delta R.T. 0.000 min

Lab File: BM035135.D

Acq: 18 May 2022 09:43




Tgt Ion: 45 Resp: 321195


Ion Ratio Lower Upper

45 100

77 13.5 10.6 15.8

79 10.8 8.1 12.1




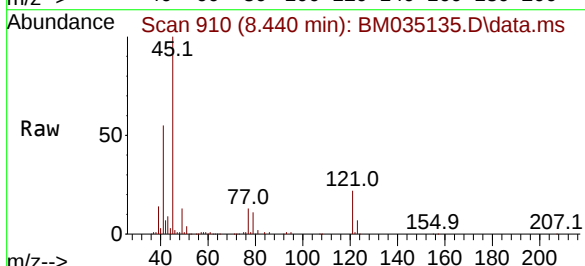




#16
Acetophenone
Concen: 20.526 ng/ul
RT: 8.728 min Scan# 959
Delta R.T. 0.000 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43




Instrument :
BNA_M
ClientSampleId :
SSTD020125


Tgt Ion:105 Resp: 342419
Ion Ratio Lower Upper
105 100
77 78.2 62.4 93.6
51 31.3 23.8 35.6



#17
N-Nitroso-di-n-propylamine
Concen: 21.102 ng/ul
RT: 8.716 min Scan# 957
Delta R.T. 0.000 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43

Tgt Ion: 70 Resp: 166900
Ion Ratio Lower Upper
70 100
42 72.0 53.3 79.9
101 9.9 8.2 12.4
130 22.2 18.3 27.5









#18
4-Methylphenol
Concen: 20.754 ng/ul
RT: 8.675 min Scan# 91
Delta R.T. -0.006 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43




Instrument :
BNA_M
ClientSampleId :
SSTD020125


Tgt Ion:108 Resp: 224470
Ion Ratio Lower Upper
108 100
107 115.7 89.7 134.5

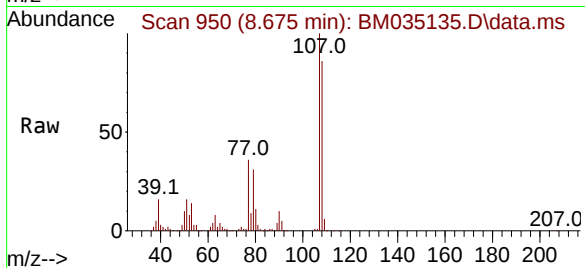

#19
Hexachloroethane
Concen: 20.727 ng/ul
RT: 8.987 min Scan# 1003
Delta R.T. -0.006 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43

Tgt Ion:117 Resp: 104619
Ion Ratio Lower Upper
117 100
201 100.2 81.3 121.9
199 63.2 53.4 80.0




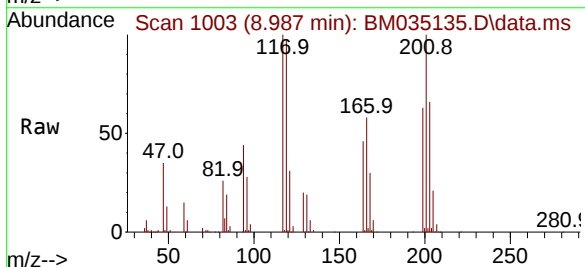




#22
Nitrobenzene
Concen: 20.664 ng/ul
RT: 9.104 min Scan# 1023
Delta R.T. 0.000 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43




Instrument :
BNA_M
ClientSampleId :
SSTD020125


Tgt Ion: 77 Resp: 262138
Ion Ratio Lower Upper
77 100
123 44.6 36.1 54.1
65 15.5 11.0 16.6



#23
Isophorone
Concen: 20.683 ng/ul
RT: 9.634 min Scan# 1113
Delta R.T. -0.006 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43

Tgt Ion: 82 Resp: 463062
Ion Ratio Lower Upper
82 100
95 7.7 6.2 9.4
138 17.7 15.3 22.9







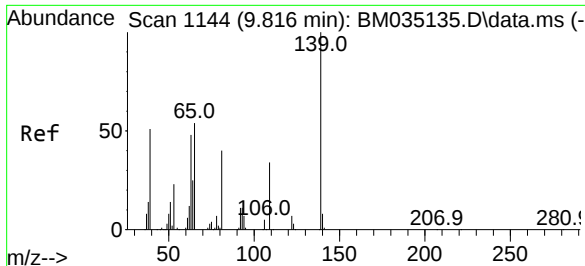

#25
2-Nitrophenol
Concen: 20.516 ng/ul
RT: 9.816 min Scan# 1144
Delta R.T. -0.006 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43




Instrument :
BNA_M
ClientSampleId :
SSTD020125


Tgt Ion:139 Resp: 130460
Ion Ratio Lower Upper
139 100
65 56.1 38.9 58.3
109 33.9 24.1 36.1

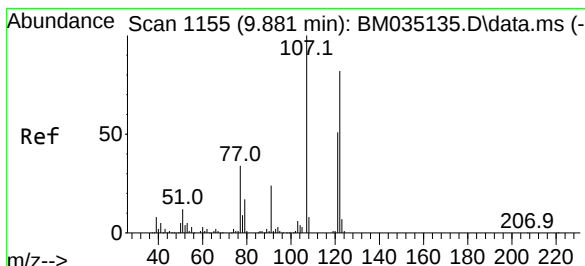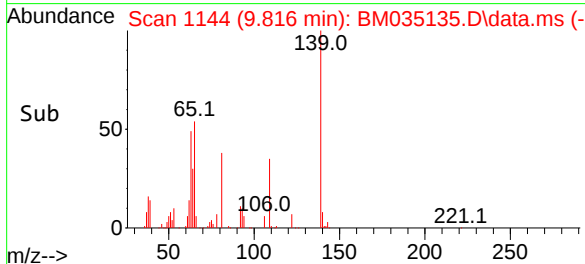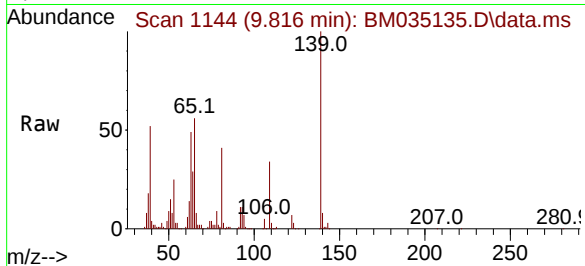

#26
2,4-Dimethylphenol
Concen: 20.605 ng/ul
RT: 9.881 min Scan# 1155
Delta R.T. -0.006 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43

Tgt Ion:107 Resp: 258257
Ion Ratio Lower Upper
107 100
121 50.8 40.3 60.5
122 83.5 66.6 100.0


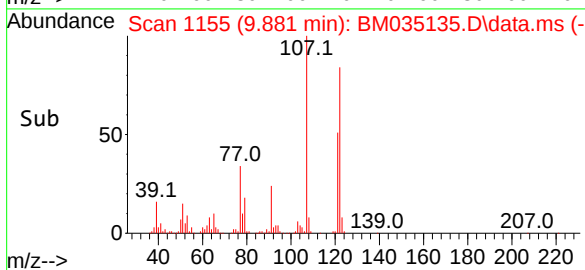

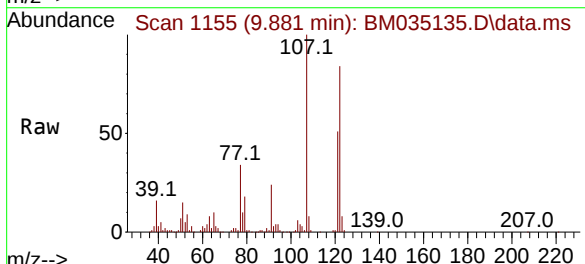




#27
 Bis(2-Chloroethoxy)methane
 Concen: 20.816 ng/ul
 RT: 10.116 min Scan# 1195
 Delta R.T. -0.006 min
 Lab File: BM035135.D
 Acq: 18 May 2022 09:43




Instrument :
 BNA_M
 ClientSampleId :
 SSTD020125


Tgt Ion: 93 Resp: 280529
 Ion Ratio Lower Upper
 93 100
 95 32.4 25.8 38.6
 123 11.5 9.2 13.8

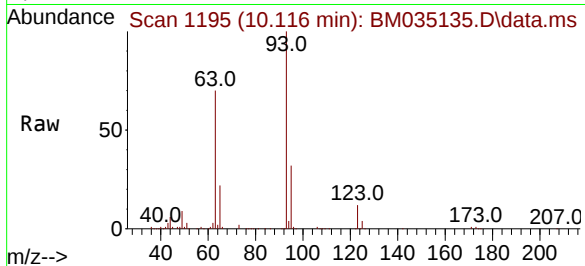

#29
 2,4-Dichlorophenol
 Concen: 20.105 ng/ul
 RT: 10.351 min Scan# 1235
 Delta R.T. -0.006 min
 Lab File: BM035135.D
 Acq: 18 May 2022 09:43

Tgt Ion: 162 Resp: 214184
 Ion Ratio Lower Upper
 162 100
 164 63.1 53.0 79.4
 98 35.2 27.4 41.0




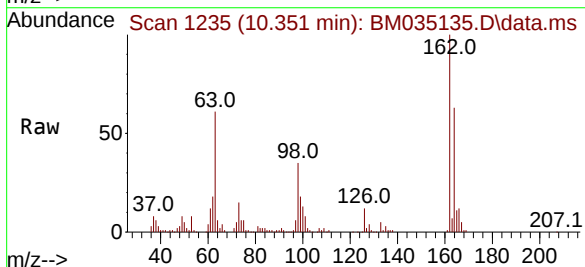




#30
Naphthalene
Concen: 20.552 ng/ul
RT: 10.757 min Scan# 1304
Delta R.T. 0.000 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43




Instrument :
BNA_M
ClientSampleId :
SSTD020125


Tgt Ion:128 Resp: 719300
Ion Ratio Lower Upper
128 100
129 11.3 9.1 13.7
127 13.5 10.6 16.0

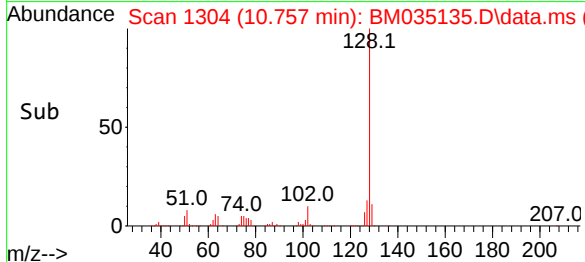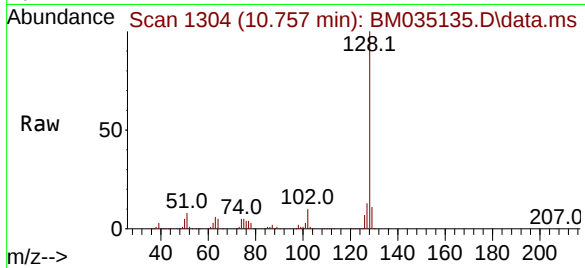

#32
4-Chloroaniline
Concen: 20.135 ng/ul
RT: 10.863 min Scan# 1322
Delta R.T. -0.006 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43

Tgt Ion:127 Resp: 293339
Ion Ratio Lower Upper
127 100
129 32.4 25.4 38.2


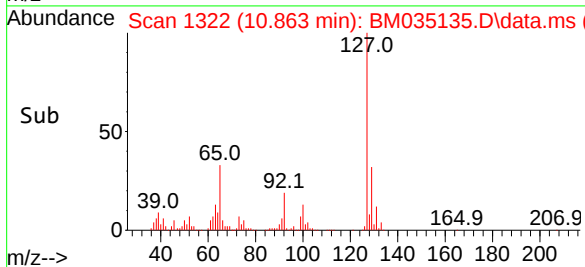

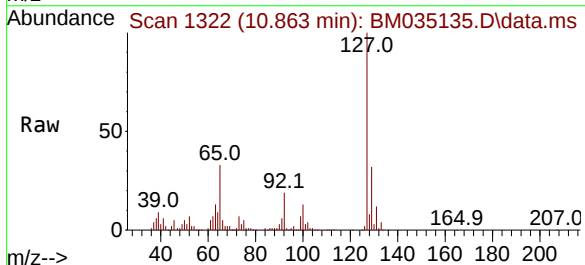




#33
Hexachlorobutadiene
Concen: 19.757 ng/ul
RT: 11.051 min Scan# 11
Delta R.T. 0.000 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43




Instrument :
BNA_M
ClientSampleId :
SSTD020125


Tgt Ion:225 Resp: 153052
Ion Ratio Lower Upper
225 100
223 62.6 49.8 74.8
227 63.8 49.6 74.4



#34
Caprolactam
Concen: 19.871 ng/ul
RT: 11.628 min Scan# 1452
Delta R.T. -0.006 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43

Tgt Ion:113 Resp: 60994
Ion Ratio Lower Upper
113 100
55 178.1 130.6 195.8
56 134.2 104.3 156.5




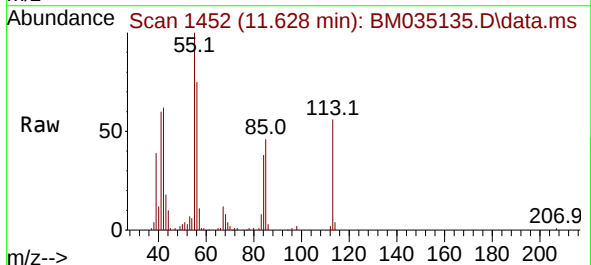




#35
4-Chloro-3-methylphenol
Concen: 20.618 ng/ul
RT: 11.992 min Scan# 11
Delta R.T. 0.000 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43




Instrument :
BNA_M
ClientSampleId :
SSTD020125


Tgt Ion:107 Resp: 220505
Ion Ratio Lower Upper
107 100
144 25.8 21.5 32.3
142 80.9 66.8 100.2

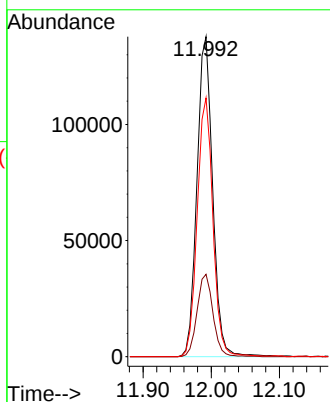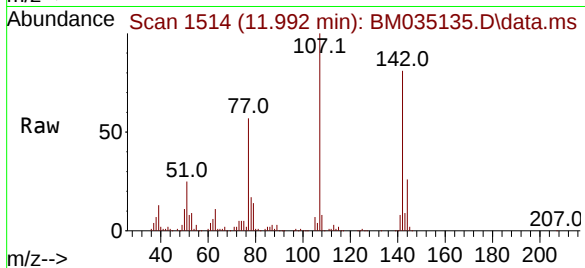

#36
2-Methylnaphthalene
Concen: 20.753 ng/ul
RT: 12.369 min Scan# 1578
Delta R.T. 0.000 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43

Tgt Ion:142 Resp: 486554
Ion Ratio Lower Upper
142 100
141 88.9 72.2 108.2

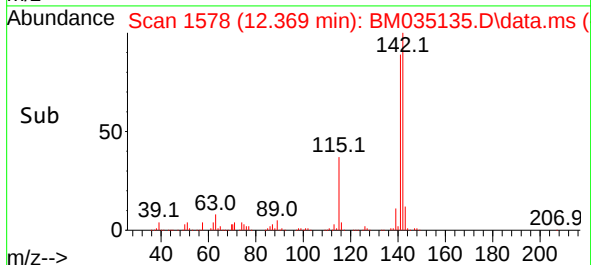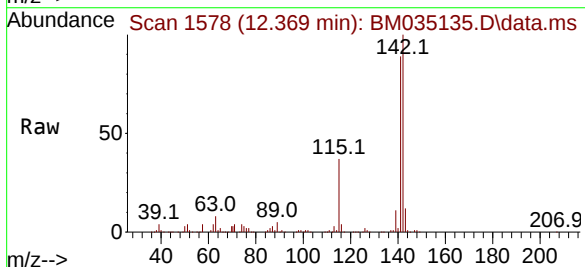



#37

1-Methylnaphthalene

Concen: 20.751 ng/ul

RT: 12.586 min Scan# 1

Delta R.T. 0.000 min

Lab File: BM035135.D

Acq: 18 May 2022 09:43

Instrument :

BNA_M

ClientSampleId :

SSTD020125





Tgt Ion:142 Resp: 487627

Ion Ratio Lower Upper

142 100

141 92.7 73.0 109.4

116 4.1 3.2 4.8

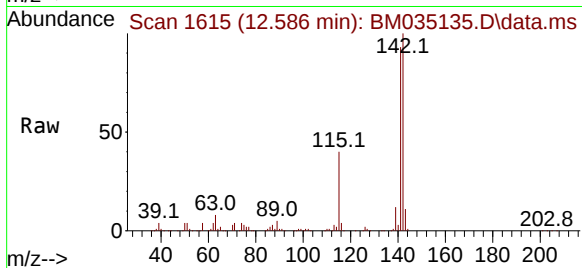

#39

1,2,4,5-Tetrachlorobenzene

Concen: 20.204 ng/ul

RT: 12.739 min Scan# 1641

Delta R.T. 0.000 min

Lab File: BM035135.D

Acq: 18 May 2022 09:43

Tgt Ion:216 Resp: 262050




Ion Ratio Lower Upper


216 100

214 78.6 64.5 96.7

179 21.7 17.9 26.9

108 18.0 15.0 22.4



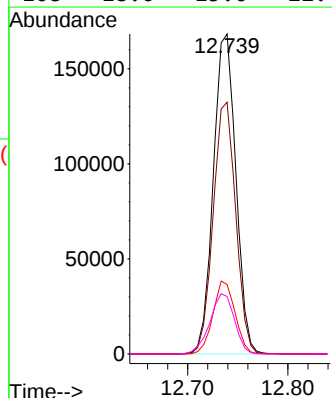
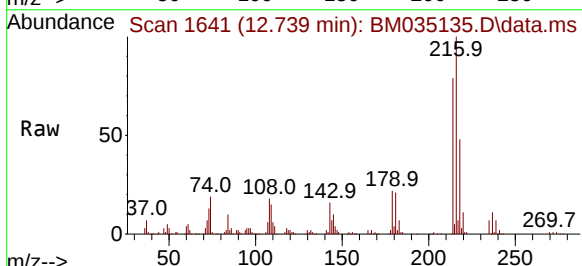




#40
Hexachlorocyclopentadiene
Concen: 18.683 ng/ul
RT: 12.722 min Scan# 1638
Delta R.T. 0.000 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43




Instrument :
BNA_M
ClientSampleId :
SSTD020125


Tgt Ion:237 Resp: 172792
Ion Ratio Lower Upper
237 100
235 62.2 49.2 73.8
272 12.1 10.0 15.0



#41
2,4,6-Trichlorophenol
Concen: 20.470 ng/ul
RT: 12.975 min Scan# 1681
Delta R.T. -0.006 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43

Tgt Ion:196 Resp: 169559
Ion Ratio Lower Upper
196 100
198 93.9 78.5 117.7
200 29.7 25.0 37.6




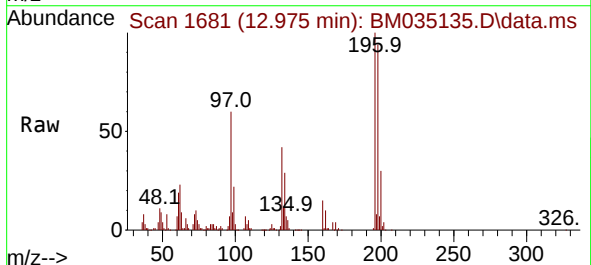




#42
2,4,5-Trichlorophenol
Concen: 20.406 ng/ul
RT: 13.045 min Scan# 1
Delta R.T. 0.000 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43




Instrument :
BNA_M
ClientSampleId :
SSTD020125


Tgt Ion:196 Resp: 179404
Ion Ratio Lower Upper
196 100
198 96.4 77.7 116.5
200 30.9 25.0 37.4



#43
1,1'-Biphenyl
Concen: 20.901 ng/ul
RT: 13.375 min Scan# 1749
Delta R.T. -0.006 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43

Tgt Ion:154 Resp: 652713
Ion Ratio Lower Upper
154 100
153 40.8 32.2 48.2
76 12.1 8.6 12.8





#44

2-Chloronaphthalene

Concen: 20.654 ng/ul

RT: 13.416 min Scan# 1756

Delta R.T. 0.000 min

Lab File: BM035135.D

Acq: 18 May 2022 09:43

Instrument :

BNA_M

ClientSampleId :

SSTD020125





Tgt Ion:162 Resp: 500135

Ion Ratio Lower Upper

162 100

164 32.7 25.7 38.5

127 39.5 29.8 44.8

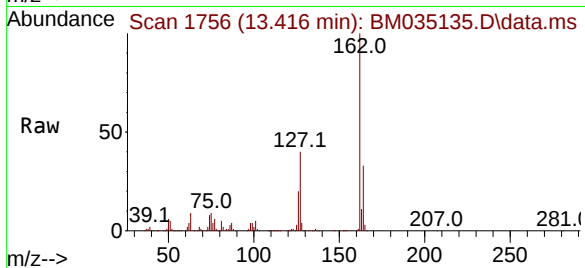

#45

2-Nitroaniline

Concen: 20.801 ng/ul

RT: 13.616 min Scan# 1790

Delta R.T. 0.000 min

Lab File: BM035135.D

Acq: 18 May 2022 09:43




Tgt Ion: 65 Resp: 141539


Ion Ratio Lower Upper

65 100

92 67.9 55.9 83.9

138 104.4 87.3 130.9




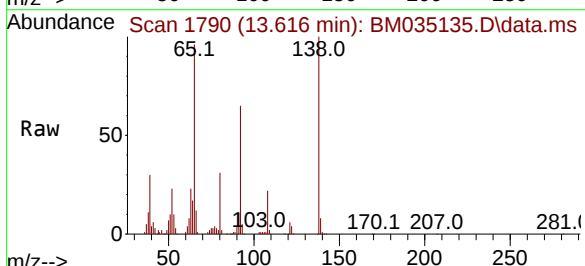


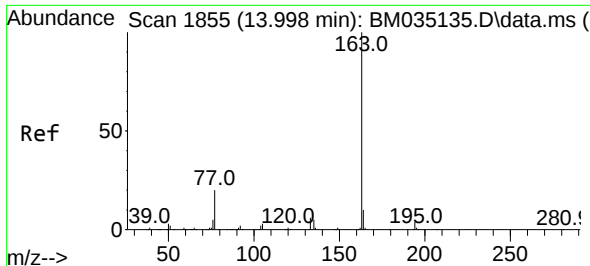

#47
Dimethylphthalate
Concen: 20.982 ng/ul
RT: 13.998 min Scan# 1855
Delta R.T. 0.000 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43




Instrument :
BNA_M
ClientSampleId :
SSTD020125


Tgt Ion:163 Resp: 617352
Ion Ratio Lower Upper
163 100
194 3.9 3.4 5.0
164 9.8 8.2 12.4

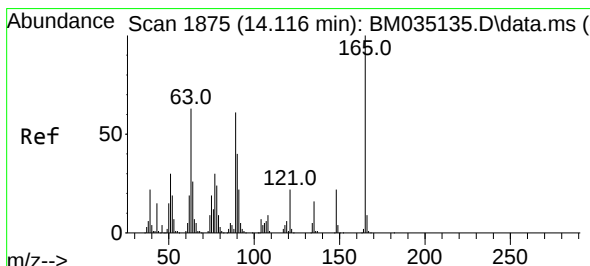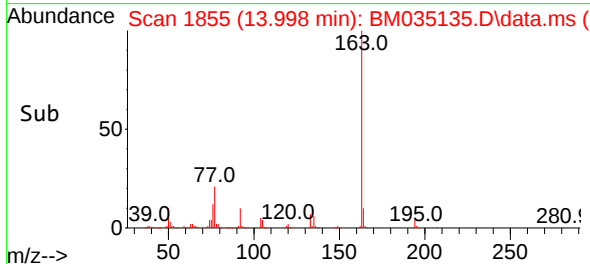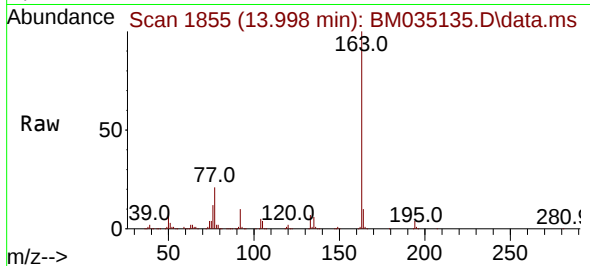

#48
2,6-Dinitrotoluene
Concen: 20.882 ng/ul
RT: 14.116 min Scan# 1875
Delta R.T. 0.000 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43

Tgt Ion:165 Resp: 122377
Ion Ratio Lower Upper
165 100
89 60.8 43.1 64.7
121 21.8 16.6 24.8


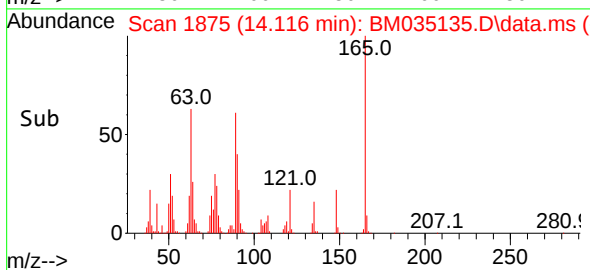

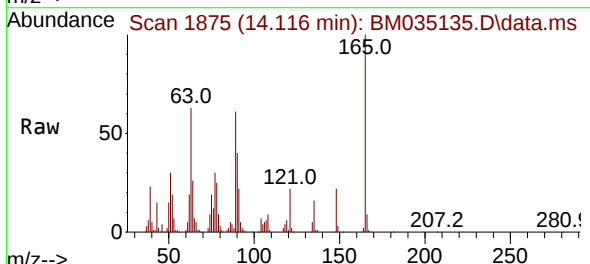




#50
Acenaphthylene
Concen: 21.068 ng/ul
RT: 14.263 min Scan# 1900
Delta R.T. 0.000 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43




Instrument :
BNA_M
ClientSampleId :
SSTD020125


Tgt Ion:152 Resp: 795219
Ion Ratio Lower Upper
152 100
151 19.6 15.3 22.9
153 13.3 10.2 15.4

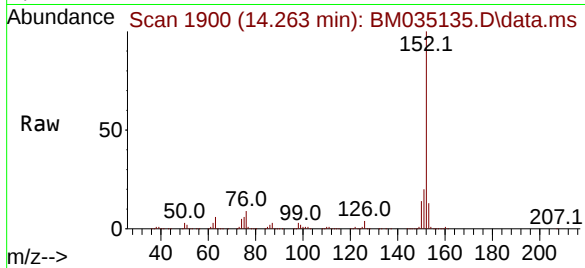

#51
3-Nitroaniline
Concen: 21.001 ng/ul
RT: 14.439 min Scan# 1930
Delta R.T. 0.000 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43

Tgt Ion:138 Resp: 118024
Ion Ratio Lower Upper
138 100
108 11.0 10.2 15.4
92 116.1 85.4 128.0


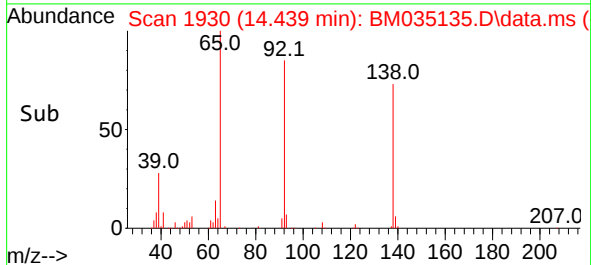

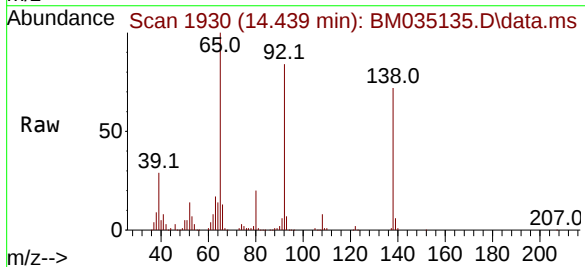


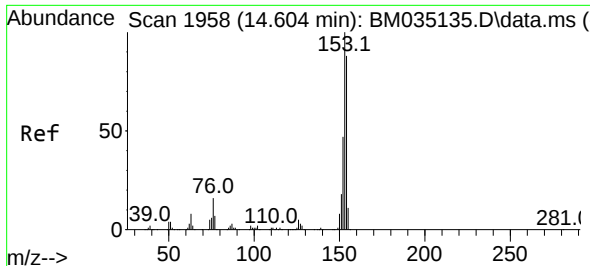

#52
Acenaphthene
Concen: 20.692 ng/ul
RT: 14.604 min Scan# 1958
Delta R.T. -0.006 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43




Instrument :
BNA_M
ClientSampleId :
SSTD020125


Tgt Ion:153 Resp: 520152
Ion Ratio Lower Upper
153 100
152 46.7 37.5 56.3
154 87.6 71.0 106.4

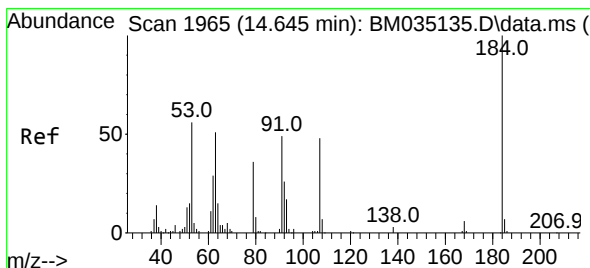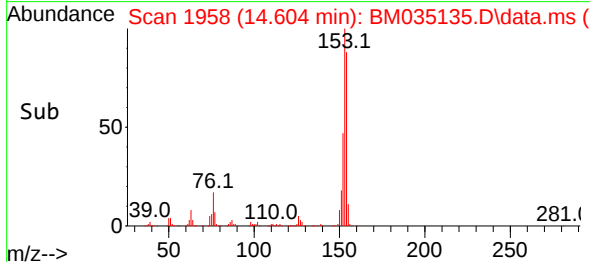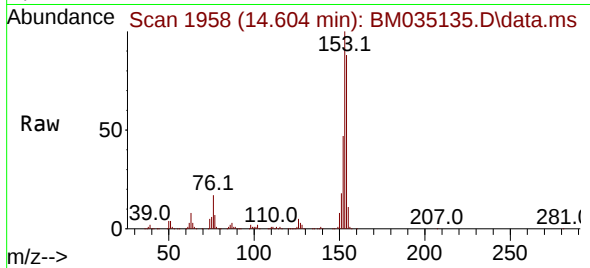

#53
2,4-Dinitrophenol
Concen: 18.018 ng/ul
RT: 14.645 min Scan# 1965
Delta R.T. -0.006 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43

Tgt Ion:184 Resp: 69177
Ion Ratio Lower Upper
184 100
63 76.0 51.8 77.6
154 67.7 54.3 81.5


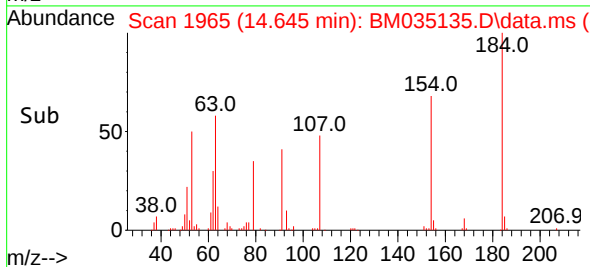

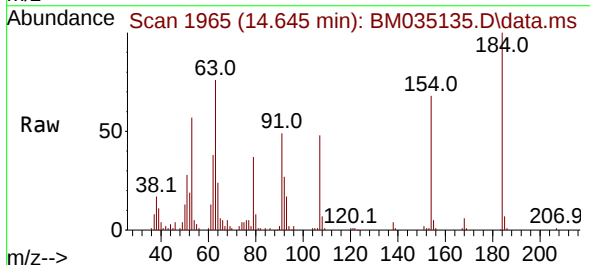




#55
4-Nitrophenol
Concen: 19.833 ng/ul
RT: 14.745 min Scan# 1982
Delta R.T. -0.006 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43




Instrument :
BNA_M
ClientSampleId :
SSTD020125


Tgt Ion:109 Resp: 96933
Ion Ratio Lower Upper
109 100
139 115.2 104.6 156.8
65 128.5 100.6 150.8

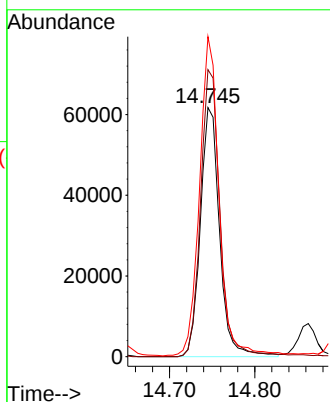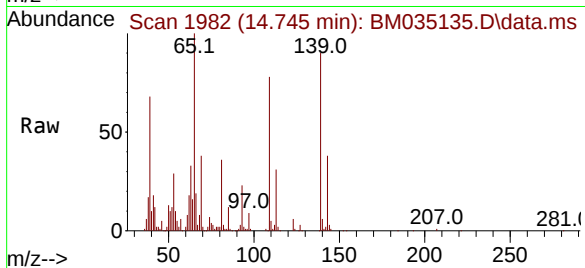

#56
Dibenzofuran
Concen: 20.820 ng/ul
RT: 14.939 min Scan# 2015
Delta R.T. 0.000 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43

Tgt Ion:168 Resp: 731962
Ion Ratio Lower Upper
168 100
139 40.1 30.0 45.0


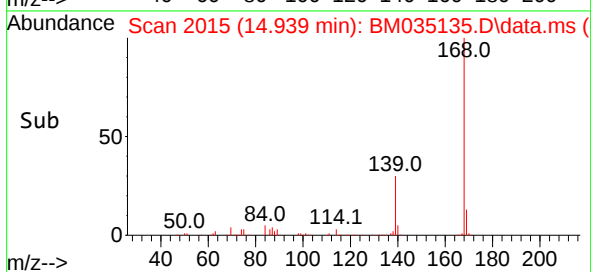
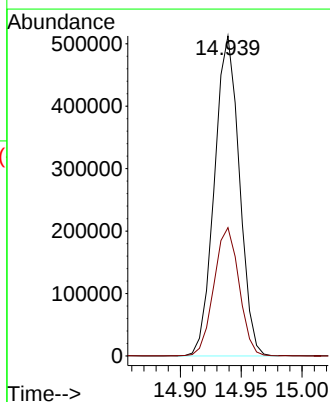
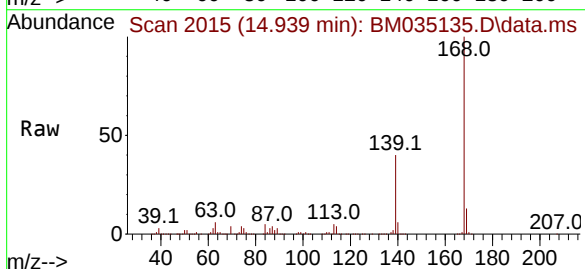




#57
2,4-Dinitrotoluene
Concen: 21.045 ng/ul
RT: 14.904 min Scan# 2009
Delta R.T. 0.000 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43




Instrument :
BNA_M
ClientSampleId :
SSTD020125


Tgt Ion:165 Resp: 173185
Ion Ratio Lower Upper
165 100
63 46.8 34.2 51.4
182 2.7 2.2 3.2

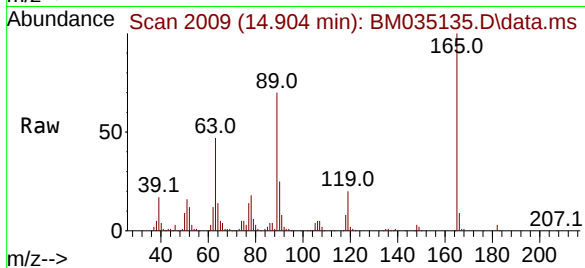

#58
2,3,4,6-Tetrachlorophenol
Concen: 20.479 ng/ul
RT: 15.169 min Scan# 2054
Delta R.T. 0.000 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43

Tgt Ion:232 Resp: 145860
Ion Ratio Lower Upper
232 100
131 47.5 39.6 59.4
130 2.7 2.1 3.1
166 31.6 27.7 41.5



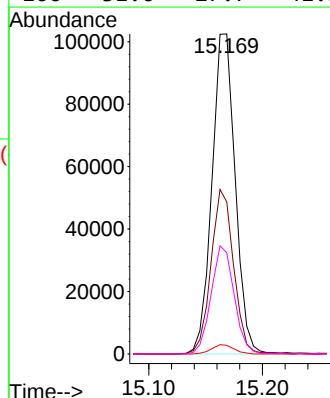
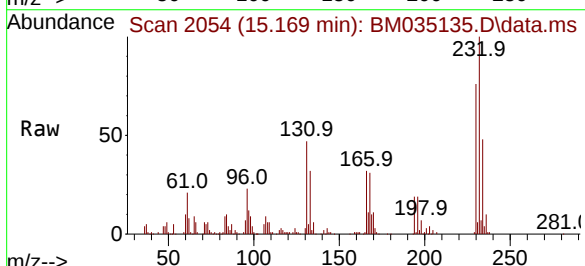




#59
Diethylphthalate
Concen: 20.975 ng/ul
RT: 15.363 min Scan# 2087
Delta R.T. -0.006 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43




Instrument :
BNA_M
ClientSampleId :
SSTD020125


Tgt Ion:149 Resp: 624938
Ion Ratio Lower Upper
149 100
177 20.8 17.2 25.8
150 12.6 9.8 14.6



#61
Fluorene
Concen: 20.898 ng/ul
RT: 15.586 min Scan# 2125
Delta R.T. -0.006 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43

Tgt Ion:166 Resp: 597773
Ion Ratio Lower Upper
166 100
165 98.9 77.9 116.9
167 13.2 10.3 15.5









#62
4-Chlorophenyl-phenylether
Concen: 20.539 ng/ul
RT: 15.580 min Scan# 2124
Delta R.T. -0.006 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43




Instrument :
BNA_M
ClientSampleId :
SSTD020125


Tgt Ion:204 Resp: 298257
Ion Ratio Lower Upper
204 100
206 32.9 26.2 39.4
141 64.4 49.5 74.3



#63
4-Nitroaniline
Concen: 22.512 ng/ul
RT: 15.598 min Scan# 2127
Delta R.T. -0.006 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43

Tgt Ion:138 Resp: 114624
Ion Ratio Lower Upper
138 100
92 53.0 37.2 55.8
108 87.5 58.4 87.6




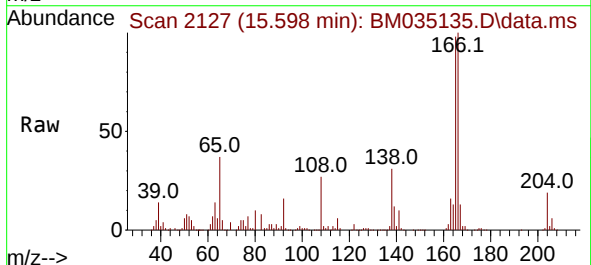




#66
4,6-Dinitro-2-methylphenol
Concen: 19.388 ng/ul
RT: 15.669 min Scan# 2139
Delta R.T. 0.000 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43




Instrument :
BNA_M
ClientSampleId :
SSTD020125


Tgt Ion:198 Resp: 100934
Ion Ratio Lower Upper
198 100
182 3.8 4.6 6.8#
77 25.0 22.2 33.2



#67
N-Nitrosodiphenylamine
Concen: 20.725 ng/ul
RT: 15.792 min Scan# 2160
Delta R.T. -0.006 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43

Tgt Ion:169 Resp: 504298
Ion Ratio Lower Upper
169 100
168 67.6 54.8 82.2
167 36.3 28.9 43.3




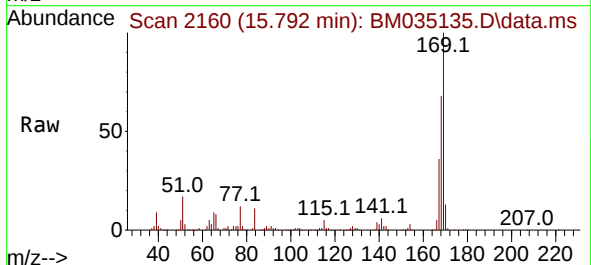




#68
4-Bromophenyl-phenylether
Concen: 20.227 ng/ul
RT: 16.474 min Scan# 21
Delta R.T. -0.006 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43




Instrument :
BNA_M
ClientSampleId :
SSTD020125


Tgt Ion:248 Resp: 172311
Ion Ratio Lower Upper
248 100
250 95.6 77.9 116.9
141 84.1 61.0 91.4



#69
Hexachlorobenzene
Concen: 20.251 ng/ul
RT: 16.598 min Scan# 2297
Delta R.T. 0.000 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43

Tgt Ion:284 Resp: 197007
Ion Ratio Lower Upper
284 100
142 38.2 31.2 46.8
249 32.2 25.9 38.9

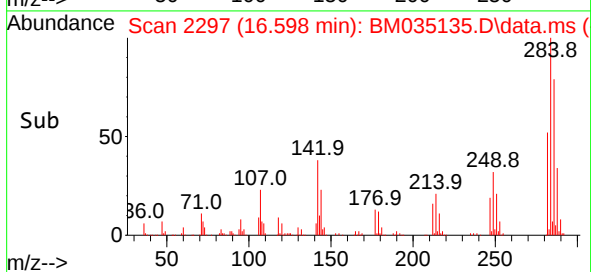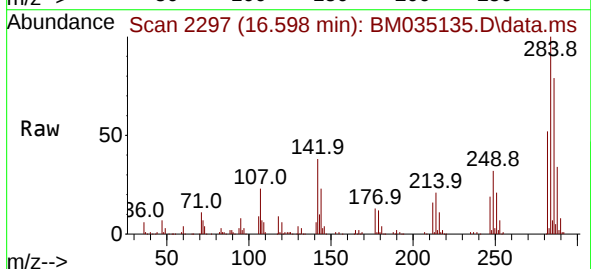



#70

Atrazine

Concen: 19.461 ng/ul

RT: 16.751 min Scan# 21

Delta R.T. 0.000 min

Lab File: BM035135.D

Acq: 18 May 2022 09:43

Instrument :

BNA_M

ClientSampleId :

SSTD020125





Tgt Ion:200 Resp: 184769

Ion Ratio Lower Upper

200 100

173 25.8 21.3 31.9

215 46.2 37.1 55.7



#71

Pentachlorophenol

Concen: 18.729 ng/ul

RT: 16.933 min Scan# 2354

Delta R.T. -0.006 min

Lab File: BM035135.D

Acq: 18 May 2022 09:43




Tgt Ion:266 Resp: 121755


Ion Ratio Lower Upper

266 100

264 60.8 48.4 72.6

268 62.8 50.6 76.0









#72
Phenanthrene
Concen: 20.582 ng/ul
RT: 17.327 min Scan# 2421
Delta R.T. 0.000 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43




Instrument :
BNA_M
ClientSampleId :
SSTD020125


Tgt Ion:178 Resp: 896428
Ion Ratio Lower Upper
178 100
179 15.0 12.2 18.4
176 19.2 15.0 22.6

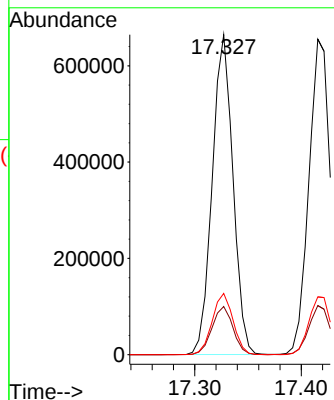

#74
Anthracene
Concen: 20.872 ng/ul
RT: 17.415 min Scan# 2436
Delta R.T. -0.006 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43

Tgt Ion:178 Resp: 926349
Ion Ratio Lower Upper
178 100
179 15.6 12.2 18.4
176 18.3 14.6 22.0



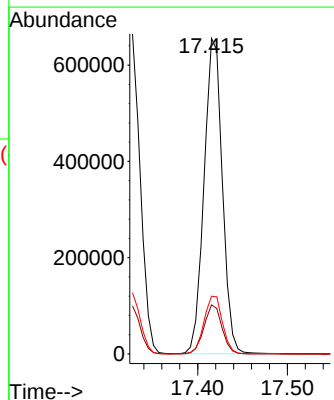





#75
1,2,3,4-Tetrachlorobenzene
Concen: 19.364 ng/uL
RT: 13.339 min Scan# 11
Delta R.T. -0.006 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43




Instrument :
BNA_M
ClientSampleId :
SSTD020125


Tgt Ion:216 Resp: 271324
Ion Ratio Lower Upper
216 100
214 77.7 62.6 94.0
218 47.6 37.1 55.7



#76
Pentachlorobenzene
Concen: 20.314 ng/uL
RT: 14.863 min Scan# 2002
Delta R.T. 0.000 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43

Tgt Ion:250 Resp: 244516
Ion Ratio Lower Upper
250 100
248 63.2 49.9 74.9
252 63.0 51.5 77.3




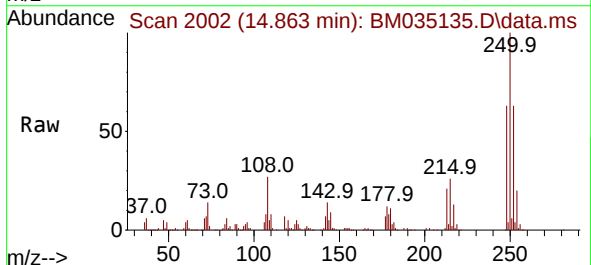




#77
 Carbazole
 Concen: 20.671 ng/ul
 RT: 17.686 min Scan# 2482
 Delta R.T. 0.000 min
 Lab File: BM035135.D
 Acq: 18 May 2022 09:43




Instrument :
 BNA_M
 ClientSampleId :
 SSTD020125


Tgt Ion:167 Resp: 811911
 Ion Ratio Lower Upper
 167 100
 166 21.6 17.1 25.7
 139 12.9 10.5 15.7

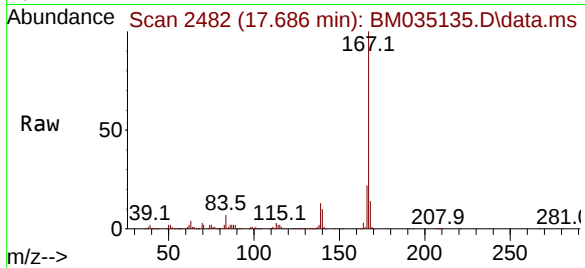

#78
 Di-n-butylphthalate
 Concen: 18.229 ng/ul
 RT: 18.257 min Scan# 2579
 Delta R.T. -0.006 min
 Lab File: BM035135.D
 Acq: 18 May 2022 09:43

Tgt Ion:149 Resp: 1024650
 Ion Ratio Lower Upper
 149 100
 150 9.5 7.1 10.7
 104 5.7 4.1 6.1


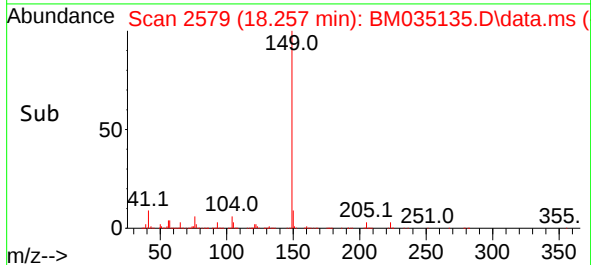

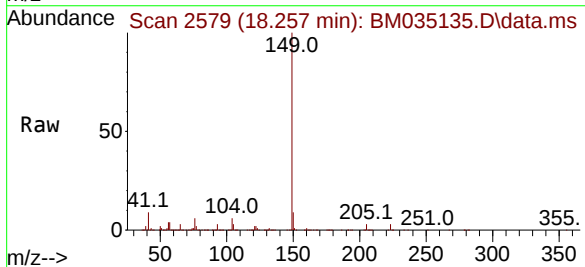




#80
Fluoranthene
Concen: 20.376 ng/u1
RT: 19.339 min Scan# 21
Delta R.T. -0.006 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43




Instrument :
BNA_M
ClientSampleId :
SSTD020125


Tgt Ion:202 Resp: 1028251
Ion Ratio Lower Upper
202 100
101 9.7 7.4 11.2
100 7.7 5.8 8.6

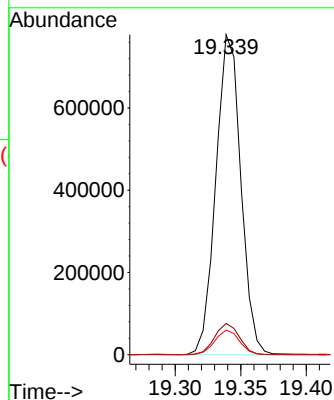

#82
Pyrene
Concen: 20.525 ng/u1
RT: 19.704 min Scan# 2825
Delta R.T. -0.006 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43

Tgt Ion:202 Resp: 1066109
Ion Ratio Lower Upper
202 100
101 10.9 9.4 14.0
100 9.6 7.8 11.6



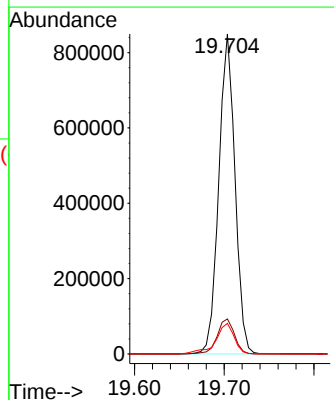
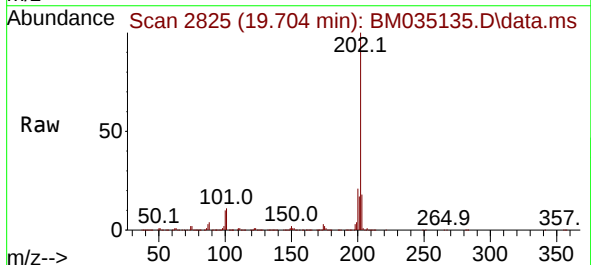




#83
 Butylbenzylphthalate
 Concen: 20.214 ng/ul
 RT: 20.603 min Scan# 2978
 Delta R.T. -0.006 min
 Lab File: BM035135.D
 Acq: 18 May 2022 09:43




Instrument :
 BNA_M
 ClientSampleId :
 SSTD020125


Tgt Ion:149 Resp: 449763
 Ion Ratio Lower Upper
 149 100
 91 72.0 54.3 81.5
 206 19.1 15.8 23.6



#84
 3,3'-Dichlorobenzidine
 Concen: 20.861 ng/ul
 RT: 21.386 min Scan# 3111
 Delta R.T. 0.000 min
 Lab File: BM035135.D
 Acq: 18 May 2022 09:43

Tgt Ion:252 Resp: 338273
 Ion Ratio Lower Upper
 252 100
 254 65.2 51.0 76.4
 126 10.0 9.0 13.6





#85

Benzo(a)anthracene

Concen: 20.716 ng/ul

RT: 21.450 min Scan# 3122

Delta R.T. -0.006 min

Lab File: BM035135.D

Acq: 18 May 2022 09:43

Instrument :

BNA_M

ClientSampleId :

SSTD020125





Tgt Ion:228 Resp: 1043918

Ion Ratio Lower Upper

228 100

229 20.1 15.4 23.0

226 27.3 21.7 32.5

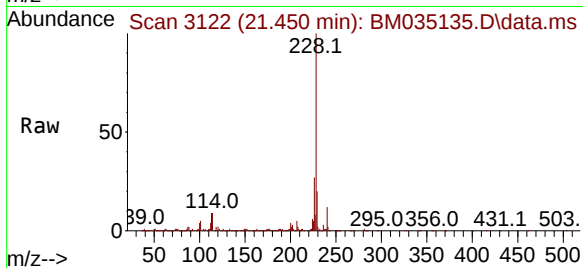

#86

Bis(2-ethylhexyl)phthalate

Concen: 20.634 ng/ul

RT: 21.386 min Scan# 3111

Delta R.T. -0.006 min

Lab File: BM035135.D

Acq: 18 May 2022 09:43




Tgt Ion:149 Resp: 690334


Ion Ratio Lower Upper

149 100

167 26.5 21.4 32.0

279 3.7 3.4 5.2




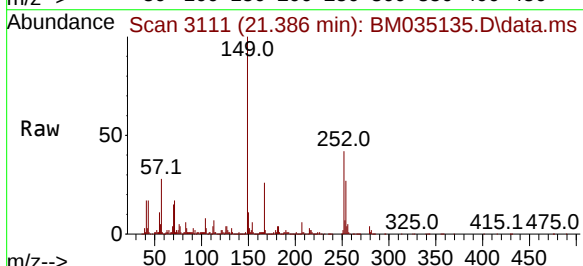




#87
Chrysene
Concen: 20.834 ng/ul
RT: 21.503 min Scan# 3131
Delta R.T. -0.006 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43




Instrument :
BNA_M
ClientSampleId :
SSTD020125


Tgt Ion:228 Resp: 1023634
Ion Ratio Lower Upper
228 100
226 30.1 23.7 35.5
229 19.4 15.7 23.5



#89
Di-n-octyl phthalate
Concen: 19.950 ng/ul
RT: 22.309 min Scan# 3268
Delta R.T. -0.006 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43

Tgt Ion:149 Resp: 1144898









#90
Benzo(b)fluoranthene
Concen: 20.913 ng/ul
RT: 23.127 min Scan# 3407
Delta R.T. -0.006 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43




Instrument :
BNA_M
ClientSampleId :
SSTD020125


Tgt Ion:252 Resp: 1088583
Ion Ratio Lower Upper
252 100
253 21.5 17.4 26.0
125 8.7 7.6 11.4



#91
Benzo(k)fluoranthene
Concen: 20.472 ng/ul
RT: 23.174 min Scan# 3415
Delta R.T. -0.006 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43

Tgt Ion:252 Resp: 1012359
Ion Ratio Lower Upper
252 100
253 22.1 17.4 26.2
125 9.7 7.8 11.6









#93
Benzo(a)pyrene
Concen: 20.807 ng/ul
RT: 23.744 min Scan# 3512
Delta R.T. -0.012 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43




Instrument :
BNA_M
ClientSampleId :
SSTD020125


Tgt Ion:252 Resp: 1055234
Ion Ratio Lower Upper
252 100
253 21.5 16.6 25.0
125 10.5 6.2 9.2#



#94
Indeno(1,2,3-cd)pyrene
Concen: 20.745 ng/ul
RT: 26.321 min Scan# 3950
Delta R.T. -0.012 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43

Tgt Ion:276 Resp: 1208990
Ion Ratio Lower Upper
276 100
138 22.7 15.3 22.9
277 24.0 19.6 29.4









#95
Dibenzo(a,h)anthracene
Concen: 20.656 ng/ul
RT: 26.333 min Scan# 3952
Delta R.T. -0.012 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43

Instrument :
BNA_M
ClientSampleId :
SSTD020125

Tgt Ion:278 Resp: 1034021
Ion Ratio Lower Upper
278 100
139 15.4 9.7 14.5#
279 24.1 18.8 28.2



#96
Benzo(g,h,i)perylene
Concen: 20.785 ng/ul
RT: 27.080 min Scan# 4079
Delta R.T. -0.006 min
Lab File: BM035135.D
Acq: 18 May 2022 09:43

Tgt Ion:276 Resp: 1007631
Ion Ratio Lower Upper
276 100
138 18.9 13.0 19.6
277 23.1 18.6 28.0

