




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051822\
 Data File : BM035137.D
 Acq On : 18 May 2022 10:55
 Operator : CG/JU
 Sample : N2766-04
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4F4

Manual IntegrationsAPPROVED

Quant Time: May 19 00:49:13 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM051722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 17 16:13:52 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/19/2022
 Supervised By :mohammad ahmed 05/19/2022

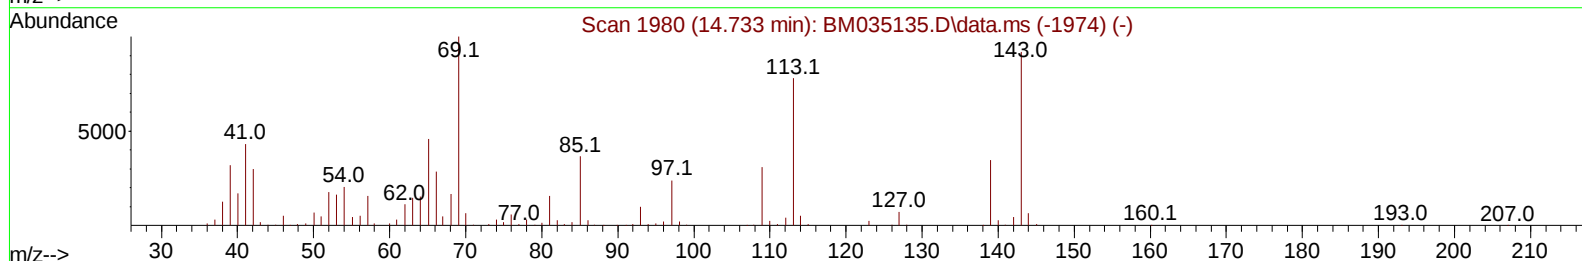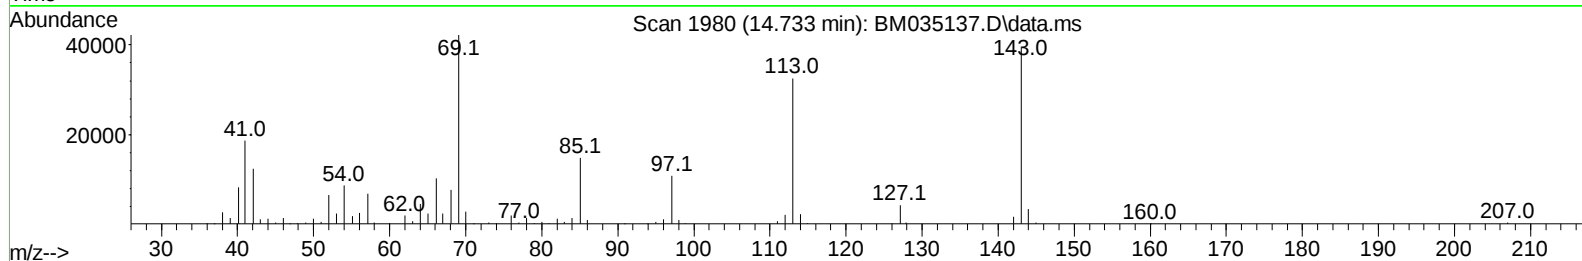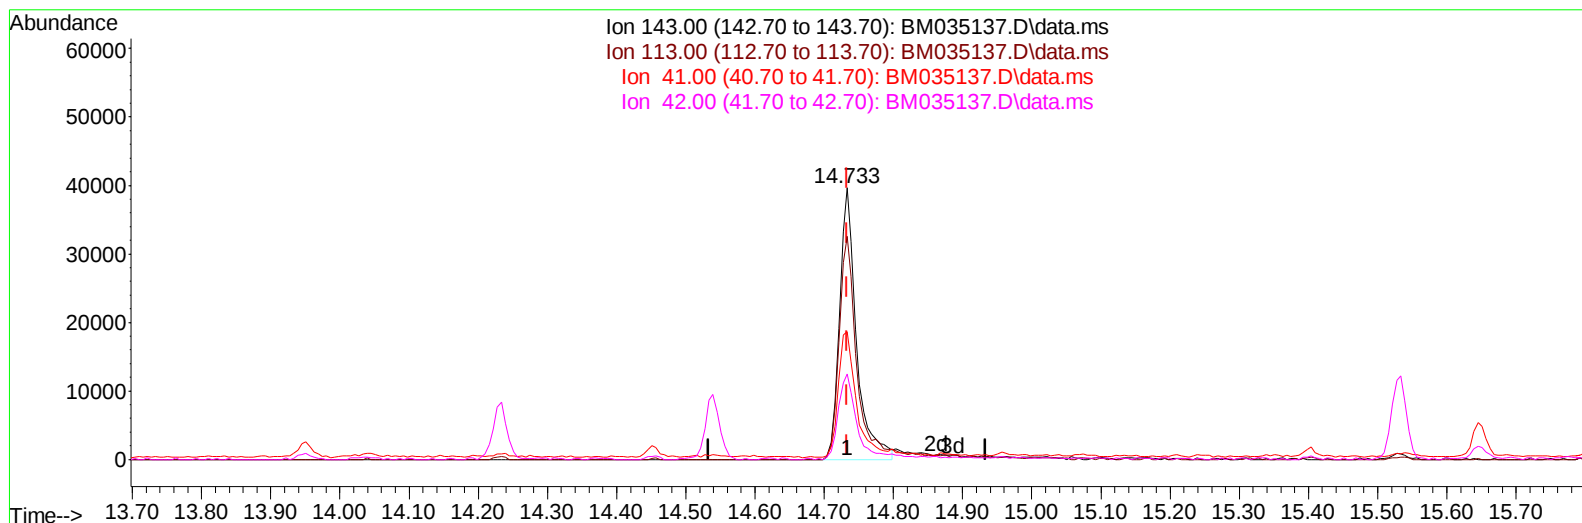

TIC: BM035137.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.733min (+ 0.000) 15.26 ng/u1

response 67301

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	80.00	82.16
41.00	42.20	47.08
42.00	28.30	31.38




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051822\
Data File : BM035137.D
Acq On : 18 May 2022 10:55
Operator : CG/JU
Sample : N2766-04
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4F4

Manual IntegrationsAPPROVED

Quant Time: May 19 00:49:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM051722.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 17 16:13:52 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/19/2022
Supervised By :mohammad ahmed 05/19/2022

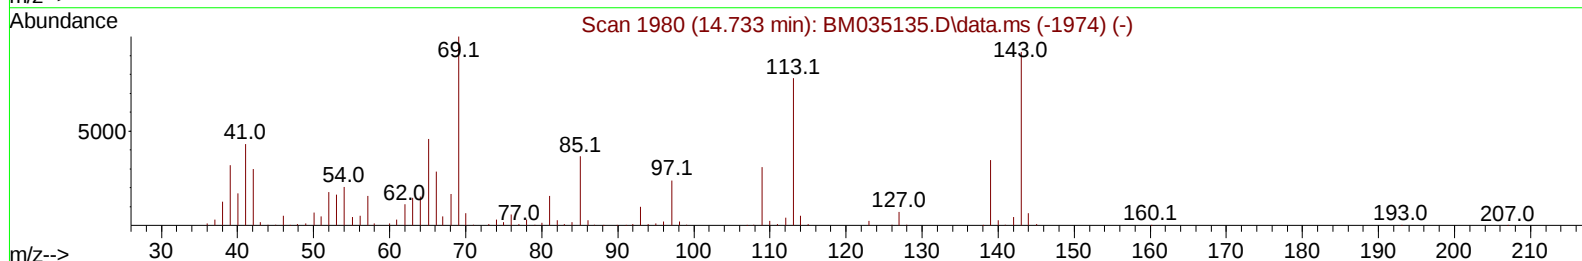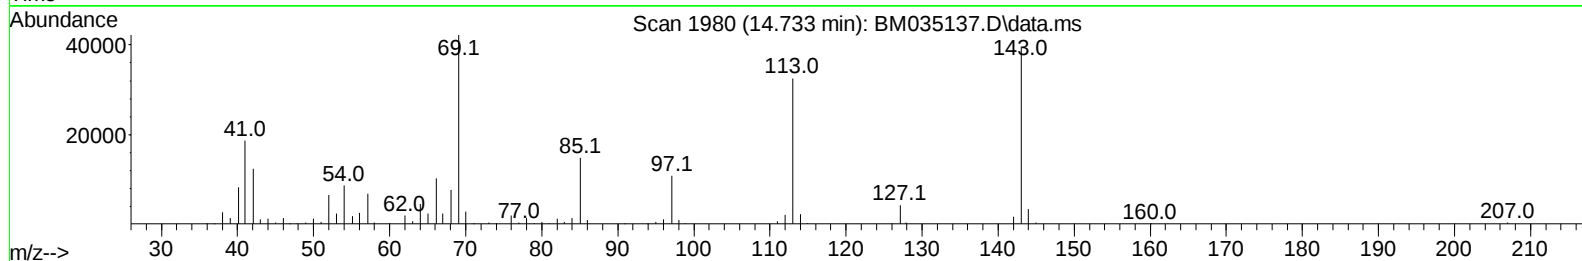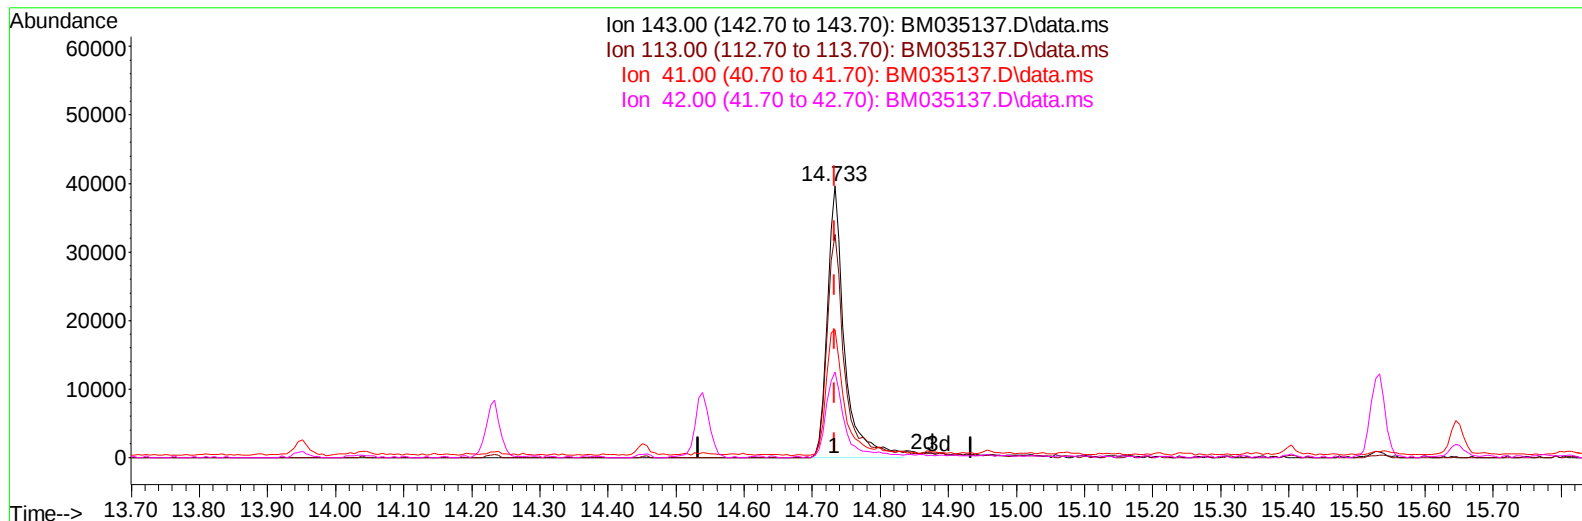

TIC: BM035137.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.733min (+ 0.000) 15.81 ng/ul m

response 69700

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	80.00	82.16
41.00	42.20	47.08
42.00	28.30	31.38

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051822\
 Data File : BM035137.D
 Acq On : 18 May 2022 10:55
 Operator : CG/JU
 Sample : N2766-04
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4F4

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/19/2022
 Supervised By :mohammad ahmed 05/19/2022

Quant Time: May 19 00:49:13 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM051722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 17 16:13:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.904	152	147064	20.000	ng/ul	0.00
20) Naphthalene-d8	10.704	136	571833	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.539	164	341372	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.286	188	667199	20.000	ng/ul	0.00
79) Chrysene-d12	21.468	240	613770	20.000	ng/ul	0.00
88) Perylene-d12	23.850	264	632834	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.369	96	15603	4.384	ng/uL	0.00
4) Pyridine-d5	3.781	84	200204	21.805	ng/ul	0.00
7) Phenol-d5	7.069	99	247278	22.815	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.234	67	168598	24.655	ng/ul	0.00
11) 2-Chlorophenol-d4	7.440	132	221657	23.070	ng/ul	0.00
15) 4-Methylphenol-d8	8.610	113	209847	23.048	ng/ul	0.00
21) Nitrobenzene-d5	9.063	128	103395	23.062	ng/ul	0.00
24) 2-Nitrophenol-d4	9.787	143	113268	22.564	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.328	165	192592	21.570	ng/ul	0.00
31) 4-Chloroaniline-d4	10.839	131	270645	21.982	ng/ul	0.00
46) Dimethylphthalate-d6	13.951	166	663665	26.684	ng/ul	0.00
49) Acenaphthylene-d8	14.233	160	765419	25.750	ng/ul	0.00
54) 4-Nitrophenol-d4	14.733	143	69700m	15.807	ng/ul	0.00
60) Fluorene-d10	15.533	176	563835	26.797	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.651	200	66532	15.443	ng/ul	0.00
73) Anthracene-d10	17.380	188	840030	27.049	ng/ul	0.00
81) Pyrene-d10	19.674	212	944810	28.902	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.697	264	894056	27.877	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051822\
Data File : BM035137.D
Acq On : 18 May 2022 10:55
Operator : CG/JU
Sample : N2766-04
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4F4

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/19/2022
Supervised By :mohammad ahmed 05/19/2022

Quant Time: May 19 00:49:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM051722.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 17 16:13:52 2022
Response via : Initial Calibration

