




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051822\
 Data File : BM035146.D
 Acq On : 18 May 2022 16:21
 Operator : CG/JU
 Sample : N2766-11
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4G1

Manual IntegrationsAPPROVED

Quant Time: May 19 00:50:00 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM051722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 17 16:13:52 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/19/2022
 Supervised By :mohammad ahmed 05/19/2022

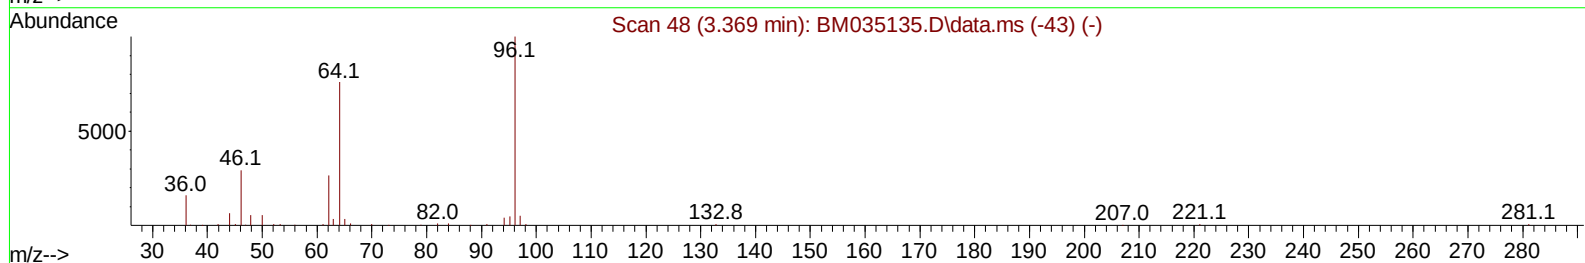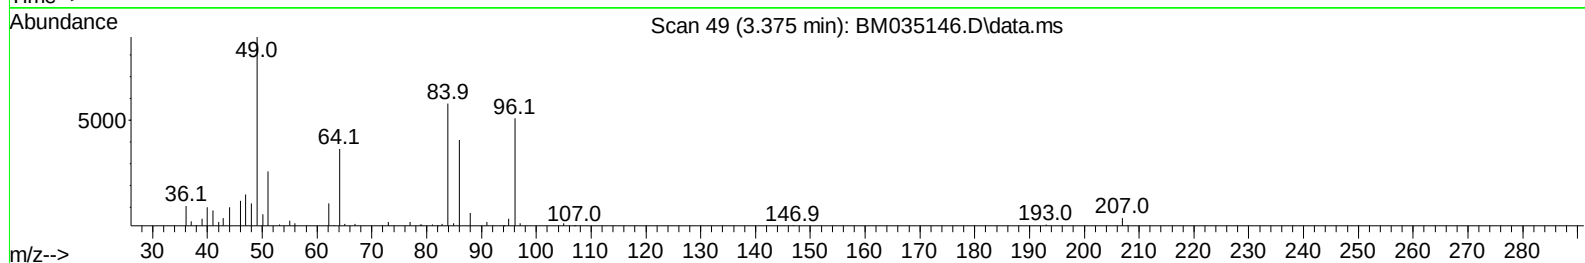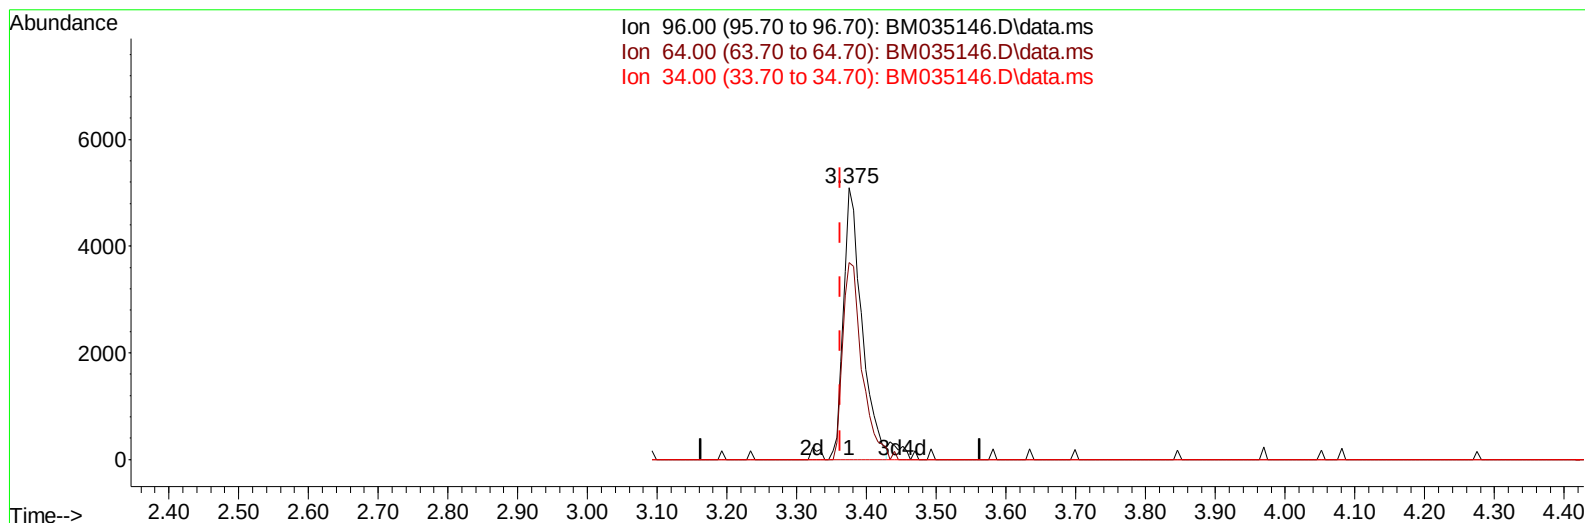

TIC: BM035146.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.375min (+ 0.012) 2.32 ng/uL

response 9397

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	72.40	72.53
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051822\
 Data File : BM035146.D
 Acq On : 18 May 2022 16:21
 Operator : CG/JU
 Sample : N2766-11
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4G1

Manual IntegrationsAPPROVED

Quant Time: May 19 00:50:00 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM051722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 17 16:13:52 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/19/2022
 Supervised By :mohammad ahmed 05/19/2022

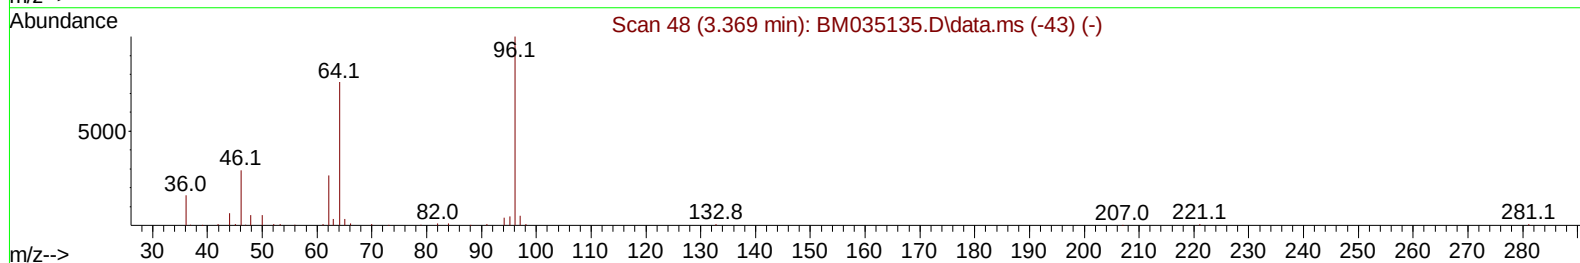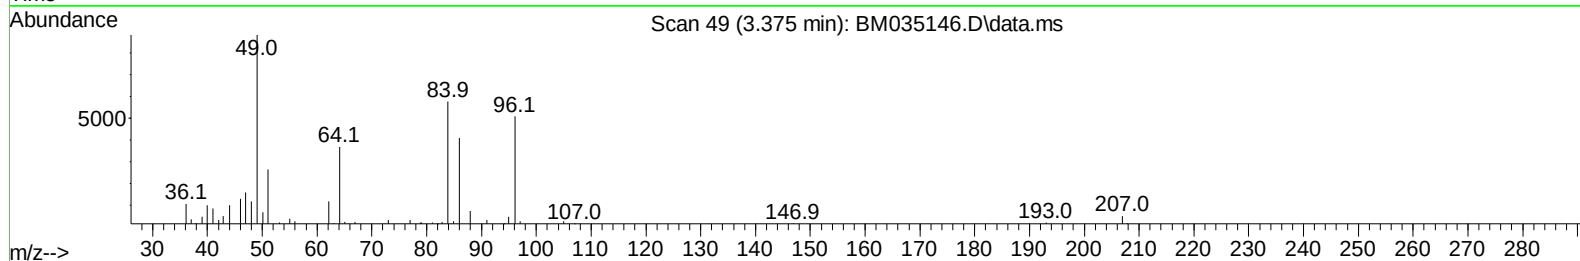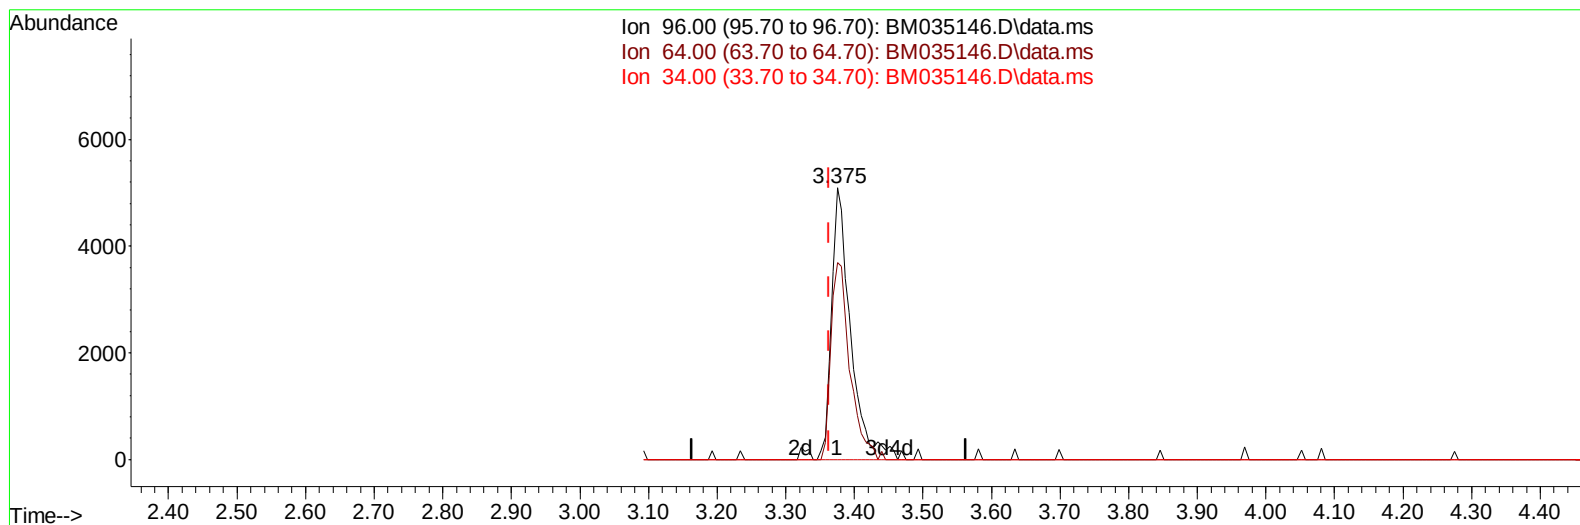

TIC: BM035146.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.375min (+ 0.012) 2.43 ng/uL m

response 9810

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	72.40	72.53
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051822\
 Data File : BM035146.D
 Acq On : 18 May 2022 16:21
 Operator : CG/JU
 Sample : N2766-11
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4G1

Manual IntegrationsAPPROVED

Quant Time: May 19 00:50:00 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM051722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 17 16:13:52 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/19/2022
 Supervised By :mohammad ahmed 05/19/2022

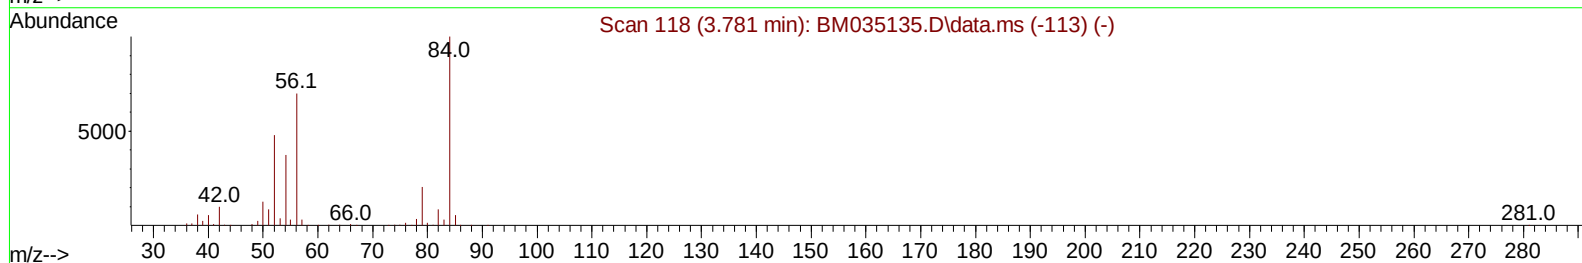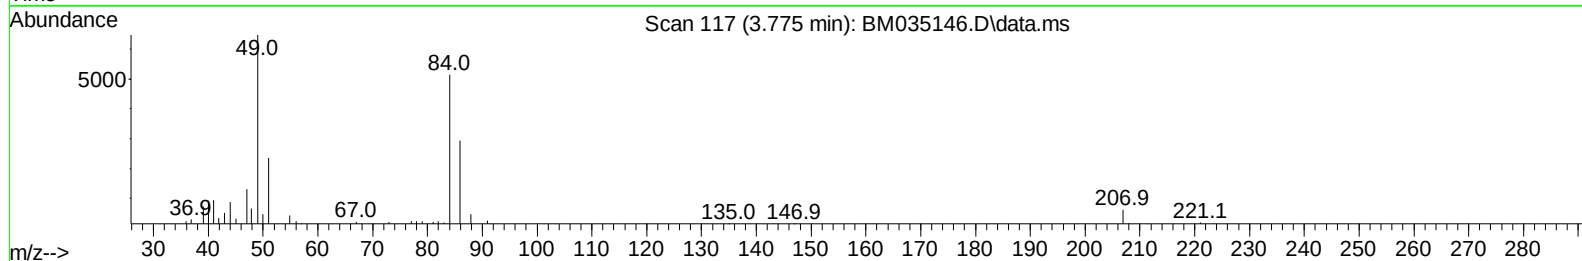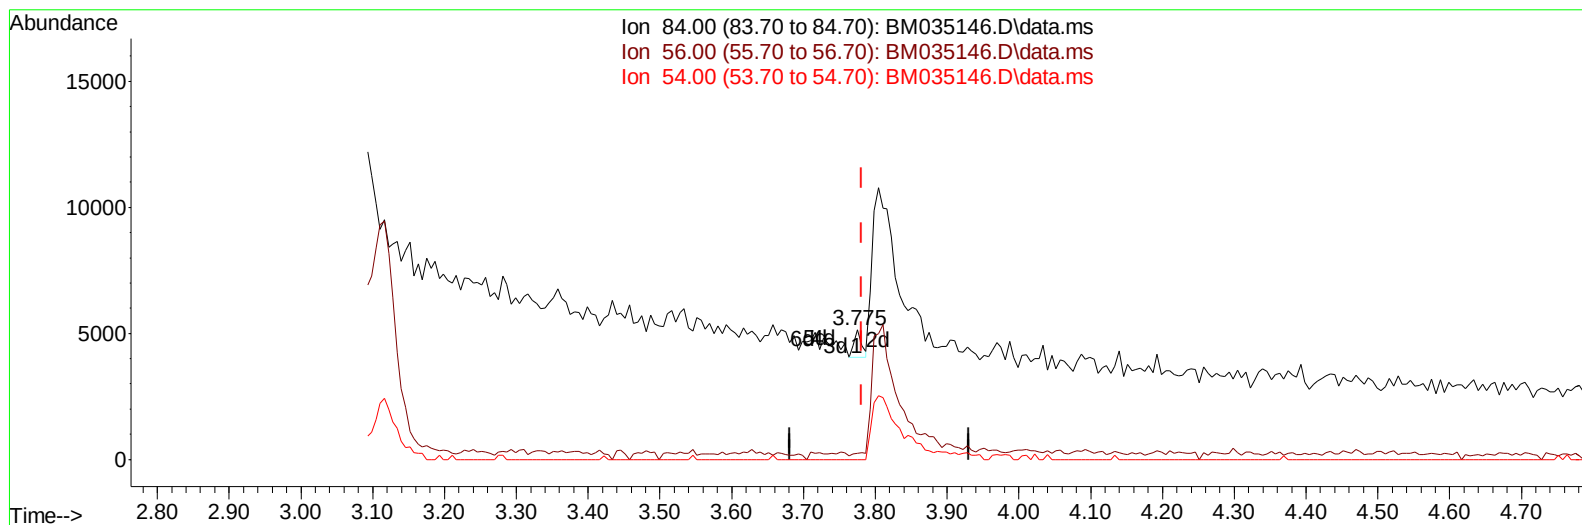

TIC: BM035146.D\data.ms

(4) Pyridine-d5 (S)

3.775min (-0.006) 0.08 ng/u1

response 795

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	68.20	4.60#
54.00	34.50	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051822\
Data File : BM035146.D
Acq On : 18 May 2022 16:21
Operator : CG/JU
Sample : N2766-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4G1

Manual IntegrationsAPPROVED

Quant Time: May 19 00:50:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM051722.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 17 16:13:52 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/19/2022
Supervised By :mohammad ahmed 05/19/2022

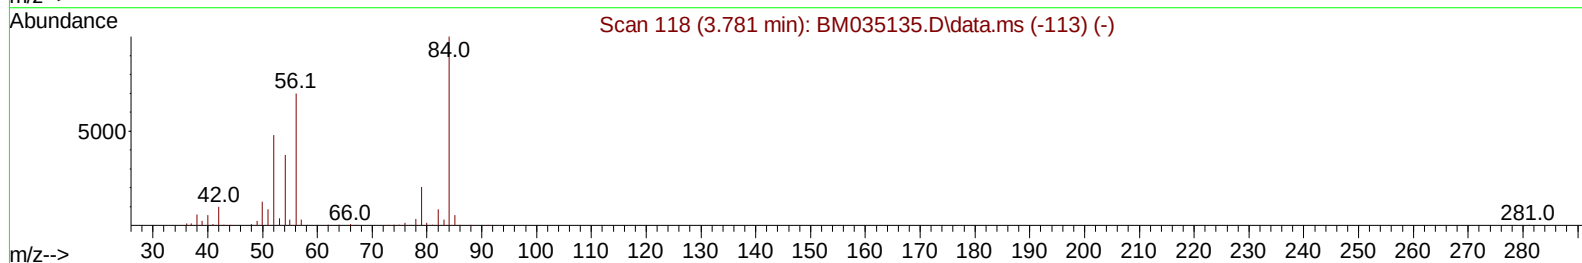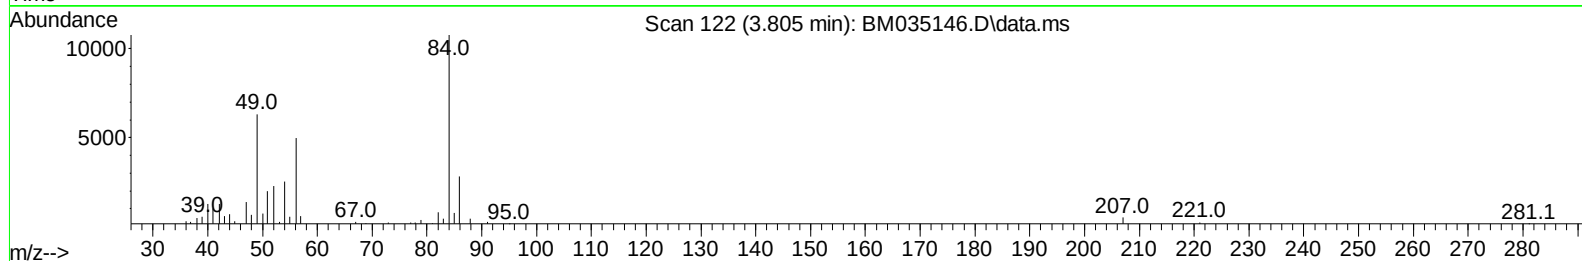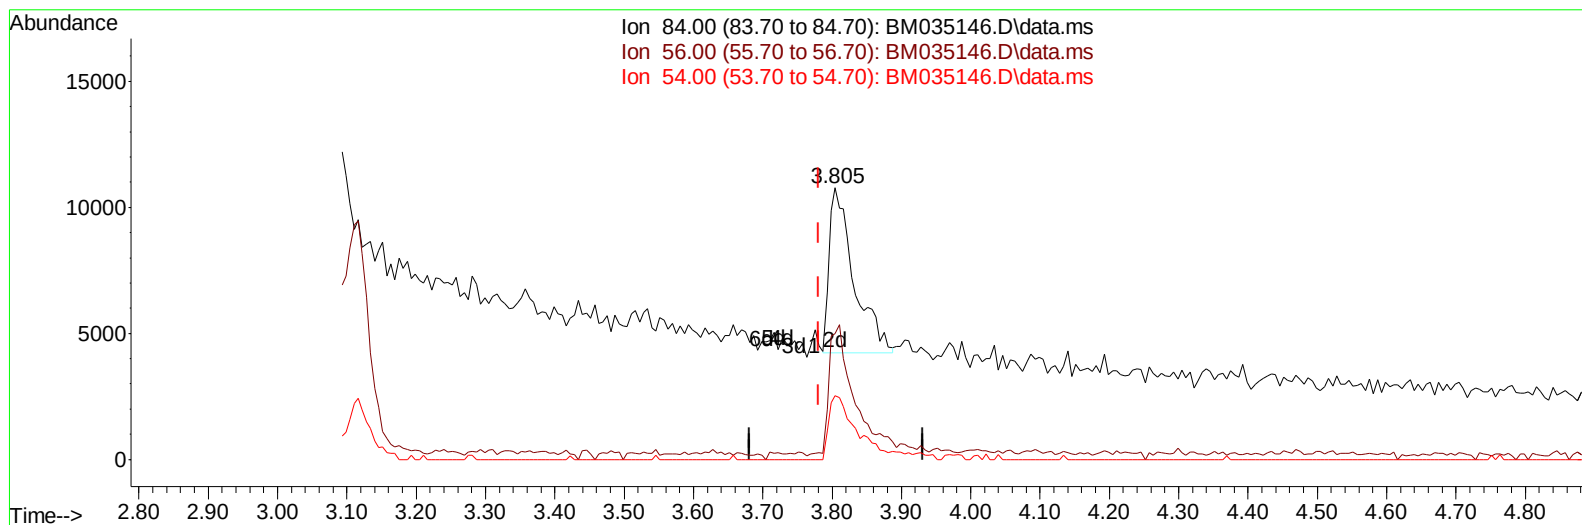

TIC: BM035146.D\data.ms

(4) Pyridine-d5 (S)

3.805min (+ 0.024) 1.57 ng/ul m

response 16327

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	68.20	46.36#
54.00	34.50	23.43#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051822\
Data File : BM035146.D
Acq On : 18 May 2022 16:21
Operator : CG/JU
Sample : N2766-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4G1

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/19/2022
Supervised By :mohammad ahmed 05/19/2022

Quant Time: May 19 00:50:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM051722.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 17 16:13:52 2022
Response via : Initial Calibration

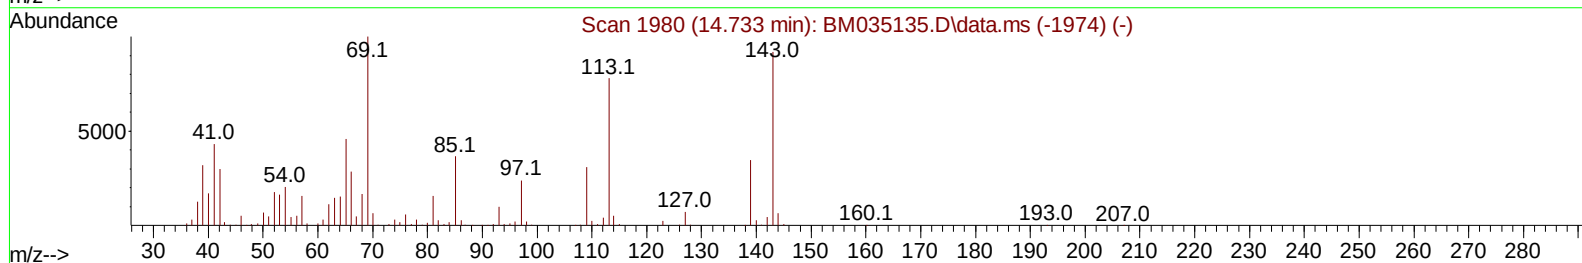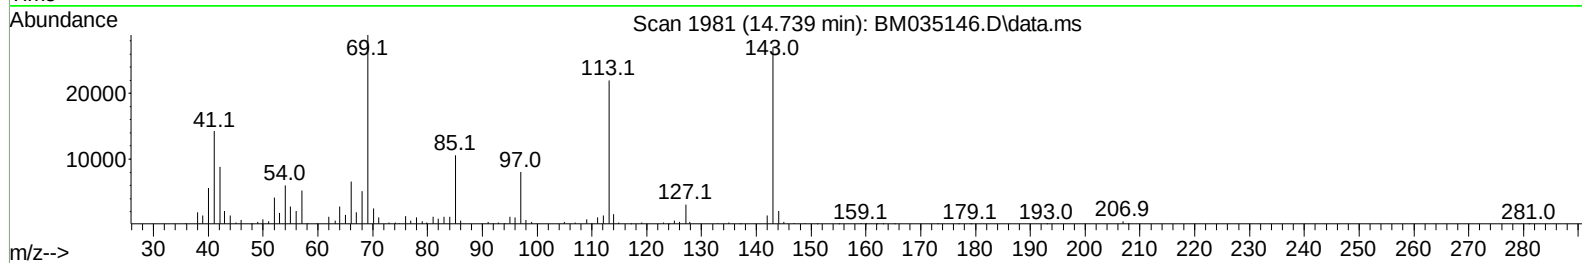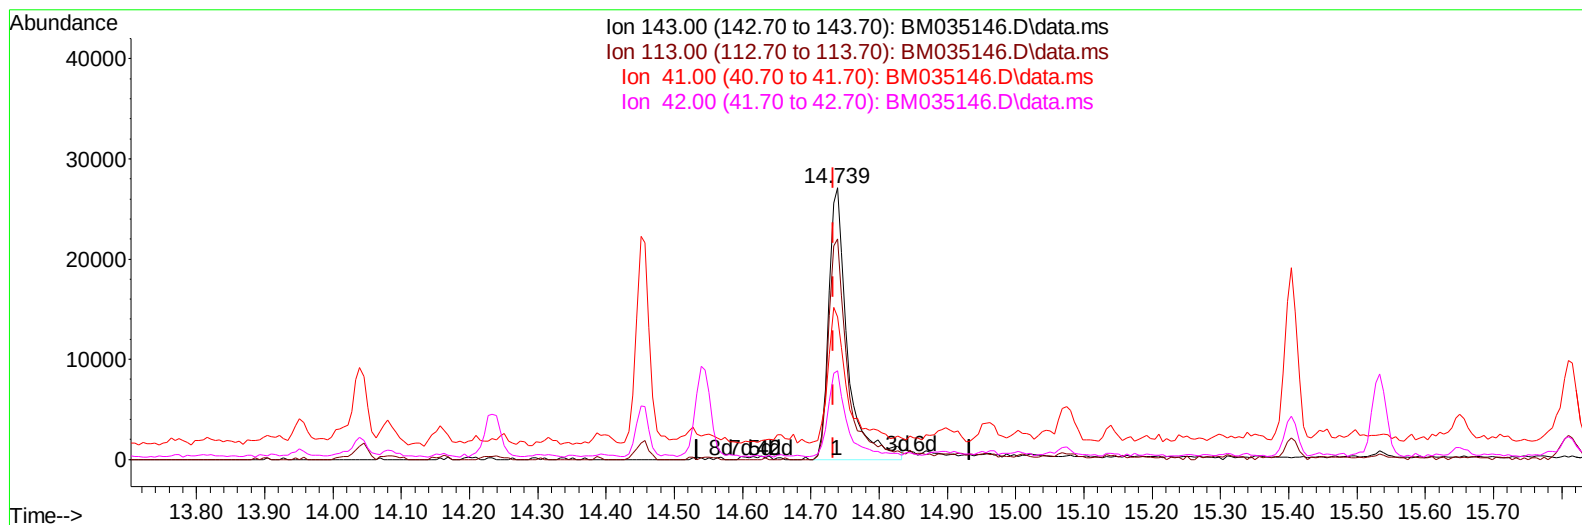

TIC: BM035146.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.739min (+ 0.006) 10.56 ng/ul m

response 52054

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	80.00	81.23
41.00	42.20	52.58#
42.00	28.30	32.71

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051822\
 Data File : BM035146.D
 Acq On : 18 May 2022 16:21
 Operator : CG/JU
 Sample : N2766-11
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4G1

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/19/2022
 Supervised By :mohammad ahmed 05/19/2022

Quant Time: May 19 00:50:00 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM051722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 17 16:13:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.910	152	167038	20.000	ng/ul	0.00
20) Naphthalene-d8	10.710	136	646347	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.545	164	381475	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.286	188	747574	20.000	ng/ul	0.00
79) Chrysene-d12	21.468	240	681129	20.000	ng/ul	0.00
88) Perylene-d12	23.856	264	710086	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.375	96	9810m	2.427	ng/uL	0.01
4) Pyridine-d5	3.805	84	16327m	1.566	ng/ul	0.02
7) Phenol-d5	7.075	99	163720	13.299	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.240	67	111637	14.373	ng/ul	0.00
11) 2-Chlorophenol-d4	7.440	132	149227	13.674	ng/ul	0.00
15) 4-Methylphenol-d8	8.616	113	128480	12.424	ng/ul	0.00
21) Nitrobenzene-d5	9.069	128	69166	13.649	ng/ul	0.00
24) 2-Nitrophenol-d4	9.792	143	75645	13.332	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.328	165	130441	12.925	ng/ul	0.00
31) 4-Chloroaniline-d4	10.845	131	169130	12.153	ng/ul	0.00
46) Dimethylphthalate-d6	13.951	166	449187	16.162	ng/ul	0.00
49) Acenaphthylene-d8	14.233	160	508213	15.300	ng/ul	0.00
54) 4-Nitrophenol-d4	14.739	143	52054m	10.564	ng/ul	0.00
60) Fluorene-d10	15.533	176	387510	16.481	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.651	200	32935	6.823	ng/ul	0.00
73) Anthracene-d10	17.386	188	606546	17.431	ng/ul	0.00
81) Pyrene-d10	19.674	212	714364	19.692	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.697	264	675594	18.773	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051822\
Data File : BM035146.D
Acq On : 18 May 2022 16:21
Operator : CG/JU
Sample : N2766-11
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4G1

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/19/2022
Supervised By :mohammad ahmed 05/19/2022

Quant Time: May 19 00:50:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM051722.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 17 16:13:52 2022
Response via : Initial Calibration

