




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051822\
 Data File : BM035148.D
 Acq On : 18 May 2022 17:34
 Operator : CG/JU
 Sample : N2766-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4F7

Manual IntegrationsAPPROVED

Quant Time: May 19 00:50:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM051722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 17 16:13:52 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/19/2022
 Supervised By :mohammad ahmed 05/19/2022

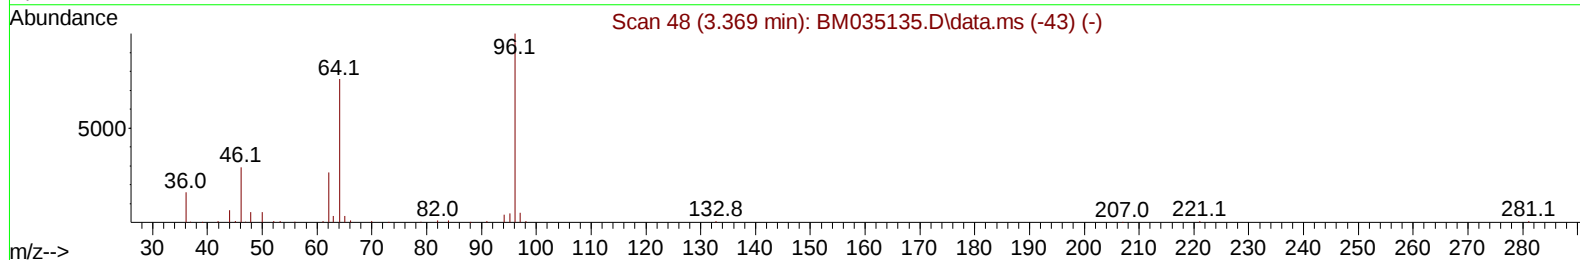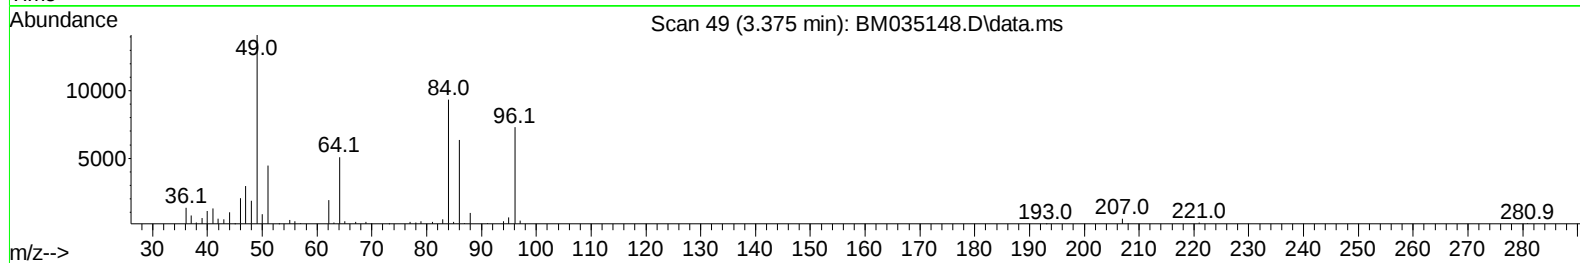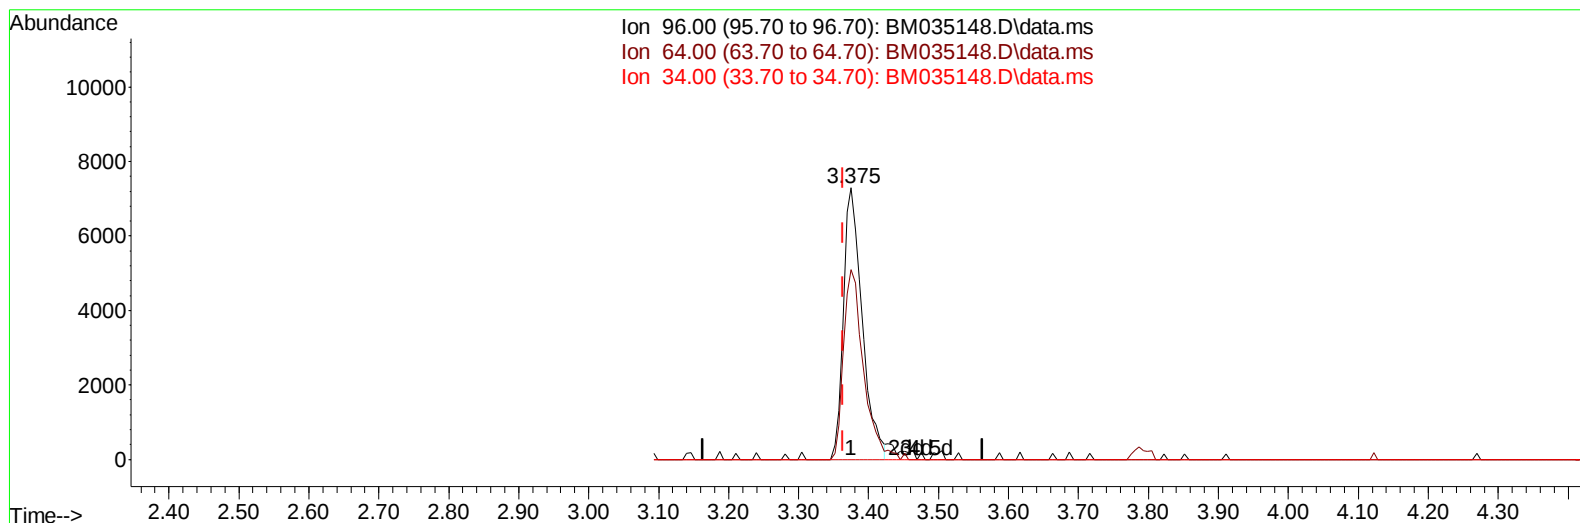

TIC: BM035148.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.375min (+ 0.012) 2.66 ng/uL

response 13467

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	72.40	69.93
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051822\
 Data File : BM035148.D
 Acq On : 18 May 2022 17:34
 Operator : CG/JU
 Sample : N2766-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4F7

Manual IntegrationsAPPROVED

Quant Time: May 19 00:50:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM051722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 17 16:13:52 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/19/2022
 Supervised By :mohammad ahmed 05/19/2022

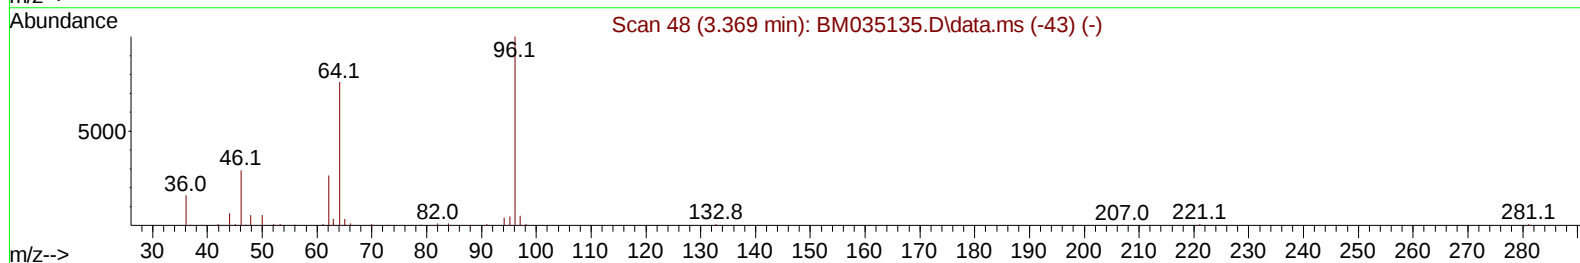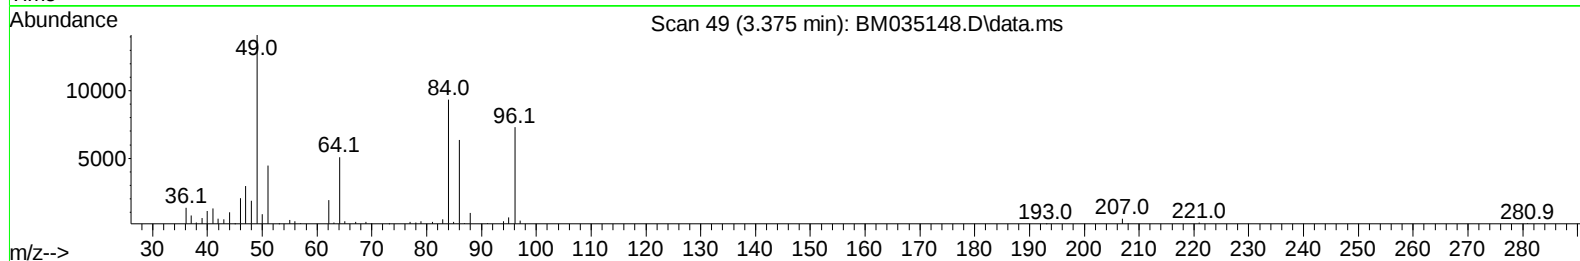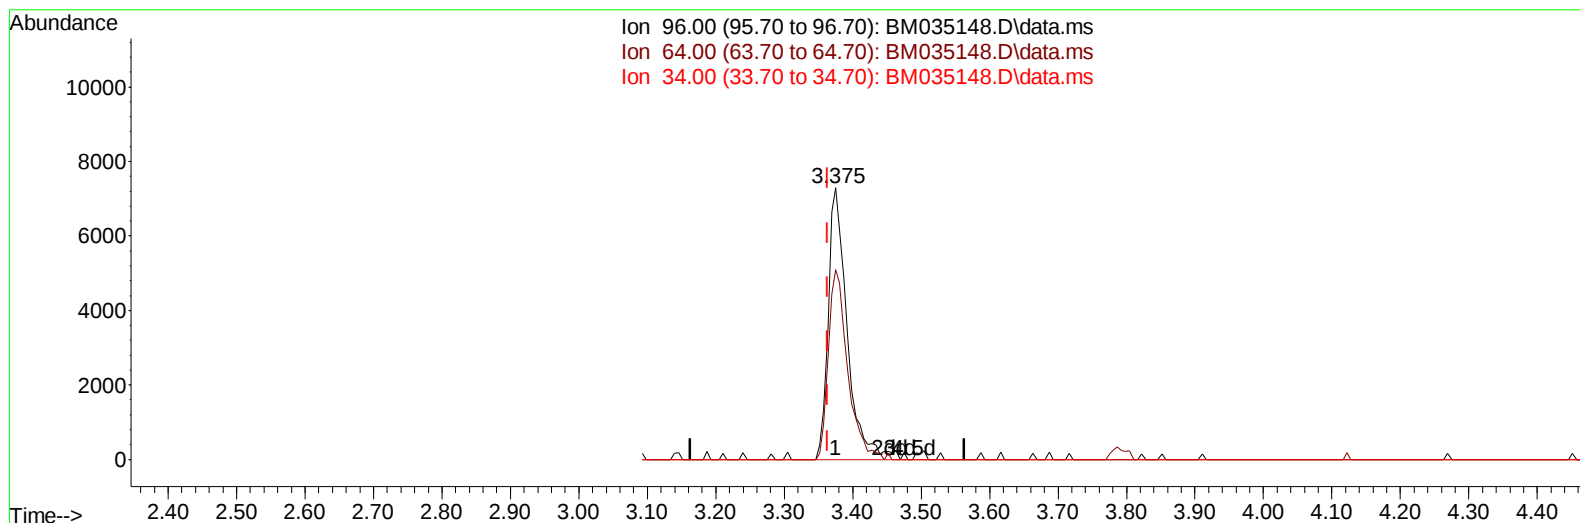

TIC: BM035148.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.375min (+ 0.012) 2.79 ng/uL m

response 14118

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	72.40	69.93
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051822\
 Data File : BM035148.D
 Acq On : 18 May 2022 17:34
 Operator : CG/JU
 Sample : N2766-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4F7

Manual IntegrationsAPPROVED

Quant Time: May 19 00:50:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM051722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 17 16:13:52 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/19/2022
 Supervised By :mohammad ahmed 05/19/2022

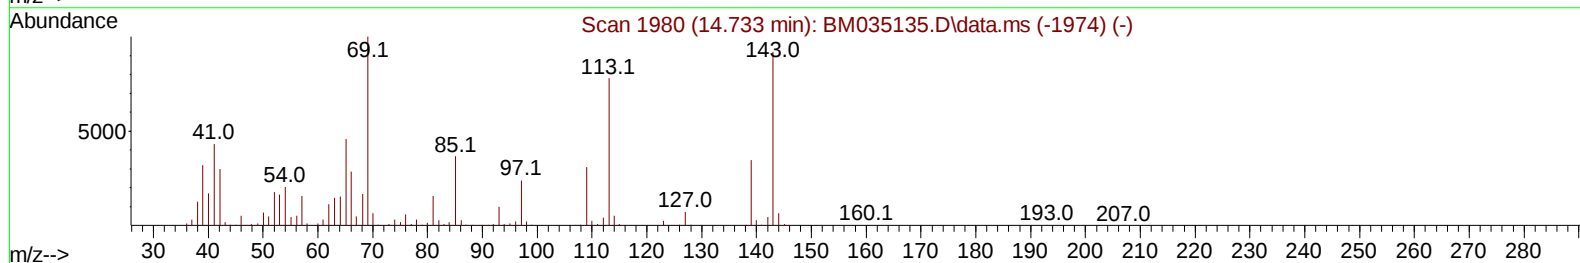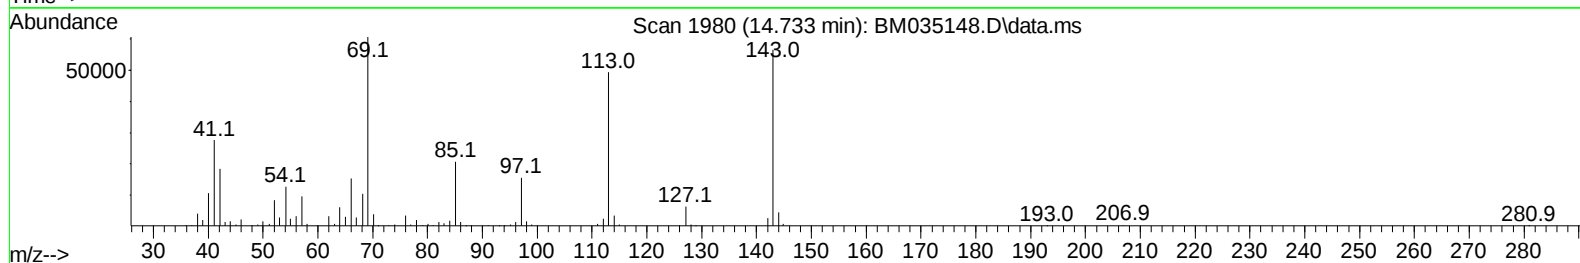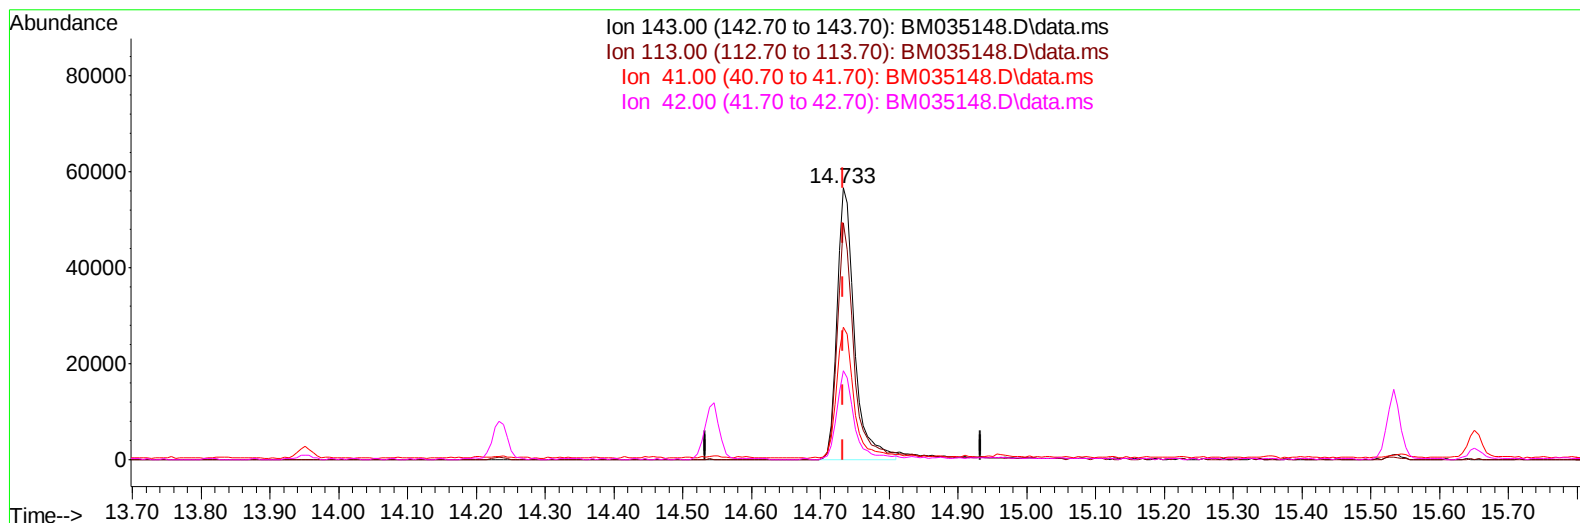

TIC: BM035148.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.733min (+ 0.000) 16.15 ng/u1

response 99257

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	80.00	87.17
41.00	42.20	48.73
42.00	28.30	32.59




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051822\
 Data File : BM035148.D
 Acq On : 18 May 2022 17:34
 Operator : CG/JU
 Sample : N2766-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4F7

Manual IntegrationsAPPROVED

Quant Time: May 19 00:50:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM051722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 17 16:13:52 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 05/19/2022
 Supervised By :mohammad ahmed 05/19/2022

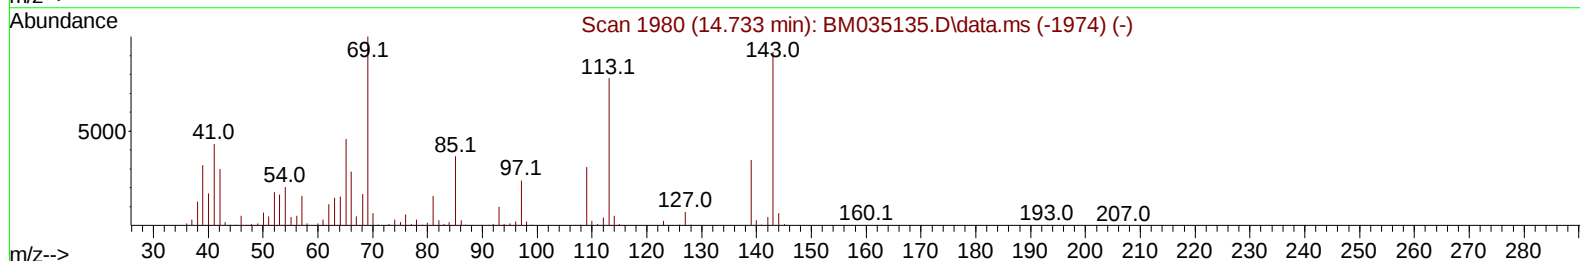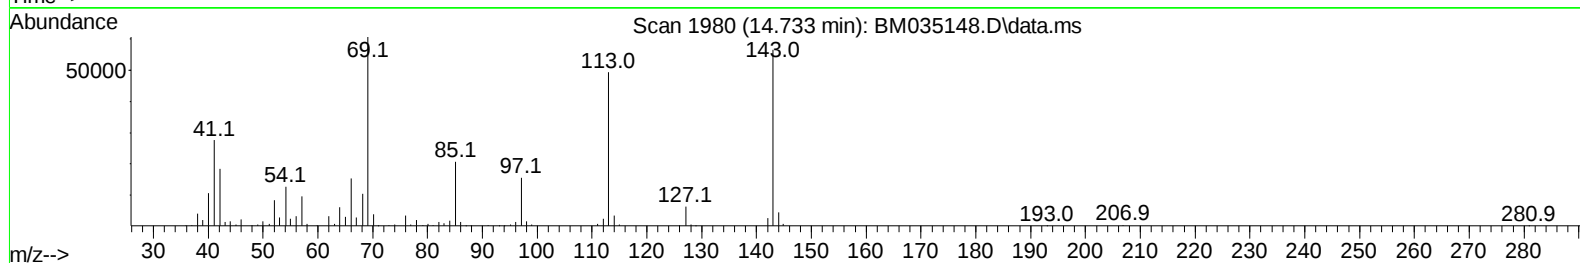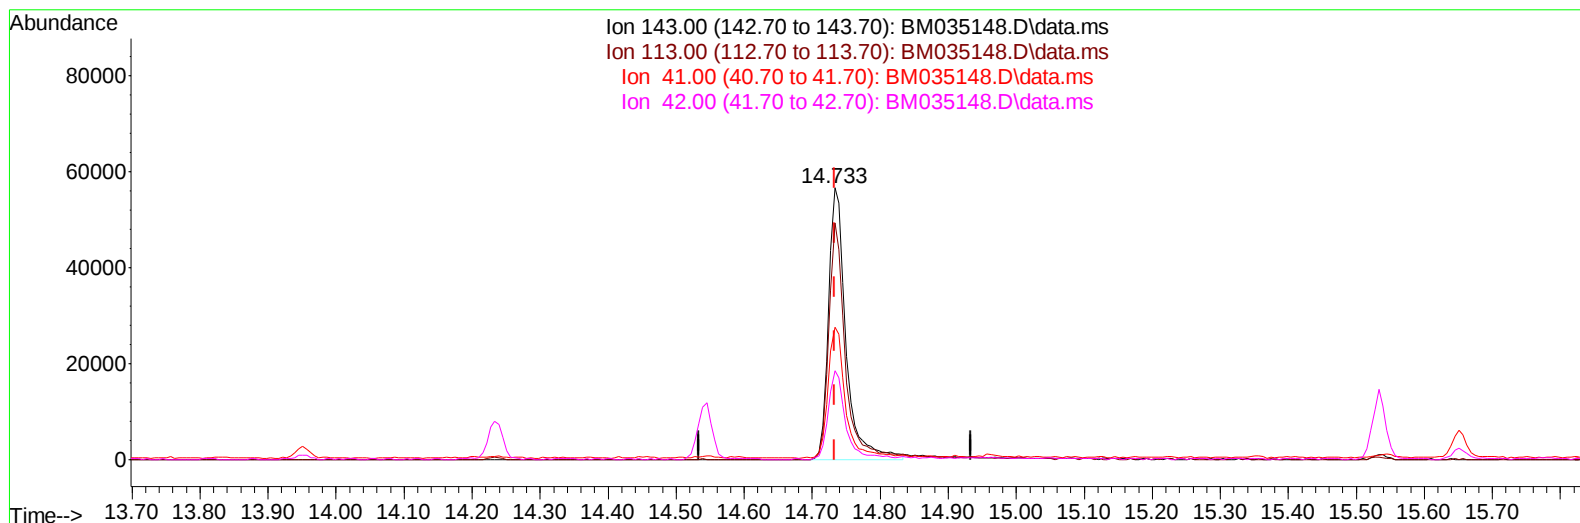

TIC: BM035148.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.733min (+ 0.000) 16.42 ng/ul m

response 100937

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	80.00	87.17
41.00	42.20	48.73
42.00	28.30	32.59

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051822\
 Data File : BM035148.D
 Acq On : 18 May 2022 17:34
 Operator : CG/JU
 Sample : N2766-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4F7

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/19/2022
 Supervised By :mohammad ahmed 05/19/2022

Quant Time: May 19 00:50:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM051722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 17 16:13:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.910	152	209007	20.000	ng/ul	0.00
20) Naphthalene-d8	10.710	136	802446	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.545	164	475852	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.286	188	948017	20.000	ng/ul	0.00
79) Chrysene-d12	21.468	240	878924	20.000	ng/ul	0.00
88) Perylene-d12	23.856	264	918167	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.375	96	14118m	2.791	ng/uL	0.01
4) Pyridine-d5	3.787	84	177981	13.640	ng/ul	0.00
7) Phenol-d5	7.075	99	248647	16.142	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.240	67	163204	16.793	ng/ul	0.00
11) 2-Chlorophenol-d4	7.440	132	223826	16.391	ng/ul	0.00
15) 4-Methylphenol-d8	8.616	113	205727	15.899	ng/ul	0.00
21) Nitrobenzene-d5	9.069	128	112508	17.883	ng/ul	0.00
24) 2-Nitrophenol-d4	9.792	143	128399	18.227	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.328	165	221323	17.664	ng/ul	0.00
31) 4-Chloroaniline-d4	10.845	131	287360	16.632	ng/ul	0.00
46) Dimethylphthalate-d6	13.951	166	764749	22.059	ng/ul	0.00
49) Acenaphthylene-d8	14.233	160	873827	21.089	ng/ul	0.00
54) 4-Nitrophenol-d4	14.733	143	100937m	16.422	ng/ul	0.00
60) Fluorene-d10	15.533	176	649155	22.133	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.651	200	82196	13.427	ng/ul	0.00
73) Anthracene-d10	17.386	188	970991	22.004	ng/ul	0.00
81) Pyrene-d10	19.680	212	1096760	23.429	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.703	264	1055827	22.690	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051822\
Data File : BM035148.D
Acq On : 18 May 2022 17:34
Operator : CG/JU
Sample : N2766-08
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4F7

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 05/19/2022
Supervised By :mohammad ahmed 05/19/2022

Quant Time: May 19 00:50:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM051722.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 17 16:13:52 2022
Response via : Initial Calibration

