

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051822\
 Data File : BM035143.D
 Acq On : 18 May 2022 14:31
 Operator : CG/JU
 Sample : N2766-14
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4G4

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 05/19/2022
 Supervised By :mohammad ahmed 05/19/2022

Quant Time: May 19 00:49:43 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM051722.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue May 17 16:13:52 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.910	152	189341	20.000	ng/u1	0.00
20) Naphthalene-d8	10.710	136	728537	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.545	164	424883	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.286	188	822209	20.000	ng/u1	0.00
79) Chrysene-d12	21.468	240	748632	20.000	ng/u1	0.00
88) Perylene-d12	23.856	264	773576	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.375	96	6846m	1.494	ng/uL	0.01
4) Pyridine-d5	0.000	84	0d	0.000	ng/u1	
7) Phenol-d5	7.075	99	117099	8.392	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.239	67	82946	9.421	ng/u1	0.00
11) 2-Chlorophenol-d4	7.439	132	110057	8.897	ng/u1	0.00
15) 4-Methylphenol-d8	8.616	113	86187	7.353	ng/u1	0.00
21) Nitrobenzene-d5	9.063	128	50792	8.892	ng/u1	0.00
24) 2-Nitrophenol-d4	9.792	143	53355	8.342	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.328	165	94719	8.326	ng/u1	0.00
31) 4-Chloroaniline-d4	10.845	131	118431	7.550	ng/u1	0.00
46) Dimethylphthalate-d6	13.951	166	302950	9.787	ng/u1	0.00
49) Acenaphthylene-d8	14.233	160	350493	9.474	ng/u1	0.00
54) 4-Nitrophenol-d4	14.739	143	24609m	4.484	ng/u1	0.00
60) Fluorene-d10	15.533	176	258066	9.854	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.657	200	12731	2.398	ng/u1	0.00
73) Anthracene-d10	17.386	188	371262	9.701	ng/u1	0.00
81) Pyrene-d10	19.674	212	419797	10.528	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.703	264	382586	9.759	ng/u1	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.733	105	19501	1.074	ng/u1	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM051822\
Data File : BM035143.D
Acq On : 18 May 2022 14:31
Operator : CG/JU
Sample : N2766-14
Misc :
ALS Vial : 10 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
EW4G4

Quant Time: May 19 00:49:43 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM051722.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue May 17 16:13:52 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 05/19/2022
Supervised By :mohammad ahmed 05/19/2022

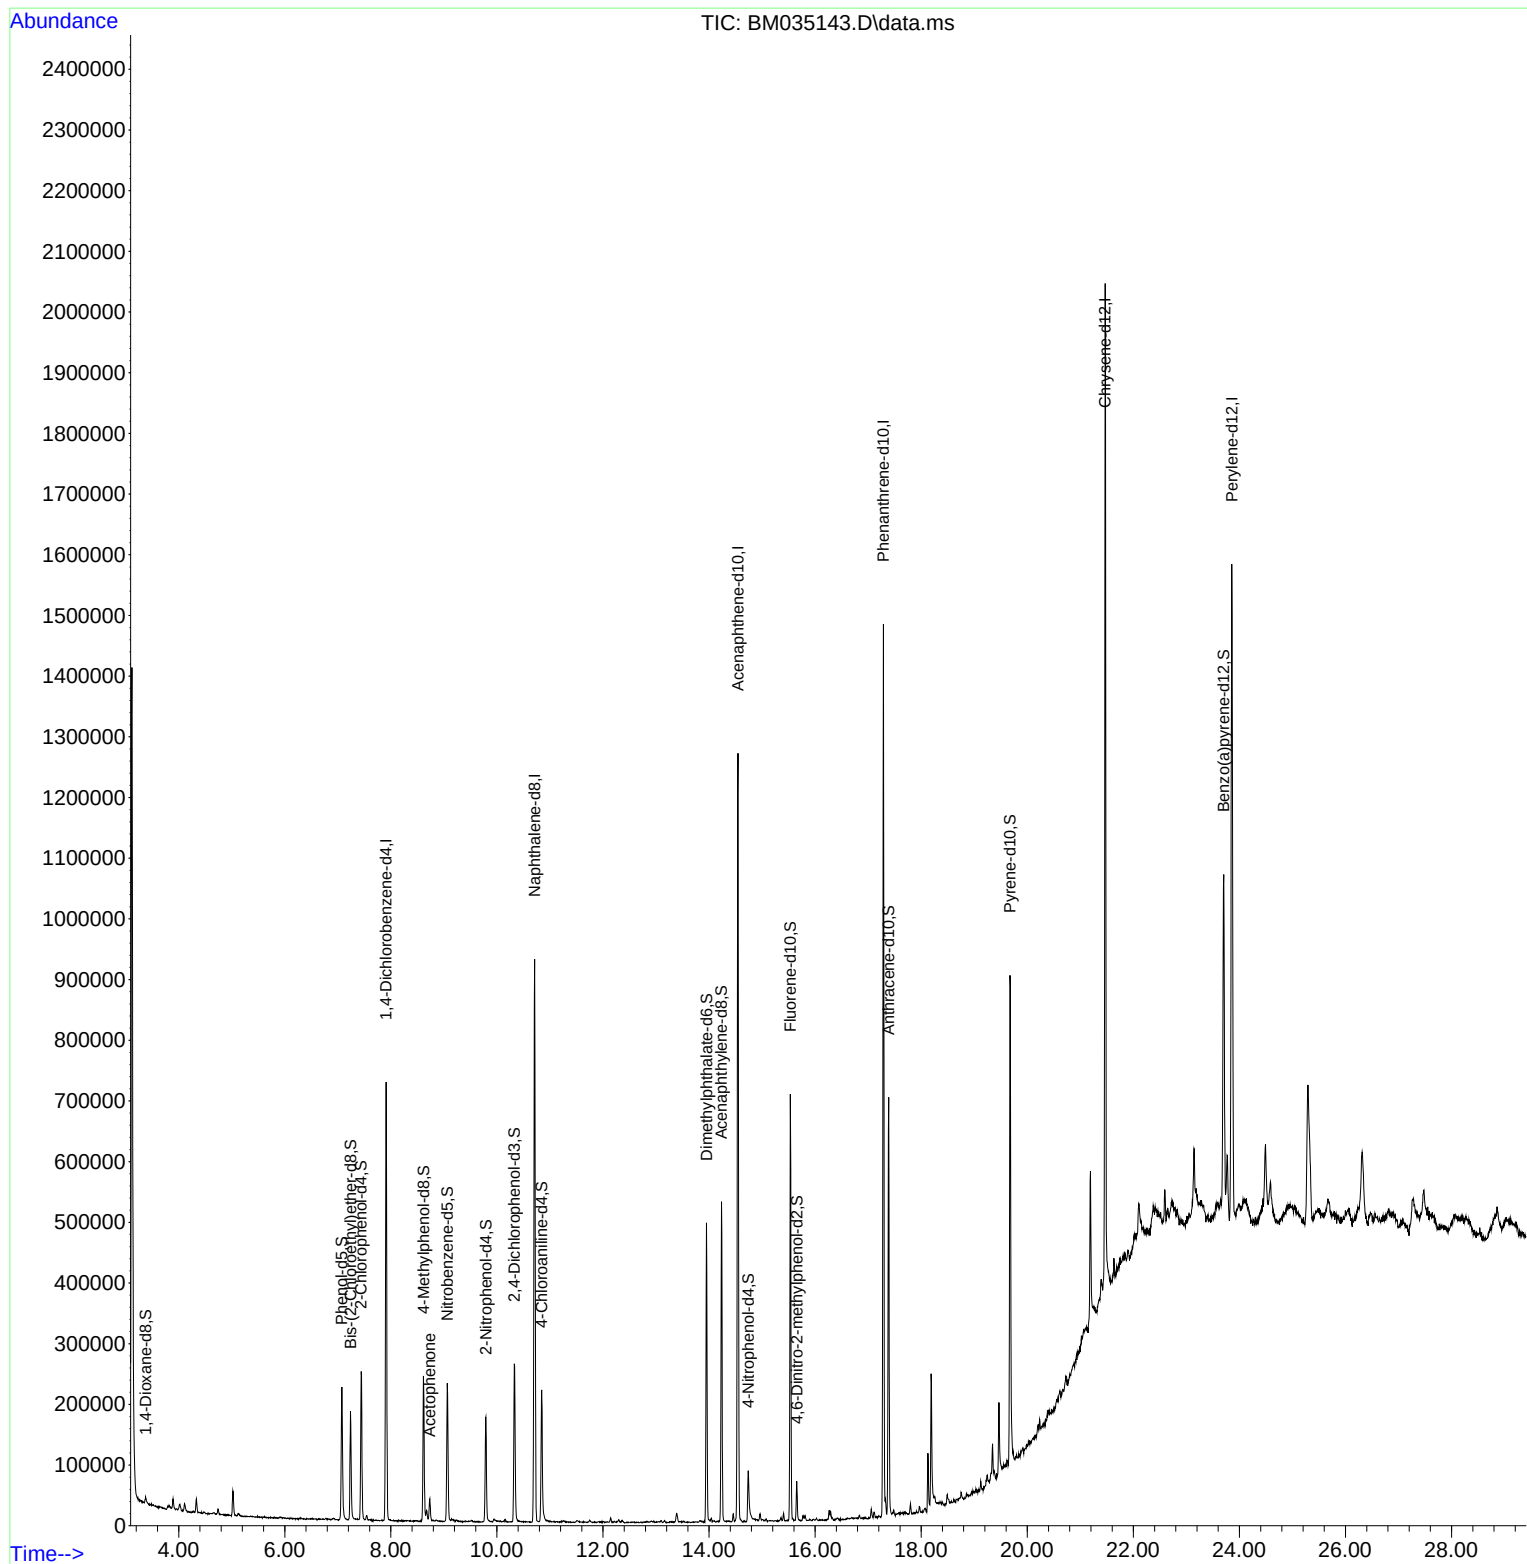

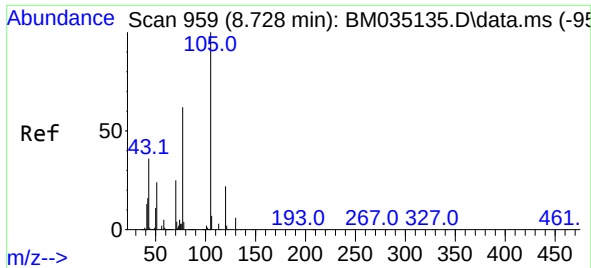

#16
Acetophenone
Concen: 1.074 ng/ul
RT: 8.733 min Scan# 90
Delta R.T. 0.006 min
Lab File: BM035143.D
Acq: 18 May 2022 14:31

Instrument :
BNA_M
ClientSampleId :
EW4G4

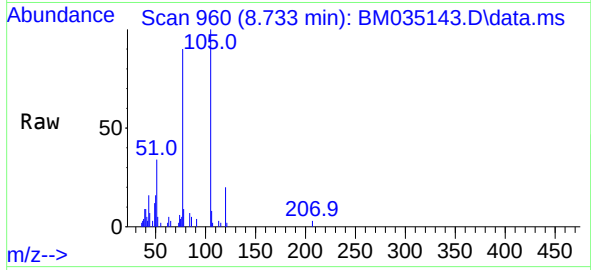

Tgt Ion:	105	Resp:	1950
Ion Ratio	Lower	Upper	
105	100		
77	89.9	62.4	93.6
51	33.5	23.8	35.6

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 05/19/2022
Supervised By :mohammad ahmed 05/19/2022

