

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052422\
 Data File : BM035228.D
 Acq On : 24 May 2022 20:33
 Operator : CG/JU
 Sample : N2981-15
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SB-8(0.5-1)

Quant Time: May 25 05:44:33 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 20 04:53:59 2022
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Reviewed By :Christian Giraldo 05/25/2022
 Supervised By :Jagrut Upadhyay 05/25/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.899	152	124064	20.000	ng	0.00
21) Naphthalene-d8	10.698	136	484025	20.000	ng	-0.01
39) Acenaphthene-d10	14.533	164	298693	20.000	ng	-0.01
64) Phenanthrene-d10	17.280	188	630559	20.000	ng	0.00
76) Chrysene-d12	21.462	240	670353	20.000	ng	#-0.01
86) Perylene-d12	23.850	264	728766	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.475	112	590532	83.975	ng	0.00
7) Phenol-d6	7.069	99	755981	83.274	ng	0.00
23) Nitrobenzene-d5	9.057	82	513461	57.286	ng	0.00
42) 2,4,6-Tribromophenol	16.027	330	311615	95.906	ng	0.00
45) 2-Fluorobiphenyl	13.163	172	1185068	57.595	ng	0.00
79) Terphenyl-d14	19.904	244	1810457	52.292	ng	-0.01
Target Compounds						
						Qvalue
71) Phenanthrene	17.321	178	110859	3.155	ng	99
75) Fluoranthene	19.339	202	252417	6.541	ng	98
78) Pyrene	19.698	202	227736	5.137	ng	99
81) Benzo(a)anthracene	21.451	228	183444	4.101	ng	98
83) Chrysene	21.498	228	159858	3.742	ng	98
87) Indeno(1,2,3-cd)pyrene	26.309	276	111500	2.012	ng	95
88) Benzo(b)fluoranthene	23.127	252	226649m	4.945	ng	
90) Benzo(a)pyrene	23.739	252	162742	4.274	ng	96
92) Benzo(g,h,i)perylene	27.068	276	100364	2.247	ng	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052422\
Data File : BM035228.D
Acq On : 24 May 2022 20:33
Operator : CG/JU
Sample : N2981-15
Misc :
ALS Vial : 15 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
SB-8(0.5-1)

Quant Time: May 25 05:44:33 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 20 04:53:59 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 05/25/2022
Supervised By :Jagrut Upadhyay 05/25/2022

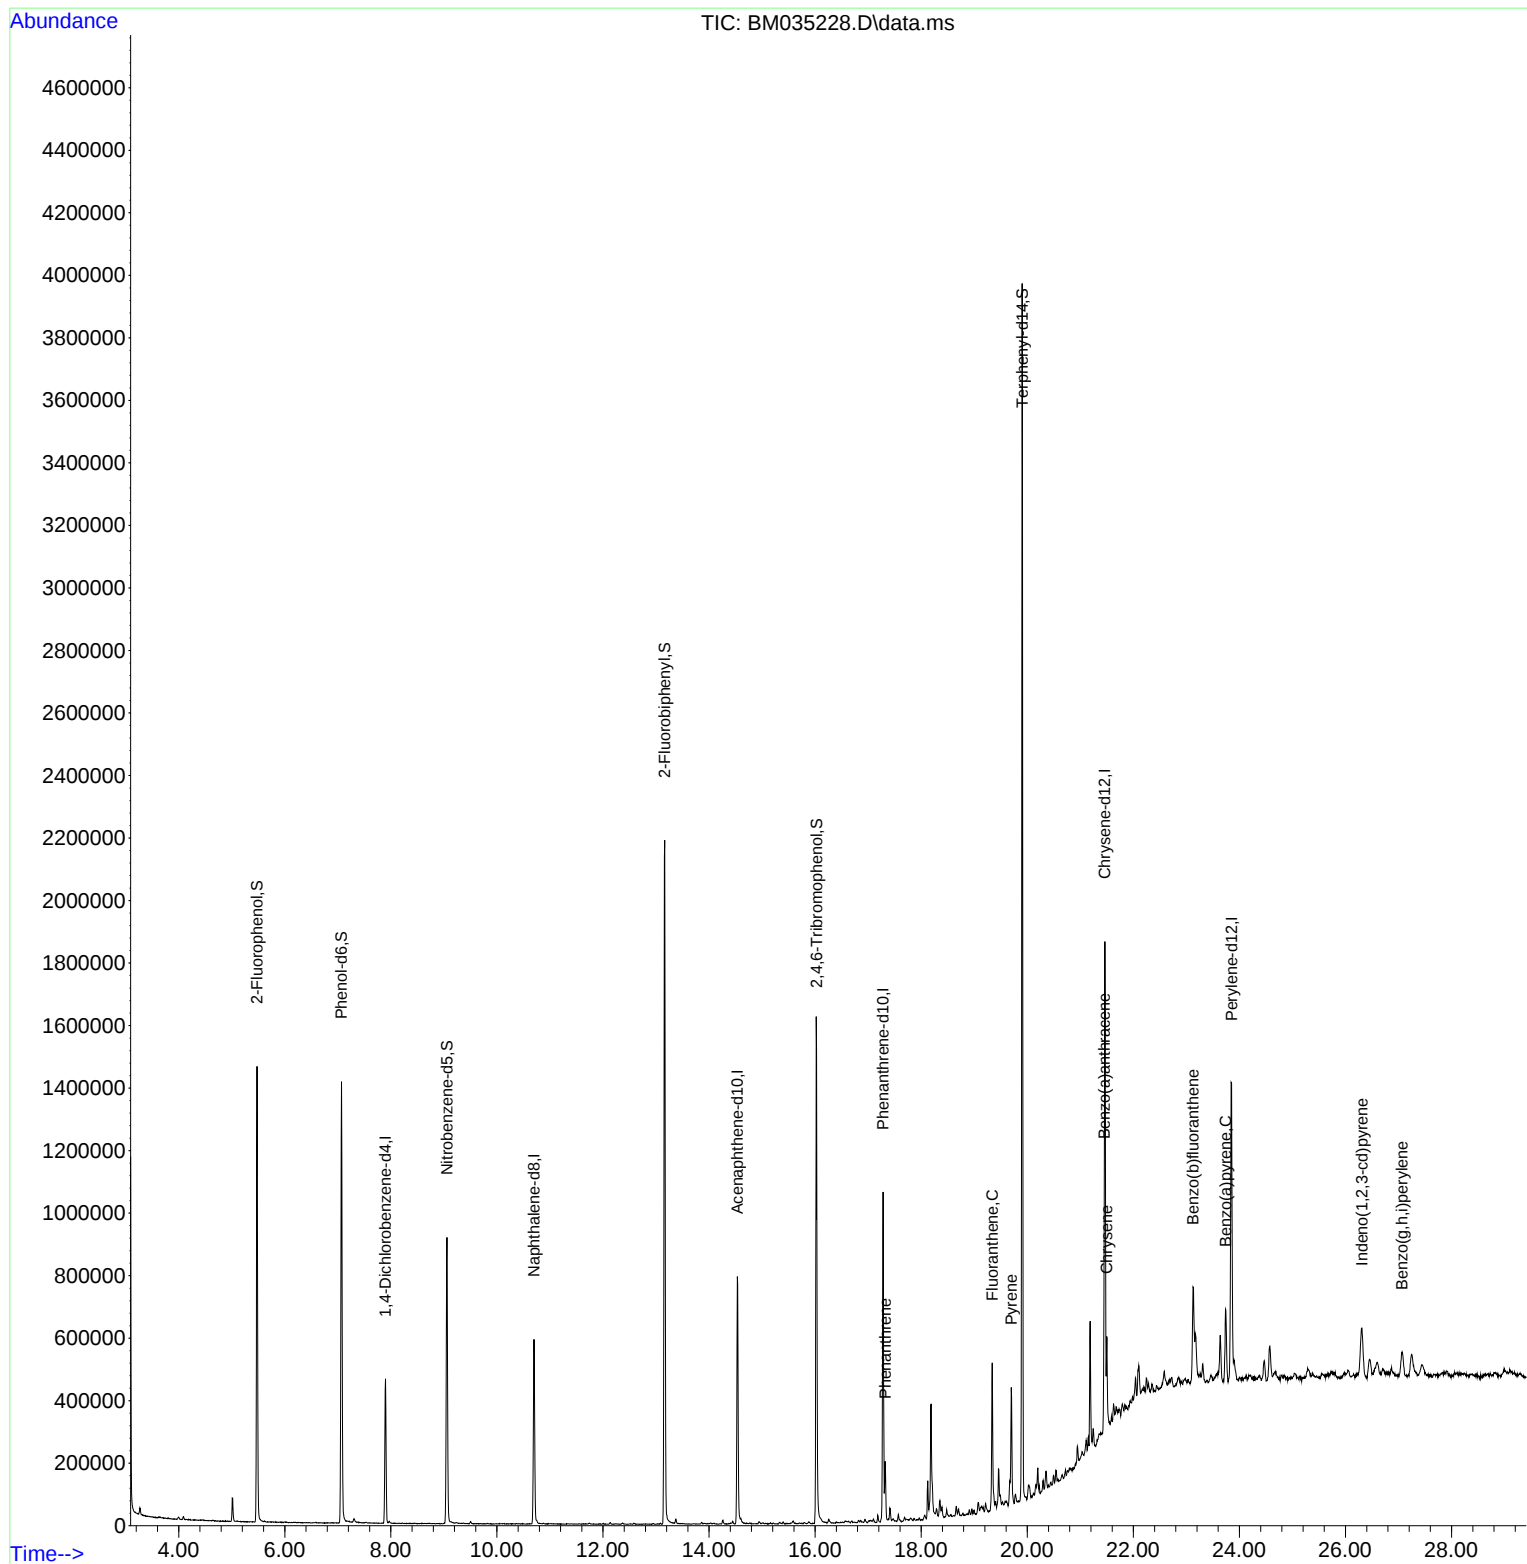



#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.899 min Scan# 81
Delta R.T. -0.005 min
Lab File: BM035228.D
Acq: 24 May 2022 20:33




Instrument :
BNA_M
ClientSampleId :
SB-8(0.5-1)




Tgt Ion:152 Resp: 124064
Ion Ratio Lower Upper
152 100
150 155.6 124.9 187.3
115 61.7 47.9 71.9

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 05/25/2022
Supervised By :Jagrut Upadhyay 05/25/2022

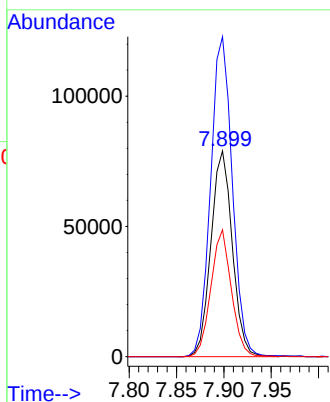

#5
2-Fluorophenol
Concen: 83.975 ng
RT: 5.475 min Scan# 406
Delta R.T. -0.006 min
Lab File: BM035228.D
Acq: 24 May 2022 20:33

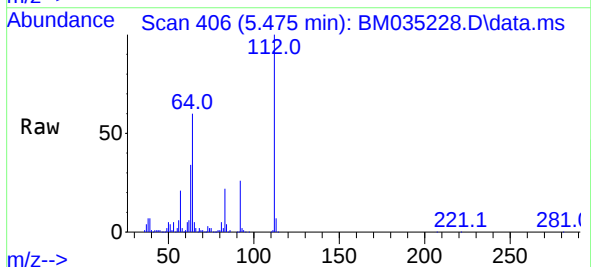


Tgt Ion:112 Resp: 590532
Ion Ratio Lower Upper
112 100
64 60.4 47.8 71.6
63 33.7 26.6 40.0

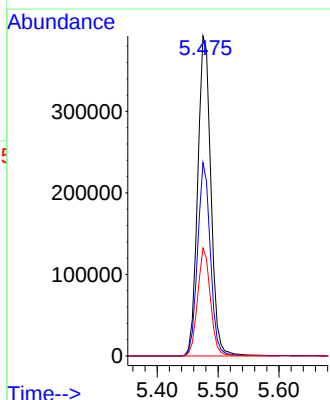



#7
Phenol-d6
Concen: 83.274 ng
RT: 7.069 min Scan# 61
Delta R.T. -0.006 min
Lab File: BM035228.D
Acq: 24 May 2022 20:33




Instrument :
BNA_M
ClientSampleId :
SB-8(0.5-1)




Tgt Ion: 99 Resp: 75598
Ion Ratio Lower Upper
99 100
42 21.4 18.8 28.2
71 37.4 30.2 45.2

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 05/25/2022
Supervised By :Jagrut Upadhyay 05/25/2022

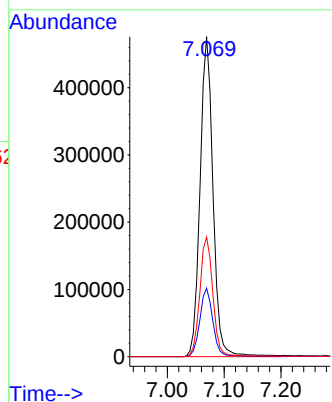

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.698 min Scan# 1294
Delta R.T. -0.012 min
Lab File: BM035228.D
Acq: 24 May 2022 20:33




Tgt Ion:136 Resp: 484025
Ion Ratio Lower Upper
136 100
137 11.0 8.9 13.3
54 7.9 7.0 10.4
68 5.0 4.3 6.5

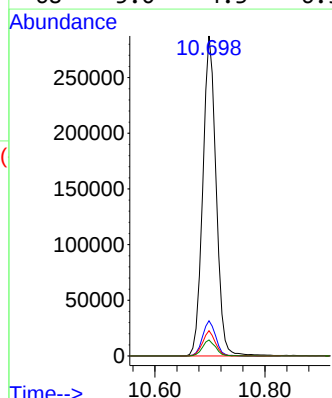



#23
Nitrobenzene-d5
Concen: 57.286 ng
RT: 9.057 min Scan# 1015
Delta R.T. -0.006 min
Lab File: BM035228.D
Acq: 24 May 2022 20:33




Instrument :
BNA_M
ClientSampleId :
SB-8(0.5-1)




Tgt Ion: 82 Resp: 51346
Ion Ratio Lower Upper
82 100
128 43.0 33.7 50.5
54 52.0 43.2 64.8

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 05/25/2022
Supervised By :Jagrut Upadhyay 05/25/2022

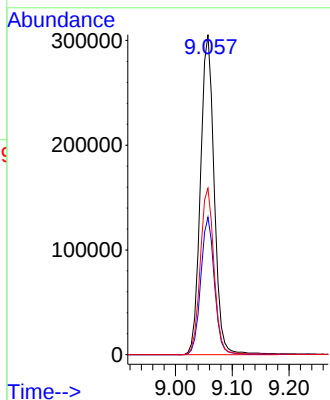


#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.533 min Scan# 1946
Delta R.T. -0.012 min
Lab File: BM035228.D
Acq: 24 May 2022 20:33




Tgt Ion:164 Resp: 298693
Ion Ratio Lower Upper
164 100
162 105.9 83.0 124.6
160 46.0 37.0 55.4

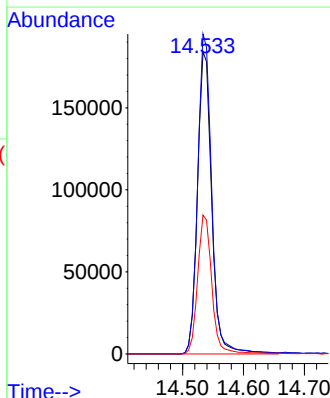



#42
2,4,6-Tribromophenol
Concen: 95.906 ng
RT: 16.027 min Scan# 211
Delta R.T. -0.006 min
Lab File: BM035228.D
Acq: 24 May 2022 20:33




Instrument :
BNA_M
ClientSampleId :
SB-8(0.5-1)




Tgt Ion:330 Resp: 31161
Ion Ratio Lower Upper
330 100
332 97.0 77.0 115.4
141 37.6 35.3 52.9

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 05/25/2022
Supervised By :Jagrut Upadhyay 05/25/2022

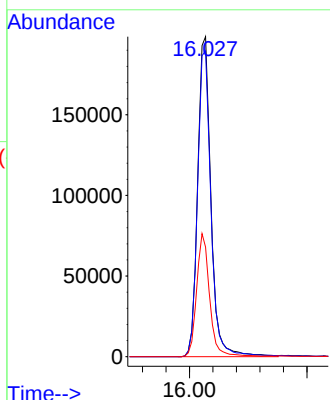


#45
2-Fluorobiphenyl
Concen: 57.595 ng
RT: 13.163 min Scan# 1713
Delta R.T. -0.006 min
Lab File: BM035228.D
Acq: 24 May 2022 20:33



Tgt Ion:172 Resp: 1185068
Ion Ratio Lower Upper
172 100
171 35.6 28.5 42.7
170 23.6 18.7 28.1

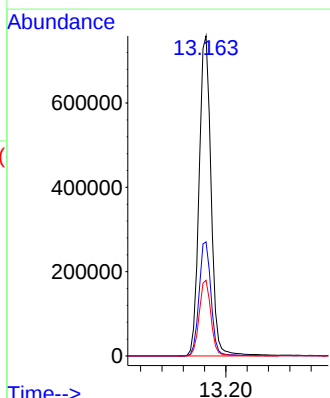



#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.280 min Scan# 2417
Delta R.T. -0.006 min
Lab File: BM035228.D
Acq: 24 May 2022 20:33

Instrument :

BNA_M

ClientSampleId :





SB-8(0.5-1)

Tgt Ion:188 Resp: 630559
Ion Ratio Lower Upper
188 100
94 7.3 7.0 10.4
80 8.3 7.6 11.4

Manual Integrations




APPROVED


Reviewed By :Christian Giraldo 05/25/2022
Supervised By :Jagrut Upadhyay 05/25/2022

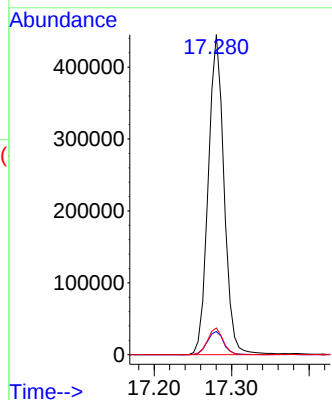

#71
Phenanthrene
Concen: 3.155 ng
RT: 17.321 min Scan# 2420
Delta R.T. -0.006 min
Lab File: BM035228.D
Acq: 24 May 2022 20:33

Tgt Ion:178 Resp: 110859
Ion Ratio Lower Upper
178 100
176 19.3 15.4 23.0
179 16.4 12.4 18.6

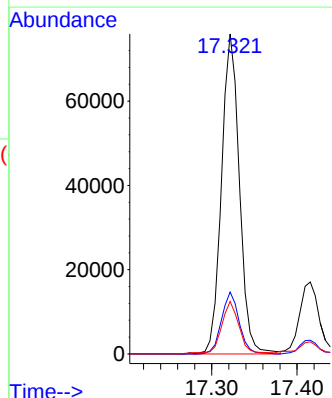







#75
Fluoranthene
Concen: 6.541 ng
RT: 19.339 min Scan# 21
Delta R.T. -0.006 min
Lab File: BM035228.D
Acq: 24 May 2022 20:33

Instrument :
BNA_M
ClientSampleId :
SB-8(0.5-1)

Tgt Ion:202 Resp: 25241
Ion Ratio Lower Upper
202 100
101 8.8 0.0 30.6
203 17.3 0.0 37.4




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 05/25/2022
Supervised By :Jagrut Upadhyay 05/25/2022

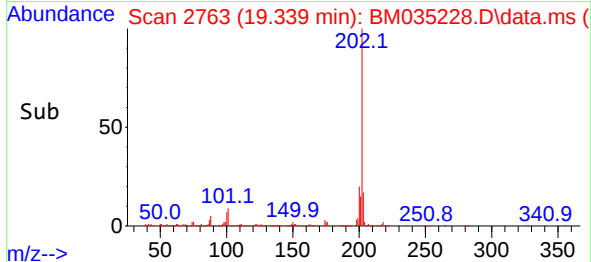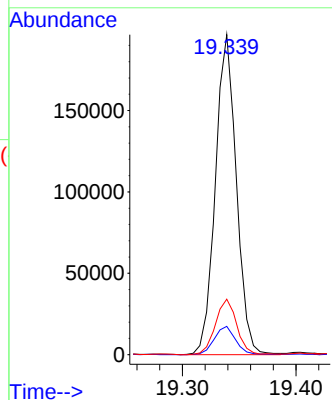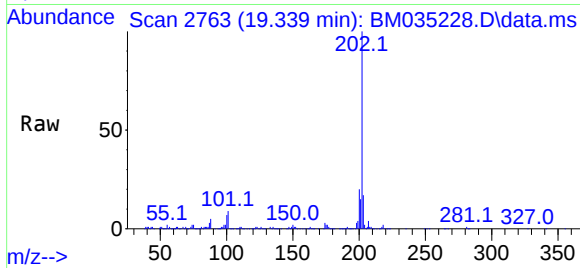

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.462 min Scan# 3124
Delta R.T. -0.012 min
Lab File: BM035228.D
Acq: 24 May 2022 20:33


Tgt Ion:240 Resp: 670353
Ion Ratio Lower Upper
240 100
120 8.9 9.4 14.0#
236 25.3 20.6 30.8

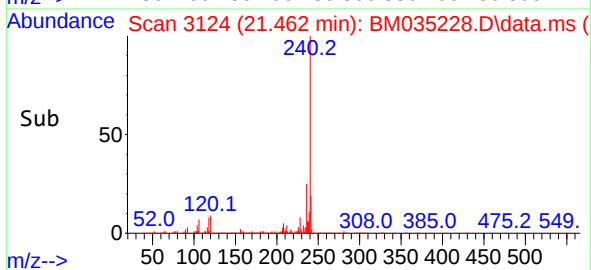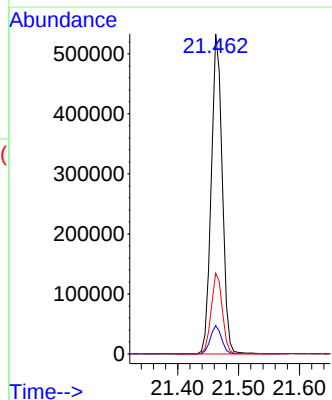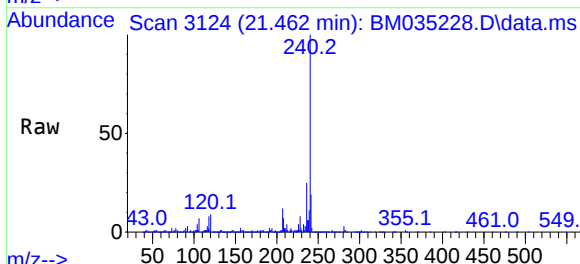



#78
Pyrene
Concen: 5.137 ng
RT: 19.698 min Scan# 2824
Delta R.T. -0.012 min
Lab File: BM035228.D
Acq: 24 May 2022 20:33




Instrument :
BNA_M
ClientSampleId :
SB-8(0.5-1)

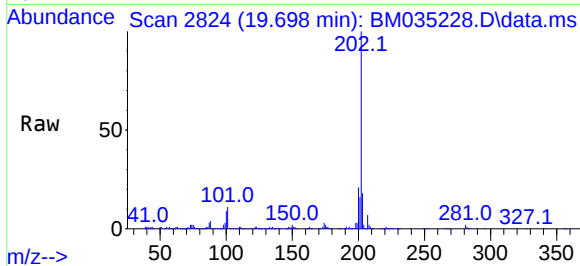


Tgt Ion:202 Resp: 227730
Ion Ratio Lower Upper
202 100
200 20.6 16.7 25.1
203 17.6 13.9 20.9

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 05/25/2022
Supervised By :Jagrut Upadhyay 05/25/2022

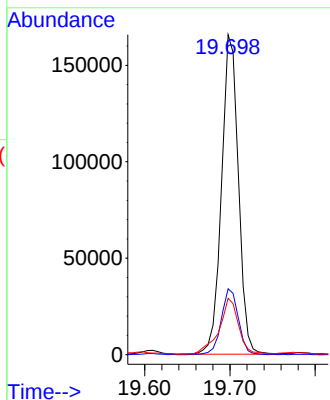


#79
Terphenyl-d14
Concen: 52.292 ng
RT: 19.904 min Scan# 2859
Delta R.T. -0.012 min
Lab File: BM035228.D
Acq: 24 May 2022 20:33

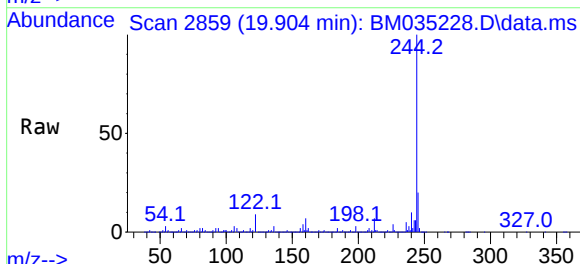

Tgt Ion:244 Resp: 1810457
Ion Ratio Lower Upper
244 100
212 7.3 6.2 9.4
122 9.1 8.3 12.5

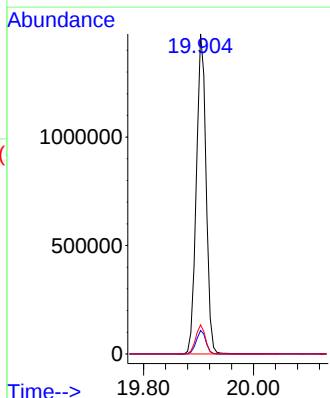







#81
Benzo(a)anthracene
Concen: 4.101 ng
RT: 21.451 min Scan# 31
Delta R.T. -0.006 min
Lab File: BM035228.D
Acq: 24 May 2022 20:33

Instrument :
BNA_M
ClientSampleId :
SB-8(0.5-1)

Tgt Ion:228 Resp: 18344
Ion Ratio Lower Upper
228 100
226 29.2 22.3 33.5
229 20.2 15.8 23.6




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 05/25/2022
Supervised By :Jagrut Upadhyay 05/25/2022

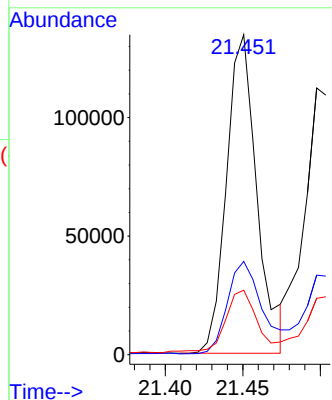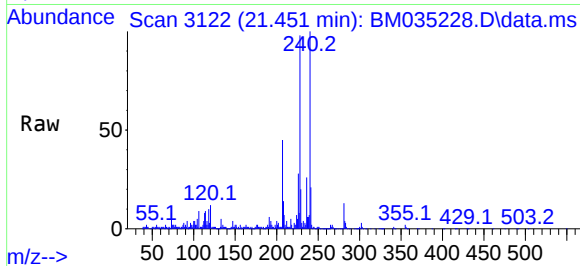

#83
Chrysene
Concen: 3.742 ng
RT: 21.498 min Scan# 3130
Delta R.T. -0.012 min
Lab File: BM035228.D
Acq: 24 May 2022 20:33

Tgt Ion:228 Resp: 159858
Ion Ratio Lower Upper
228 100
226 29.8 24.4 36.6
229 21.1 15.8 23.8

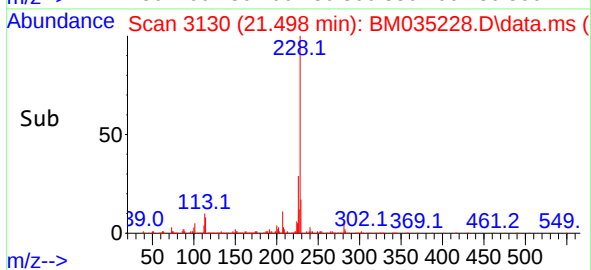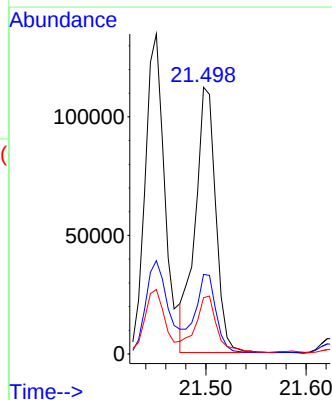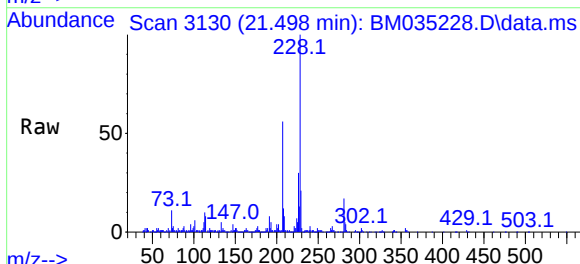







#86
Perylene-d12
Concen: 20.000 ng
RT: 23.850 min Scan# 31
Delta R.T. -0.006 min
Lab File: BM035228.D
Acq: 24 May 2022 20:33

Instrument :
BNA_M
ClientSampleId :
SB-8(0.5-1)

Tgt Ion:264 Resp: 728760
Ion Ratio Lower Upper
264 100
260 23.5 18.9 28.3
265 22.4 17.5 26.3




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 05/25/2022
Supervised By :Jagrut Upadhyay 05/25/2022

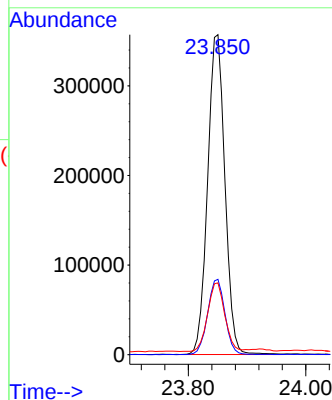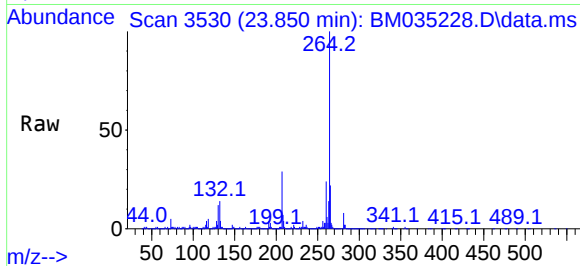

#87
Indeno(1,2,3-cd)pyrene
Concen: 2.012 ng
RT: 26.309 min Scan# 3948
Delta R.T. -0.023 min
Lab File: BM035228.D
Acq: 24 May 2022 20:33


Tgt Ion:276 Resp: 111500
Ion Ratio Lower Upper
276 100
138 21.3 20.2 30.4
277 24.3 20.2 30.2

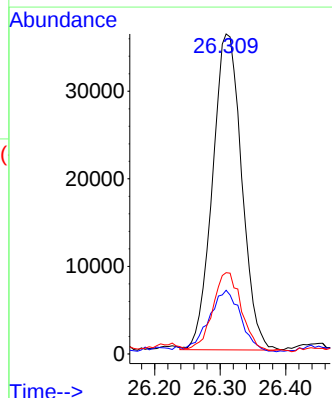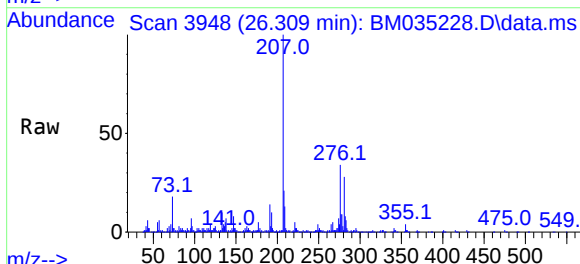



#88
Benzo(b)fluoranthene
Concen: 4.945 ng m
RT: 23.127 min Scan# 3411
Delta R.T. -0.006 min
Lab File: BM035228.D
Acq: 24 May 2022 20:33




Instrument :
BNA_M
ClientSampleId :
SB-8(0.5-1)

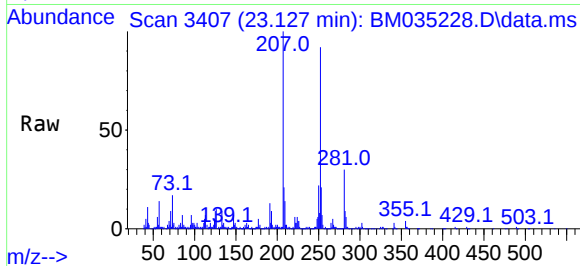


Tgt Ion:252 Resp: 226649
Ion Ratio Lower Upper
252 100
253 23.4 17.6 26.4
125 10.1 7.6 11.4

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 05/25/2022
Supervised By :Jagrut Upadhyay 05/25/2022

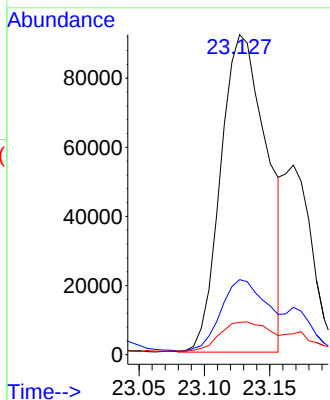


#90
Benzo(a)pyrene
Concen: 4.274 ng
RT: 23.739 min Scan# 3511
Delta R.T. -0.012 min
Lab File: BM035228.D
Acq: 24 May 2022 20:33

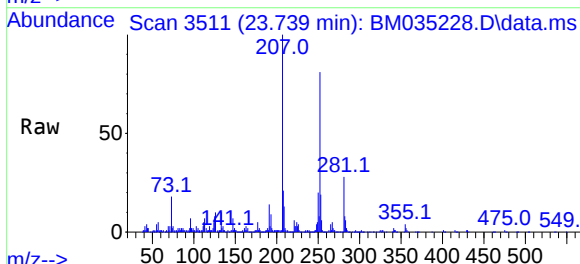


Tgt Ion:252 Resp: 162742
Ion Ratio Lower Upper
252 100
253 23.7 17.2 25.8
125 10.2 8.7 13.1

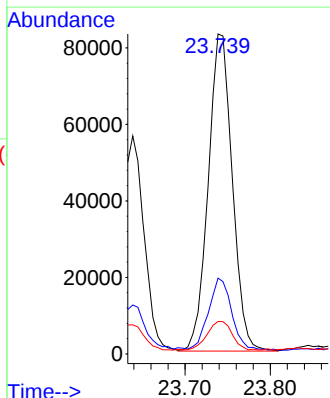



#92
 Benzo(g,h,i)perylene
 Concen: 2.247 ng
 RT: 27.068 min Scan# 40
 Delta R.T. -0.023 min
 Lab File: BM035228.D
 Acq: 24 May 2022 20:33

Instrument :
 BNA_M
 ClientSampleId :
 SB-8(0.5-1)



Tgt Ion: 276 Resp: 100364

Ion	Ratio	Lower	Upper
276	100		
277	24.6	18.7	28.1
138	19.8	17.6	26.4

Manual Integrations
 APPROVED

Reviewed By :Christian Giraldo 05/25/2022
 Supervised By :Jagrut Upadhyay 05/25/2022

