

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052422\
 Data File : BM035216.D
 Acq On : 24 May 2022 13:15
 Operator : CG/JU
 Sample : PB145012BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB145012BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM035216.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.481	400	407	426	rBV	2671015	3783168	53.58%	10.935%
2	7.075	670	678	691	rBV	2382328	3775036	53.47%	10.911%
3	7.898	812	818	828	rBV	506880	807423	11.44%	2.334%
4	9.063	1007	1016	1039	rBV	1487722	2506194	35.50%	7.244%
5	10.704	1287	1295	1311	rBV	623187	1068283	15.13%	3.088%
6	13.163	1706	1713	1731	rBV	3872013	5734916	81.23%	16.576%
7	14.539	1940	1947	1963	rBV	894766	1354134	19.18%	3.914%
8	16.027	2193	2200	2225	rBV	2486004	3853640	54.58%	11.138%
9	17.280	2407	2413	2426	rBV	970188	1458622	20.66%	4.216%
10	18.186	2561	2567	2577	rBV	59038	116684	1.65%	0.337%
11	19.462	2780	2784	2792	rBV5	38095	76928	1.09%	0.222%
12	19.909	2854	2860	2868	rBV	5701765	7060372	100.00%	20.407%
13	21.468	3120	3125	3133	rBV	1131466	1492339	21.14%	4.313%
14	23.856	3525	3531	3541	rVB2	707665	1510527	21.39%	4.366%




Sum of corrected areas: 34598266

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052422\
Data File : BM035216.D
Acq On : 24 May 2022 13:15
Operator : CG/JU
Sample : PB145012BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145012BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

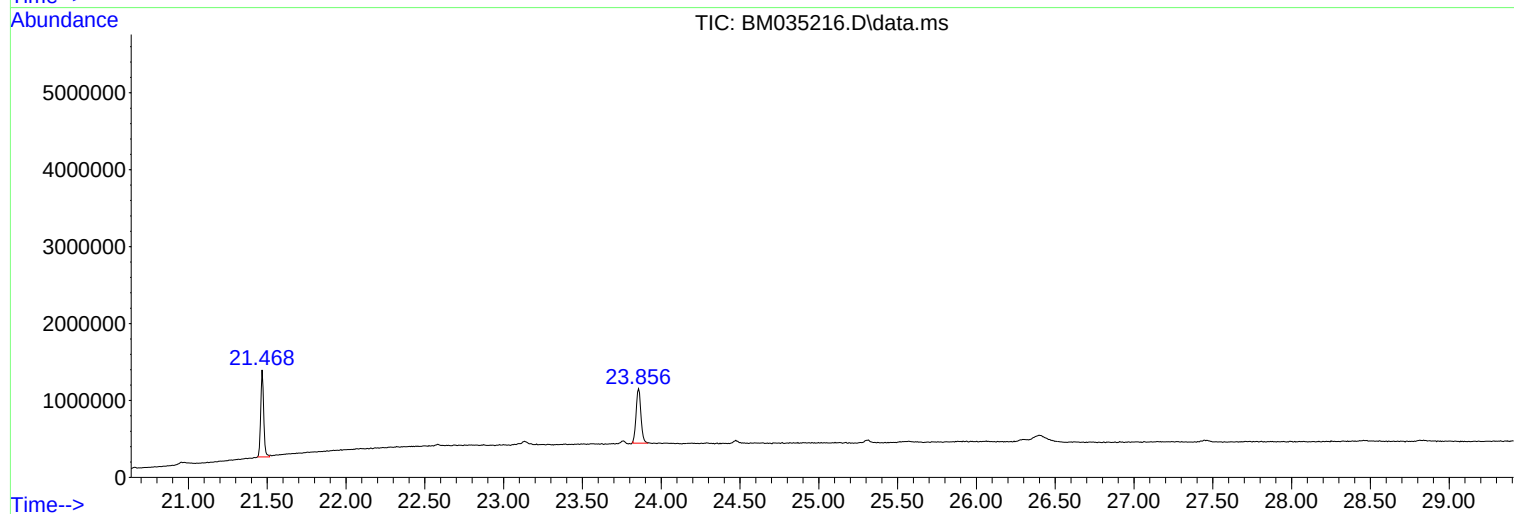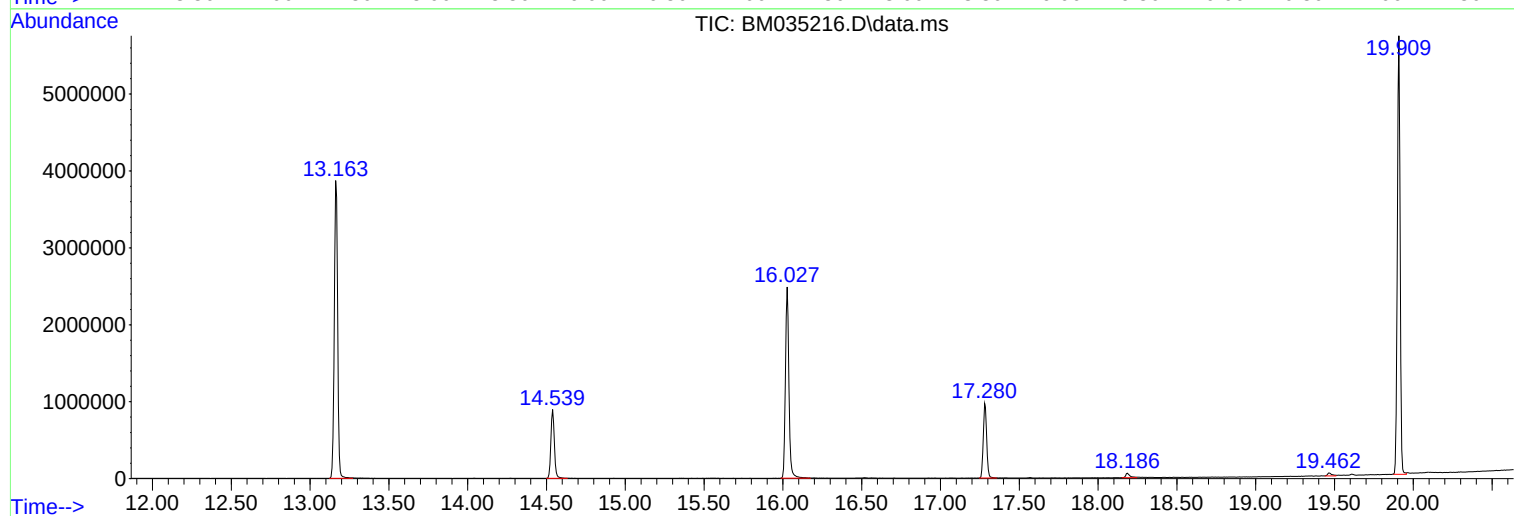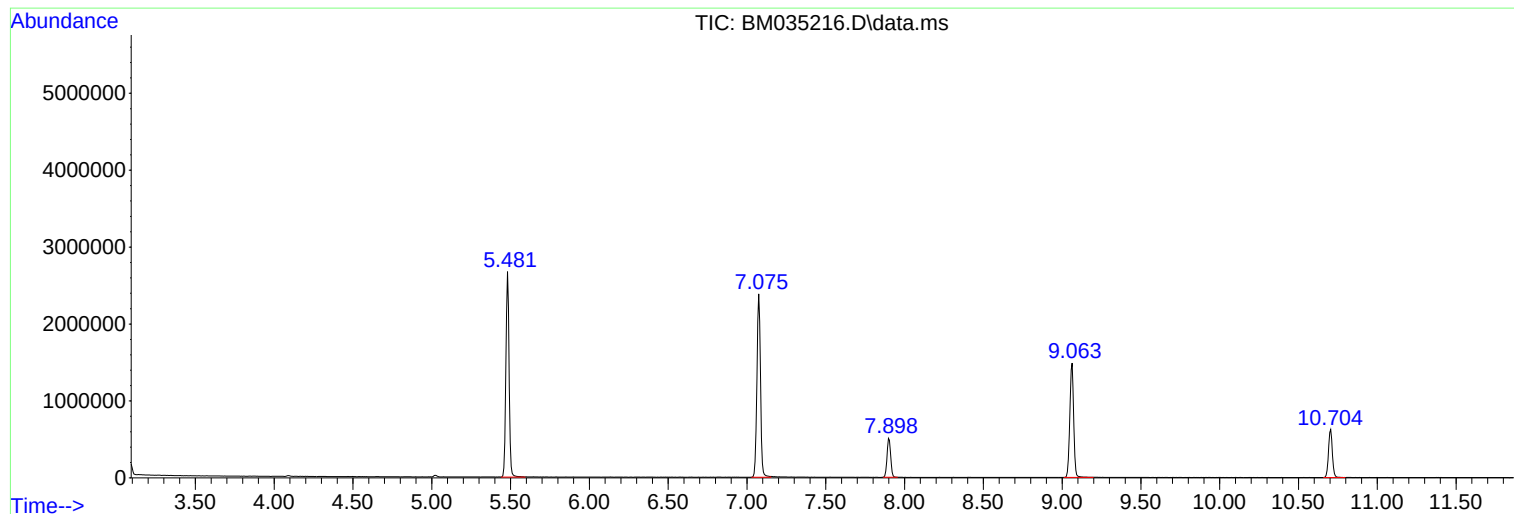

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052422\
Data File : BM035216.D
Acq On : 24 May 2022 13:15
Operator : CG/JU
Sample : PB145012BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145012BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052422\
Data File : BM035216.D
Acq On : 24 May 2022 13:15
Operator : CG/JU
Sample : PB145012BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145012BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------