

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052422\
 Data File : BM035226.D
 Acq On : 24 May 2022 19:20
 Operator : CG/JU
 Sample : N2981-14
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SB-9(4.5-5)

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM035226.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	28	31	42	rVB	47386	71110	1.31%	0.236%
2	5.481	400	407	426	rBV	1662895	2539507	46.89%	8.421%
3	7.069	670	677	696	rBV	1625170	2659814	49.11%	8.820%
4	7.898	810	818	827	rBV	469096	740990	13.68%	2.457%
5	9.057	1007	1015	1026	rBV	1050937	1753486	32.37%	5.814%
6	10.698	1287	1294	1310	rBV	578832	1008020	18.61%	3.342%
7	13.163	1706	1713	1727	rBV	2598889	3878181	71.60%	12.860%
8	14.539	1940	1947	1955	rBV	821062	1272383	23.49%	4.219%
9	16.027	2193	2200	2221	rBV	1803142	2907464	53.68%	9.641%
10	17.280	2404	2413	2418	rBV	1030496	1515381	27.98%	5.025%
11	17.321	2418	2420	2428	rVV	126293	172996	3.19%	0.574%
12	17.409	2428	2435	2443	rVB2	43352	75143	1.39%	0.249%
13	18.186	2560	2567	2578	rVV2	225728	418144	7.72%	1.387%
14	19.339	2756	2763	2771	rBV	267500	423376	7.82%	1.404%
15	19.462	2779	2784	2793	rBV3	111283	169573	3.13%	0.562%
16	19.668	2815	2819	2821	rBV	49801	70438	1.30%	0.234%
17	19.703	2821	2825	2833	rVB	204277	311384	5.75%	1.033%
18	19.903	2853	2859	2865	rBV	4497716	5416378	100.00%	17.960%
19	20.027	2876	2880	2887	rBV5	24178	55362	1.02%	0.184%
20	21.186	3073	3077	3083	rBV2	215785	283394	5.23%	0.940%
21	21.462	3118	3124	3128	rBV2	1515876	2122048	39.18%	7.036%
22	21.497	3128	3130	3139	rVB	161638	227927	4.21%	0.756%
23	23.850	3523	3530	3548	rVB2	979522	2065321	38.13%	6.848%




Sum of corrected areas: 30157820

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052422\
Data File : BM035226.D
Acq On : 24 May 2022 19:20
Operator : CG/JU
Sample : N2981-14
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SB-9(4.5-5)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

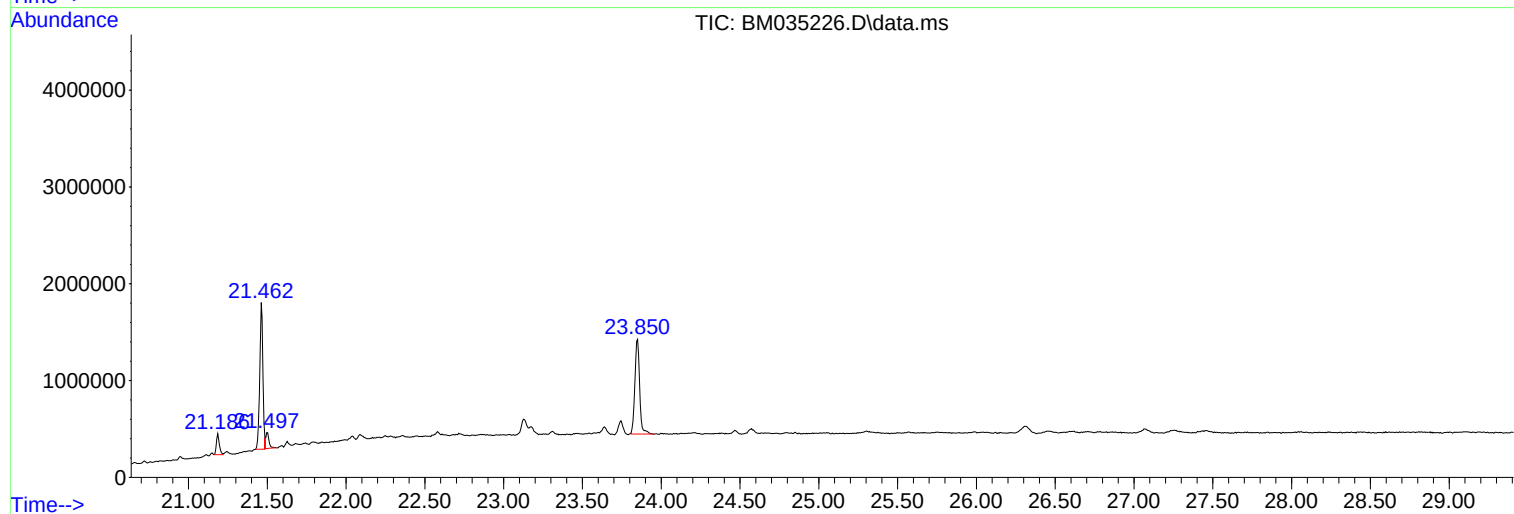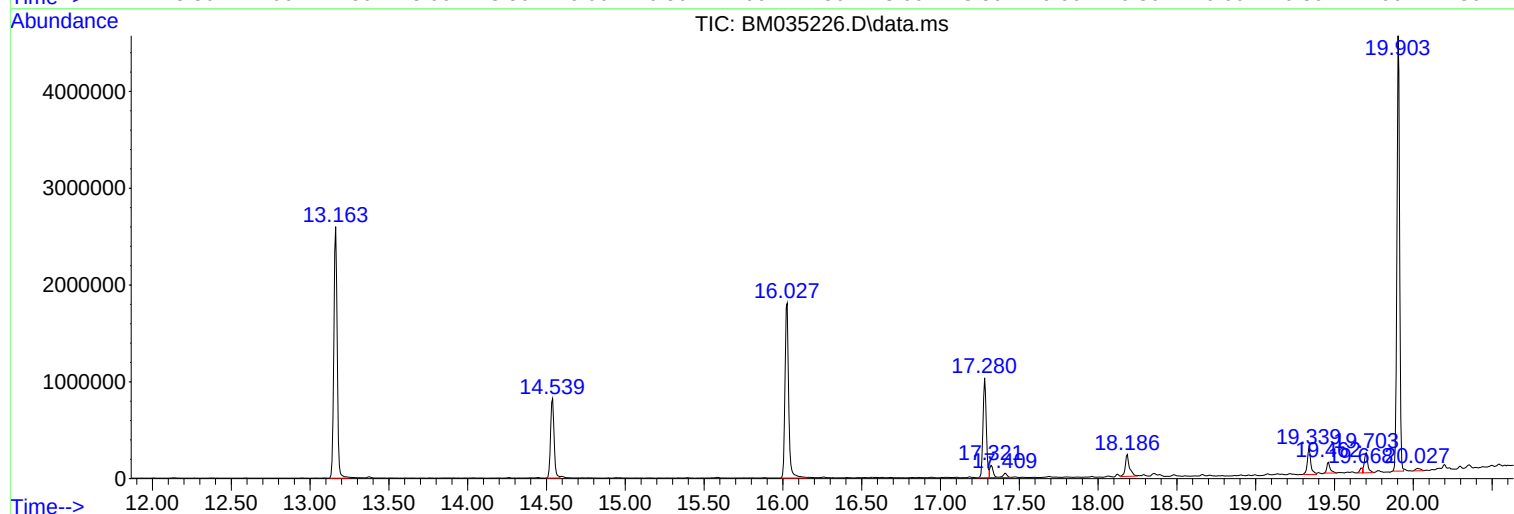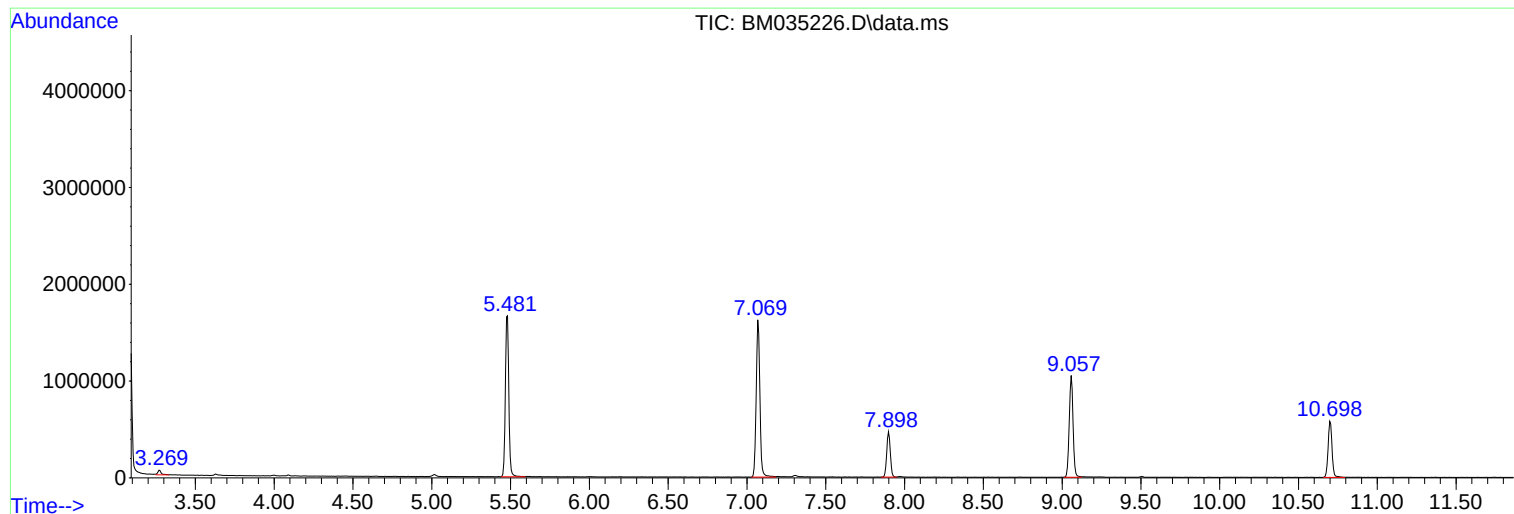

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052422\
Data File : BM035226.D
Acq On : 24 May 2022 19:20
Operator : CG/JU
Sample : N2981-14
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SB-9(4.5-5)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052422\
Data File : BM035226.D
Acq On : 24 May 2022 19:20
Operator : CG/JU
Sample : N2981-14
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SB-9(4.5-5)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------