


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052422\
 Data File : BM035214.D
 Acq On : 24 May 2022 12:00
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri May 20 04:53:59 2022

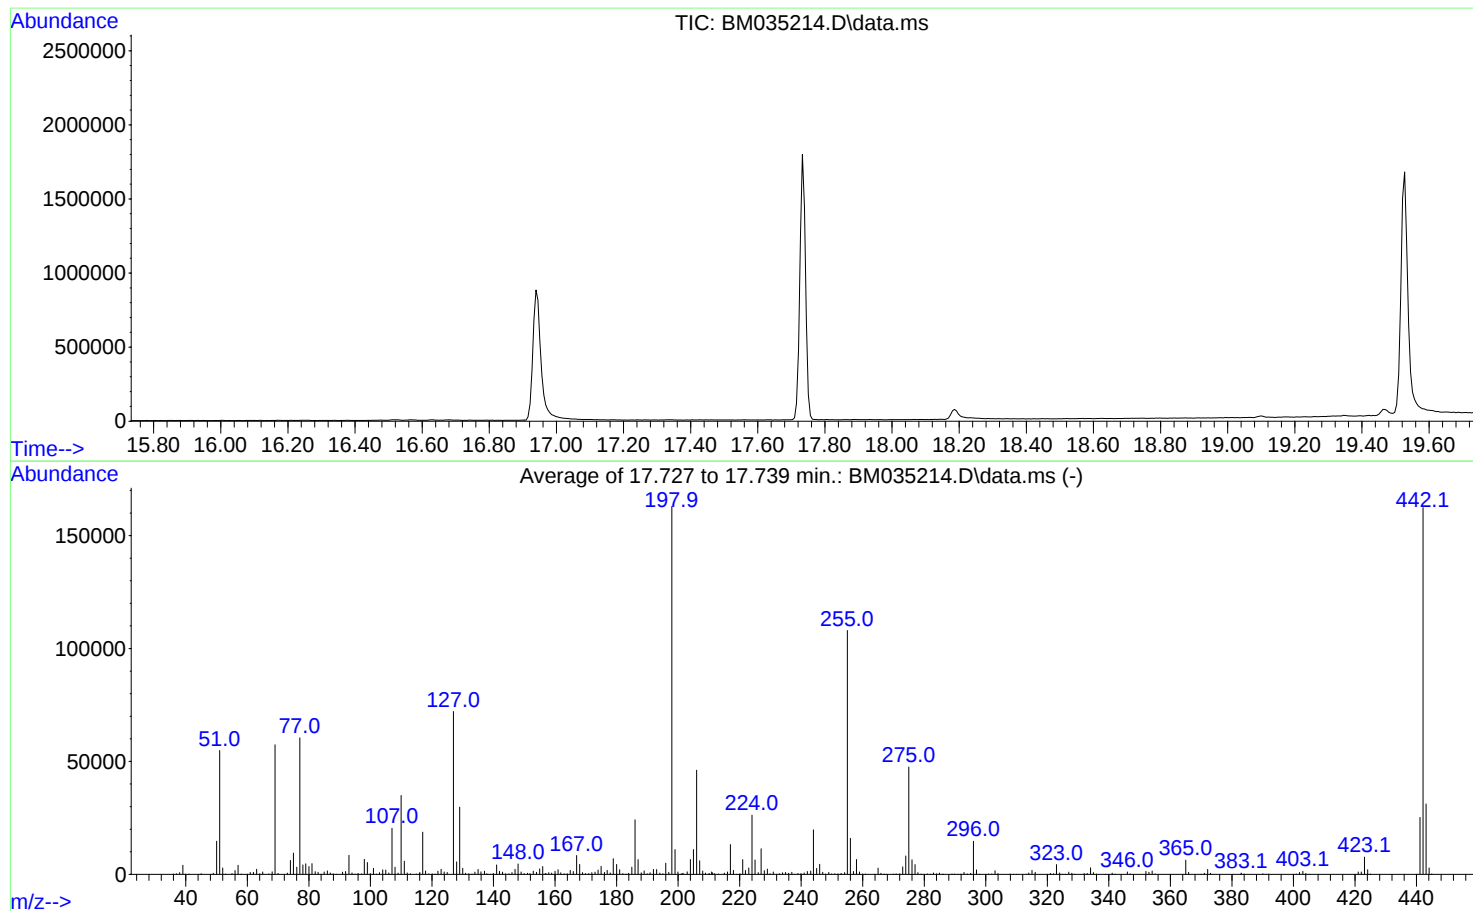




AutoFind: Scans 2489, 2490, 2491; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.7	54867	PASS
68	69	0.00	2	2.0	1130	PASS
69	198	0.00	100	35.2	57371	PASS
70	69	0.00	2	0.7	393	PASS
127	198	10	80	44.3	72128	PASS
197	198	0.00	2	0.6	903	PASS
198	198	100	100	100.0	162880	PASS
199	198	5	9	6.8	11011	PASS
275	198	10	60	29.2	47571	PASS
365	198	1	100	3.9	6342	PASS
441	198	0.01	100	15.5	25244	PASS
442	442	50	100	100.0	162360	PASS
443	442	15	24	19.2	31160	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052422\
 Data File : BM035214.D
 Acq On : 24 May 2022 12:00
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: May 25 07:28:54 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri May 20 04:53:59 2022
 Response via : Initial Calibration

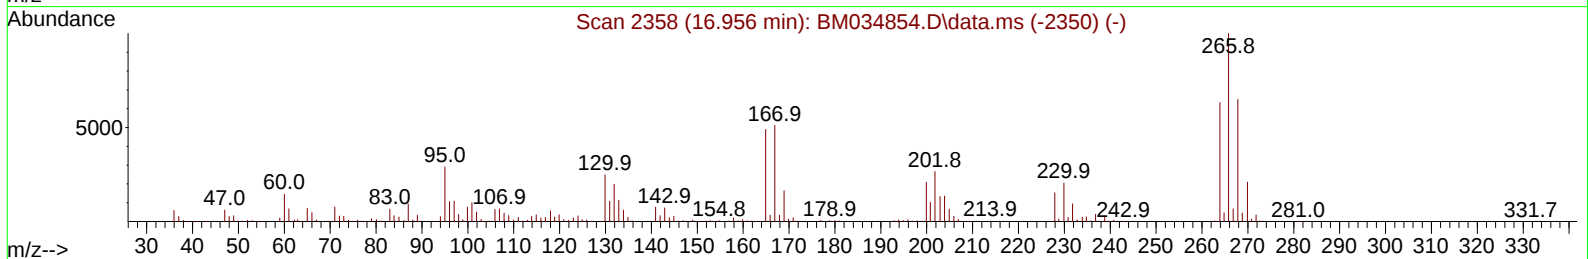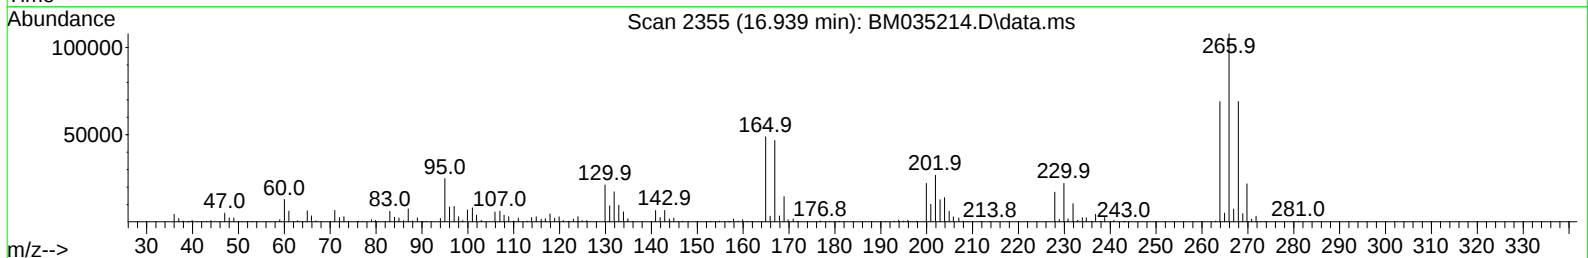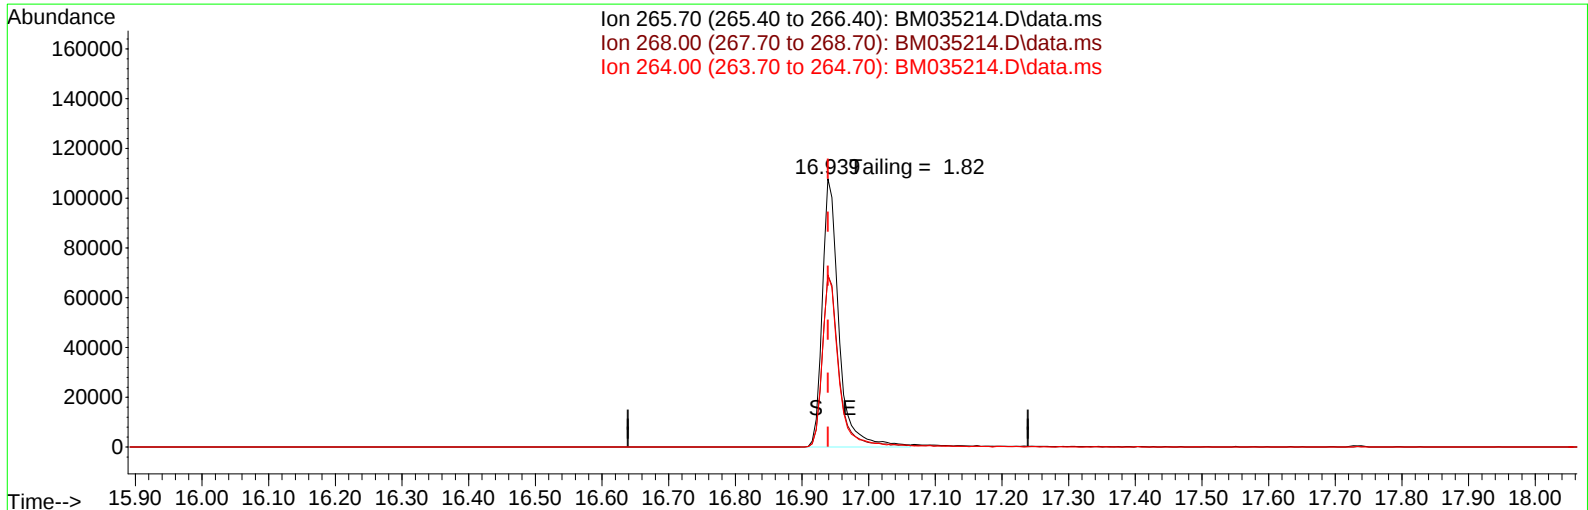

TIC: BM035214.D\data.ms

(70) Pentachlorophenol (C)

16.939min (-0.000) 43519.18 ng




response 187131

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	64.05
264.00	63.30	64.01
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052422\
Data File : BM035214.D
Acq On : 24 May 2022 12:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: May 25 07:28:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri May 20 04:53:59 2022
Response via : Initial Calibration

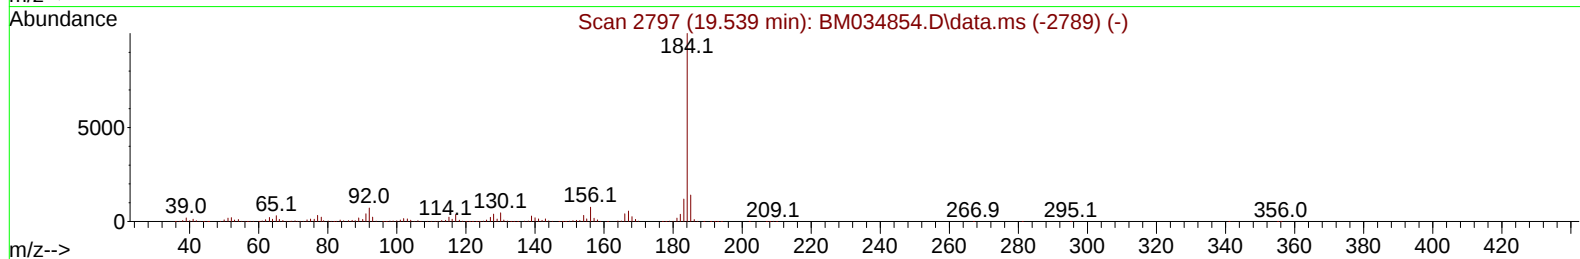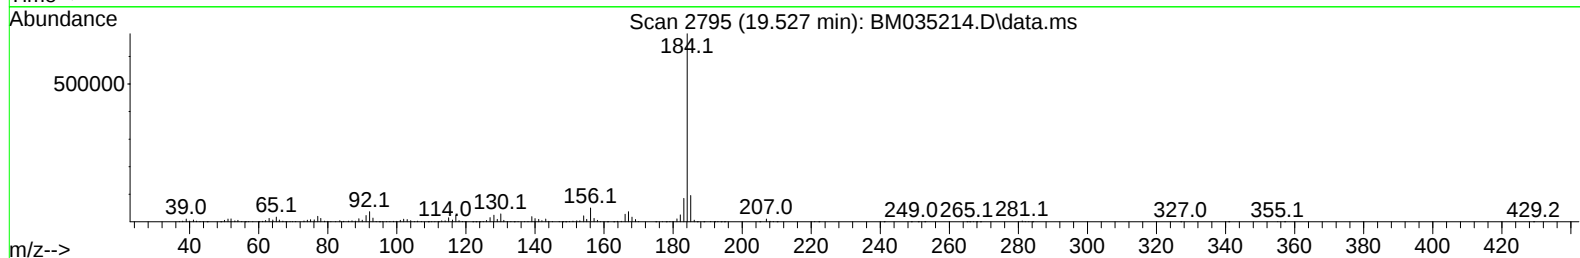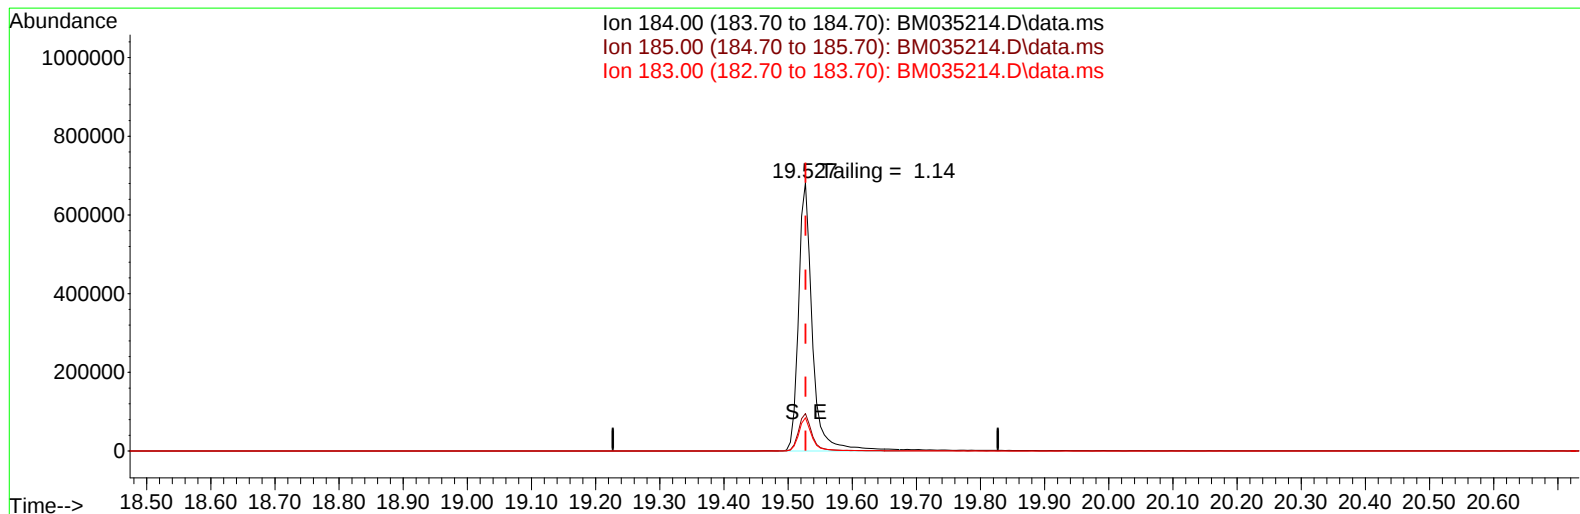

TIC: BM035214.D\data.ms

(77) Benzidine

19.527min (-0.000) 18195.68 ng

response 1036690

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.97
183.00	11.90	12.42
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/24/2022	BNA_M	<u>BM035214.D</u>
Compound Name	Response	Retention Time
DDT	573892	20.762
DDD	8111	20.327
DDE	1379	19.821
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9490	583382	1.63

Instrument :
BNA_M
ClientSampleId :
DFTPP