
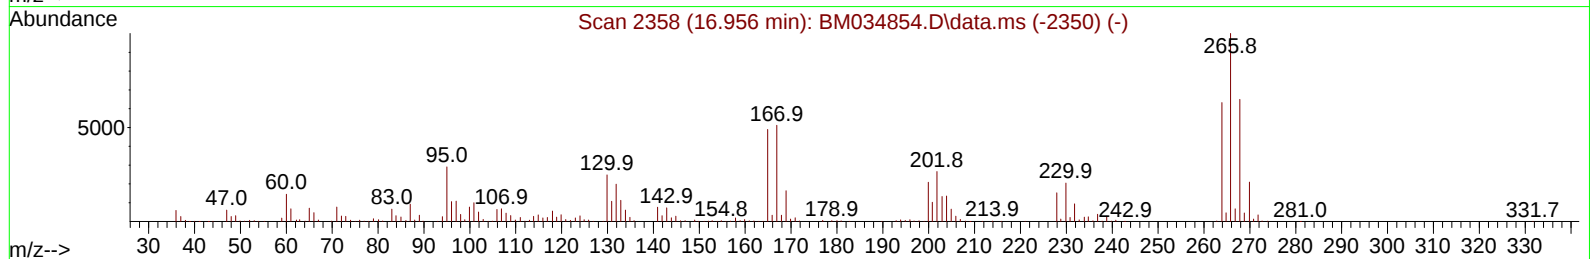
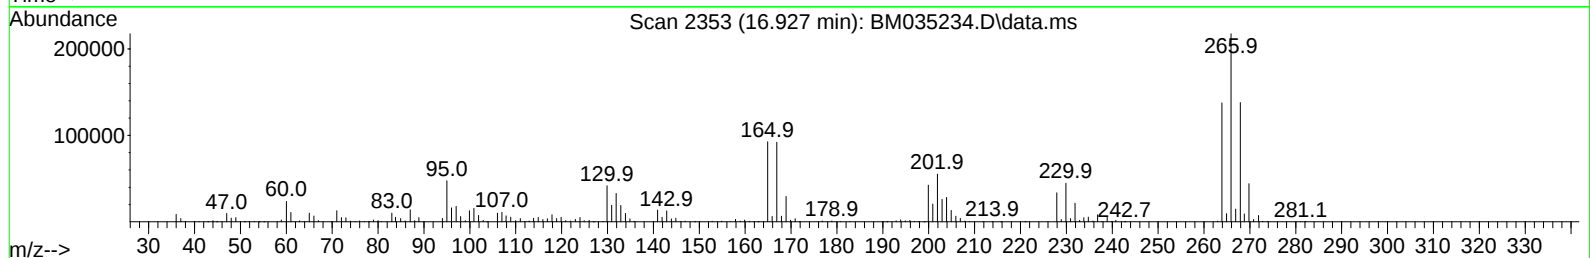


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052522\
 Data File : BM035234.D
 Acq On : 25 May 2022 09:30
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 26 08:29:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 26 05:05:10 2022
 Response via : Initial Calibration

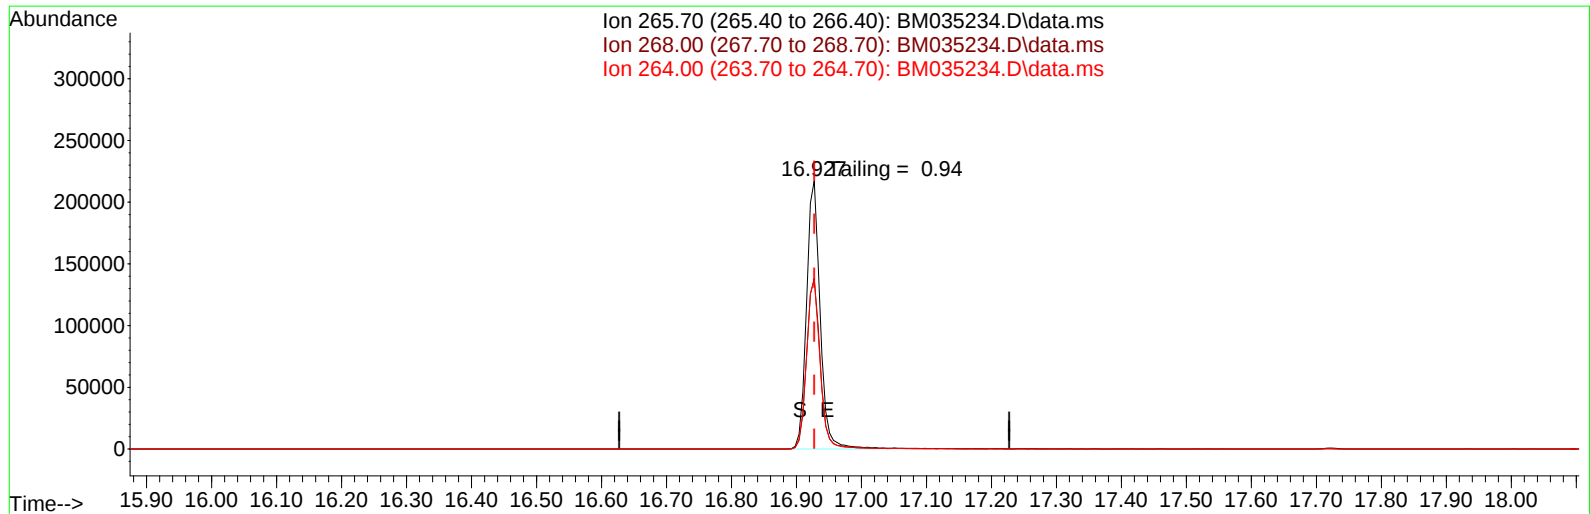

TIC: BM035234.D\data.ms

(70) Pentachlorophenol (C)




16.927min (+ 0.000) 796858.59 ng

response 320873

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	63.42
264.00	63.30	63.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052522\
 Data File : BM035234.D
 Acq On : 25 May 2022 09:30
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 26 08:29:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 26 05:05:10 2022
 Response via : Initial Calibration

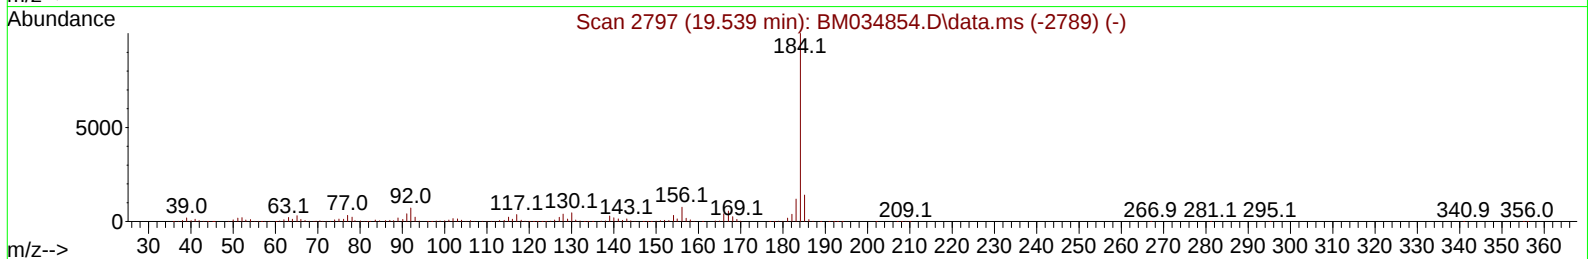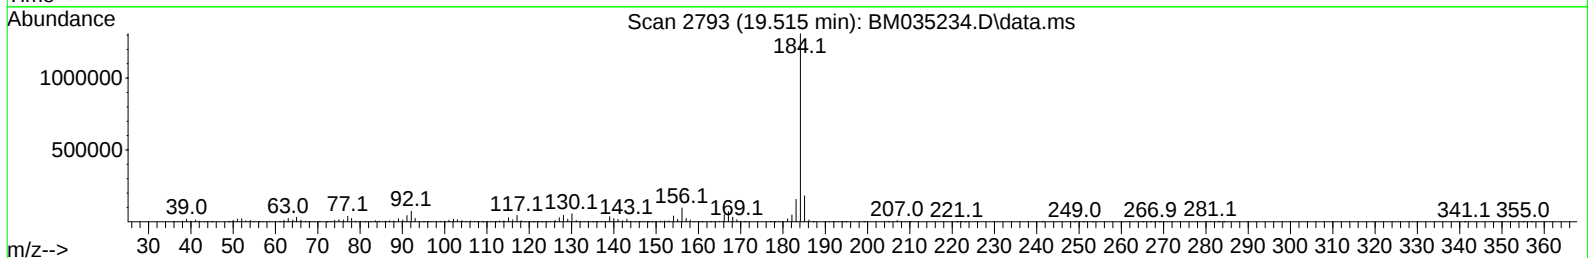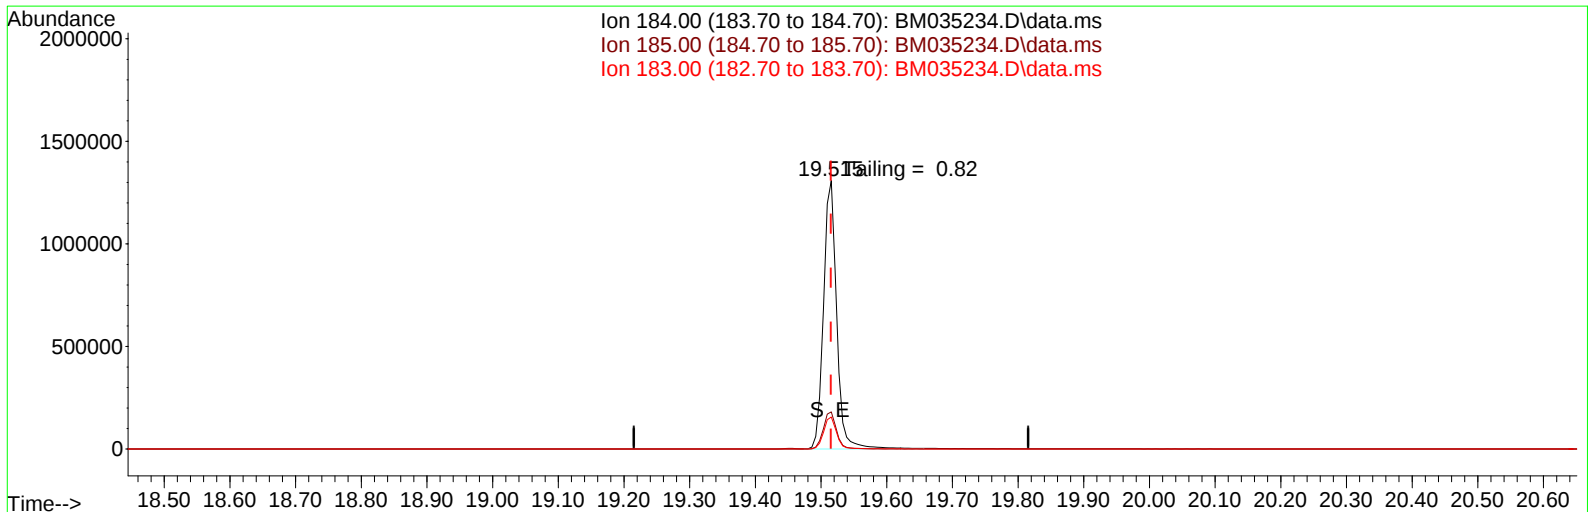

TIC: BM035234.D\data.ms

(77) Benzidine**19.515min (+ 0.000) 127779.95 ng****response 1815171**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.84
183.00	11.90	11.91
0.00	0.00	0.00