
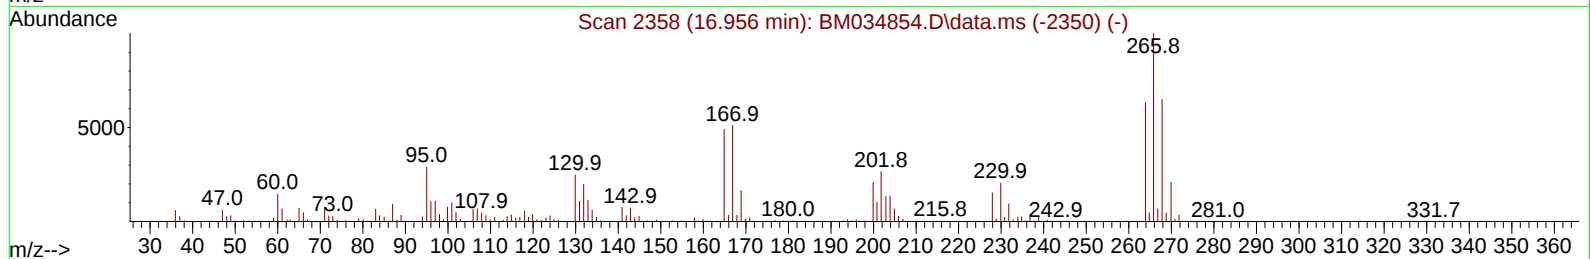
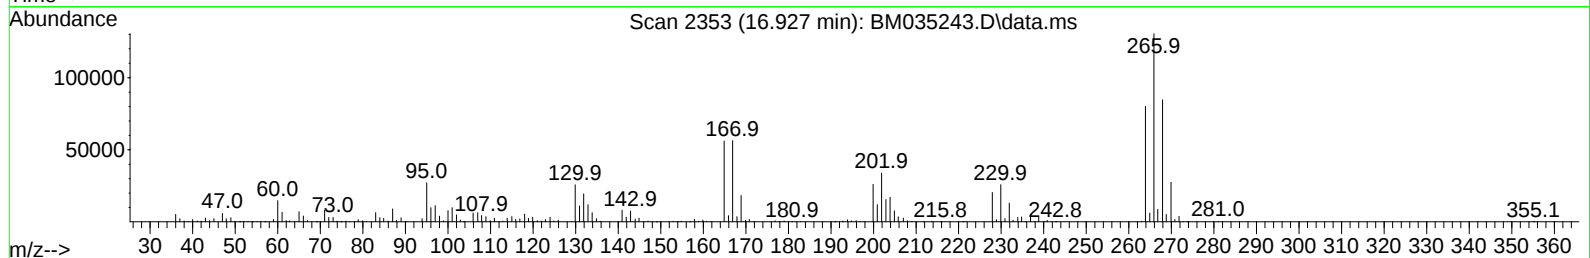


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052522\
 Data File : BM035243.D
 Acq On : 25 May 2022 16:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 26 08:44:36 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 26 05:05:10 2022
 Response via : Initial Calibration

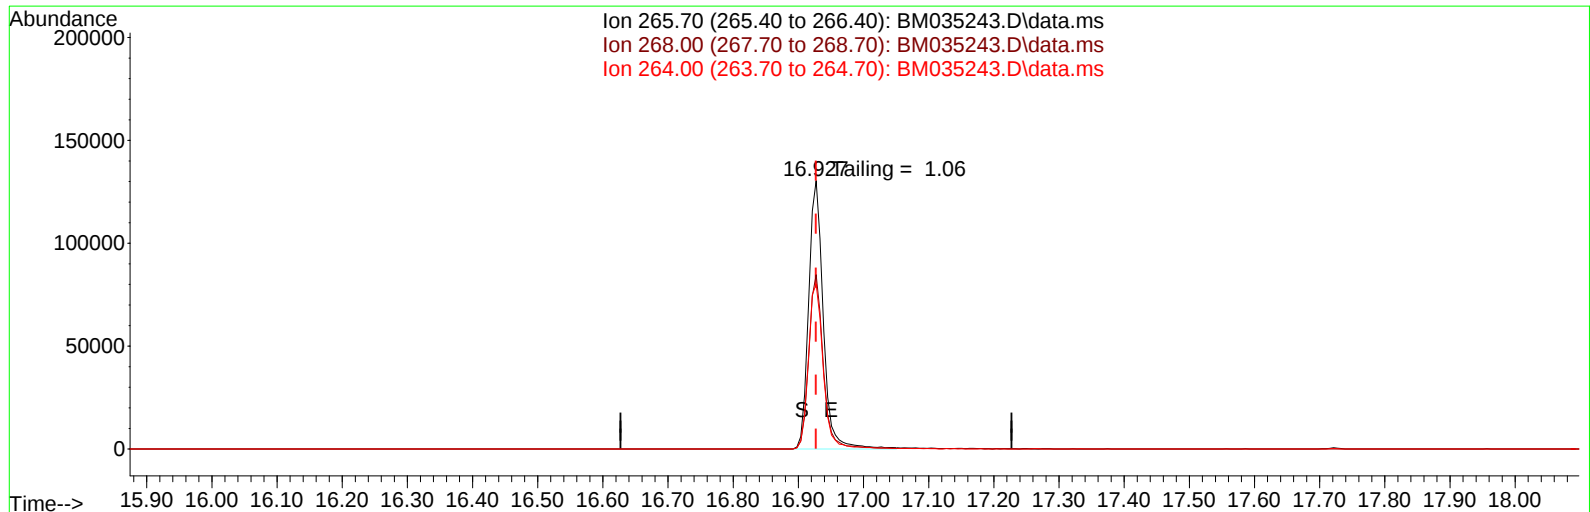

TIC: BM035243.D\data.ms

(70) Pentachlorophenol (C)




16.927min (+ 0.000) 0.00 ng

response 205035

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	64.92
264.00	63.30	61.40
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052522\
Data File : BM035243.D
Acq On : 25 May 2022 16:05
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: May 26 08:44:36 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 26 05:05:10 2022
Response via : Initial Calibration

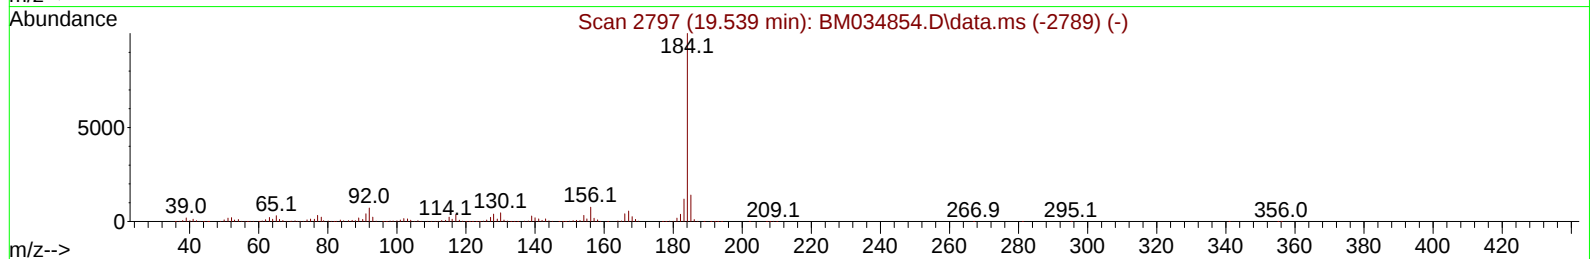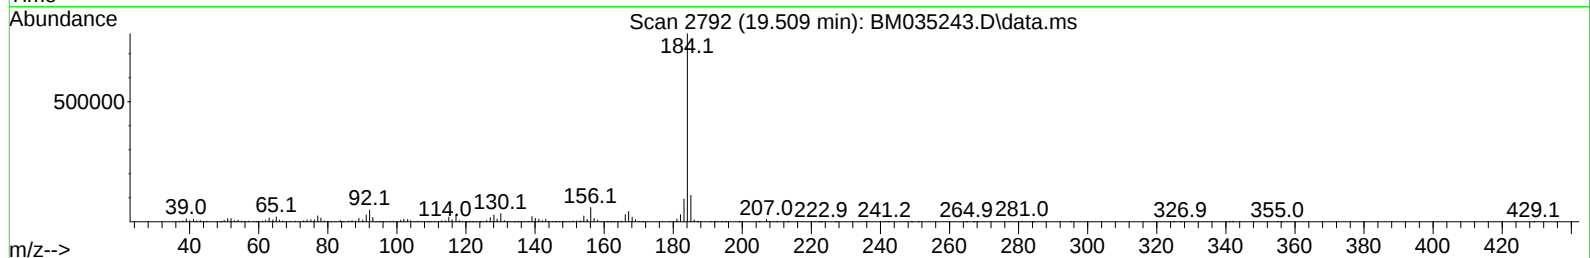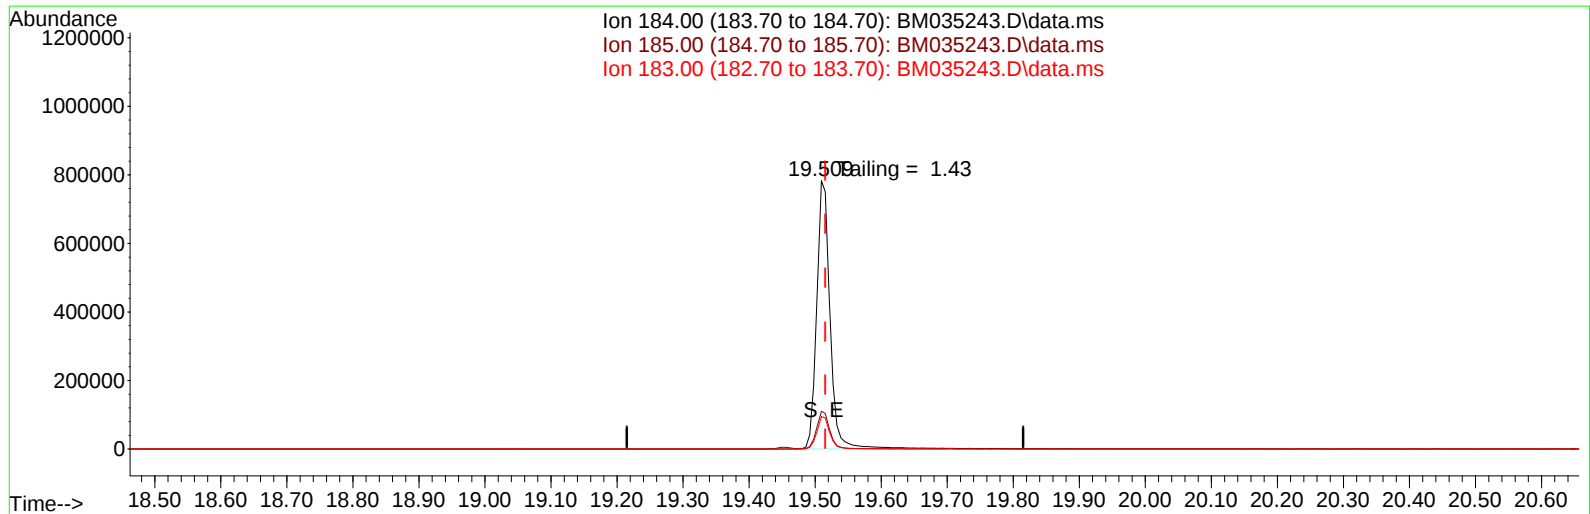

TIC: BM035243.D\data.ms

(77) Benzidine**19.509min (-0.006) 35448.50 ng****response 1102421**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.07
183.00	11.90	12.12
0.00	0.00	0.00