

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052522\
 Data File : BM035247.D
 Acq On : 25 May 2022 18:33
 Operator : CG/JU
 Sample : N2922-09
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 P024-SS001-2430-01

Quant Time: May 26 05:35:55 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 26 05:05:10 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.887	152	108626	20.000	ng	0.00
21) Naphthalene-d8	10.692	136	417333	20.000	ng	0.00
39) Acenaphthene-d10	14.527	164	265575	20.000	ng	0.00
64) Phenanthrene-d10	17.268	188	567918	20.000	ng	0.00
76) Chrysene-d12	21.450	240	595849	20.000	ng	# 0.00
86) Perylene-d12	23.827	264	633163	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.469	112	679723	110.395	ng	0.00
7) Phenol-d6	7.063	99	872315	109.745	ng	0.00
23) Nitrobenzene-d5	9.045	82	568728	73.592	ng	0.00
42) 2,4,6-Tribromophenol	16.015	330	371151	128.474	ng	0.00
45) 2-Fluorobiphenyl	13.151	172	1338133	73.144	ng	0.00
79) Terphenyl-d14	19.898	244	2253069	73.213	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052522\
Data File : BM035247.D
Acq On : 25 May 2022 18:33
Operator : CG/JU
Sample : N2922-09
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P024-SS001-2430-01

Quant Time: May 26 05:35:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 26 05:05:10 2022
Response via : Initial Calibration




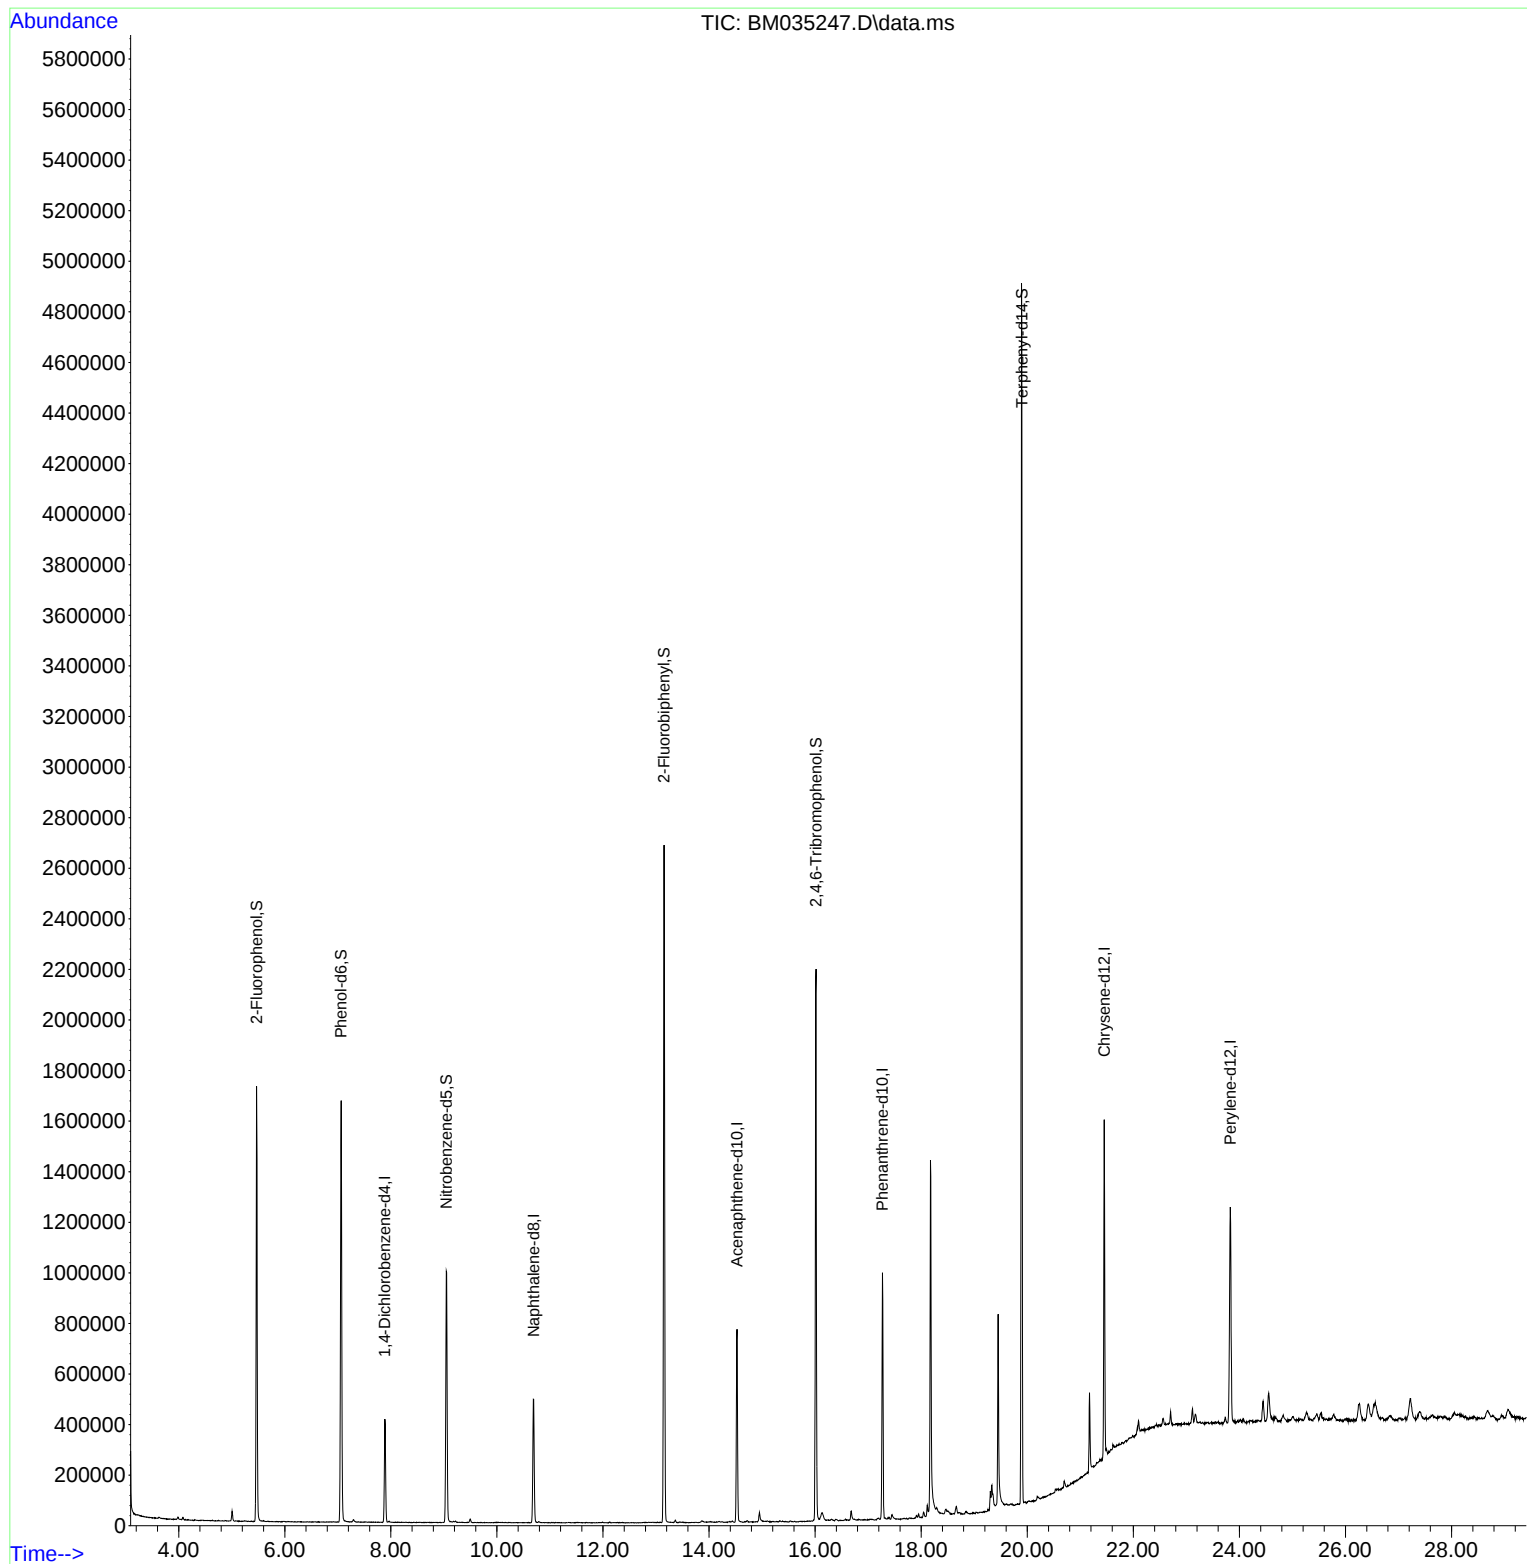




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.887 min Scan# 81
Delta R.T. -0.000 min
Lab File: BM035247.D
Acq: 25 May 2022 18:33




Instrument :
BNA_M
ClientSampleId :
P024-SS001-2430-01

Tgt Ion:152 Resp: 108626
Ion Ratio Lower Upper
152 100
150 156.1 124.9 187.3
115 60.0 47.9 71.9

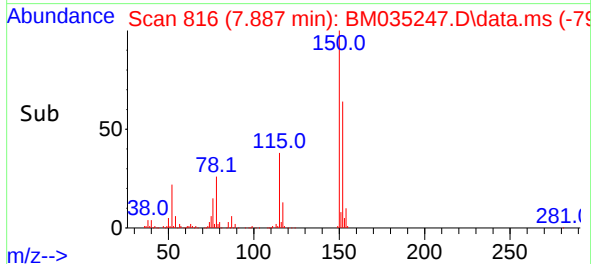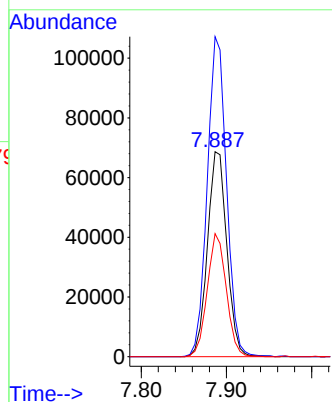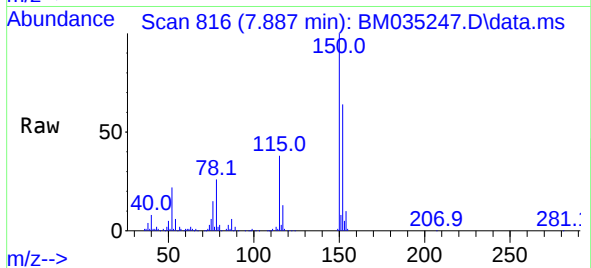

#5
2-Fluorophenol
Concen: 110.395 ng
RT: 5.469 min Scan# 405
Delta R.T. -0.000 min
Lab File: BM035247.D
Acq: 25 May 2022 18:33

Tgt Ion:112 Resp: 679723
Ion Ratio Lower Upper
112 100
64 59.0 47.8 71.6
63 33.3 26.6 40.0


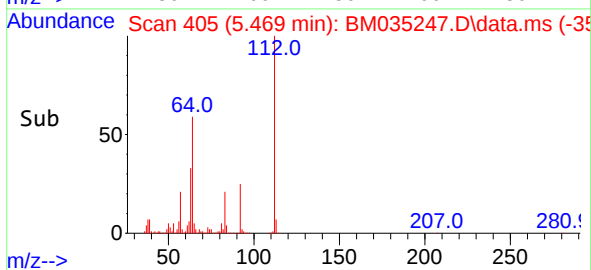
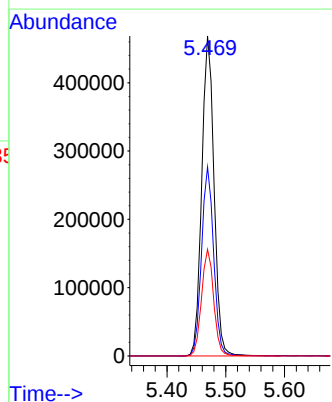
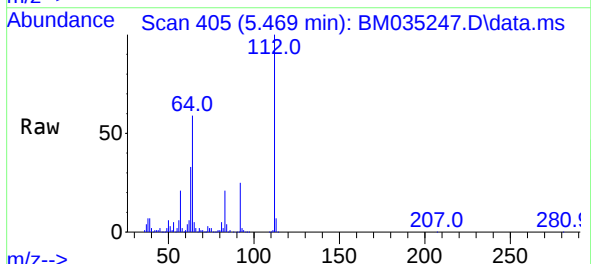




#7
Phenol-d6
Concen: 109.745 ng
RT: 7.063 min Scan# 61
Delta R.T. -0.000 min
Lab File: BM035247.D
Acq: 25 May 2022 18:33




Instrument :
BNA_M
ClientSampleId :
P024-SS001-2430-01

Tgt Ion: 99 Resp: 872315
Ion Ratio Lower Upper
99 100
42 21.6 18.8 28.2
71 38.0 30.2 45.2

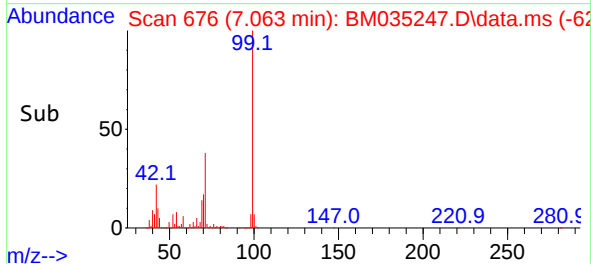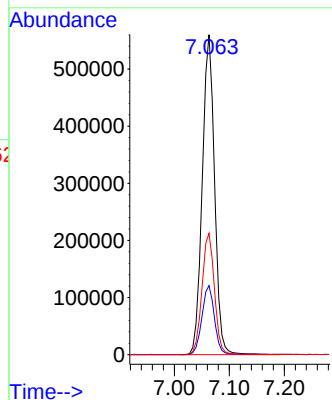

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.692 min Scan# 1293
Delta R.T. -0.000 min
Lab File: BM035247.D
Acq: 25 May 2022 18:33

Tgt Ion: 136 Resp: 417333
Ion Ratio Lower Upper
136 100
137 10.8 8.9 13.3
54 7.2 7.0 10.4
68 5.0 4.3 6.5


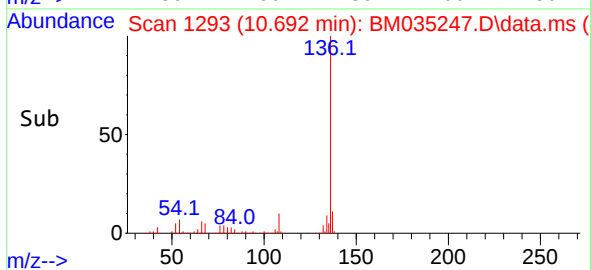
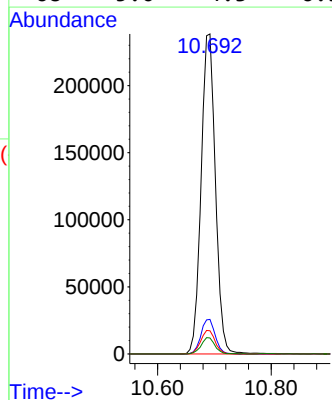
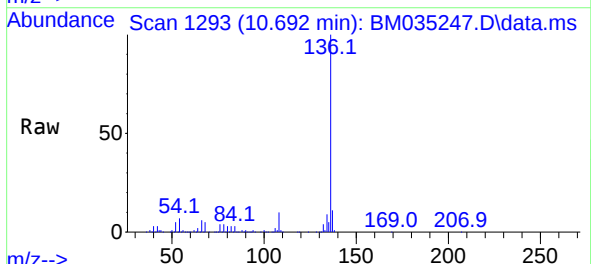




#23
Nitrobenzene-d5
Concen: 73.592 ng
RT: 9.045 min Scan# 1013
Delta R.T. -0.006 min
Lab File: BM035247.D
Acq: 25 May 2022 18:33




Instrument :
BNA_M
ClientSampleId :
P024-SS001-2430-01


Tgt Ion: 82 Resp: 568728
Ion Ratio Lower Upper
82 100
128 42.3 33.7 50.5
54 52.4 43.2 64.8

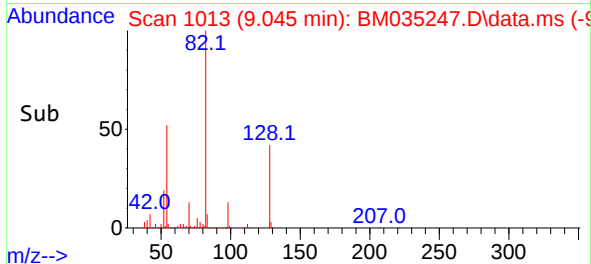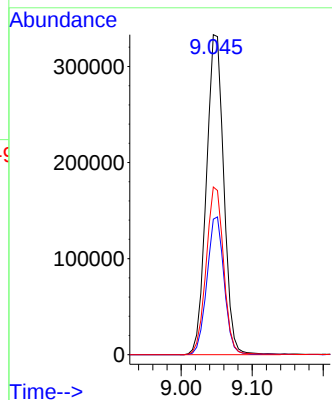

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.527 min Scan# 1945
Delta R.T. -0.000 min
Lab File: BM035247.D
Acq: 25 May 2022 18:33


Tgt Ion: 164 Resp: 265575
Ion Ratio Lower Upper
164 100
162 102.4 83.0 124.6
160 44.8 37.0 55.4

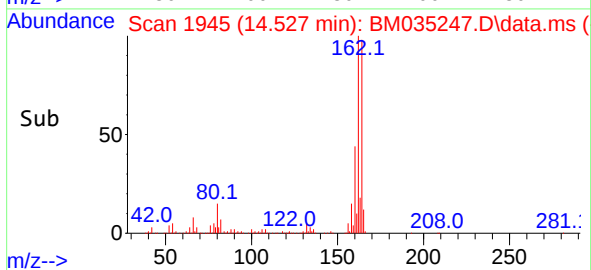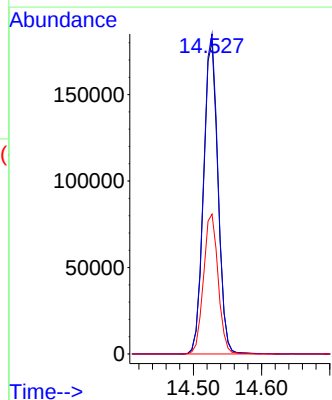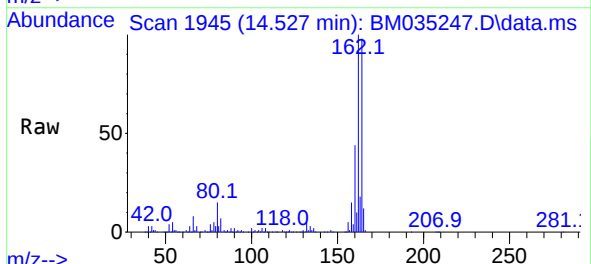






#42
2,4,6-Tribromophenol
Concen: 128.474 ng
RT: 16.015 min Scan# 21
Delta R.T. -0.000 min
Lab File: BM035247.D
Acq: 25 May 2022 18:33

Instrument :
BNA_M
ClientSampleId :
P024-SS001-2430-01



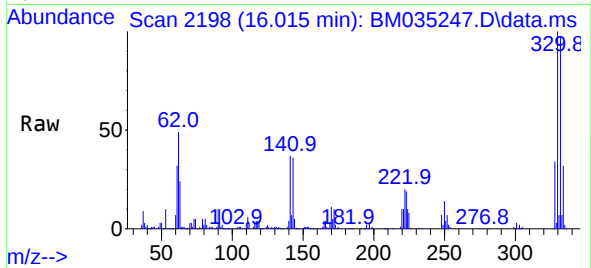



Tgt Ion:330 Resp: 371151
Ion Ratio Lower Upper
330 100
332 96.8 77.0 115.4
141 39.4 35.3 52.9

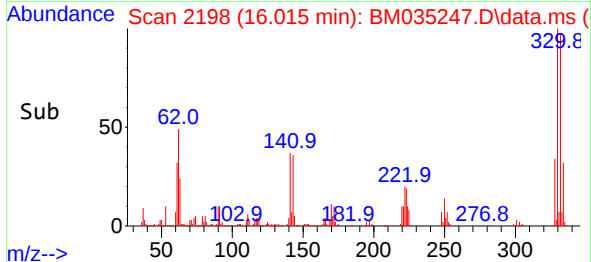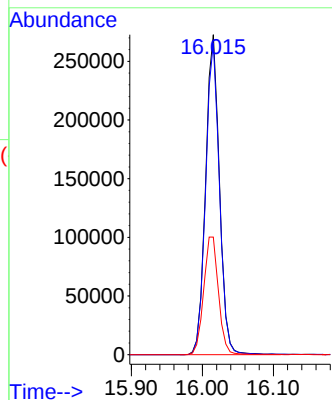

#45
2-Fluorobiphenyl
Concen: 73.144 ng
RT: 13.151 min Scan# 1711
Delta R.T. -0.006 min
Lab File: BM035247.D
Acq: 25 May 2022 18:33

Tgt Ion:172 Resp: 1338133
Ion Ratio Lower Upper
172 100
171 35.0 28.5 42.7
170 23.4 18.7 28.1


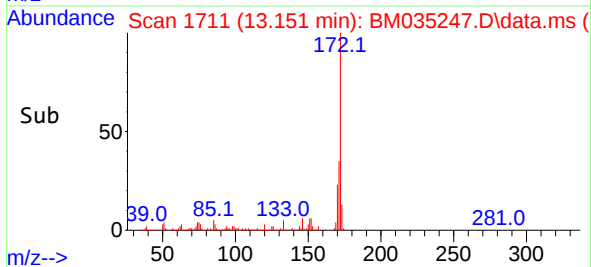
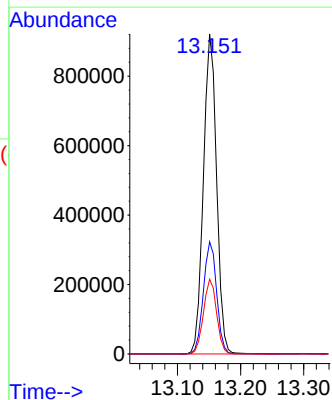
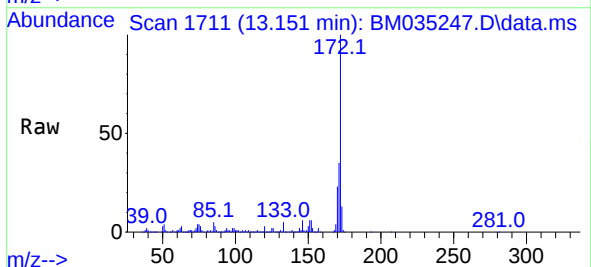




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.268 min Scan# 2417
Delta R.T. -0.000 min
Lab File: BM035247.D
Acq: 25 May 2022 18:33




Instrument :
BNA_M
ClientSampleId :
P024-SS001-2430-01


Tgt Ion:188 Resp: 567918
Ion Ratio Lower Upper
188 100
94 7.4 7.0 10.4
80 8.4 7.6 11.4

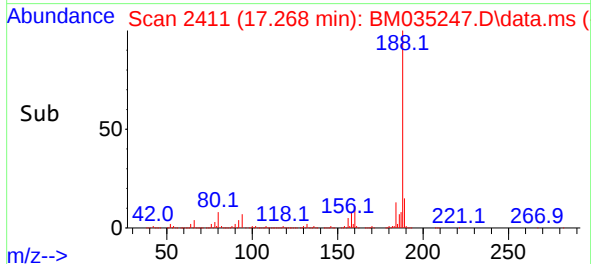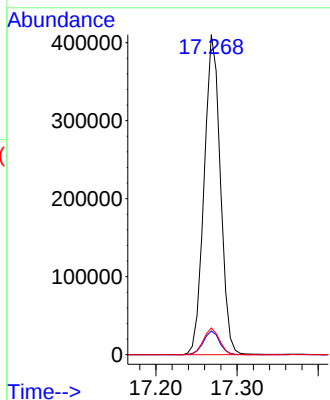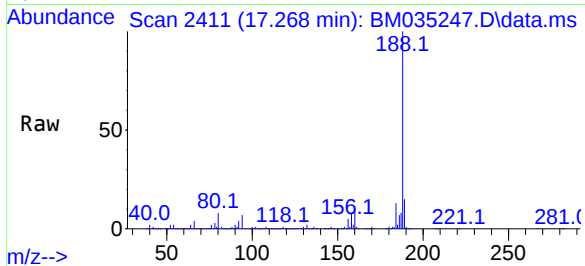

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.450 min Scan# 3122
Delta R.T. -0.006 min
Lab File: BM035247.D
Acq: 25 May 2022 18:33

Tgt Ion:240 Resp: 595849
Ion Ratio Lower Upper
240 100
120 9.1 9.4 14.0#
236 26.2 20.6 30.8


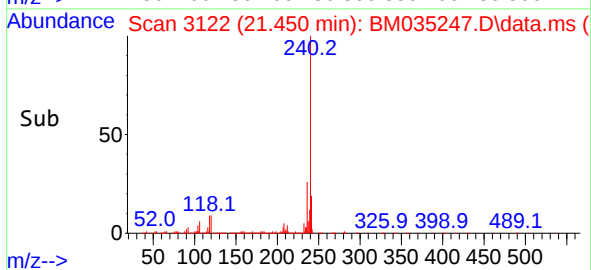
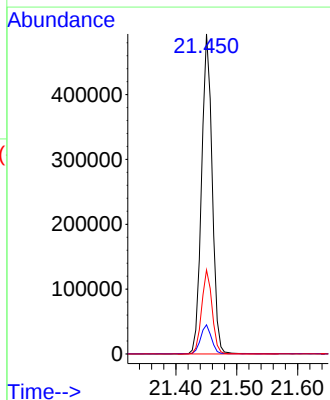
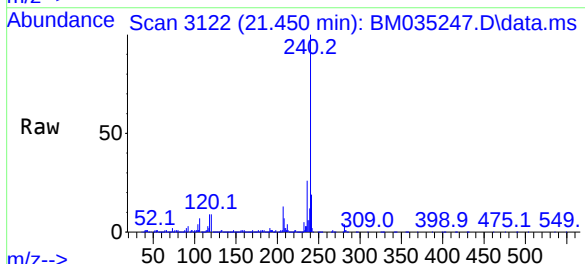




#79
 Terphenyl-d14
 Concen: 73.213 ng
 RT: 19.898 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: BM035247.D
 Acq: 25 May 2022 18:33

Instrument :
 BNA_M
 ClientSampleId :
 P024-SS001-2430-01

Tgt Ion:244 Resp: 2253069
 Ion Ratio Lower Upper
 244 100
 212 7.2 6.2 9.4
 122 8.4 8.3 12.5

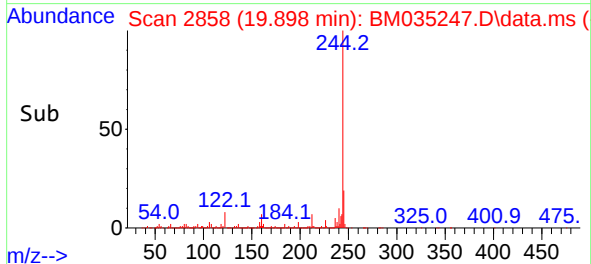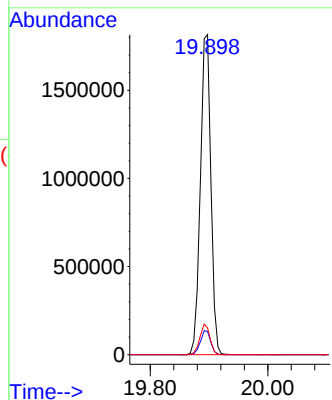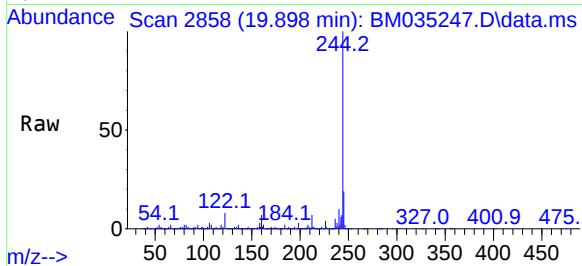

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 23.827 min Scan# 3526
 Delta R.T. -0.006 min
 Lab File: BM035247.D
 Acq: 25 May 2022 18:33

Tgt Ion:264 Resp: 633163
 Ion Ratio Lower Upper
 264 100
 260 23.4 18.9 28.3
 265 22.2 17.5 26.3

