

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM052522\  
 Data File : BM035236.D  
 Acq On : 25 May 2022 10:42  
 Operator : CG/JU  
 Sample : PB145067BL  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 PB145067BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM042722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM035236.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.469       | 398           | 405         | 426          | rBV      | 2971193        | 4367441       | 39.02%          | 9.253%        |
| 2         | 7.069       | 668           | 677         | 695          | rBV      | 2795507        | 4619166       | 41.27%          | 9.786%        |
| 3         | 7.887       | 810           | 816         | 828          | rBV      | 565968         | 910937        | 8.14%           | 1.930%        |
| 4         | 9.051       | 1005          | 1014        | 1030         | rBV      | 1853113        | 3037495       | 27.14%          | 6.435%        |
| 5         | 10.692      | 1285          | 1293        | 1306         | rBV      | 754726         | 1302118       | 11.63%          | 2.759%        |
| 6         | 13.157      | 1703          | 1712        | 1726         | rBV      | 5399436        | 7700023       | 68.79%          | 16.313%       |
| 7         | 14.527      | 1938          | 1945        | 1957         | rBV      | 1285597        | 1867701       | 16.69%          | 3.957%        |
| 8         | 16.015      | 2191          | 2198        | 2221         | rBV      | 4185104        | 5876050       | 52.50%          | 12.449%       |
| 9         | 17.268      | 2405          | 2411        | 2424         | rBV      | 1475625        | 2206647       | 19.71%          | 4.675%        |
| 10        | 18.174      | 2560          | 2565        | 2575         | rBV      | 81589          | 147433        | 1.32%           | 0.312%        |
| 11        | 19.898      | 2852          | 2858        | 2863         | rBV      | 8682442        | 11193079      | 100.00%         | 23.713%       |
| 12        | 21.456      | 3118          | 3123        | 3128         | rBV      | 1688137        | 2121863       | 18.96%          | 4.495%        |
| 13        | 23.833      | 3521          | 3527        | 3536         | rVB2     | 904655         | 1852456       | 16.55%          | 3.924%        |




Sum of corrected areas: 47202409

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM052522\  
Data File : BM035236.D  
Acq On : 25 May 2022 10:42  
Operator : CG/JU  
Sample : PB145067BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
PB145067BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM042722.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

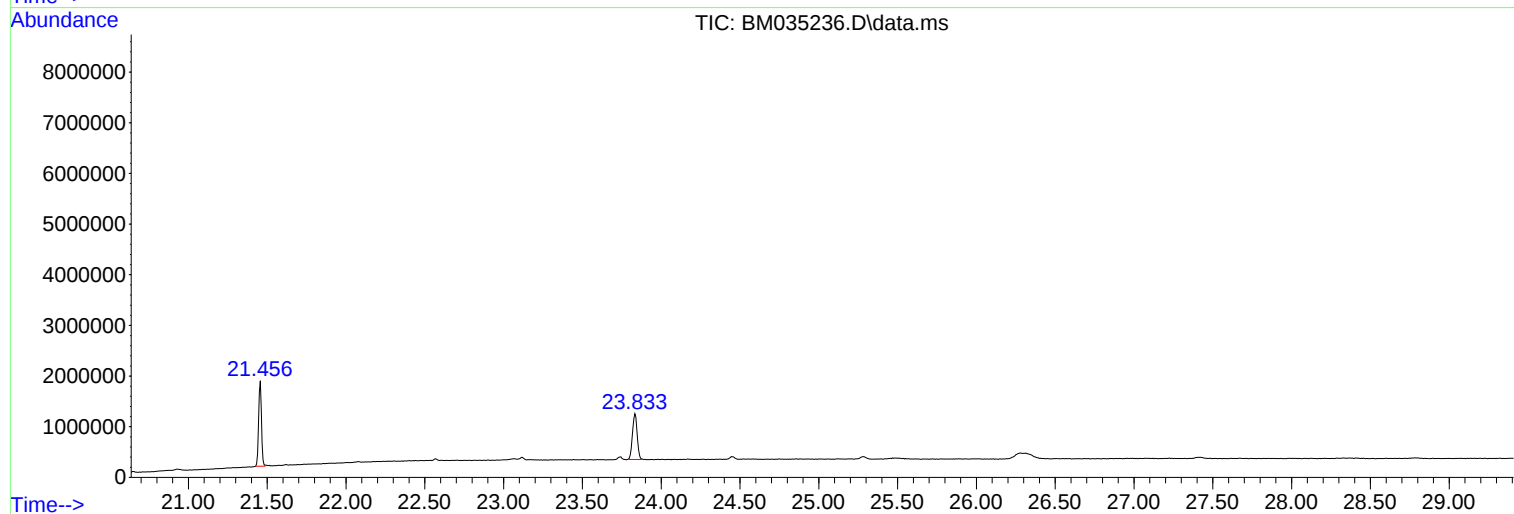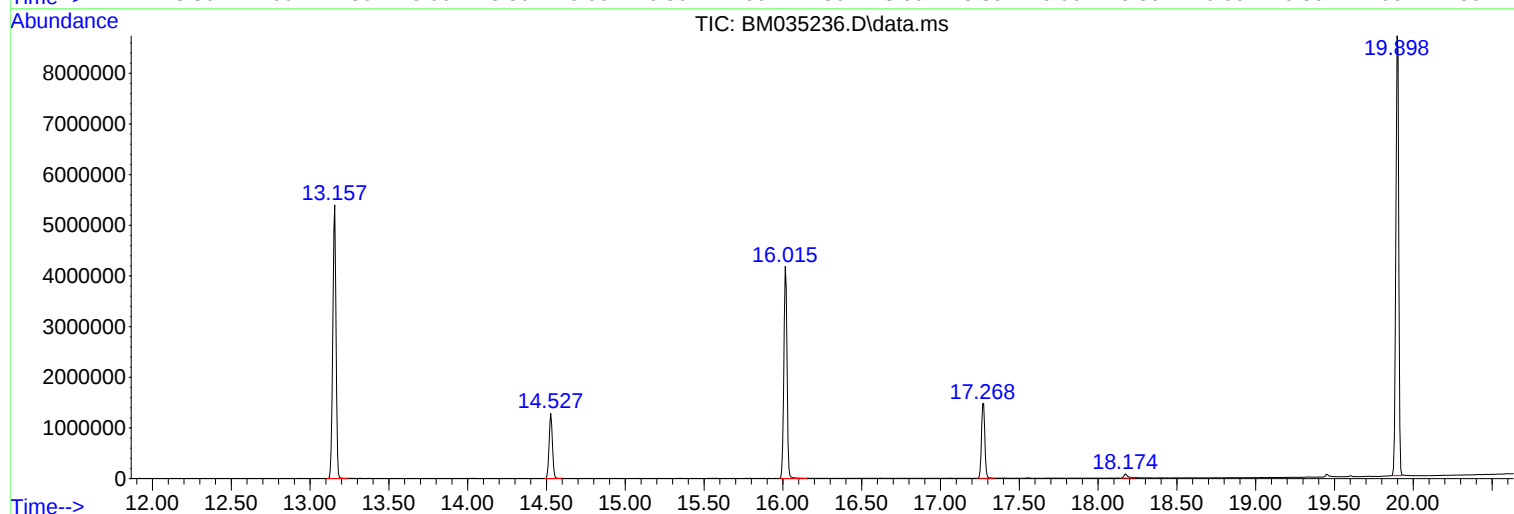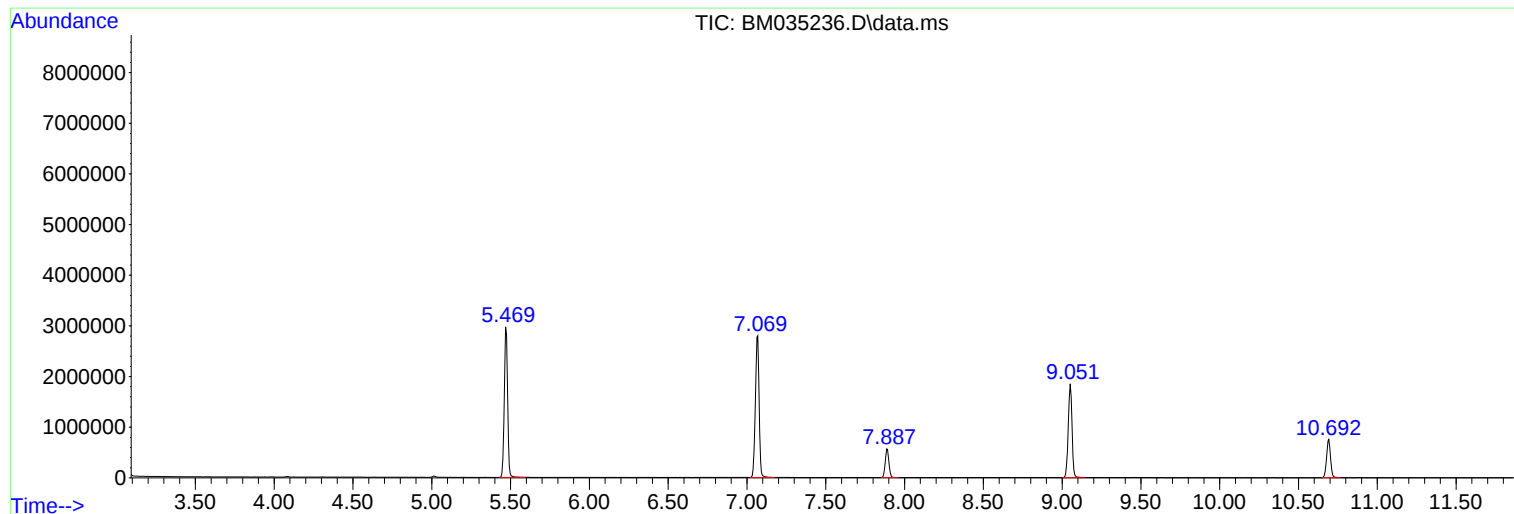

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM052522\  
Data File : BM035236.D  
Acq On : 25 May 2022 10:42  
Operator : CG/JU  
Sample : PB145067BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
PB145067BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM042722.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM052522\  
Data File : BM035236.D  
Acq On : 25 May 2022 10:42  
Operator : CG/JU  
Sample : PB145067BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
PB145067BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM042722.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|