


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052522\
 Data File : BM035234.D
 Acq On : 25 May 2022 09:30
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 26 05:05:10 2022

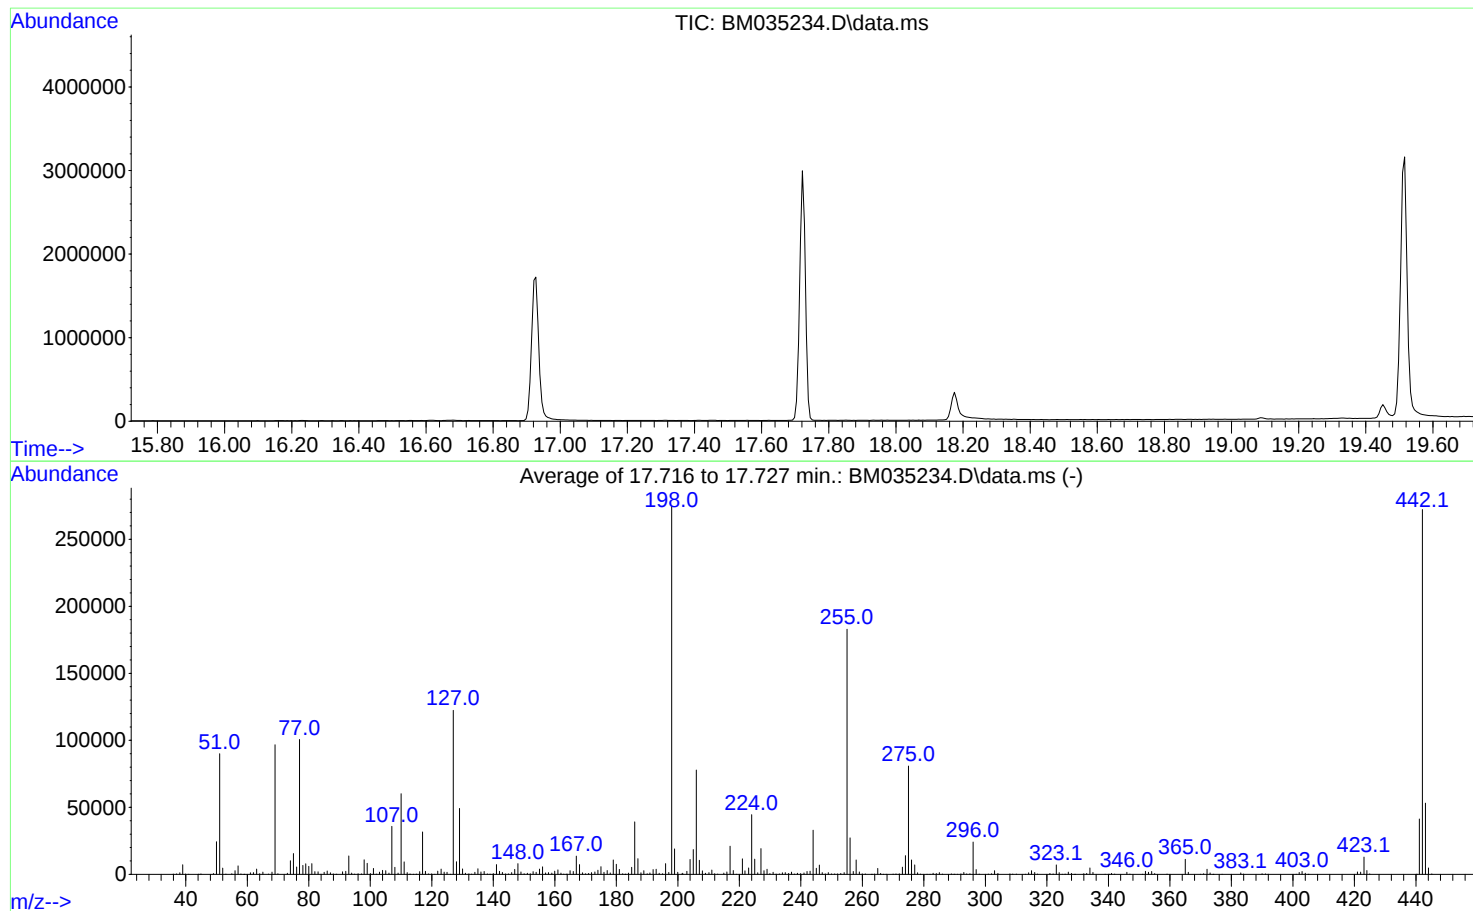




AutoFind: Scans 2487, 2488, 2489; Background Corrected with Scan 2480

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.8	89981	PASS
68	69	0.00	2	1.8	1741	PASS
69	198	0.00	100	35.2	96720	PASS
70	69	0.00	2	0.5	499	PASS
127	198	10	80	44.6	122387	PASS
197	198	0.00	2	0.5	1464	PASS
198	198	100	100	100.0	274453	PASS
199	198	5	9	6.9	19011	PASS
275	198	10	60	29.4	80816	PASS
365	198	1	100	4.1	11283	PASS
441	198	0.01	100	15.0	41280	PASS
442	442	50	100	100.0	272213	PASS
443	442	15	24	19.5	53171	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052522\
Data File : BM035234.D
Acq On : 25 May 2022 09:30
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: May 26 08:29:14 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 26 05:05:10 2022
Response via : Initial Calibration

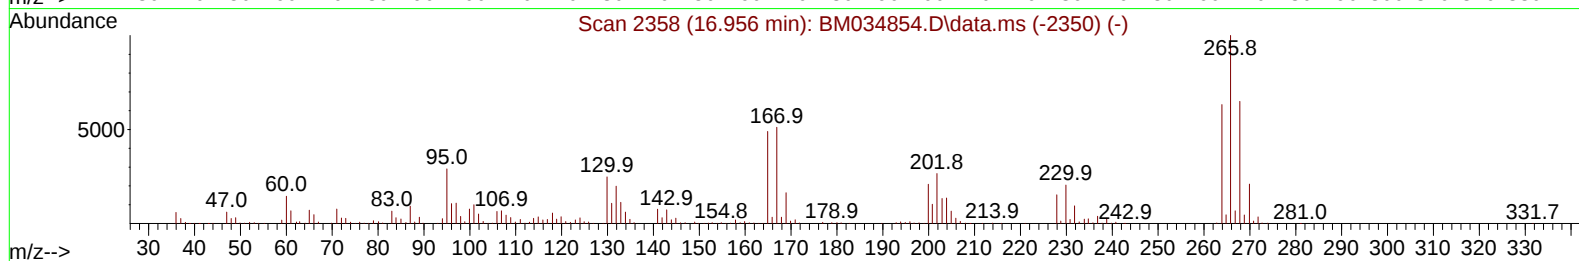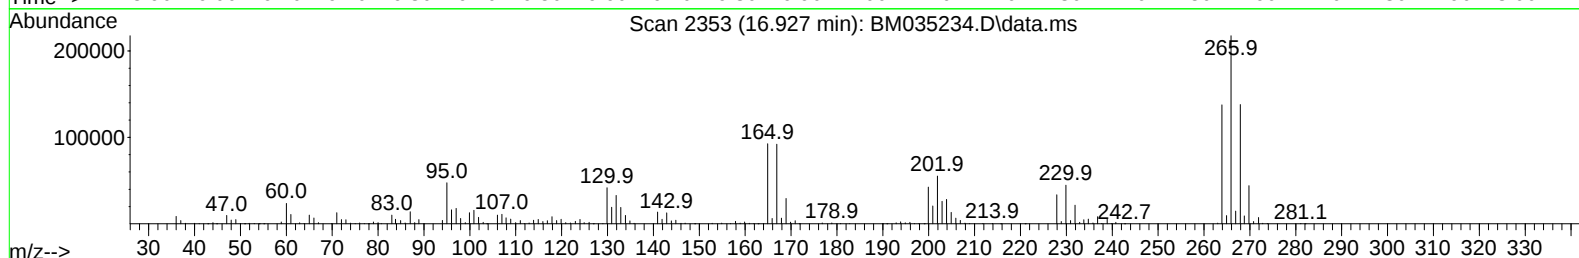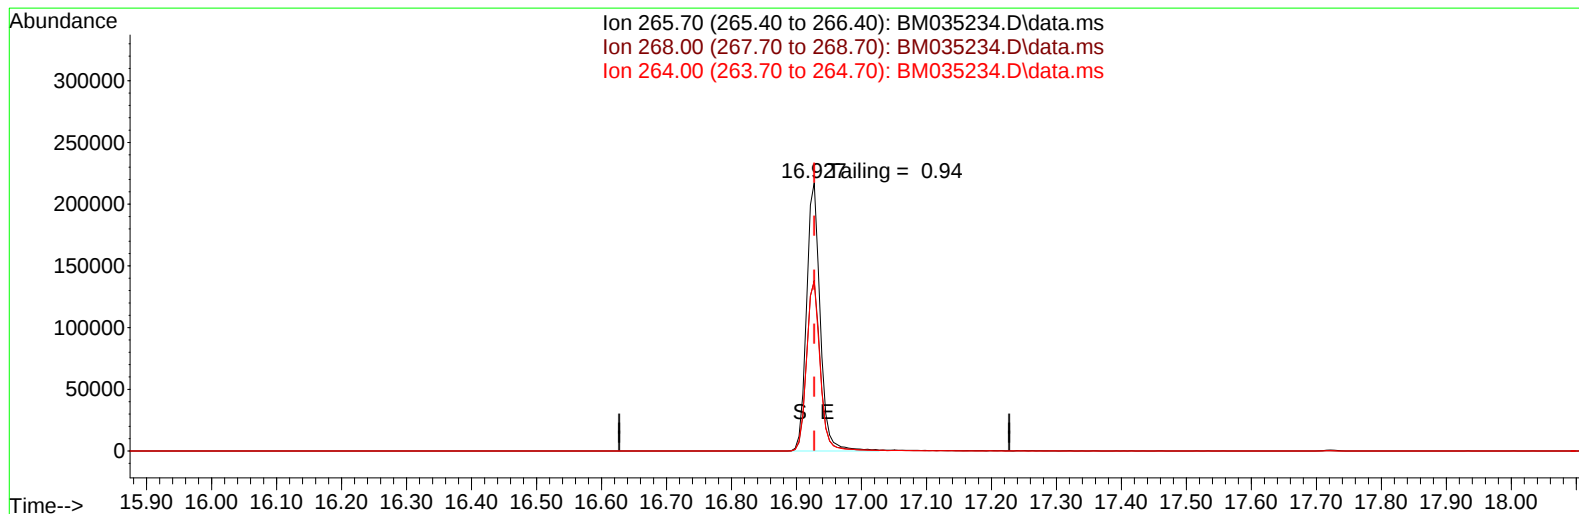

TIC: BM035234.D\data.ms

(70) Pentachlorophenol (C)

16.927min (+ 0.000) 796858.59 ng




response 320873

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	63.42
264.00	63.30	63.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052522\
Data File : BM035234.D
Acq On : 25 May 2022 09:30
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: May 26 08:29:14 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 26 05:05:10 2022
Response via : Initial Calibration

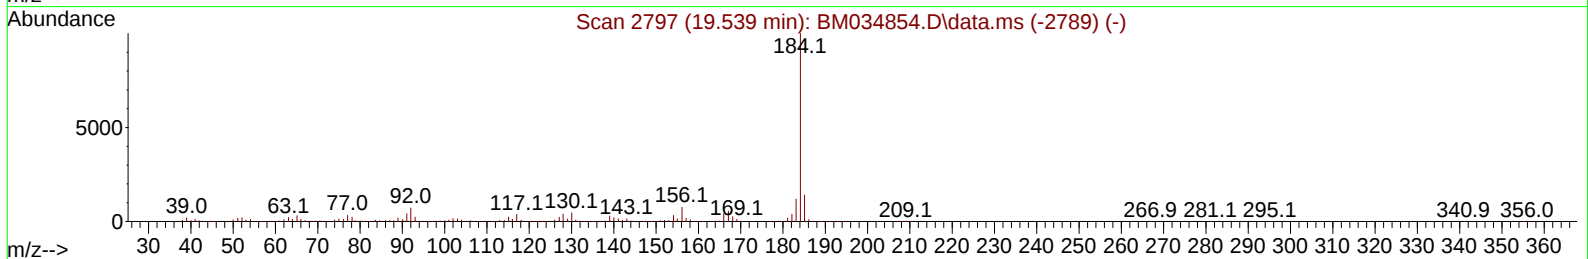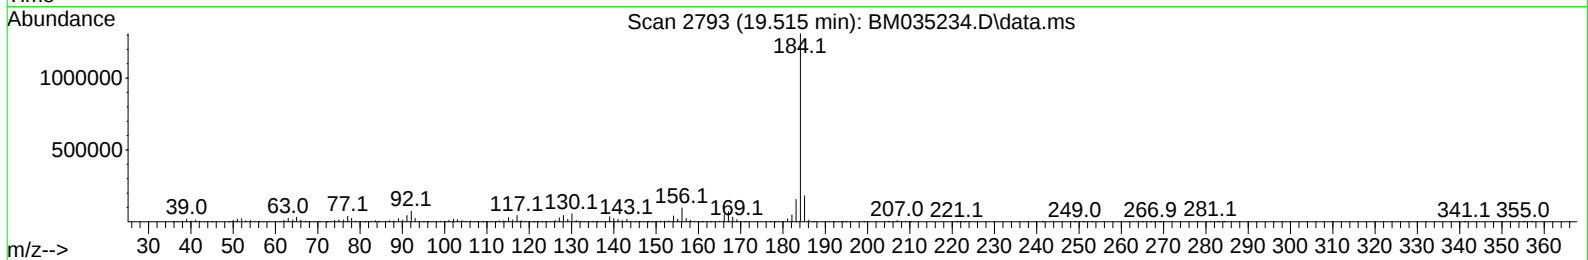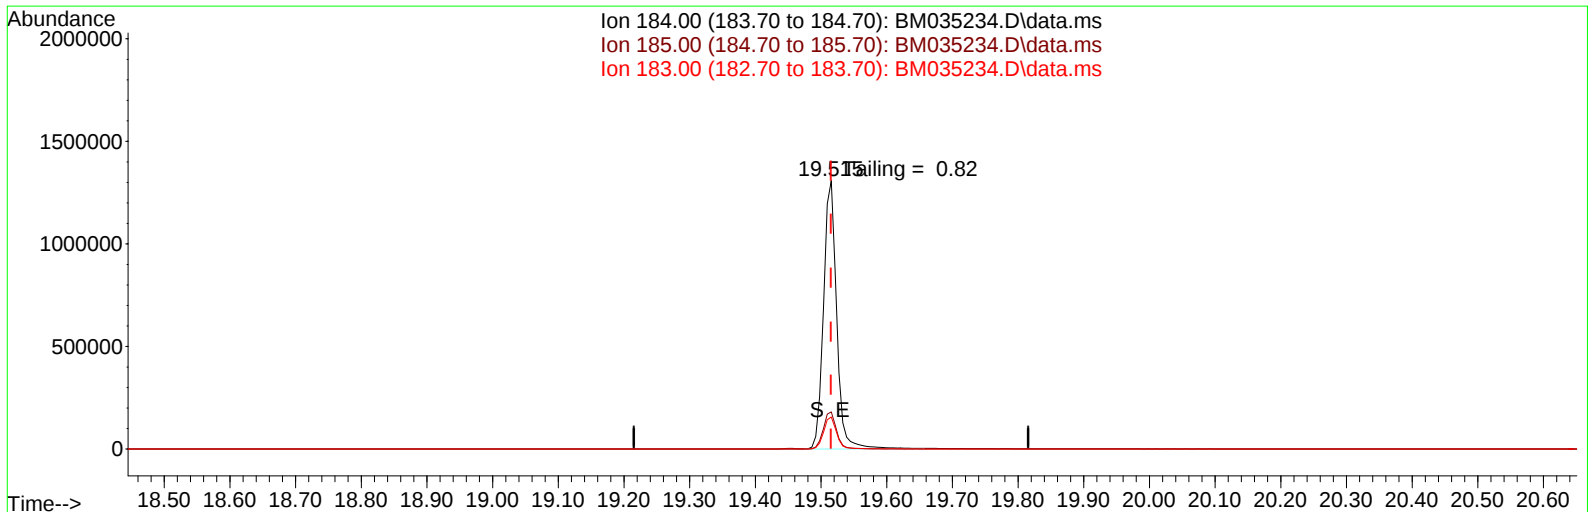

TIC: BM035234.D\data.ms

(77) Benzidine

19.515min (+ 0.000) 127779.95 ng

response 1815171

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	13.84
183.00	11.90	11.91
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/25/2022	BNA_M	<u>BM035234.D</u>
Compound Name	Response	Retention Time
DDT	1030883	20.751
DDD	17336	20.309
DDE	1733	19.804
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19069	1049952	1.82

Instrument :
BNA_M
ClientSampleId :
DFTPP