


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052522\
 Data File : BM035243.D
 Acq On : 25 May 2022 16:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu May 26 05:05:10 2022

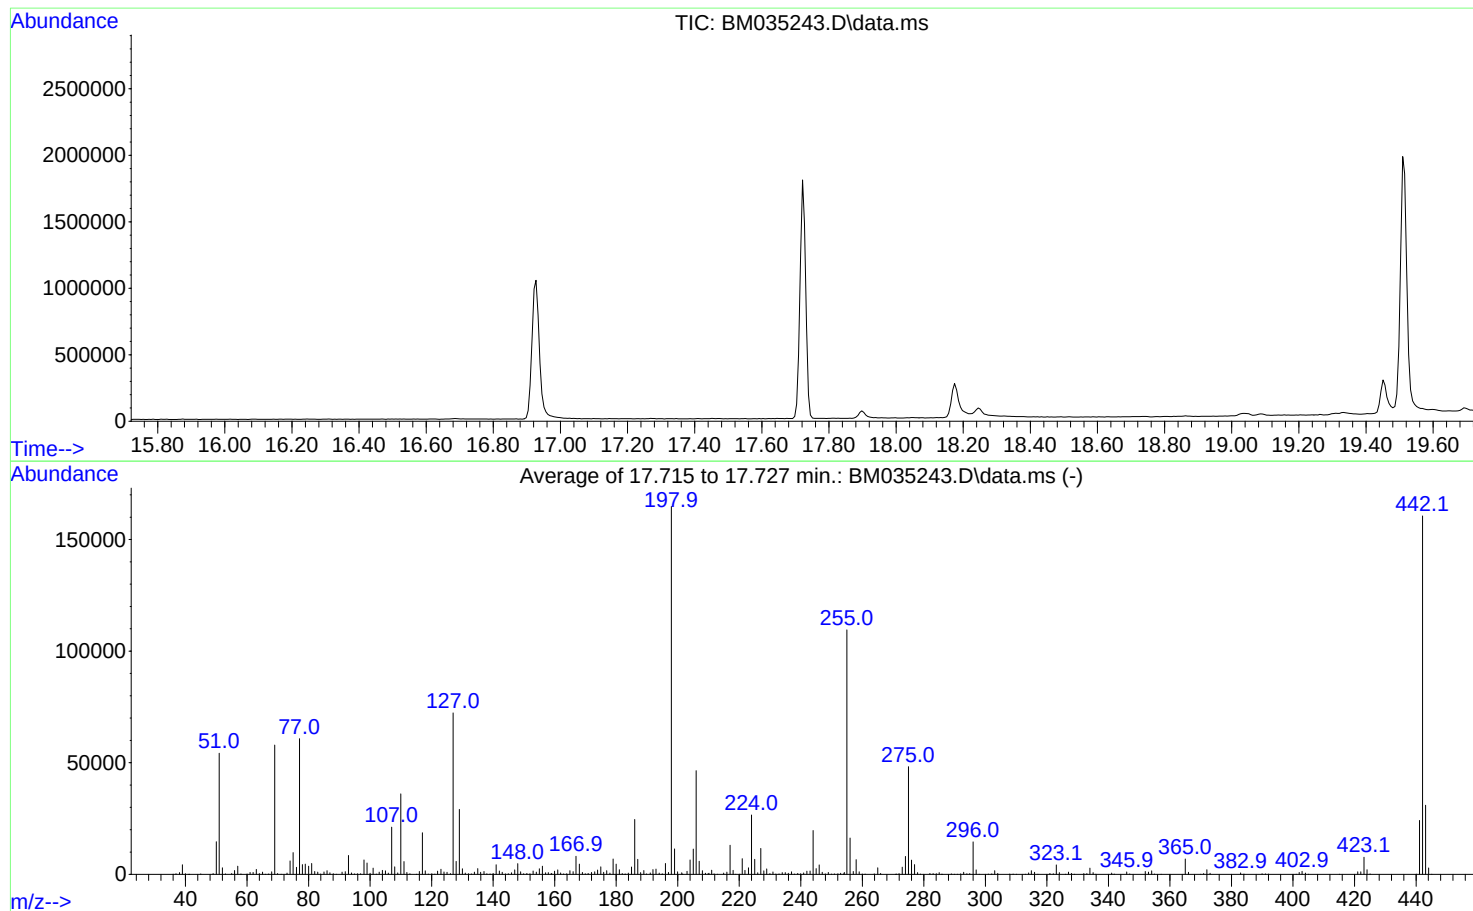




AutoFind: Scans 2487, 2488, 2489; Background Corrected with Scan 2480

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.9	54278	PASS
68	69	0.00	2	1.9	1130	PASS
69	198	0.00	100	35.2	57949	PASS
70	69	0.00	2	0.6	354	PASS
127	198	10	80	43.9	72339	PASS
197	198	0.00	2	0.5	858	PASS
198	198	100	100	100.0	164779	PASS
199	198	5	9	6.9	11386	PASS
275	198	10	60	29.3	48251	PASS
365	198	1	100	4.2	6868	PASS
441	198	0.01	100	14.7	24191	PASS
442	442	50	100	100.0	160571	PASS
443	442	15	24	19.3	30979	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052522\
 Data File : BM035243.D
 Acq On : 25 May 2022 16:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: May 26 08:44:36 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu May 26 05:05:10 2022
 Response via : Initial Calibration

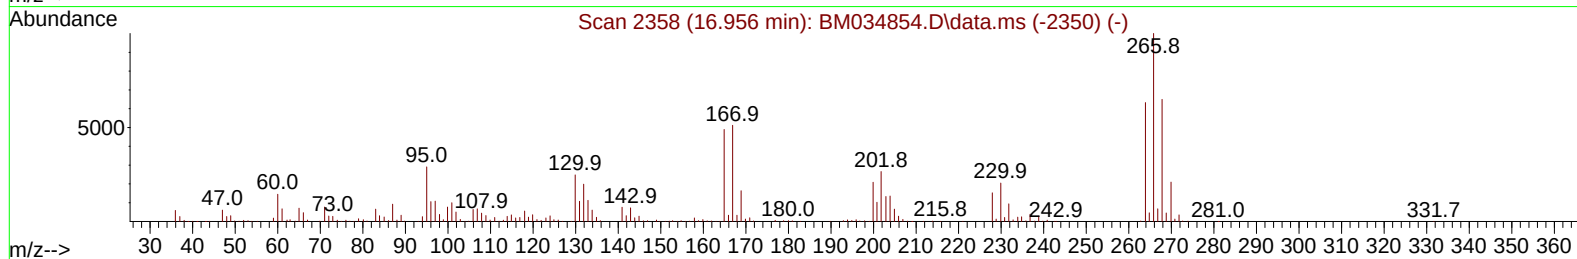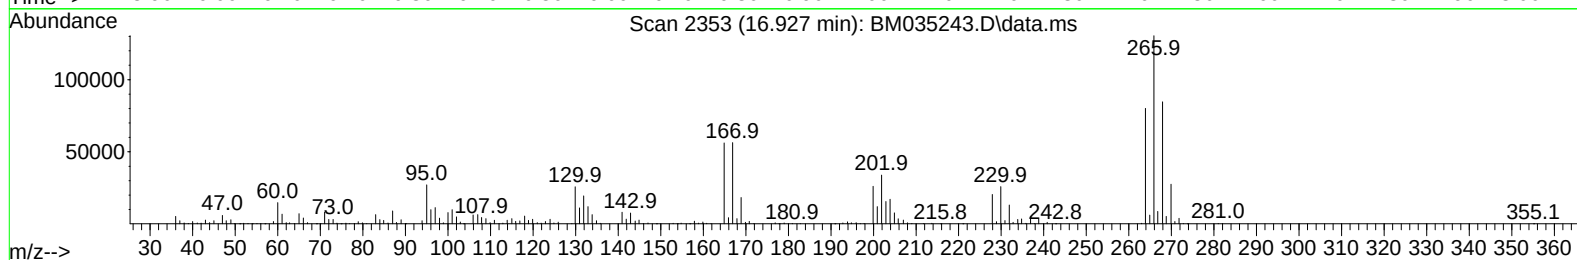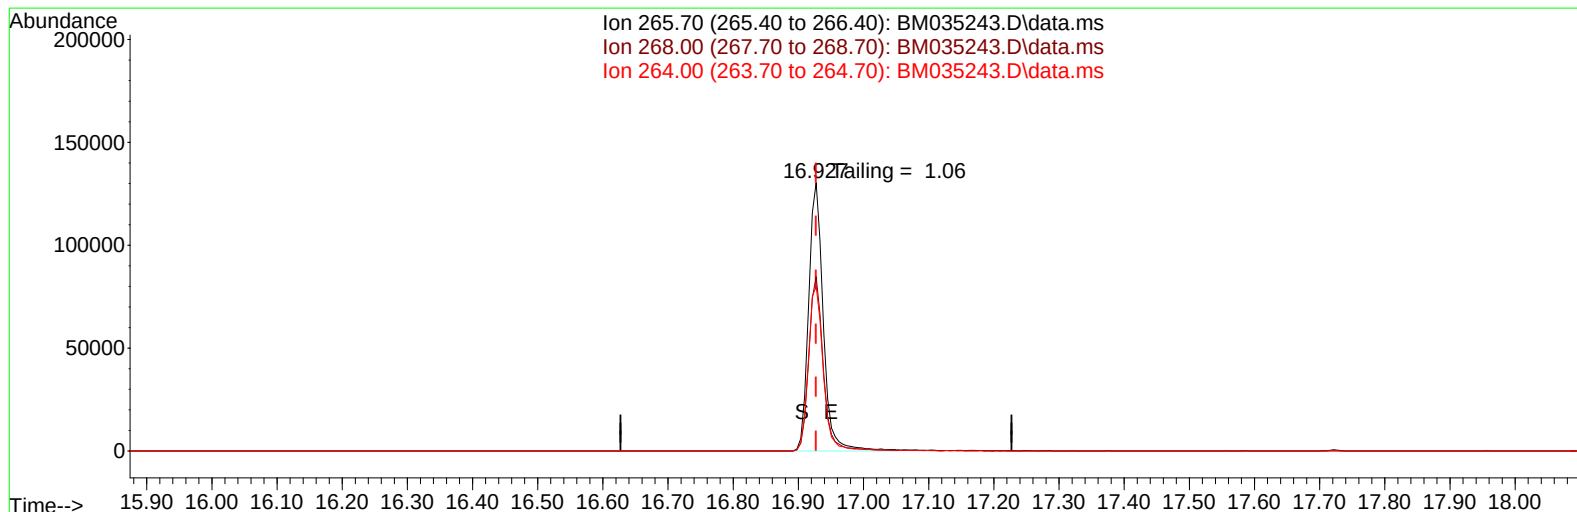

TIC: BM035243.D\data.ms

(70) Pentachlorophenol (C)

16.927min (+ 0.000) 0.00 ng




response 205035

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	64.92
264.00	63.30	61.40
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052522\
Data File : BM035243.D
Acq On : 25 May 2022 16:05
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: May 26 08:44:36 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM042722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu May 26 05:05:10 2022
Response via : Initial Calibration

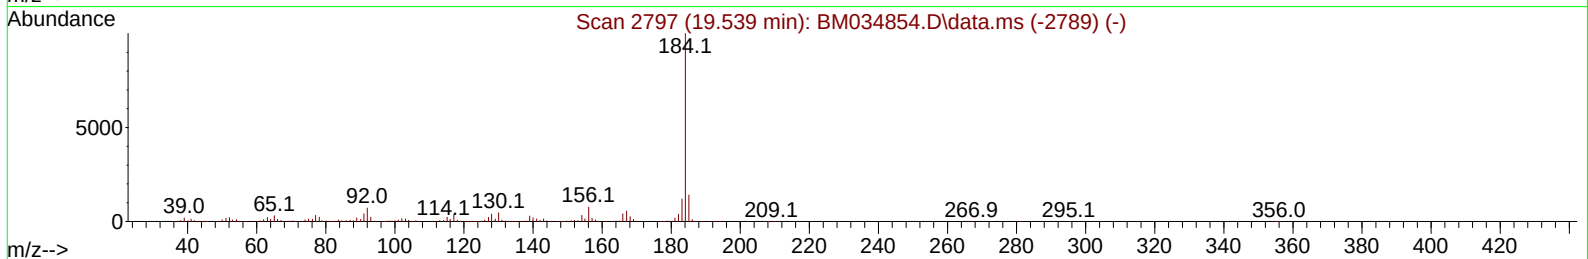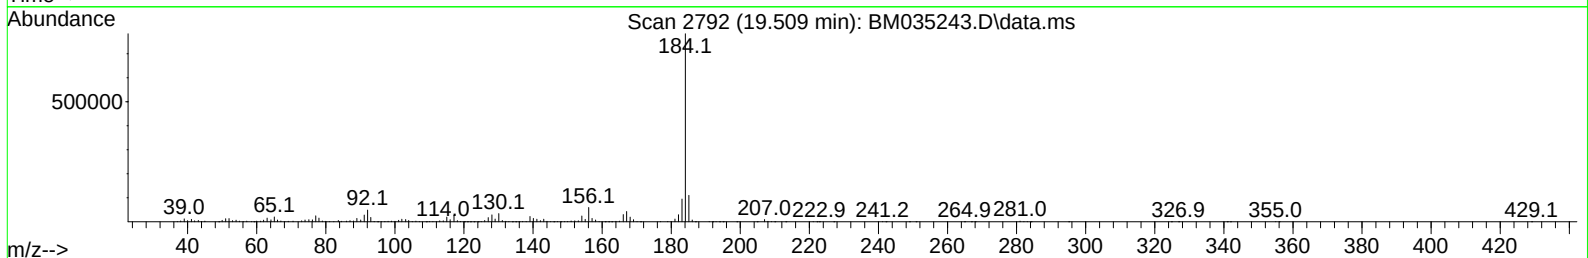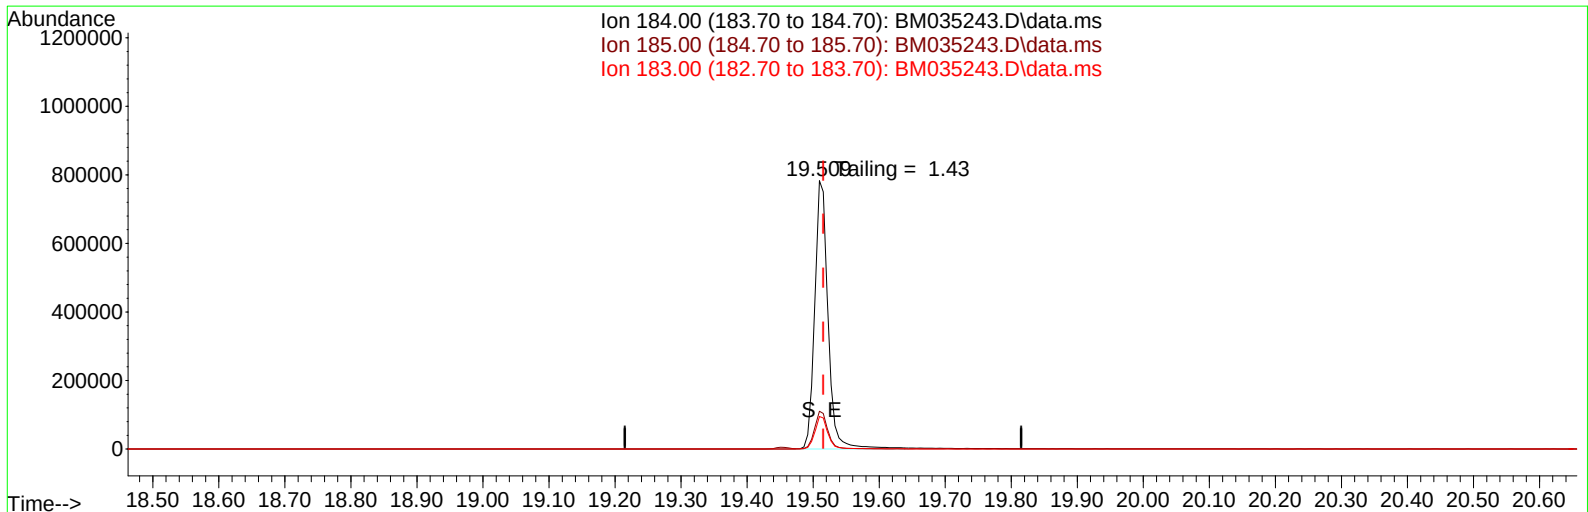

TIC: BM035243.D\data.ms

(77) Benzidine

19.509min (-0.006) 35448.50 ng

response 1102421

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.07
183.00	11.90	12.12
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
5/25/2022	BNA_M	<u>BM035243.D</u>
Compound Name	Response	Retention Time
DDT	625375	20.751
DDD	6313	20.362
DDE	811	19.804
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7124	632499	1.13

Instrument :
BNA_M
ClientSampleId :
DFTPP