

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052721\
 Data File : BM030203.D
 Acq On : 27 May 2021 16:08
 Operator : CG/JU
 Sample : M2474-16
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB449

Quant Time: May 27 16:39:12 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 27 12:44:50 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.875	152	424318	20.00	ng/ul	0.00
20) Naphthalene-d8	10.669	136	1785816	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.498	164	1146742	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.227	188	2207345	20.00	ng/ul	0.00
79) Chrysene-d12	21.386	240	1916086	20.00	ng/ul	0.00
88) Perylene-d12	23.680	264	1910988	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.340	96	19013	1.83	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.00	ng/ul	0.00
7) Phenol-d5	7.028	99	105935	2.84	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.204	67	350577	14.89	ng/ul	0.00
11) 2-Chlorophenol-d4	7.404	132	338000	12.09	ng/ul	0.00
15) 4-Methylphenol-d8	8.563	113	188028	6.35	ng/ul	0.00
21) Nitrobenzene-d5	9.028	128	202386	17.36	ng/ul	0.00
24) 2-Nitrophenol-d4	9.745	143	195737	17.63	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.281	165	410507	14.33	ng/ul	0.00
31) 4-Chloroaniline-d4	10.798	131	9018	0.21	ng/ul	0.00
46) Dimethylphthalate-d6	13.904	166	1371722	15.65	ng/ul	0.00
49) Acenaphthylene-d8	14.186	160	1697846	15.02	ng/ul	0.00
54) 4-Nitrophenol-d4	14.686	143	32999	2.33	ng/ul	0.01
60) Fluorene-d10	15.486	176	1238854	16.19	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.592	200	176324	16.48	ng/ul	0.00
73) Anthracene-d10	17.327	188	1984982	18.17	ng/ul	0.00
81) Pyrene-d10	19.610	212	2113052	20.57	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.533	264	1971796	18.20	ng/ul	0.00
Target Compounds						
47) Dimethylphthalate	13.945	163	173109	2.00	ng/ul	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052721\
Data File : BM030203.D
Acq On : 27 May 2021 16:08
Operator : CG/JU
Sample : M2474-16
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB449

Quant Time: May 27 16:39:12 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 27 12:44:50 2021
Response via : Initial Calibration

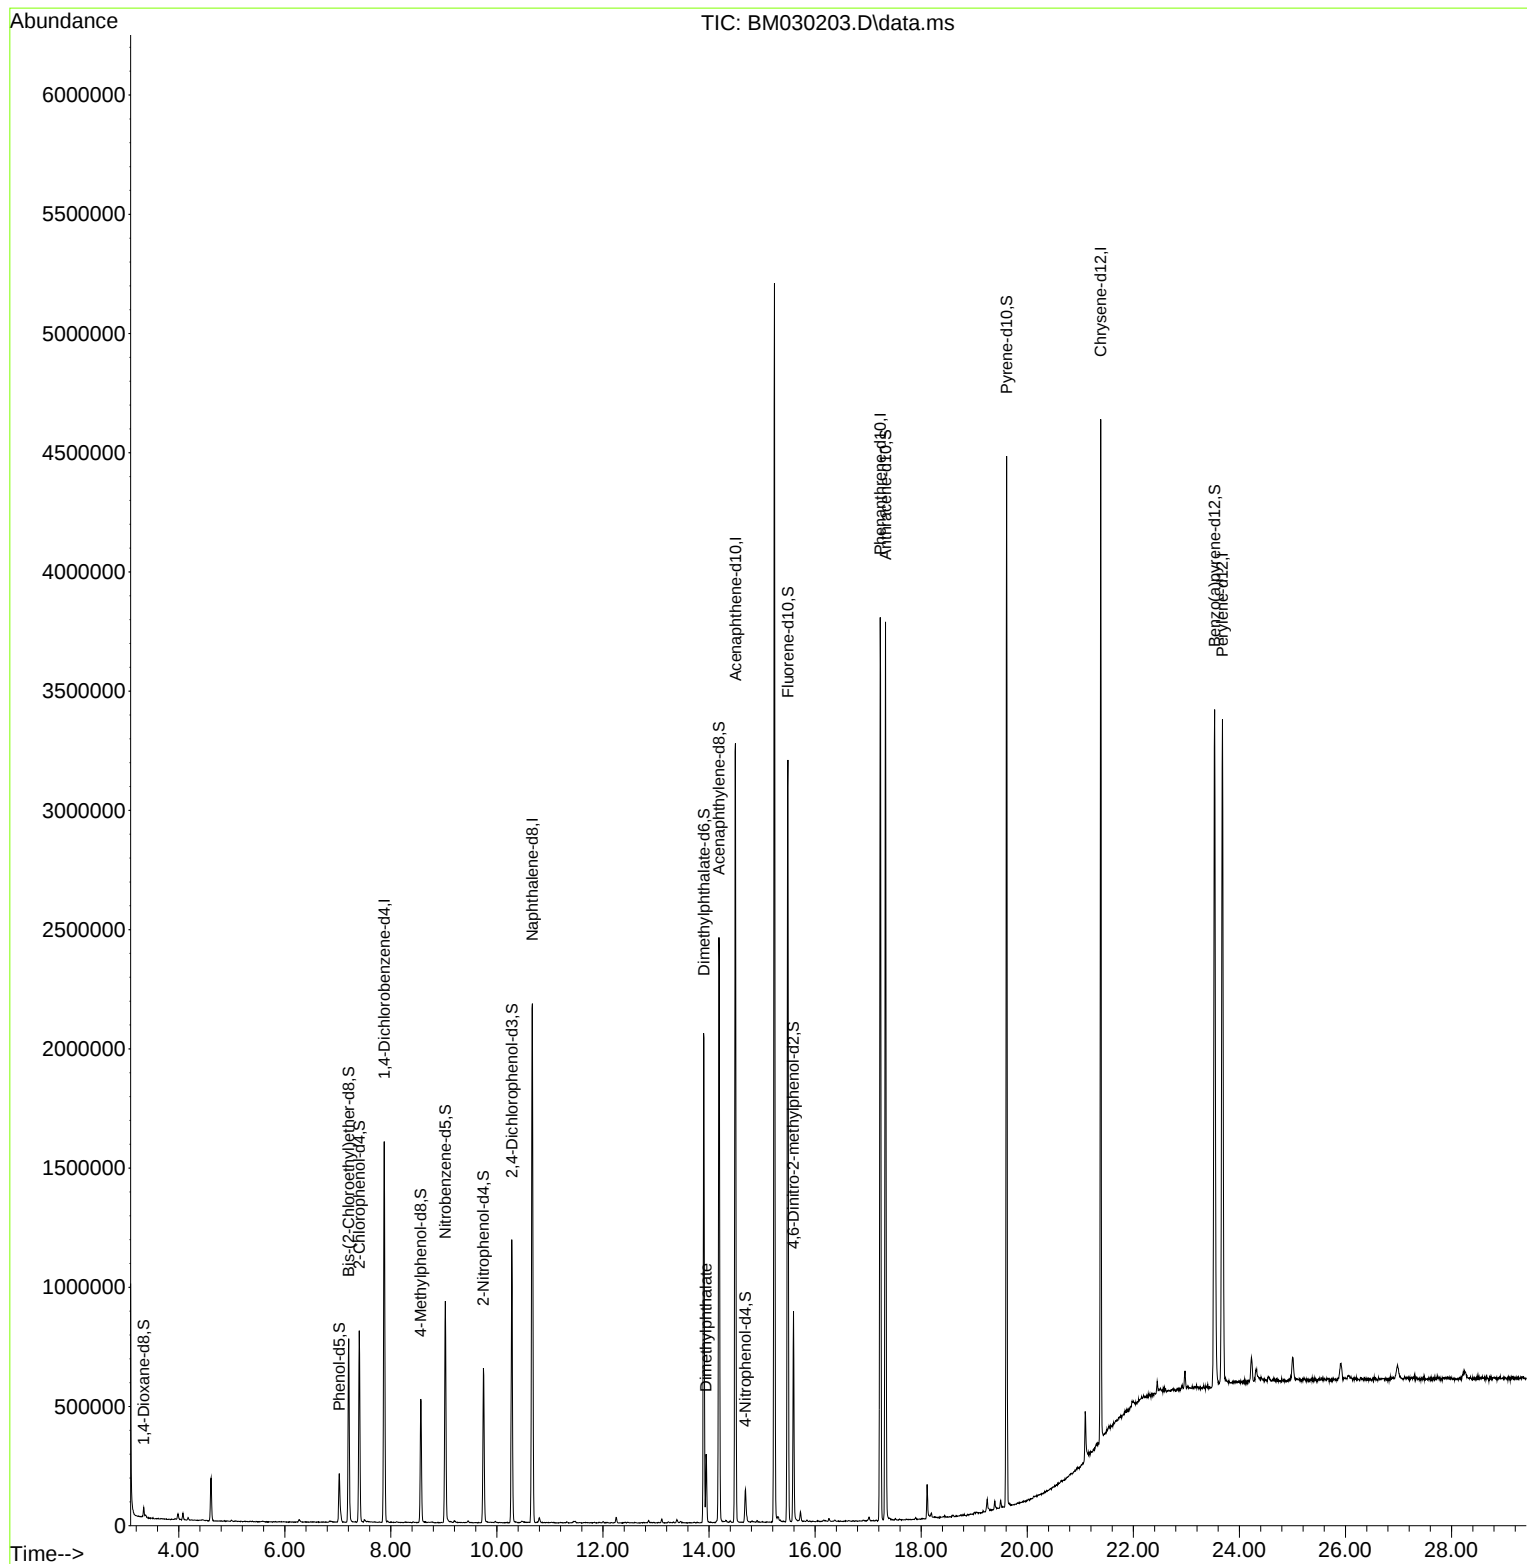

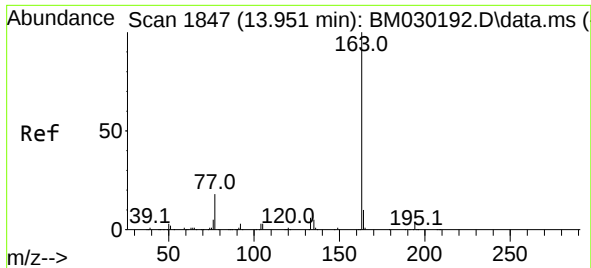

#47
 Dimethylphthalate
 Concen: 2.00 ng/ul
 RT: 13.945 min Scan# 1846
 Delta R.T. -0.006 min
 Lab File: BM030203.D
 Acq: 27 May 2021 16:08

Instrument :
 BNA_M
 ClientSampleId :
 GB449

Tgt Ion:163 Resp: 173109
 Ion Ratio Lower Upper
 163 100
 194 3.7 3.4 5.0
 164 10.2 8.2 12.2

