

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052721\
 Data File : BM030204.D
 Acq On : 27 May 2021 16:45
 Operator : CG/JU
 Sample : M2474-18
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB451

Quant Time: May 27 17:19:38 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 27 12:44:50 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.875	152	166841	20.00	ng/ul	0.00
20) Naphthalene-d8	10.669	136	726673	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.498	164	491890	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.227	188	1047366	20.00	ng/ul	0.00
79) Chrysene-d12	21.386	240	920780	20.00	ng/ul	0.00
88) Perylene-d12	23.680	264	800282	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.340	96	19272	4.73	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.00	ng/ul	0.00
7) Phenol-d5	7.028	99	123084	8.39	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.204	67	382982	41.36	ng/ul	0.00
11) 2-Chlorophenol-d4	7.404	132	371131	33.77	ng/ul	0.00
15) 4-Methylphenol-d8	8.563	113	239888	20.59	ng/ul	0.00
21) Nitrobenzene-d5	9.028	128	224622	47.36	ng/ul	0.00
24) 2-Nitrophenol-d4	9.745	143	221179	48.96	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.280	165	448590	38.49	ng/ul	0.00
31) 4-Chloroaniline-d4	10.798	131	19595	1.13	ng/ul	0.00
46) Dimethylphthalate-d6	13.904	166	1725125	45.87	ng/ul	0.00
49) Acenaphthylene-d8	14.186	160	2074241	42.79	ng/ul	0.00
54) 4-Nitrophenol-d4	14.668	143	45696	7.52	ng/ul	0.00
60) Fluorene-d10	15.486	176	1570462	47.84	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.592	200	237387	46.75	ng/ul	0.00
73) Anthracene-d10	17.327	188	2648677	51.10	ng/ul	0.00
81) Pyrene-d10	19.609	212	2922092	59.20	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.533	264	2343392	51.66	ng/ul	0.00
Target Compounds						
					Qvalue	
8) Phenol	7.051	94	18347	1.23	ng/ul	100
47) Dimethylphthalate	13.945	163	177157	4.77	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052721\
Data File : BM030204.D
Acq On : 27 May 2021 16:45
Operator : CG/JU
Sample : M2474-18
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB451

Quant Time: May 27 17:19:38 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 27 12:44:50 2021
Response via : Initial Calibration




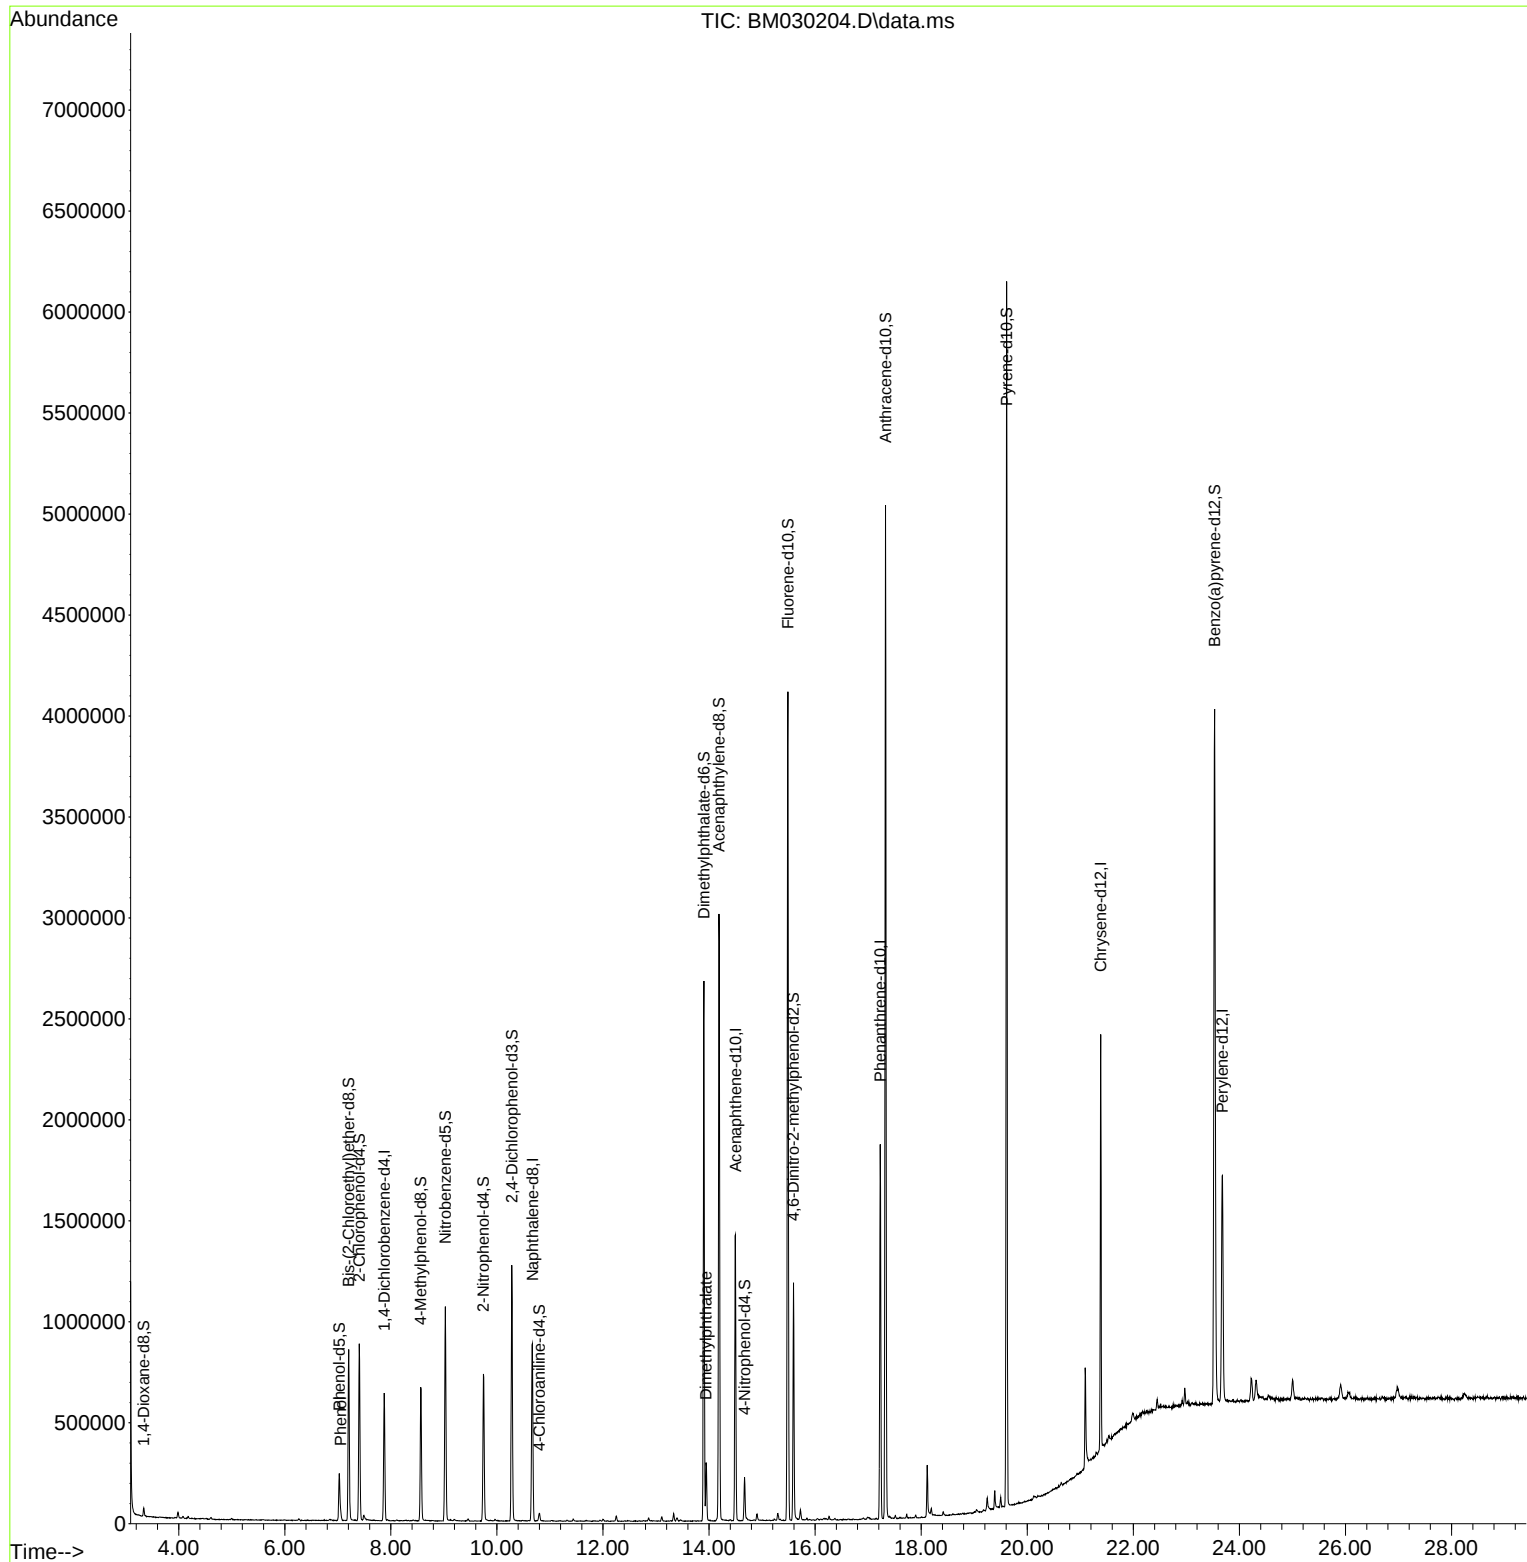


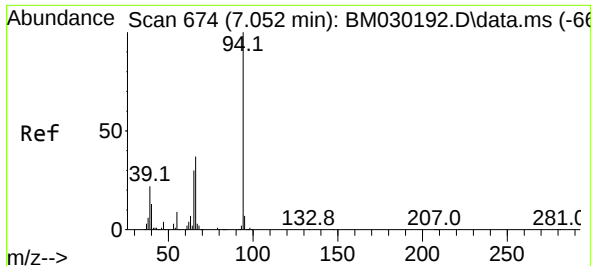

#8
Phenol
Concen: 1.23 ng/ul
RT: 7.051 min Scan# 674
Delta R.T. -0.000 min
Lab File: BM030204.D
Acq: 27 May 2021 16:45

Instrument :
BNA_M
ClientSampleId :
GB451

Tgt Ion:	94	Resp:	18347
Ion	Ratio	Lower	Upper
94	100		
65	28.8	23.3	34.9
66	37.3	29.8	44.6

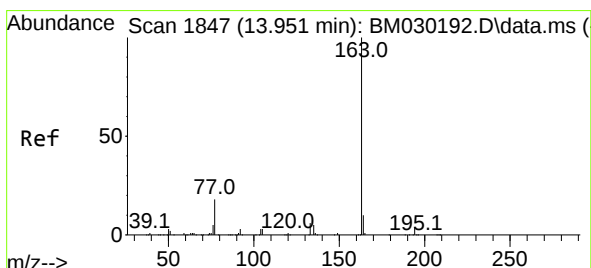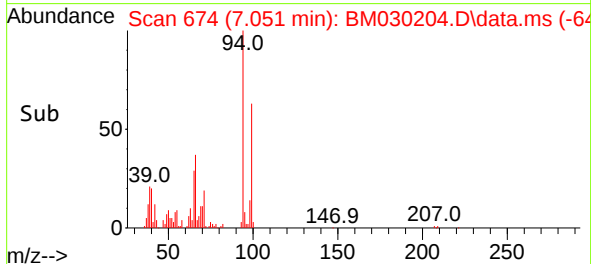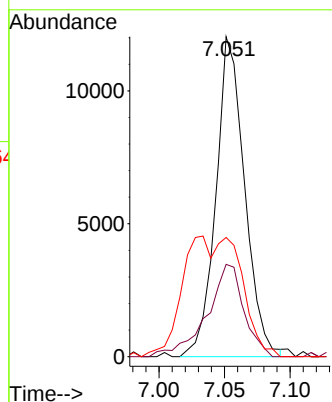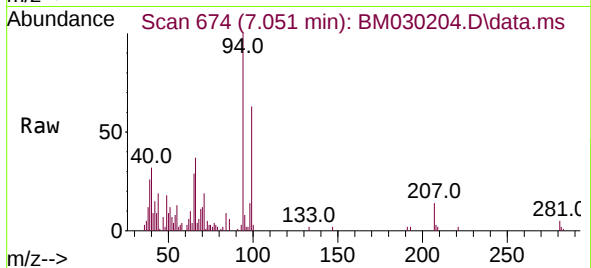

#47
Dimethylphthalate
Concen: 4.77 ng/ul
RT: 13.945 min Scan# 1846
Delta R.T. -0.006 min
Lab File: BM030204.D
Acq: 27 May 2021 16:45

Tgt Ion:	163	Resp:	177157
Ion	Ratio	Lower	Upper
163	100		
194	3.8	3.4	5.0
164	10.0	8.2	12.2

