

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052721\
 Data File : BM030205.D
 Acq On : 27 May 2021 17:22
 Operator : CG/JU
 Sample : M2474-17
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB450

Quant Time: May 27 17:52:42 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 27 12:44:50 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.875	152	220843	20.00	ng/ul	0.00
20) Naphthalene-d8	10.663	136	940624	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.492	164	636376	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.227	188	1288871	20.00	ng/ul	0.00
79) Chrysene-d12	21.386	240	1110673	20.00	ng/ul	0.00
88) Perylene-d12	23.674	264	1080029	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.340	96	17327	3.21	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.00	ng/ul	0.00
7) Phenol-d5	7.028	99	105403	5.43	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.204	67	337440	27.53	ng/ul	0.00
11) 2-Chlorophenol-d4	7.404	132	328766	22.60	ng/ul	0.00
15) 4-Methylphenol-d8	8.563	113	206772	13.41	ng/ul	0.00
21) Nitrobenzene-d5	9.028	128	197158	32.11	ng/ul	0.00
24) 2-Nitrophenol-d4	9.745	143	190400	32.56	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.280	165	388844	25.77	ng/ul	0.00
31) 4-Chloroaniline-d4	10.798	131	17771	0.79	ng/ul	0.00
46) Dimethylphthalate-d6	13.904	166	1458068	29.97	ng/ul	0.00
49) Acenaphthylene-d8	14.186	160	1767942	28.19	ng/ul	0.00
54) 4-Nitrophenol-d4	14.668	143	34405	4.38	ng/ul	0.00
60) Fluorene-d10	15.480	176	1295075	30.50	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.592	200	195360	31.27	ng/ul	0.00
73) Anthracene-d10	17.327	188	2224257	34.87	ng/ul	0.00
81) Pyrene-d10	19.609	212	2364070	39.71	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.533	264	2125313	34.71	ng/ul	0.00
Target Compounds						
47) Dimethylphthalate	13.945	163	128385	2.67	ng/ul	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052721\
Data File : BM030205.D
Acq On : 27 May 2021 17:22
Operator : CG/JU
Sample : M2474-17
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB450

Quant Time: May 27 17:52:42 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 27 12:44:50 2021
Response via : Initial Calibration

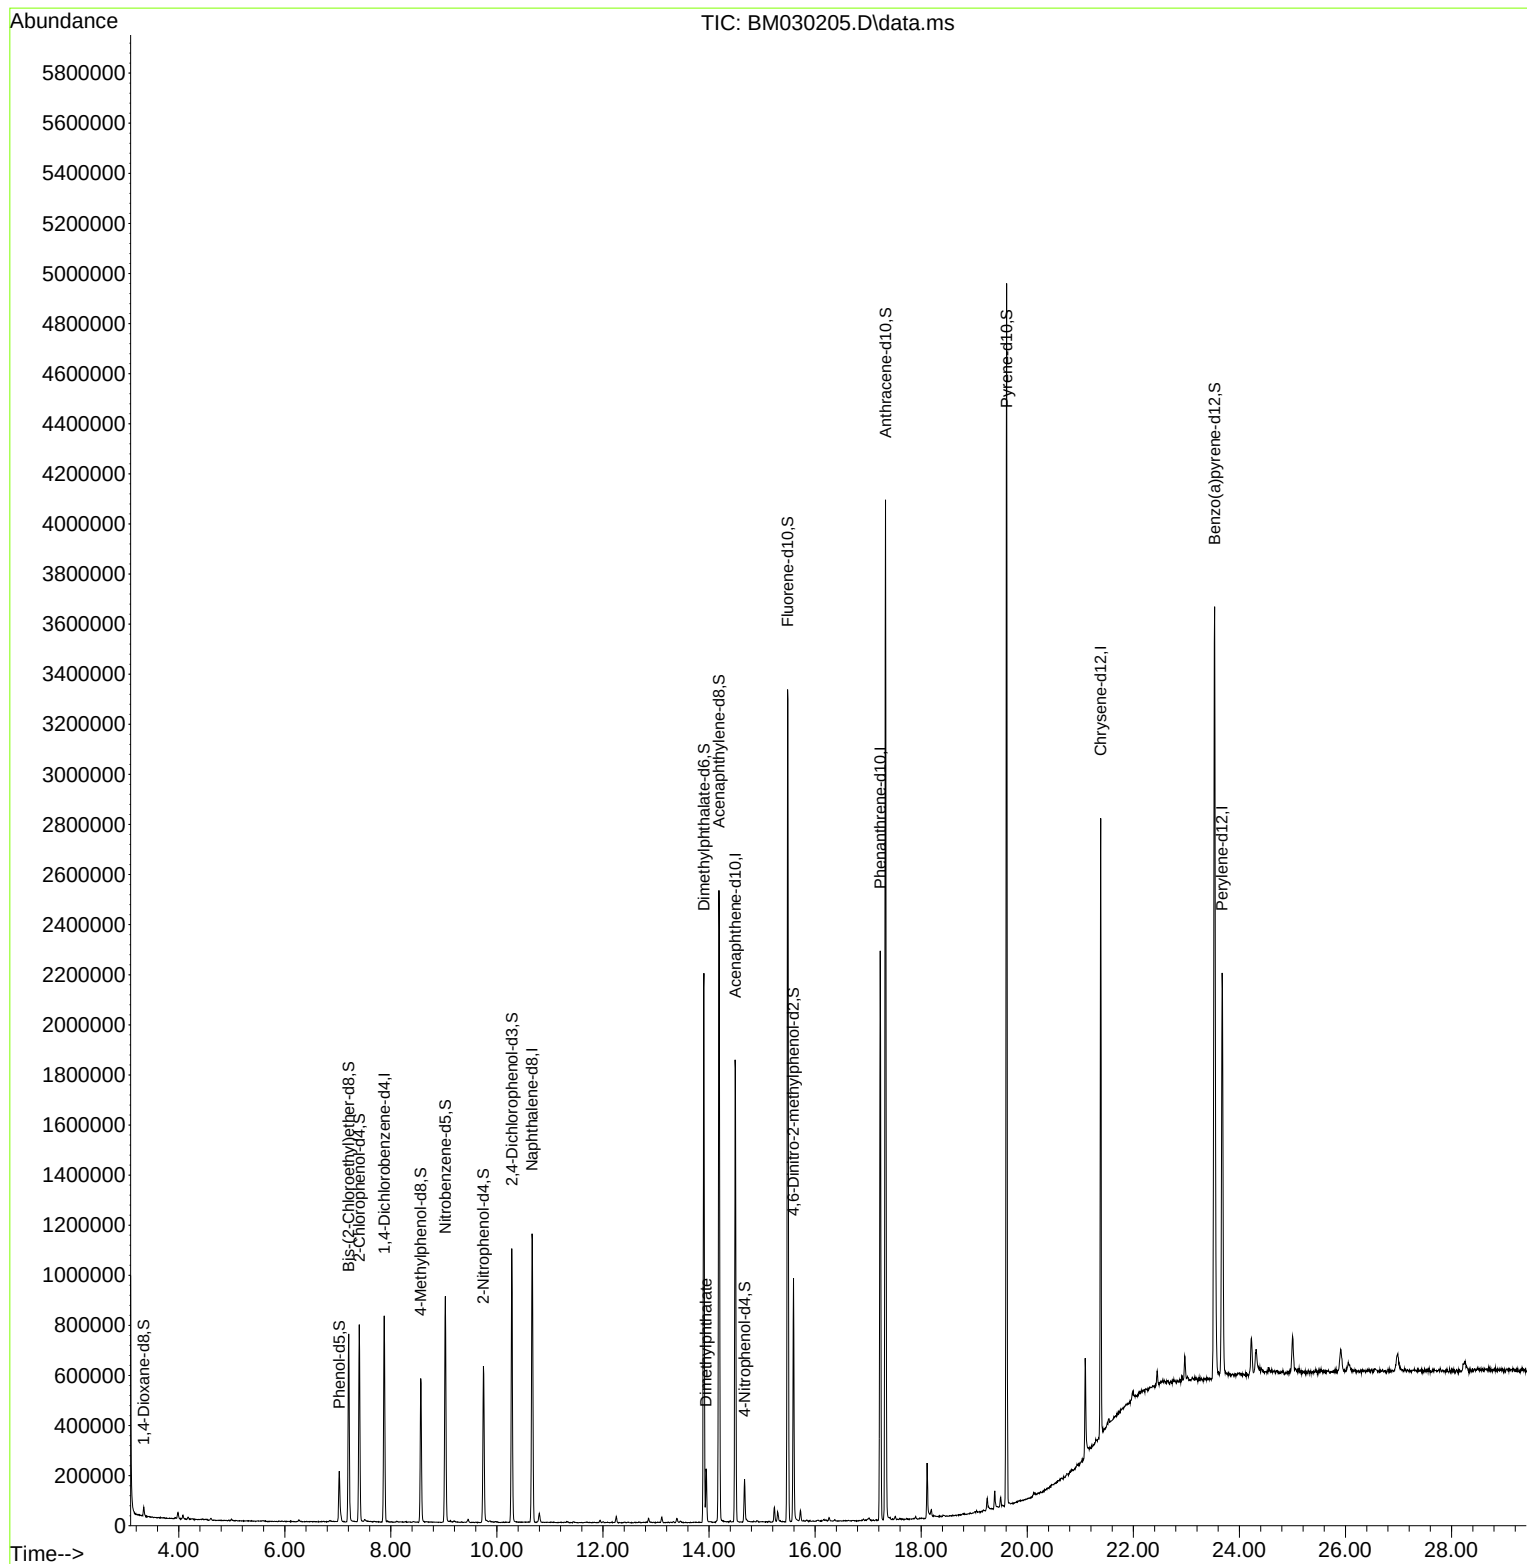

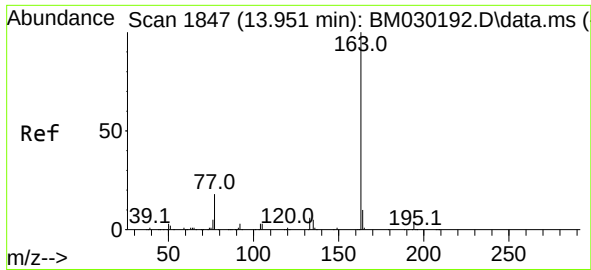

#47
 Dimethylphthalate
 Concen: 2.67 ng/ul
 RT: 13.945 min Scan# 1846
 Delta R.T. -0.006 min
 Lab File: BM030205.D
 Acq: 27 May 2021 17:22

Instrument :
 BNA_M
 ClientSampleId :
 GB450

Tgt Ion:163 Resp: 128385
 Ion Ratio Lower Upper
 163 100
 194 4.0 3.4 5.0
 164 10.4 8.2 12.2

