

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052721\
 Data File : BM030207.D
 Acq On : 27 May 2021 18:36
 Operator : CG/JU
 Sample : M2474-15
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB446

Quant Time: May 27 19:06:33 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 27 12:44:50 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.875	152	200569	20.00	ng/ul	0.00
20) Naphthalene-d8	10.663	136	840060	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.492	164	538938	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.227	188	1045951	20.00	ng/ul	0.00
79) Chrysene-d12	21.386	240	914060	20.00	ng/ul	0.00
88) Perylene-d12	23.674	264	898555	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.340	96	20250	4.13	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.00	ng/ul	0.00
7) Phenol-d5	7.028	99	104155	5.91	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.204	67	336790	30.26	ng/ul	0.00
11) 2-Chlorophenol-d4	7.404	132	323505	24.49	ng/ul	0.00
15) 4-Methylphenol-d8	8.563	113	198882	14.20	ng/ul	0.00
21) Nitrobenzene-d5	9.028	128	192579	35.12	ng/ul	0.00
24) 2-Nitrophenol-d4	9.745	143	186533	35.72	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.281	165	375533	27.87	ng/ul	0.00
31) 4-Chloroaniline-d4	10.798	131	20884	1.04	ng/ul	0.00
46) Dimethylphthalate-d6	13.898	166	1323741	32.13	ng/ul	0.00
49) Acenaphthylene-d8	14.186	160	1630423	30.70	ng/ul	0.00
54) 4-Nitrophenol-d4	14.669	143	31044	4.66	ng/ul	0.00
60) Fluorene-d10	15.486	176	1183446	32.90	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.592	200	166332	32.80	ng/ul	0.00
73) Anthracene-d10	17.327	188	1941518	37.50	ng/ul	0.00
81) Pyrene-d10	19.609	212	2043817	41.71	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.533	264	1901542	37.33	ng/ul	0.00
Target Compounds						
47) Dimethylphthalate	13.945	163	90352	2.22	ng/ul	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052721\
Data File : BM030207.D
Acq On : 27 May 2021 18:36
Operator : CG/JU
Sample : M2474-15
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB446

Quant Time: May 27 19:06:33 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 27 12:44:50 2021
Response via : Initial Calibration

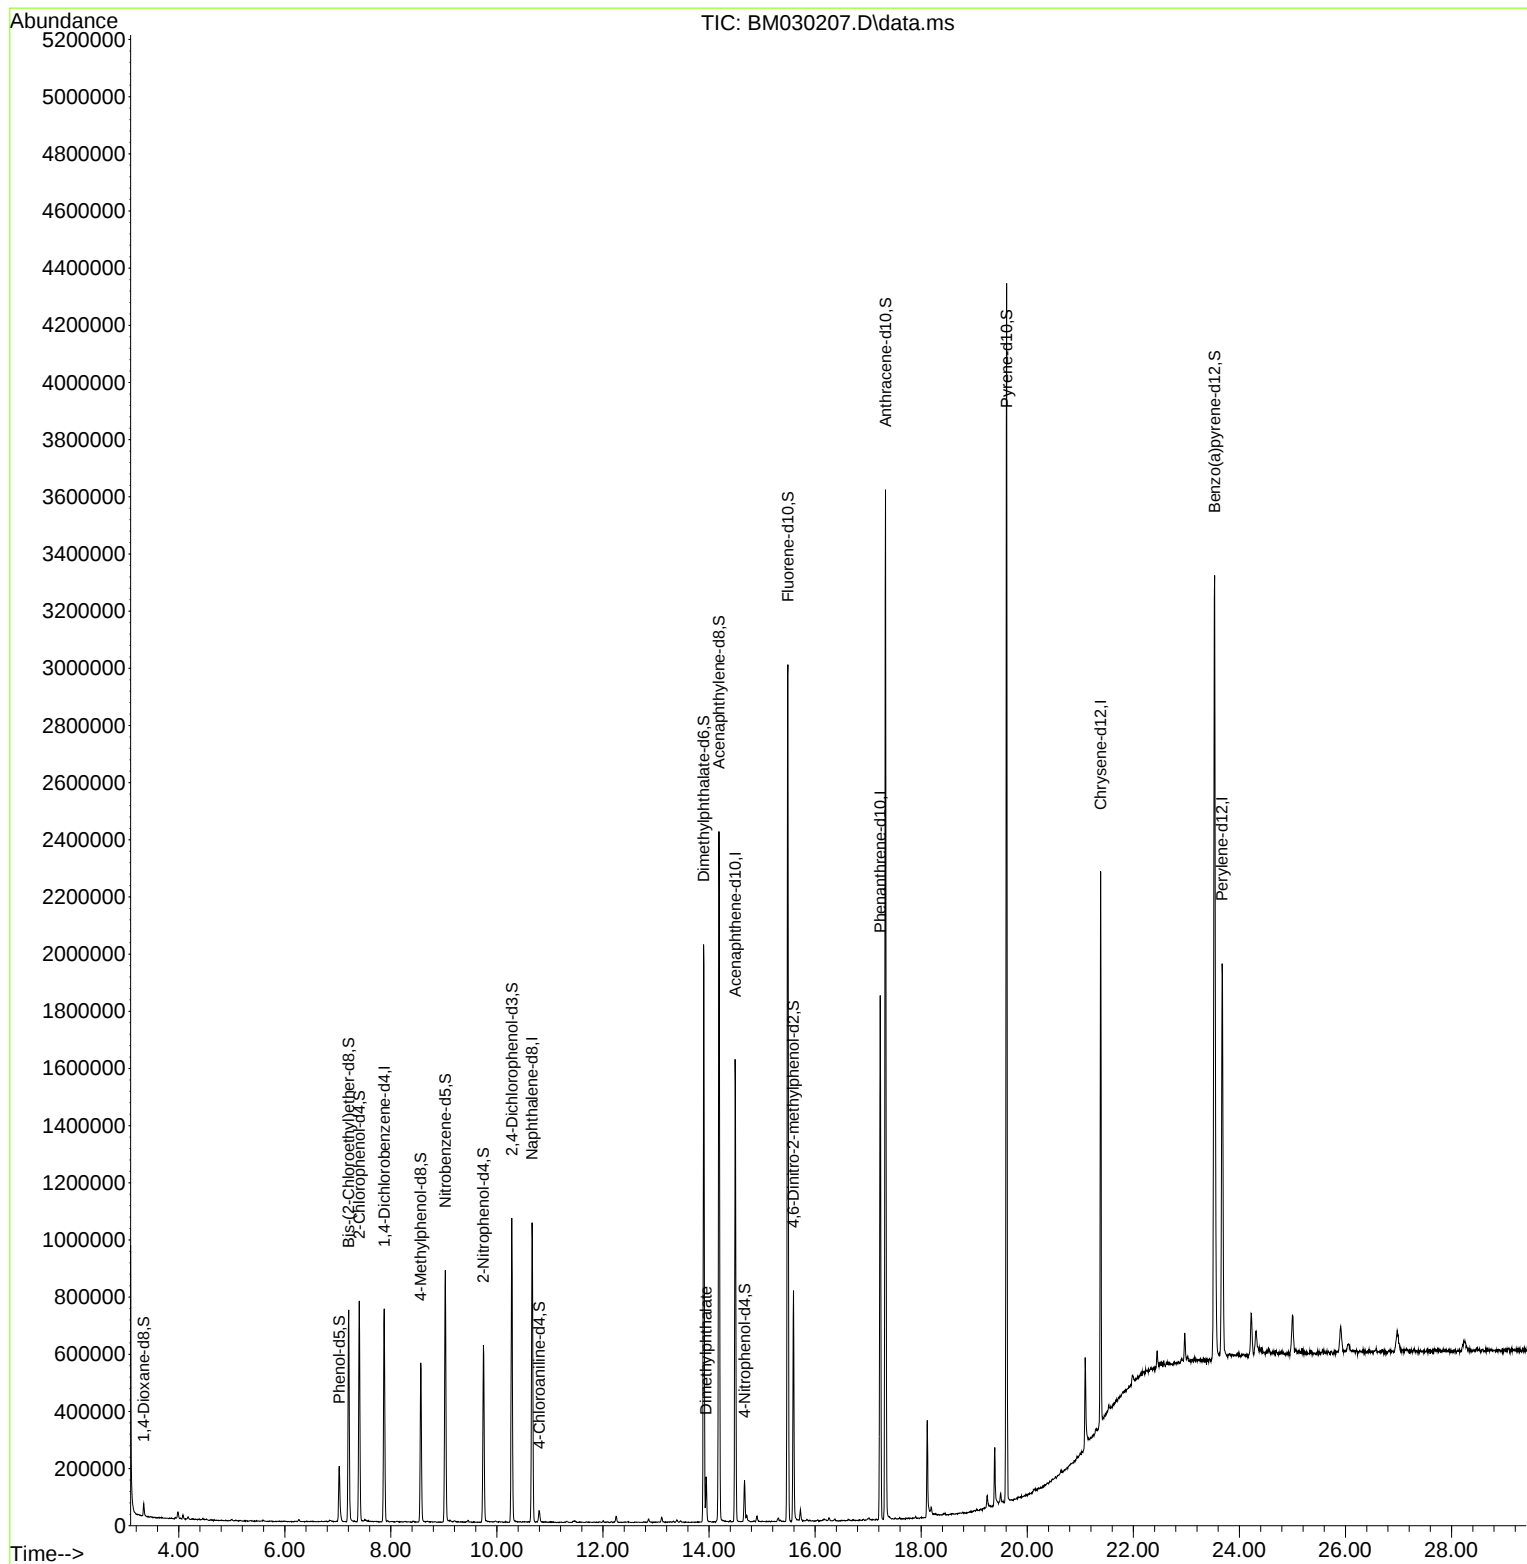

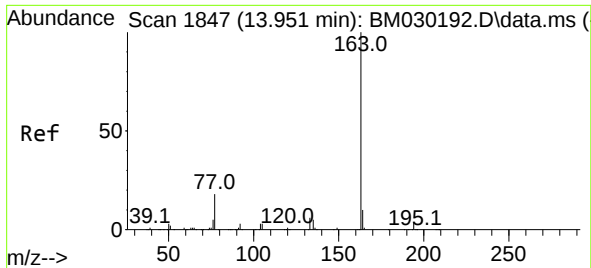

#47
 Dimethylphthalate
 Concen: 2.22 ng/ul
 RT: 13.945 min Scan# 1846
 Delta R.T. -0.006 min
 Lab File: BM030207.D
 Acq: 27 May 2021 18:36

Instrument :
 BNA_M
 ClientSampleId :
 GB446

Tgt Ion:163	Resp:	90352
Ion Ratio	Lower	Upper
163	100	
194	4.4	3.4 5.0
164	11.1	8.2 12.2

