

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052721\
 Data File : BM030213.D
 Acq On : 27 May 2021 22:52
 Operator : CG/JU
 Sample : M2528-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YARK5

Quant Time: May 28 02:08:01 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu May 27 10:27:00 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.875	152	270853	20.00	ng/ul	0.00
20) Naphthalene-d8	10.663	136	1176724	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.492	164	784105	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.227	188	1589798	20.00	ng/ul	0.00
79) Chrysene-d12	21.380	240	1322213	20.00	ng/ul	0.00
88) Perylene-d12	23.674	264	1226550	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.340	96	21080	3.19	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.00	ng/ul	0.00
7) Phenol-d5	7.028	99	126008	5.29	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.198	67	397746	26.46	ng/ul	0.00
11) 2-Chlorophenol-d4	7.404	132	385285	21.60	ng/ul	0.00
15) 4-Methylphenol-d8	8.563	113	246369	13.03	ng/ul	0.00
21) Nitrobenzene-d5	9.028	128	236624	30.81	ng/ul	0.00
24) 2-Nitrophenol-d4	9.745	143	232707	31.81	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.275	165	473490	25.09	ng/ul	0.00
31) 4-Chloroaniline-d4	10.798	131	31278	1.12	ng/ul	0.00
46) Dimethylphthalate-d6	13.898	166	1783859	29.76	ng/ul	0.00
49) Acenaphthylene-d8	14.186	160	2131068	27.58	ng/ul	0.00
54) 4-Nitrophenol-d4	14.669	143	41861	4.32	ng/ul	0.00
60) Fluorene-d10	15.480	176	1593111	30.45	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.592	200	225863	29.31	ng/ul	0.00
73) Anthracene-d10	17.327	188	2593717	32.96	ng/ul	0.00
81) Pyrene-d10	19.609	212	2709813	38.23	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.527	264	2289555	32.93	ng/ul	0.00
Target Compounds						
47) Dimethylphthalate	13.945	163	108743	1.84	ng/ul	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052721\
Data File : BM030213.D
Acq On : 27 May 2021 22:52
Operator : CG/JU
Sample : M2528-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YARK5

Quant Time: May 28 02:08:01 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu May 27 10:27:00 2021
Response via : Initial Calibration

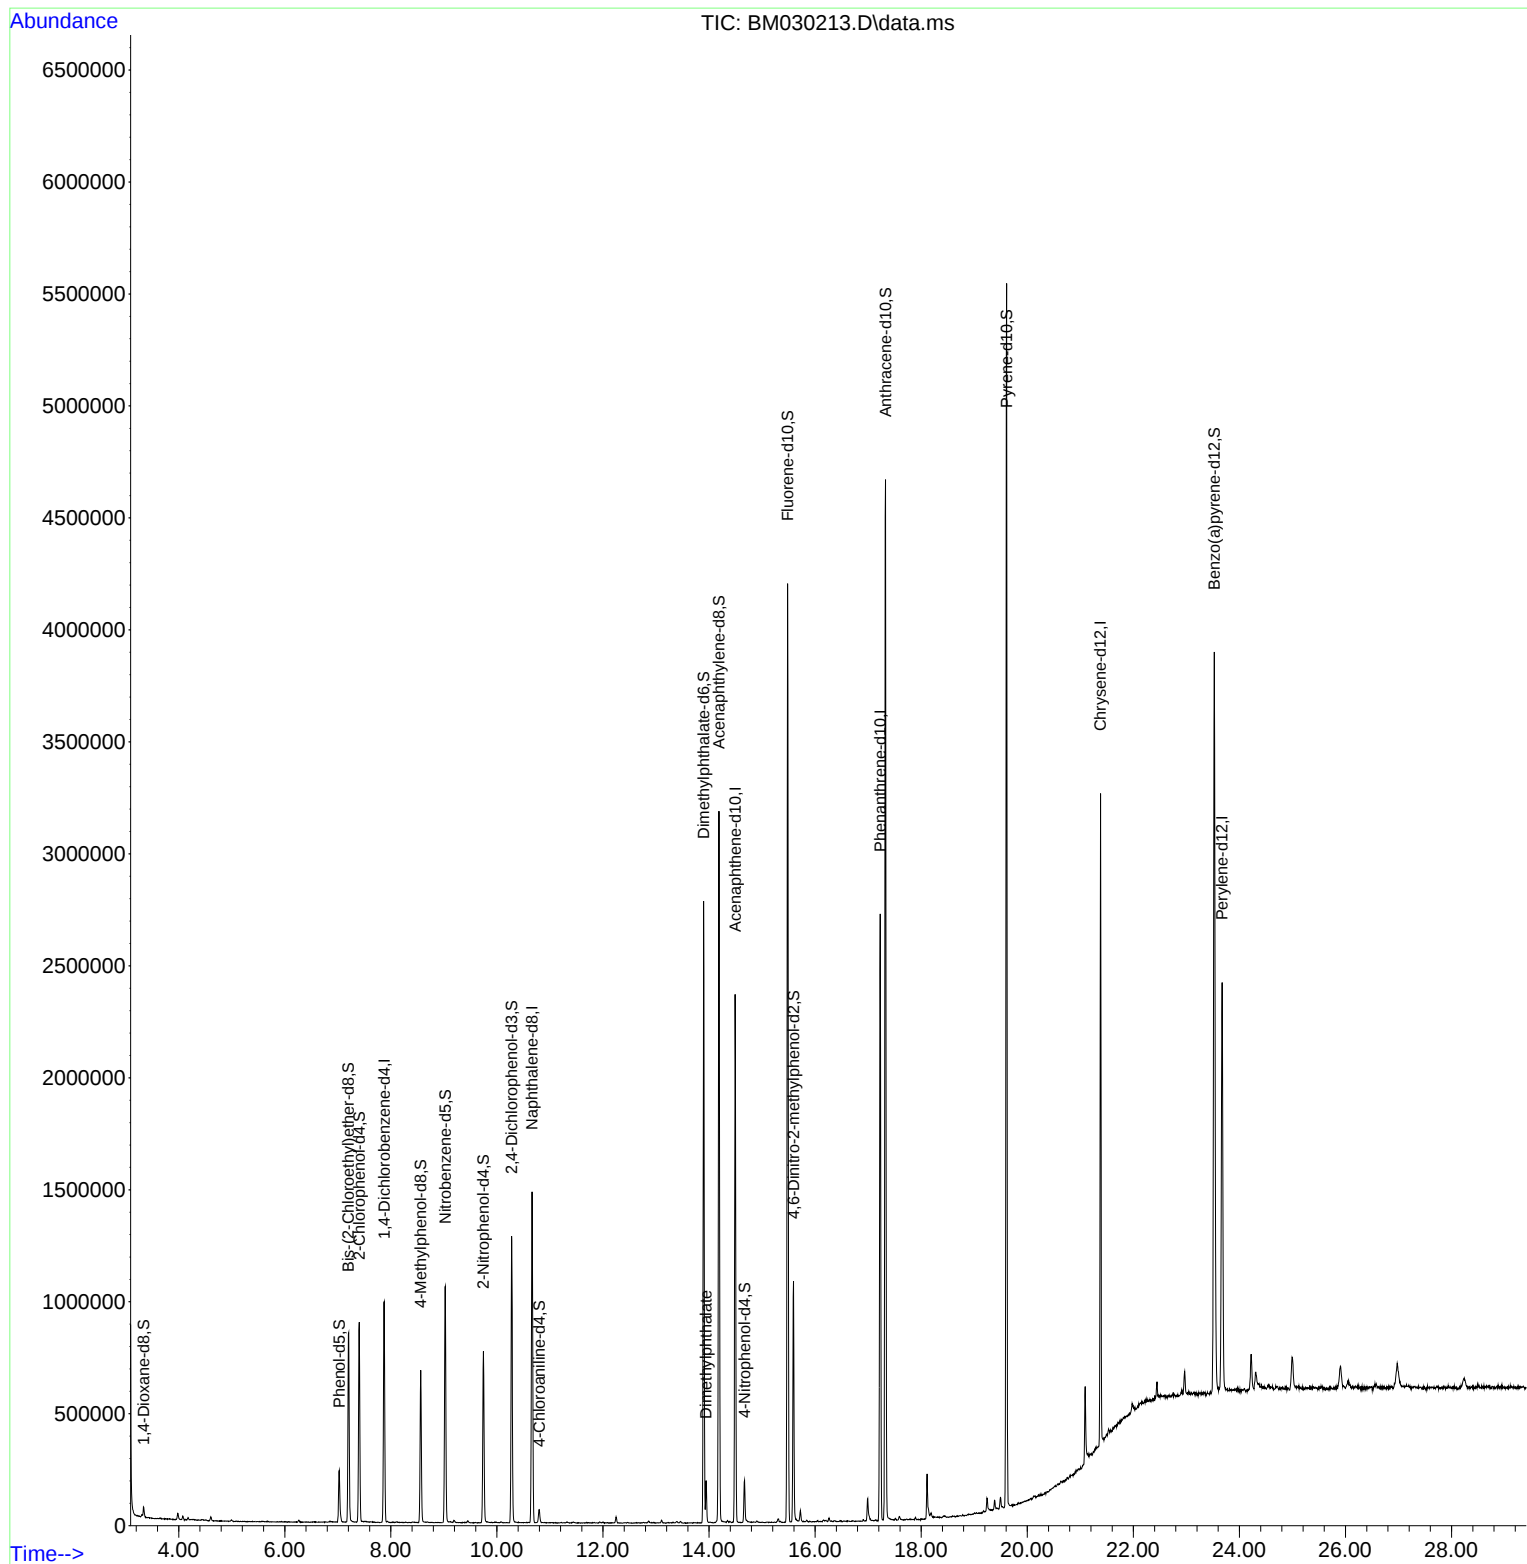

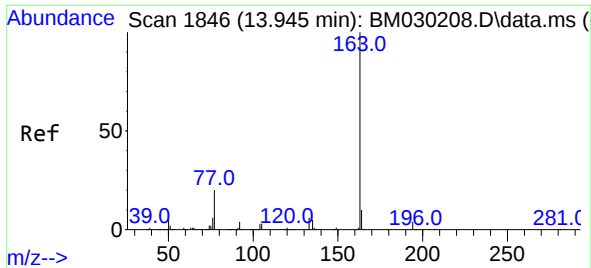

#47
 Dimethylphthalate
 Concen: 1.84 ng/ul
 RT: 13.945 min Scan# 1846
 Delta R.T. -0.006 min
 Lab File: BM030213.D
 Acq: 27 May 2021 22:52

Instrument :
 BNA_M
 ClientSampleId :
 YARK5

Tgt Ion:163 Resp: 108743

Ion	Ratio	Lower	Upper
163	100		
194	4.1	3.4	5.0
164	10.7	8.2	12.2

