

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052721\
 Data File : BM030216.D
 Acq On : 28 May 2021 00:41
 Operator : CG/JU
 Sample : M2528-04
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 YARK6

Quant Time: May 28 02:45:00 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri May 28 02:10:33 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.875	152	238217	20.00	ng/ul	0.00
20) Naphthalene-d8	10.663	136	973313	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.492	164	610550	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.227	188	1175924	20.00	ng/ul	0.00
79) Chrysene-d12	21.380	240	1086200	20.00	ng/ul	0.00
88) Perylene-d12	23.668	264	1107688	20.00	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.340	96	21022	3.61	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.00	ng/ul	
7) Phenol-d5	7.022	99	130483	6.23	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.199	67	388286	29.37	ng/ul	0.00
11) 2-Chlorophenol-d4	7.404	132	398443	25.40	ng/ul	0.00
15) 4-Methylphenol-d8	8.563	113	250495	15.06	ng/ul	0.00
21) Nitrobenzene-d5	9.022	128	234220	36.87	ng/ul	0.00
24) 2-Nitrophenol-d4	9.745	143	232561	38.43	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.275	165	463713	29.70	ng/ul	0.00
31) 4-Chloroaniline-d4	10.792	131	33288	1.44	ng/ul	0.00
46) Dimethylphthalate-d6	13.898	166	1542575	33.05	ng/ul	0.00
49) Acenaphthylene-d8	14.186	160	1934393	32.15	ng/ul	0.00
54) 4-Nitrophenol-d4	14.669	143	38692	5.13	ng/ul	0.00
60) Fluorene-d10	15.480	176	1369000	33.60	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.592	200	197905	34.72	ng/ul	0.00
73) Anthracene-d10	17.321	188	2211706	38.00	ng/ul	0.00
81) Pyrene-d10	19.604	212	2410603	41.40	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.527	264	2433973	38.76	ng/ul	0.00
Target Compounds						
47) Dimethylphthalate	13.945	163	87030	1.89	ng/ul	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052721\
Data File : BM030216.D
Acq On : 28 May 2021 00:41
Operator : CG/JU
Sample : M2528-04
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
YARK6

Quant Time: May 28 02:45:00 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri May 28 02:10:33 2021
Response via : Initial Calibration

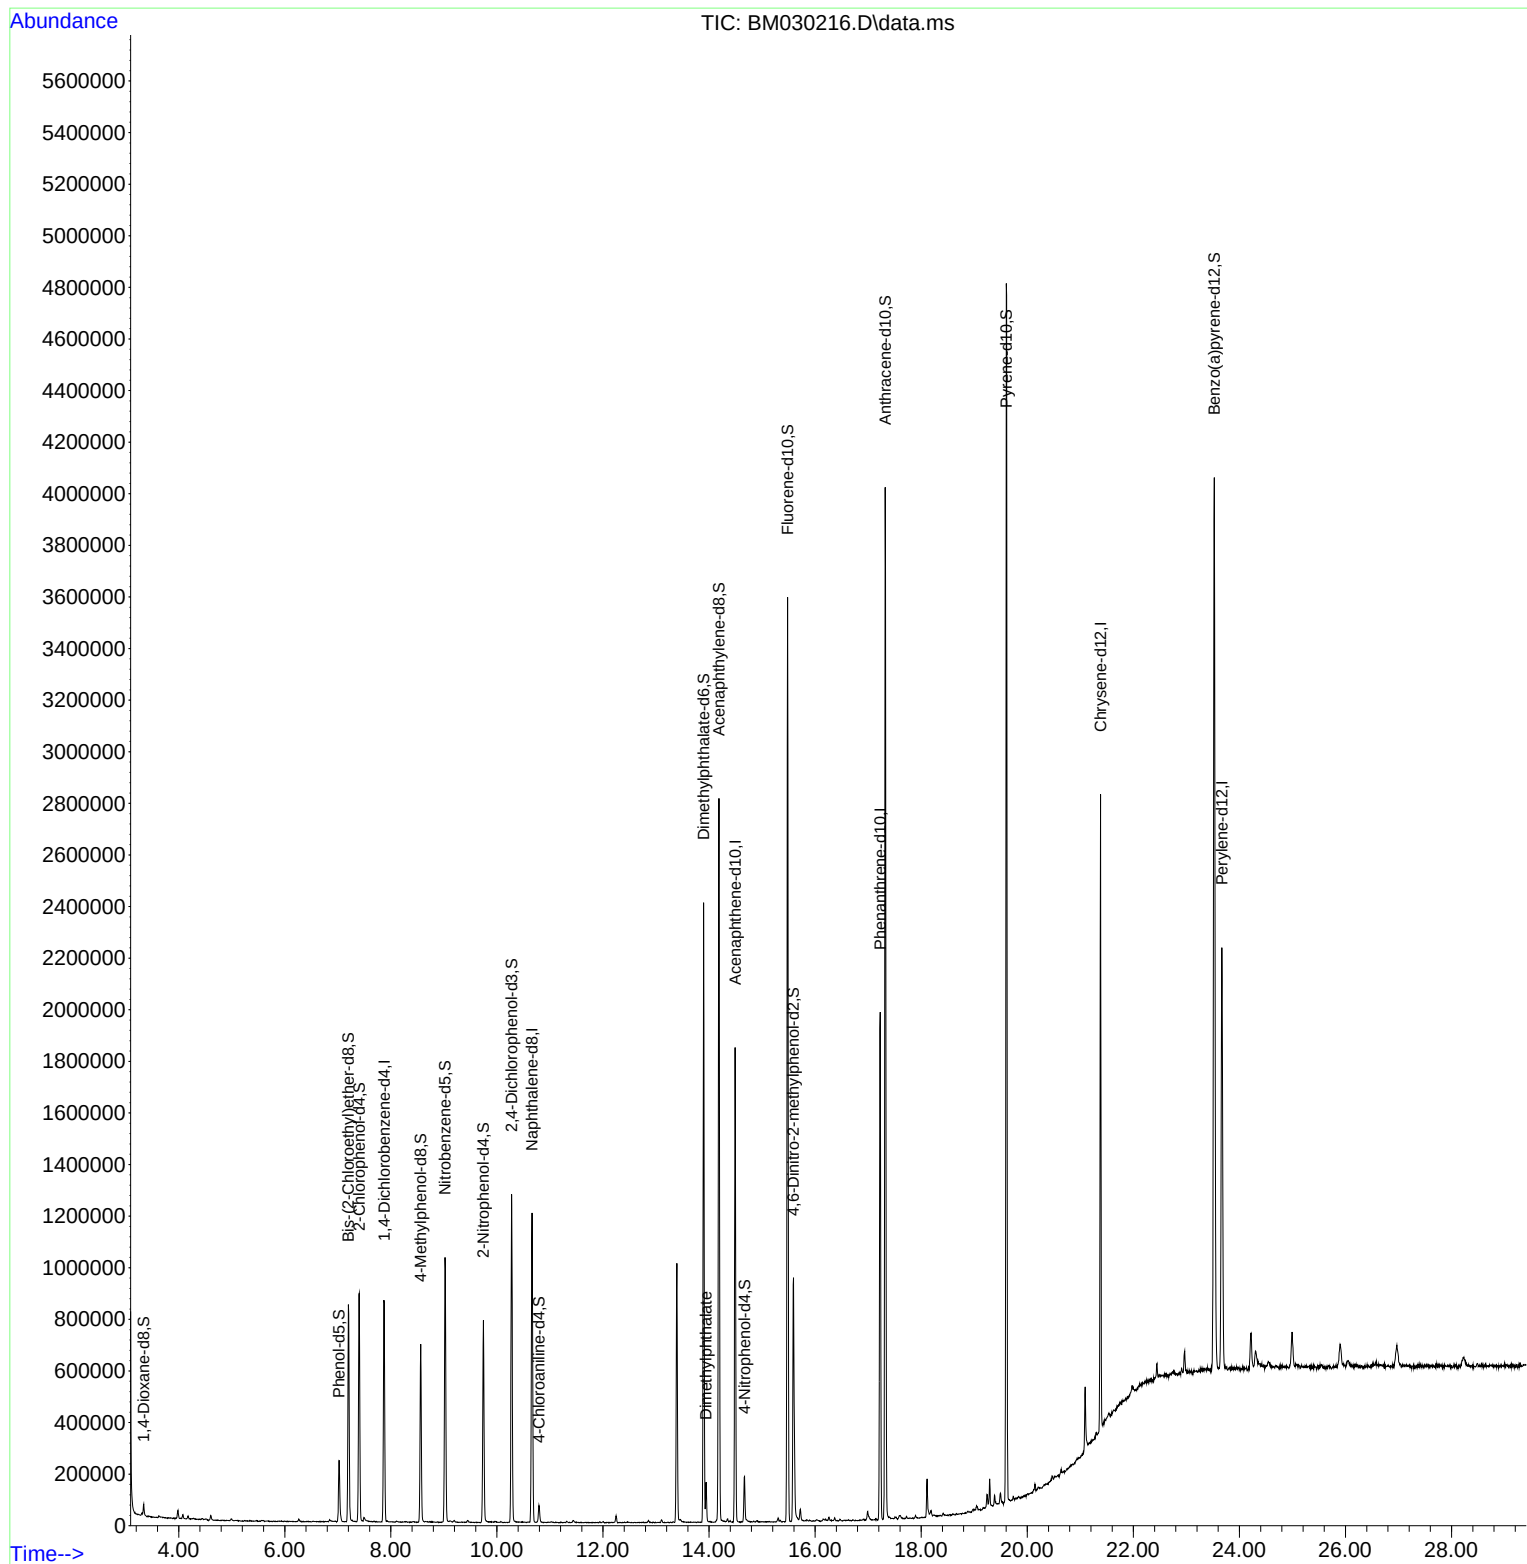

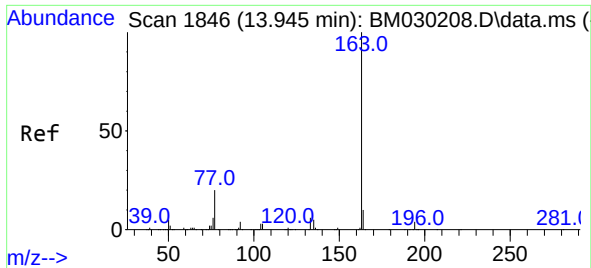

#47
Dimethylphthalate
Concen: 1.89 ng/ul
RT: 13.945 min Scan# 1846
Delta R.T. -0.006 min
Lab File: BM030216.D
Acq: 28 May 2021 00:41

Instrument :
BNA_M
ClientSampleId :
YARK6

Tgt Ion:163 Resp: 87030
Ion Ratio Lower Upper
163 100
194 4.2 3.4 5.0
164 9.8 8.2 12.2

