

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052721\
 Data File : BM030200.D
 Acq On : 27 May 2021 14:17
 Operator : CG/JU
 Sample : M2474-20
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB453

Integration Parameters: LSCINT.P

Integrator: RTE

Soothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030200.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.340	39	43	49	rVB	42103	56694	0.74%	0.087%
2	3.928	140	143	147	rBV5	4873	8880	0.12%	0.014%
3	3.987	148	153	161	rVV	29942	50226	0.65%	0.077%
4	4.081	165	169	175	rVB	15950	26388	0.34%	0.041%
5	4.175	181	185	190	rBV8	13407	18341	0.24%	0.028%
6	6.263	537	540	544	rVB5	9233	12447	0.16%	0.019%
7	7.028	663	670	680	rVB	238807	391538	5.11%	0.602%
8	7.204	693	700	713	rBV	917136	1465922	19.11%	2.255%
9	7.404	726	734	744	rBV	966353	1509628	19.68%	2.323%
10	7.498	747	750	761	rVB	4891	10920	0.14%	0.017%
11	7.875	806	814	821	rVB	860021	1342086	17.50%	2.065%
12	8.563	923	931	945	rBV	698371	1143501	14.91%	1.759%
13	9.028	1001	1010	1023	rBV	1124990	1858800	24.24%	2.860%
14	9.192	1032	1038	1043	rBV9	4643	8541	0.11%	0.013%
15	9.745	1124	1132	1141	rBV	783749	1339406	17.46%	2.061%
16	10.281	1215	1223	1234	rBV	1341146	2219037	28.93%	3.414%
17	10.663	1280	1288	1297	rBV	1187957	2022141	26.37%	3.111%
18	11.328	1396	1401	1406	rVB8	5719	10946	0.14%	0.017%
19	11.439	1415	1420	1425	rBV9	7544	13366	0.17%	0.021%
20	12.251	1552	1558	1562	rBV	28153	46705	0.61%	0.072%
21	12.475	1591	1596	1602	rBV6	7281	13044	0.17%	0.020%
22	12.863	1658	1662	1667	rBV4	12169	18990	0.25%	0.029%
23	13.110	1698	1704	1708	rBV3	21862	31660	0.41%	0.049%
24	13.692	1798	1803	1812	rBV2	70862	100616	1.31%	0.155%
25	13.904	1832	1839	1856	rBV	2679962	3804731	49.61%	5.854%
26	14.186	1879	1887	1900	rBV	3074985	4522244	58.96%	6.958%
27	14.492	1933	1939	1949	rBV	1892721	2910145	37.94%	4.478%
28	14.669	1963	1969	1973	rBV	212988	308053	4.02%	0.474%
29	14.710	1973	1976	1981	rVB	41595	58008	0.76%	0.089%
30	14.898	2004	2008	2013	rBV8	7387	10969	0.14%	0.017%
31	15.233	2058	2065	2072	rBV	37461	51866	0.68%	0.080%
32	15.304	2072	2077	2080	rVV2	16330	28172	0.37%	0.043%
33	15.345	2081	2084	2088	rVB5	12516	13907	0.18%	0.021%
34	15.486	2100	2108	2119	rBV	4106102	5996914	78.19%	9.227%
35	15.592	2119	2126	2137	rBV	1145164	1574454	20.53%	2.422%
36	15.721	2144	2148	2157	rVB	51903	80696	1.05%	0.124%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052721\
 Data File : BM030200.D
 Acq On : 27 May 2021 14:17
 Operator : CG/JU
 Sample : M2474-20
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB453

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
 Title : SVOA CALIBRATION

37	15.845	2165	2169	2172	rVB6	6897	8557	0.11%	0.013%
38	16.045	2199	2203	2209	rBV9	5496	8551	0.11%	0.013%
39	16.198	2226	2229	2237	rBV	17516	25816	0.34%	0.040%
40	16.263	2237	2240	2246	rVB4	16223	23489	0.31%	0.036%
41	16.686	2309	2312	2315	rBV5	5886	8389	0.11%	0.013%
42	16.910	2345	2350	2355	rVB7	7715	12486	0.16%	0.019%
43	16.992	2360	2364	2367	rBV	19423	27259	0.36%	0.042%
44	17.227	2398	2404	2414	rVB	2454553	3394251	44.26%	5.222%
45	17.327	2414	2421	2432	rBV	4819227	6715337	87.56%	10.332%
46	17.515	2449	2453	2459	rVB2	8173	14609	0.19%	0.022%
47	17.727	2485	2489	2492	rBV3	10682	12707	0.17%	0.020%
48	17.898	2512	2518	2524	rBV2	33995	52608	0.69%	0.081%
49	18.109	2550	2554	2559	rBV4	36042	55085	0.72%	0.085%
50	18.192	2564	2568	2572	rVB	19547	27284	0.36%	0.042%
51	18.415	2603	2606	2608	rBV4	10841	14893	0.19%	0.023%
52	19.245	2743	2747	2751	rBV	56566	86109	1.12%	0.132%
53	19.386	2768	2771	2775	rVB2	28490	31548	0.41%	0.049%
54	19.498	2786	2790	2794	rBV	48363	59170	0.77%	0.091%
55	19.609	2803	2809	2819	rBV	5854681	7669441	100.00%	11.800%
56	21.386	3106	3111	3118	rBV	2870415	3451790	45.01%	5.311%
57	23.533	3469	3476	3488	rVB2	3489005	6942863	90.53%	10.682%
58	23.680	3495	3501	3510	rVB2	1704076	3271119	42.65%	5.033%



Sum of corrected areas: 64993343

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052721\
Data File : BM030200.D
Acq On : 27 May 2021 14:17
Operator : CG/JU
Sample : M2474-20
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB453

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

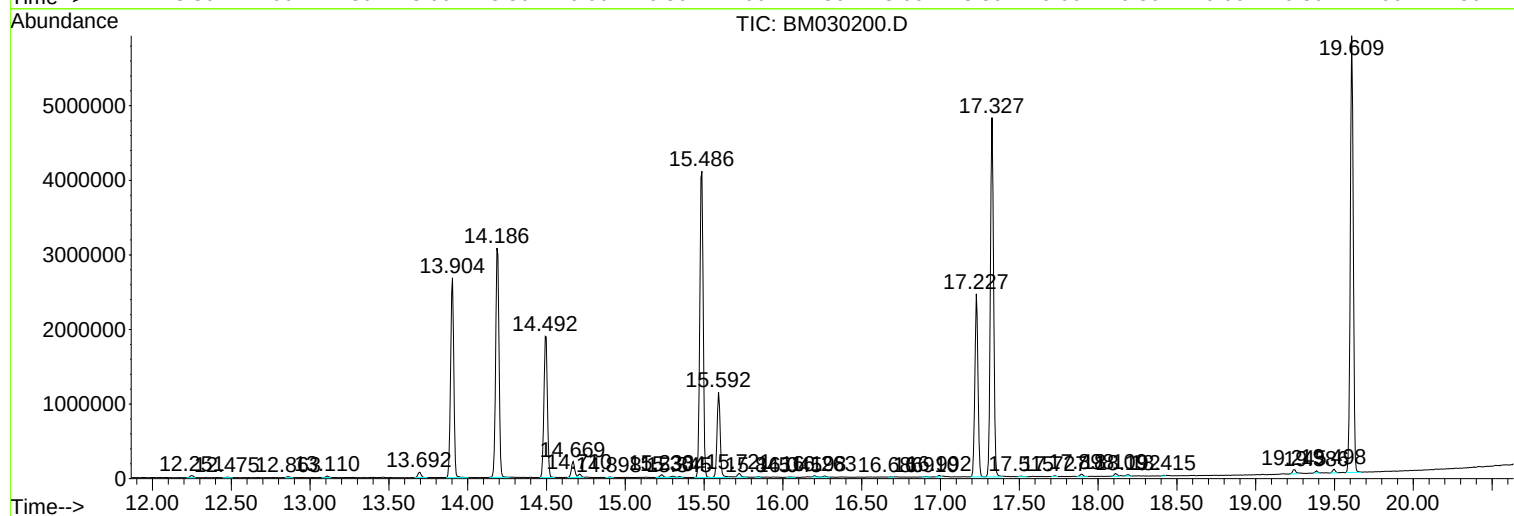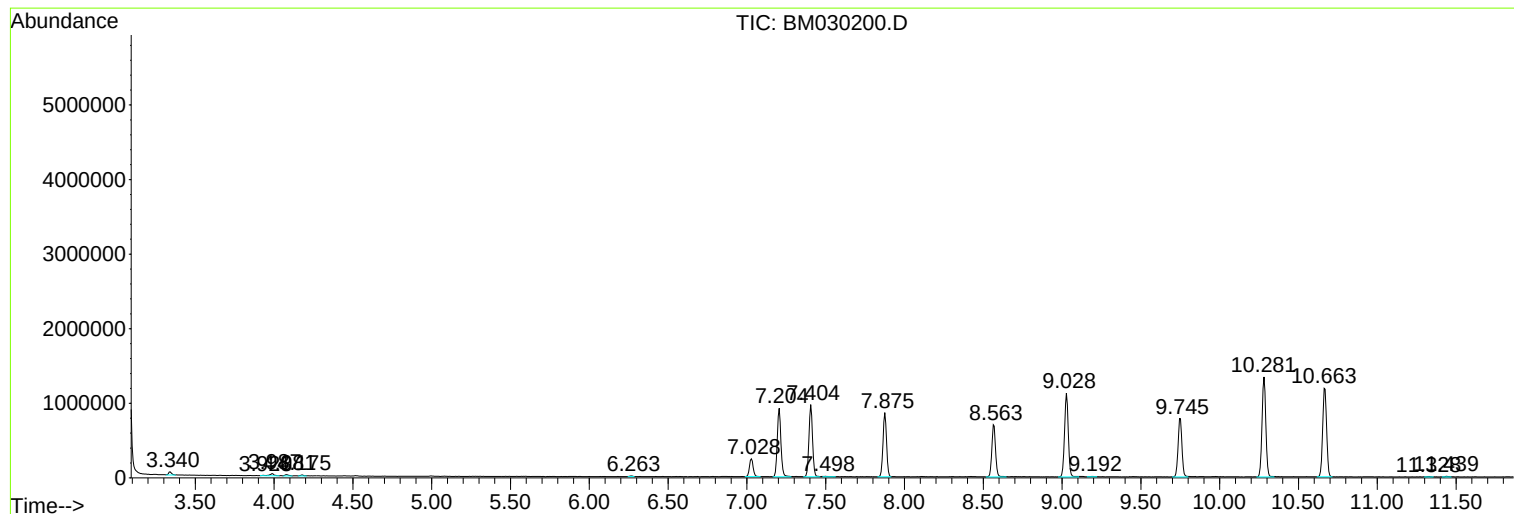

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052721\
Data File : BM030200.D
Acq On : 27 May 2021 14:17
Operator : CG/JU
Sample : M2474-20
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB453

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052721\
Data File : BM030200.D
Acq On : 27 May 2021 14:17
Operator : CG/JU
Sample : M2474-20
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB453

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
