

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052721\
 Data File : BM030201.D
 Acq On : 27 May 2021 14:54
 Operator : CG/JU
 Sample : M2474-19
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB452

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030201.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.340	39	43	51	rVB	39107	53535	0.62%	0.077%
2	3.928	138	143	146	rBV4	7108	11459	0.13%	0.017%
3	3.987	148	153	161	rVV	25194	45602	0.53%	0.066%
4	4.081	165	169	174	rVB2	14920	20060	0.23%	0.029%
5	4.175	182	185	192	rVB5	12300	20325	0.23%	0.029%
6	6.269	535	541	544	rBV2	9481	14121	0.16%	0.020%
7	7.028	662	670	677	rBV	254712	408776	4.73%	0.591%
8	7.204	693	700	716	rBV	981434	1596490	18.46%	2.308%
9	7.404	727	734	745	rBV	1022610	1630393	18.85%	2.357%
10	7.875	807	814	821	rBV	812036	1276493	14.76%	1.845%
11	8.110	846	854	857	rBV8	3880	8680	0.10%	0.013%
12	8.428	901	908	912	rBV9	5576	12510	0.14%	0.018%
13	8.563	925	931	939	rBV	731073	1199742	13.87%	1.734%
14	9.028	1001	1010	1019	rBV	1247043	2038310	23.57%	2.946%
15	9.751	1125	1133	1143	rBV	862971	1479928	17.11%	2.139%
16	10.281	1215	1223	1233	rBV	1489322	2451467	28.34%	3.543%
17	10.669	1281	1289	1298	rVB	1109181	1929595	22.31%	2.789%
18	11.439	1416	1420	1428	rBV8	12764	28526	0.33%	0.041%
19	12.251	1553	1558	1563	rBV2	29283	49264	0.57%	0.071%
20	12.857	1657	1661	1668	rBV3	14218	22976	0.27%	0.033%
21	13.110	1698	1704	1709	rBV2	24339	36971	0.43%	0.053%
22	13.333	1737	1742	1746	rBV	20422	29573	0.34%	0.043%
23	13.469	1758	1765	1769	rVB8	7647	15446	0.18%	0.022%
24	13.904	1831	1839	1849	rBV	3023040	4187117	48.41%	6.052%
25	14.186	1877	1887	1904	rBV	3205408	4800966	55.51%	6.940%
26	14.492	1933	1939	1951	rBV	1859260	2784991	32.20%	4.026%
27	14.668	1963	1969	1973	rBV	217658	316517	3.66%	0.458%
28	14.710	1973	1976	1982	rVB	43494	61889	0.72%	0.089%
29	14.904	2003	2009	2017	rBV9	16066	29490	0.34%	0.043%
30	15.233	2060	2065	2070	rVB	13698	20236	0.23%	0.029%
31	15.304	2070	2077	2082	rVB3	18240	34903	0.40%	0.050%
32	15.486	2100	2108	2116	rBV	4545702	6616214	76.50%	9.563%
33	15.592	2120	2126	2135	rBV	1224946	1702309	19.68%	2.461%
34	15.721	2143	2148	2155	rVB2	54842	86396	1.00%	0.125%
35	15.839	2165	2168	2173	rVB5	8417	11836	0.14%	0.017%
36	16.157	2218	2222	2224	rBV5	5759	8904	0.10%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052721\
 Data File : BM030201.D
 Acq On : 27 May 2021 14:54
 Operator : CG/JU
 Sample : M2474-19
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB452

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
 Title : SVOA CALIBRATION

37	16.262	2235	2240	2246	rBV4	17662	30827	0.36%	0.045%
38	16.374	2256	2259	2267	rVB8	7024	8937	0.10%	0.013%
39	17.015	2365	2368	2374	rVB2	9415	17087	0.20%	0.025%
40	17.227	2397	2404	2413	rBV	2331880	3302830	38.19%	4.774%
41	17.327	2414	2421	2438	rBV2	5075374	7328004	84.73%	10.592%
42	17.515	2449	2453	2461	rVB4	7786	15078	0.17%	0.022%
43	17.892	2514	2517	2524	rVB9	12190	13755	0.16%	0.020%
44	18.109	2550	2554	2563	rBV2	73249	118411	1.37%	0.171%
45	18.192	2563	2568	2572	rVB	29461	43457	0.50%	0.063%
46	19.245	2743	2747	2757	rBV	61997	104004	1.20%	0.150%
47	19.386	2767	2771	2779	rBV	75325	110944	1.28%	0.160%
48	19.498	2786	2790	2795	rBV	46906	64373	0.74%	0.093%
49	19.609	2803	2809	2819	rBV	6454982	8649066	100.00%	12.502%
50	21.386	3106	3111	3116	rBV	2770461	3541145	40.94%	5.119%
51	23.533	3469	3476	3489	rBV2	3828961	7553221	87.33%	10.918%
52	23.680	3495	3501	3511	rVB2	1713061	3239688	37.46%	4.683%




Sum of corrected areas: 69182837

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052721\
Data File : BM030201.D
Acq On : 27 May 2021 14:54
Operator : CG/JU
Sample : M2474-19
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB452

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

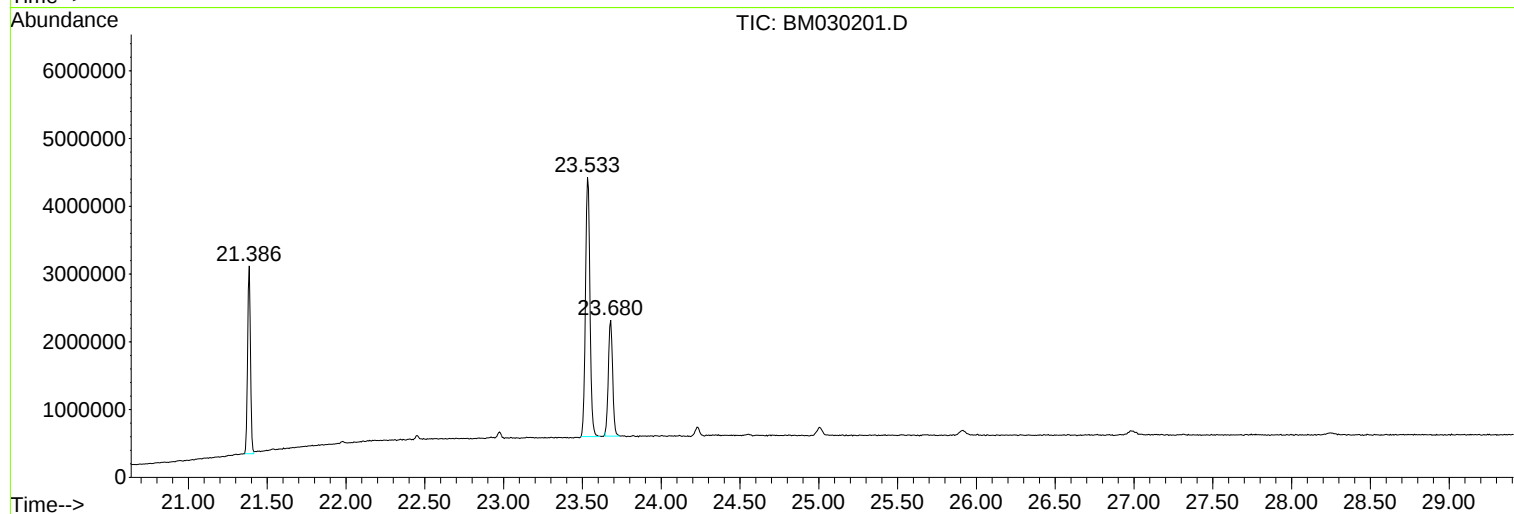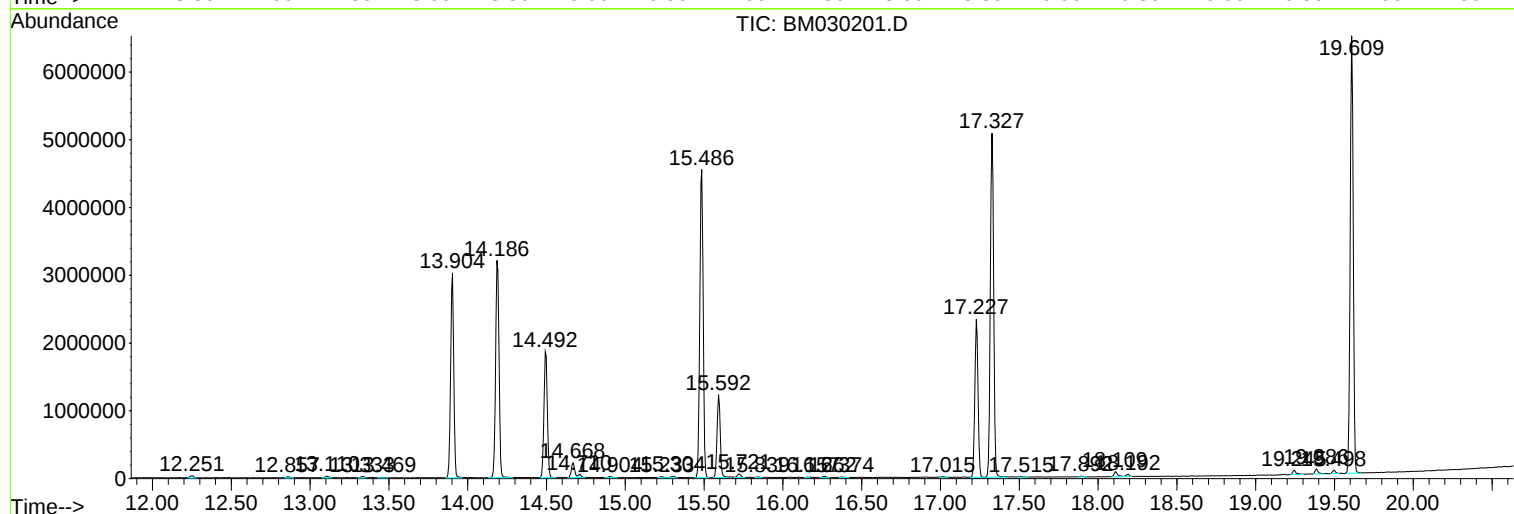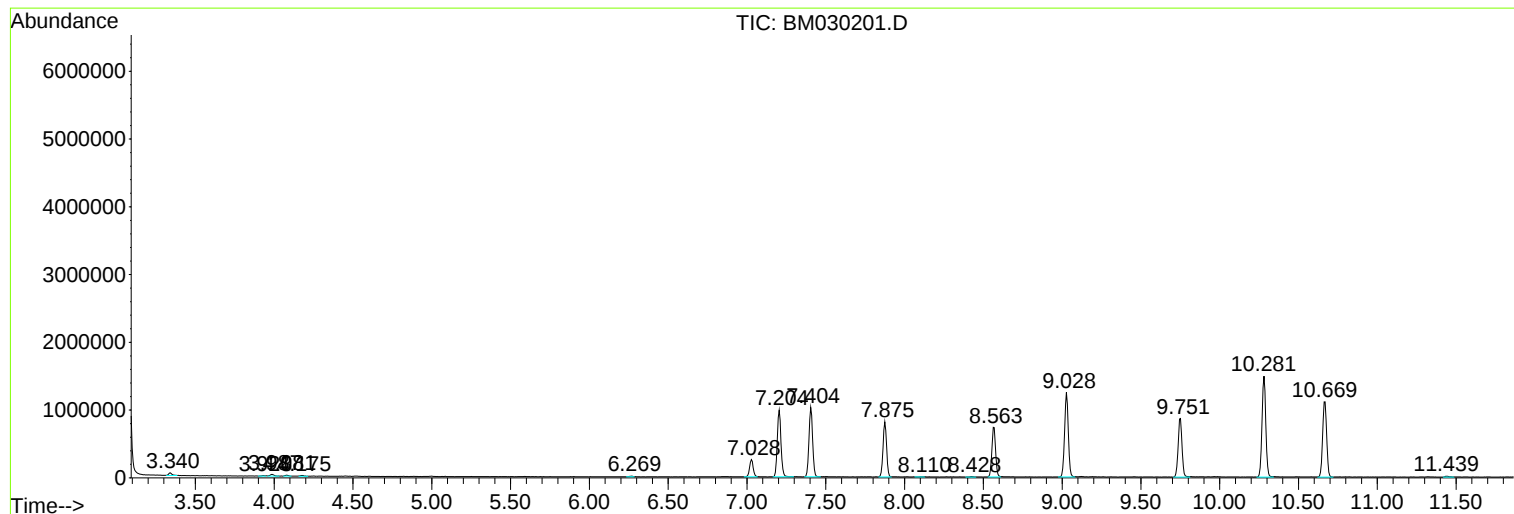

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052721\
Data File : BM030201.D
Acq On : 27 May 2021 14:54
Operator : CG/JU
Sample : M2474-19
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB452

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052721\
Data File : BM030201.D
Acq On : 27 May 2021 14:54
Operator : CG/JU
Sample : M2474-19
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB452

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc