

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052721\
 Data File : BM030202.D
 Acq On : 27 May 2021 15:31
 Operator : CG/JU
 Sample : M2474-22
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB455

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030202.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.340	39	43	49	rVB	43983	57845	0.85%	0.094%
2	3.928	140	143	146	rBV5	5497	7563	0.11%	0.012%
3	3.987	148	153	160	rVB	30612	50023	0.73%	0.081%
4	4.081	165	169	175	rVB	14613	23768	0.35%	0.039%
5	4.175	180	185	189	rBV6	14472	21863	0.32%	0.035%
6	4.610	254	259	267	rBV6	8799	17517	0.26%	0.028%
7	4.993	321	324	330	rVB3	7302	10449	0.15%	0.017%
8	6.269	534	541	546	rBV6	9841	15984	0.23%	0.026%
9	7.028	664	670	678	rBV	273070	436141	6.40%	0.707%
10	7.204	693	700	712	rBV	1038421	1653048	24.26%	2.679%
11	7.404	726	734	743	rBV	1078654	1696586	24.89%	2.750%
12	7.875	807	814	821	rBV	795925	1250116	18.34%	2.026%
13	8.122	850	856	861	rBV9	3929	8116	0.12%	0.013%
14	8.569	923	932	945	rBV	761625	1272071	18.67%	2.062%
15	9.028	1002	1010	1022	rBV	1273668	2059039	30.21%	3.338%
16	9.198	1032	1039	1043	rBV7	4287	6894	0.10%	0.011%
17	9.751	1125	1133	1145	rBV	878989	1487105	21.82%	2.410%
18	9.863	1149	1152	1158	rVV8	4537	9093	0.13%	0.015%
19	10.280	1215	1223	1235	rBV	1496496	2457363	36.06%	3.983%
20	10.669	1281	1289	1298	rVB	1064793	1833227	26.90%	2.972%
21	10.804	1307	1312	1316	rBV8	6128	12864	0.19%	0.021%
22	11.322	1395	1400	1405	rBV8	4304	8317	0.12%	0.013%
23	11.439	1415	1420	1429	rBV8	8370	20022	0.29%	0.032%
24	11.545	1434	1438	1446	rVB10	4119	7666	0.11%	0.012%
25	11.951	1502	1507	1509	rVV4	5728	8971	0.13%	0.015%
26	12.004	1511	1516	1521	rVB4	7298	12135	0.18%	0.020%
27	12.245	1551	1557	1564	rVB2	31320	53557	0.79%	0.087%
28	12.863	1657	1662	1667	rBV	15847	25111	0.37%	0.041%
29	13.110	1699	1704	1713	rBV2	25656	41702	0.61%	0.068%
30	13.333	1737	1742	1750	rBV	63410	95846	1.41%	0.155%
31	13.392	1750	1752	1757	rVV5	4845	7150	0.10%	0.012%
32	13.463	1760	1764	1769	rVV3	7782	12430	0.18%	0.020%
33	13.792	1815	1820	1823	rBV6	3579	8156	0.12%	0.013%
34	13.904	1832	1839	1849	rBV	2785619	3865491	56.72%	6.266%
35	14.186	1878	1887	1902	rBV	3208905	4777521	70.10%	7.744%
36	14.492	1933	1939	1951	rBV	1667199	2485337	36.47%	4.029%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052721\
 Data File : BM030202.D
 Acq On : 27 May 2021 15:31
 Operator : CG/JU
 Sample : M2474-22
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB455

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
 Title : SVOA CALIBRATION

37	14.668	1962	1969	1975	rBV	189051	283943	4.17%	0.460%
38	15.298	2069	2076	2084	rBV2	38863	70530	1.03%	0.114%
39	15.486	2101	2108	2116	rBV	4128193	6011997	88.22%	9.745%
40	15.592	2120	2126	2135	rBV	1085386	1416644	20.79%	2.296%
41	15.721	2143	2148	2154	rVB2	48735	72236	1.06%	0.117%
42	15.845	2166	2169	2172	rVB5	8106	8977	0.13%	0.015%
43	16.104	2210	2213	2218	rBV	9202	15263	0.22%	0.025%
44	16.168	2220	2224	2228	rVB6	4810	8752	0.13%	0.014%
45	16.262	2236	2240	2247	rBV4	13551	20074	0.29%	0.033%
46	16.727	2314	2319	2322	rBV5	4905	7660	0.11%	0.012%
47	16.909	2347	2350	2354	rVB6	8128	10825	0.16%	0.018%
48	17.015	2366	2368	2374	rVB2	10358	13421	0.20%	0.022%
49	17.227	2398	2404	2412	rBV	1876146	2682823	39.37%	4.349%
50	17.327	2414	2421	2432	rBV	4563856	6259850	91.85%	10.147%
51	17.509	2448	2452	2458	rVB	12166	17744	0.26%	0.029%
52	17.892	2514	2517	2523	rVB8	9370	12278	0.18%	0.020%
53	18.109	2550	2554	2562	rBV3	48872	78398	1.15%	0.127%
54	18.192	2564	2568	2574	rVB	23917	36187	0.53%	0.059%
55	19.245	2743	2747	2754	rBV	48658	75637	1.11%	0.123%
56	19.386	2767	2771	2778	rBV3	46625	64102	0.94%	0.104%
57	19.498	2786	2790	2794	rVB	35065	48059	0.71%	0.078%
58	19.609	2803	2809	2818	rBV	5132952	6815139	100.00%	11.047%
59	21.386	3106	3111	3116	rBV	2203198	2654235	38.95%	4.302%
60	23.533	3469	3476	3489	rVB2	3362202	6507492	95.49%	10.548%
61	23.680	3495	3501	3511	rVB2	1375576	2684818	39.39%	4.352%




Sum of corrected areas: 61693171

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052721\
Data File : BM030202.D
Acq On : 27 May 2021 15:31
Operator : CG/JU
Sample : M2474-22
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB455

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

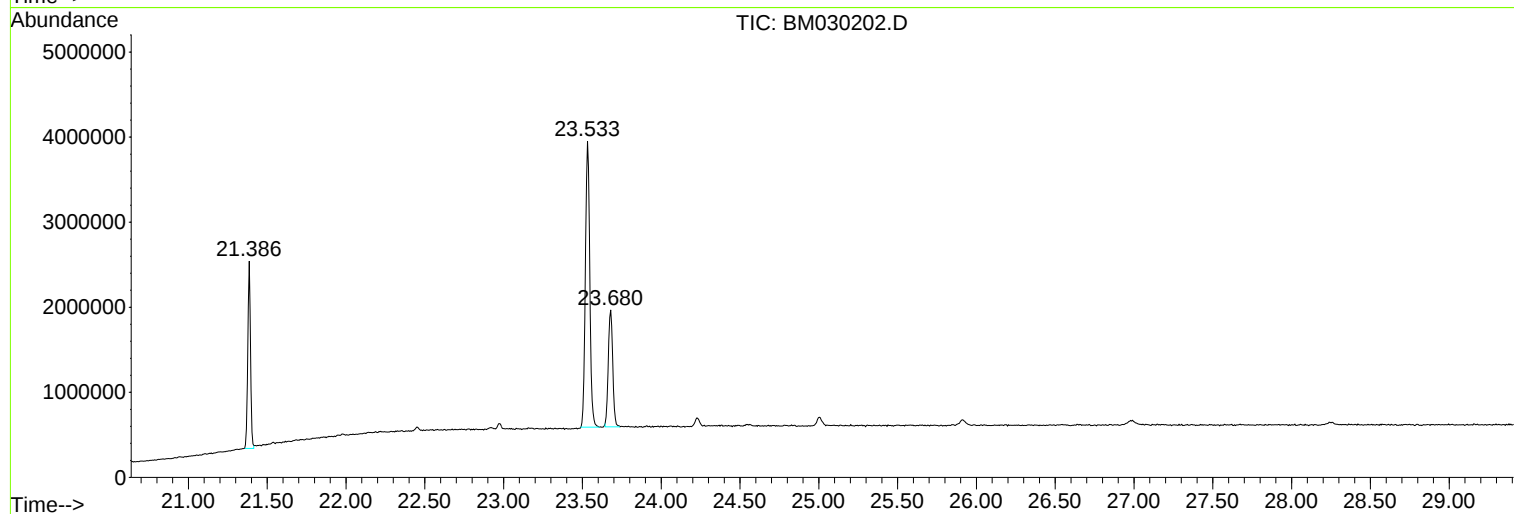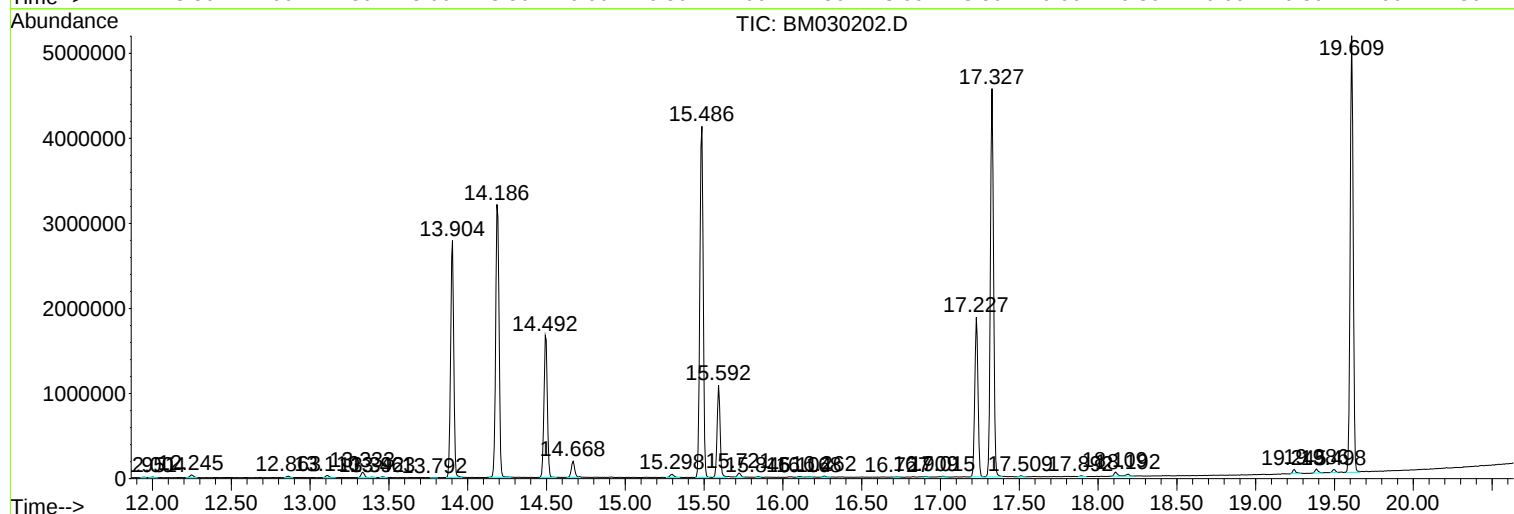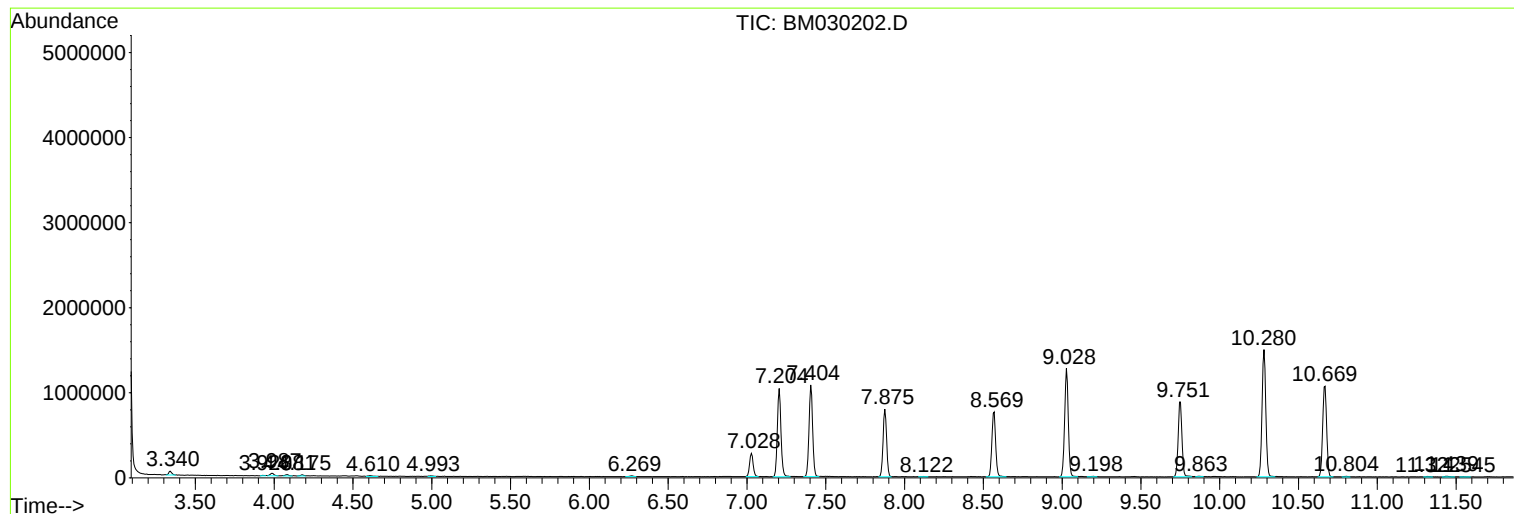

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052721\
Data File : BM030202.D
Acq On : 27 May 2021 15:31
Operator : CG/JU
Sample : M2474-22
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB455

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052721\
Data File : BM030202.D
Acq On : 27 May 2021 15:31
Operator : CG/JU
Sample : M2474-22
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB455

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
