

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052721\
 Data File : BM030206.D
 Acq On : 27 May 2021 17:59
 Operator : CG/JU
 Sample : M2474-21
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB454

Integration Parameters: LSCINT.P

Integrator: RTE

Smoother: OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030206.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.340	39	43	48	rVB	46996	58197	0.93%	0.101%
2	3.987	148	153	159	rVB	28130	41411	0.66%	0.072%
3	4.081	165	169	176	rVB2	15687	26495	0.42%	0.046%
4	4.175	179	185	190	rBV7	11398	19345	0.31%	0.033%
5	4.298	203	206	211	rVB7	4168	6959	0.11%	0.012%
6	4.610	253	259	264	rVB	22933	39171	0.63%	0.068%
7	4.993	322	324	330	rVB5	6405	9780	0.16%	0.017%
8	6.269	537	541	546	rVB2	8801	14034	0.22%	0.024%
9	7.028	663	670	677	rBV	250942	395276	6.32%	0.683%
10	7.204	693	700	713	rBV	910424	1450118	23.17%	2.506%
11	7.404	727	734	745	rBV	965209	1511955	24.16%	2.612%
12	7.875	806	814	823	rBV	838384	1322099	21.12%	2.284%
13	8.569	925	932	943	rBV	684505	1127630	18.02%	1.948%
14	9.028	1001	1010	1020	rBV	1115211	1836753	29.35%	3.174%
15	9.192	1033	1038	1043	rBV5	10205	17623	0.28%	0.030%
16	9.745	1125	1132	1142	rBV	766812	1302534	20.81%	2.251%
17	10.280	1216	1223	1234	rBV	1309043	2175344	34.76%	3.759%
18	10.663	1280	1288	1296	rBV	1140668	1970312	31.48%	3.404%
19	11.439	1416	1420	1422	rBV5	6724	8387	0.13%	0.014%
20	12.004	1510	1516	1521	rBV8	6487	11021	0.18%	0.019%
21	12.251	1552	1558	1564	rBV	27977	47002	0.75%	0.081%
22	12.480	1591	1597	1606	rVB8	4464	13337	0.21%	0.023%
23	12.857	1656	1661	1668	rBV6	8698	17595	0.28%	0.030%
24	12.945	1672	1676	1683	rVB6	6772	11055	0.18%	0.019%
25	13.110	1699	1704	1709	rBV3	12606	19081	0.30%	0.033%
26	13.463	1758	1764	1768	rVB6	5384	7789	0.12%	0.013%
27	13.698	1801	1804	1811	rVB8	11196	16622	0.27%	0.029%
28	13.904	1832	1839	1854	rBV	2524681	3545743	56.65%	6.126%
29	14.186	1880	1887	1901	rBV	2907054	4261950	68.09%	7.364%
30	14.492	1930	1939	1946	rBV	1806287	2744560	43.85%	4.742%
31	14.668	1961	1969	1973	rBV	181892	266601	4.26%	0.461%
32	14.710	1973	1976	1981	rVB	33990	46985	0.75%	0.081%
33	14.851	1998	2000	2004	rVB5	4858	6296	0.10%	0.011%
34	14.904	2004	2009	2014	rBV8	7362	13027	0.21%	0.023%
35	15.233	2060	2065	2070	rBV	73117	103375	1.65%	0.179%
36	15.304	2072	2077	2081	rVB2	12469	21680	0.35%	0.037%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052721\
 Data File : BM030206.D
 Acq On : 27 May 2021 17:59
 Operator : CG/JU
 Sample : M2474-21
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GB454

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
 Title : SVOA CALIBRATION

37	15.480	2100	2107	2115	rBV	3825203	5555658	88.76%	9.599%
38	15.592	2119	2126	2139	rBV	969827	1320820	21.10%	2.282%
39	15.721	2144	2148	2154	rVB	44192	67408	1.08%	0.116%
40	15.845	2166	2169	2173	rVB5	5916	7545	0.12%	0.013%
41	16.045	2197	2203	2209	rBV8	3382	7905	0.13%	0.014%
42	16.162	2218	2223	2229	rBV10	5463	7650	0.12%	0.013%
43	16.262	2236	2240	2247	rVB6	11910	22493	0.36%	0.039%
44	16.909	2345	2350	2352	rBV6	8555	9516	0.15%	0.016%
45	17.015	2360	2368	2372	rBV	10955	22907	0.37%	0.040%
46	17.227	2397	2404	2411	rBV	2133878	2989820	47.77%	5.166%
47	17.327	2413	2421	2434	rBV	4215261	5791721	92.53%	10.007%
48	17.504	2449	2451	2457	rVB4	4685	7822	0.12%	0.014%
49	17.892	2515	2517	2521	rBV5	7888	11339	0.18%	0.020%
50	18.109	2548	2554	2564	rBV9	26511	55005	0.88%	0.095%
51	18.186	2564	2567	2573	rVB	17509	24186	0.39%	0.042%
52	18.415	2603	2606	2609	rBV5	5652	7213	0.12%	0.012%
53	19.245	2743	2747	2751	rBV	43889	61974	0.99%	0.107%
54	19.386	2769	2771	2775	rVB5	15059	14846	0.24%	0.026%
55	19.498	2786	2790	2794	rBV	34158	41461	0.66%	0.072%
56	19.609	2803	2809	2820	rBV	4760047	6258981	100.00%	10.814%
57	21.386	3106	3111	3116	rBV	2148089	2780209	44.42%	4.804%
58	23.533	3469	3476	3486	rVB2	2896166	5599364	89.46%	9.675%
59	23.674	3494	3500	3510	rVB2	1403198	2724165	43.52%	4.707%




Sum of corrected areas: 57877150

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052721\
Data File : BM030206.D
Acq On : 27 May 2021 17:59
Operator : CG/JU
Sample : M2474-21
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB454

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

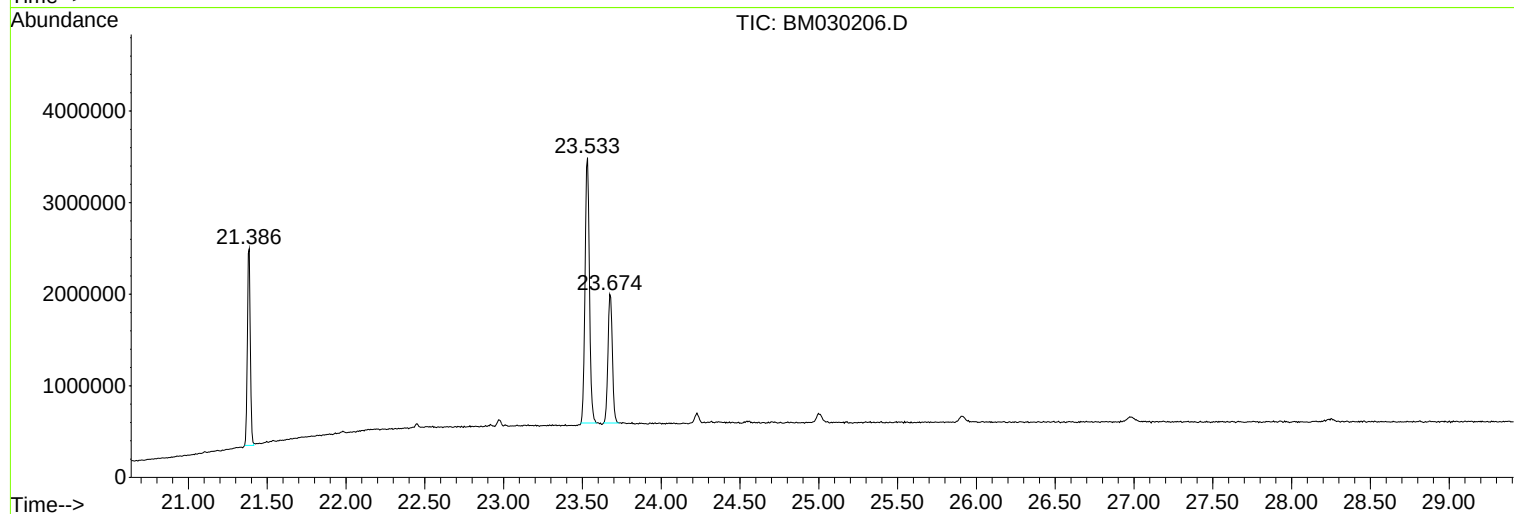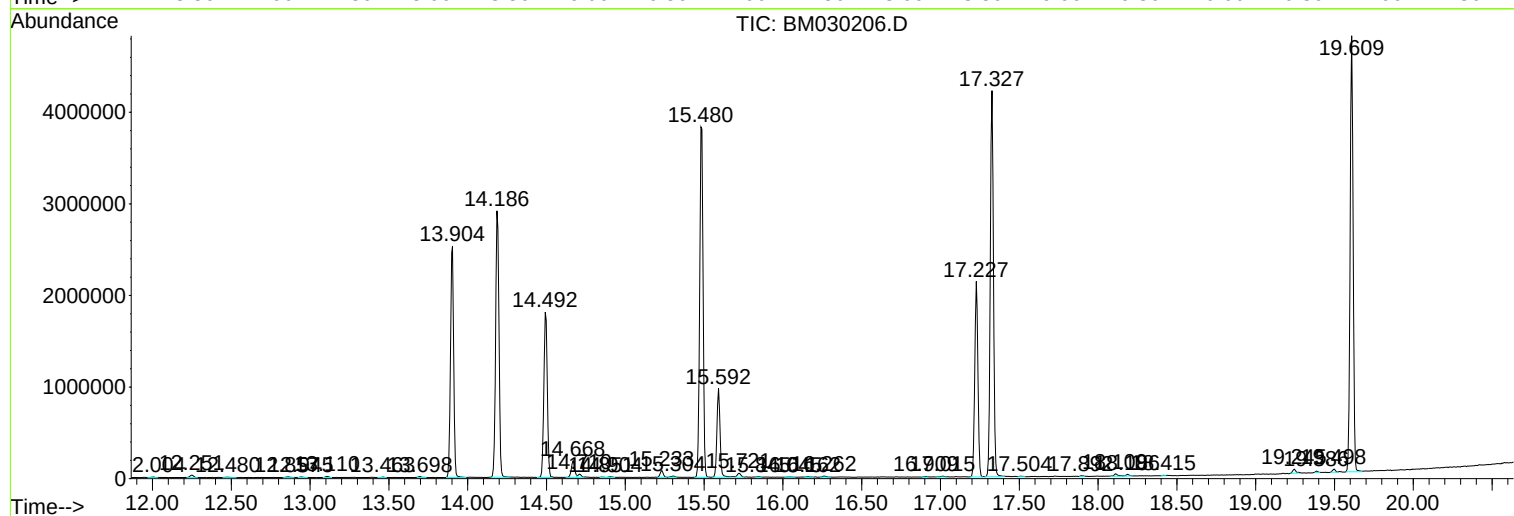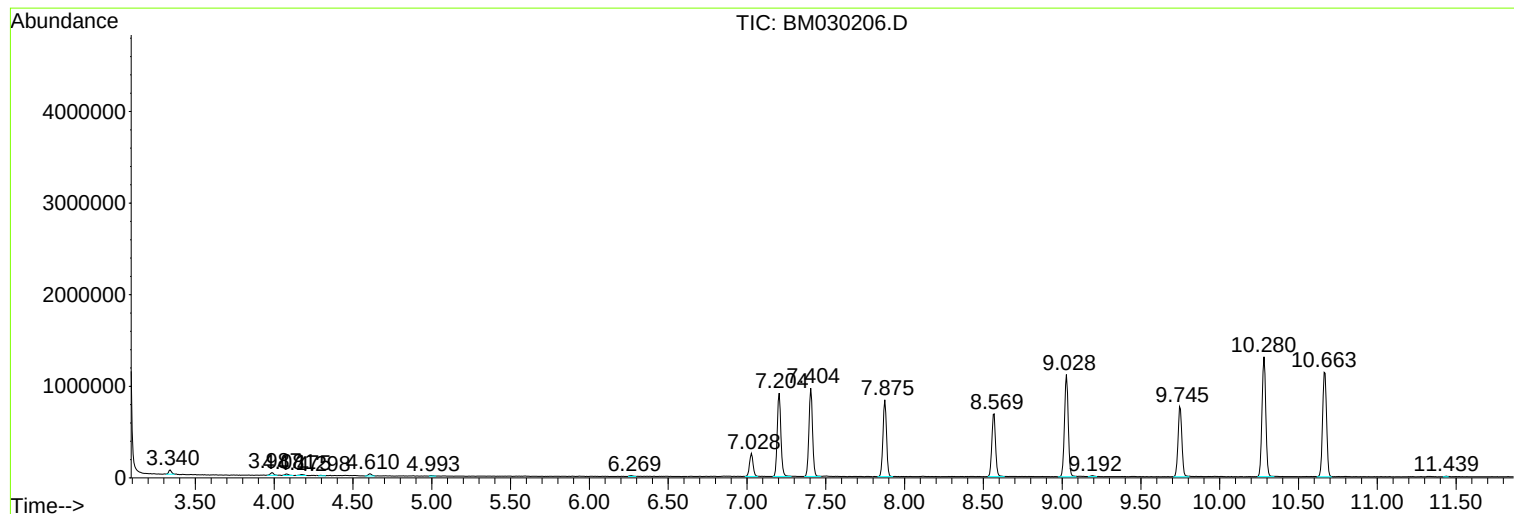

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052721\
Data File : BM030206.D
Acq On : 27 May 2021 17:59
Operator : CG/JU
Sample : M2474-21
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB454

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052721\
Data File : BM030206.D
Acq On : 27 May 2021 17:59
Operator : CG/JU
Sample : M2474-21
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GB454

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------