

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052721\
 Data File : BM030212.D
 Acq On : 27 May 2021 22:16
 Operator : CG/JU
 Sample : M2491-02
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JLX81

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030212.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.340	39	43	52	rVB	22865	36320	1.22%	0.114%
2	3.775	113	117	128	rBV	54503	131653	4.41%	0.413%
3	3.852	128	130	140	rVB7	15922	27632	0.92%	0.087%
4	3.987	147	153	161	rVB	65391	105548	3.53%	0.331%
5	4.081	164	169	175	rVB	19268	27425	0.92%	0.086%
6	4.175	181	185	192	rVB4	20787	33274	1.11%	0.104%
7	4.446	228	231	235	rVB4	9260	12985	0.43%	0.041%
8	4.681	268	271	274	rBV5	2955	4078	0.14%	0.013%
9	4.987	317	323	332	rVB	64264	99287	3.32%	0.311%
10	5.587	424	425	430	rVB4	4799	5140	0.17%	0.016%
11	5.869	468	473	476	rBV7	2873	4493	0.15%	0.014%
12	5.899	476	478	481	rVV4	3986	4220	0.14%	0.013%
13	6.263	535	540	547	rVB	16360	27255	0.91%	0.085%
14	6.857	637	641	642	rBV4	5263	6938	0.23%	0.022%
15	7.022	662	669	682	rBV	363318	640202	21.43%	2.007%
16	7.204	693	700	709	rBV	255384	427797	14.32%	1.341%
17	7.404	725	734	745	rBV	331979	542457	18.16%	1.700%
18	7.498	747	750	755	rVV6	8358	12610	0.42%	0.040%
19	7.557	757	760	765	rVB6	3972	6986	0.23%	0.022%
20	7.693	778	783	787	rBV4	5767	11150	0.37%	0.035%
21	7.869	806	813	822	rBV	791012	1299133	43.48%	4.072%
22	8.422	904	907	915	rVB9	4249	9243	0.31%	0.029%
23	8.563	925	931	941	rBV	379414	612659	20.51%	1.920%
24	8.693	948	953	959	rVB	37755	61730	2.07%	0.193%
25	9.022	1003	1009	1020	rBV	287197	494665	16.56%	1.550%
26	9.193	1032	1038	1040	rBV6	4563	7895	0.26%	0.025%
27	9.451	1077	1082	1086	rVB7	5056	8657	0.29%	0.027%
28	9.745	1121	1132	1143	rBV	191977	340306	11.39%	1.067%
29	9.863	1149	1152	1157	rBV7	3461	5244	0.18%	0.016%
30	9.969	1164	1170	1172	rBV7	3060	6562	0.22%	0.021%
31	10.104	1188	1193	1198	rVB6	4254	7876	0.26%	0.025%
32	10.281	1212	1223	1232	rBV	377532	640351	21.43%	2.007%
33	10.351	1232	1235	1239	rVB5	2326	4022	0.13%	0.013%
34	10.663	1280	1288	1300	rVB	1109091	1861997	62.32%	5.836%
35	10.792	1302	1310	1324	rVV	331917	588659	19.70%	1.845%
36	11.192	1375	1378	1387	rVB	6171	11490	0.38%	0.036%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052721\
 Data File : BM030212.D
 Acq On : 27 May 2021 22:16
 Operator : CG/JU
 Sample : M2491-02
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JLX81

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
 Title : SVOA CALIBRATION

37	11.451	1415	1422	1429	rBV5	10617	25441	0.85%	0.080%
38	11.692	1456	1463	1468	rVB5	6415	11432	0.38%	0.036%
39	11.945	1499	1506	1510	rBV9	3083	6711	0.22%	0.021%
40	12.010	1516	1517	1524	rVB7	4374	6170	0.21%	0.019%
41	12.175	1539	1545	1549	rVB9	2710	5749	0.19%	0.018%
42	12.245	1553	1557	1564	rVB6	12005	20845	0.70%	0.065%
43	12.404	1580	1584	1588	rVB7	3049	4580	0.15%	0.014%
44	12.857	1656	1661	1667	rBV6	9611	16681	0.56%	0.052%
45	13.039	1689	1692	1699	rVB6	8243	12450	0.42%	0.039%
46	13.104	1699	1703	1708	rBV2	15454	23044	0.77%	0.072%
47	13.328	1738	1741	1743	rBV3	3586	4327	0.14%	0.014%
48	13.392	1748	1752	1755	rBV4	10032	15227	0.51%	0.048%
49	13.463	1760	1764	1768	rVB6	4129	5384	0.18%	0.017%
50	13.816	1817	1824	1829	rBV2	17282	29002	0.97%	0.091%
51	13.898	1832	1838	1842	rVV	735290	985116	32.97%	3.088%
52	13.945	1842	1846	1851	rVV	190113	272410	9.12%	0.854%
53	13.986	1851	1853	1856	rVB3	8370	7802	0.26%	0.024%
54	14.051	1859	1864	1867	rVV6	5152	6249	0.21%	0.020%
55	14.186	1875	1887	1896	rBV	788451	1186804	39.72%	3.720%
56	14.492	1932	1939	1946	rBV	1651744	2454832	82.16%	7.694%
57	14.557	1946	1950	1958	rVB2	50559	75134	2.51%	0.235%
58	14.669	1963	1969	1975	rBV	237491	363578	12.17%	1.140%
59	14.898	2002	2008	2015	rBV3	79229	118087	3.95%	0.370%
60	14.969	2017	2020	2024	rVB3	9683	11747	0.39%	0.037%
61	15.110	2040	2044	2048	rVB6	5660	10355	0.35%	0.032%
62	15.163	2048	2053	2056	rBV7	5163	7930	0.27%	0.025%
63	15.304	2071	2077	2082	rVB2	17767	29652	0.99%	0.093%
64	15.480	2097	2107	2113	rBV	1083393	1573640	52.67%	4.932%
65	15.533	2113	2116	2120	rVB	19962	26323	0.88%	0.083%
66	15.586	2120	2125	2135	rBV	203182	294751	9.87%	0.924%
67	15.663	2136	2138	2141	rVB4	6411	5494	0.18%	0.017%
68	15.692	2141	2143	2144	rBV2	6053	4746	0.16%	0.015%
69	15.722	2144	2148	2150	rBV5	7467	11931	0.40%	0.037%
70	15.839	2166	2168	2173	rVB5	6769	7034	0.24%	0.022%
71	16.133	2214	2218	2219	rBV4	3881	4956	0.17%	0.016%
72	16.169	2221	2224	2227	rVV5	5664	8177	0.27%	0.026%
73	16.221	2227	2233	2238	rVV4	13001	26037	0.87%	0.082%
74	16.539	2285	2287	2290	rVB4	6191	5296	0.18%	0.017%
75	16.586	2291	2295	2300	rVB7	7347	14654	0.49%	0.046%
76	16.633	2300	2303	2306	rBV5	4241	4540	0.15%	0.014%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052721\
 Data File : BM030212.D
 Acq On : 27 May 2021 22:16
 Operator : CG/JU
 Sample : M2491-02
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JLX81

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
 Title : SVOA CALIBRATION

77	16.686	2309	2312	2315	rVB5	4507	4868	0.16%	0.015%
78	17.010	2361	2367	2368	rBV4	6000	9655	0.32%	0.030%
79	17.045	2369	2373	2379	rVB3	25410	39602	1.33%	0.124%
80	17.139	2387	2389	2393	rVB5	3709	4126	0.14%	0.013%
81	17.227	2397	2404	2408	rBV	1892142	2689707	90.02%	8.430%
82	17.268	2408	2411	2415	rVV	149678	204615	6.85%	0.641%
83	17.321	2415	2420	2431	rVV	1169596	1696486	56.78%	5.317%
84	17.410	2431	2435	2442	rVB8	22200	37368	1.25%	0.117%
85	17.586	2461	2465	2467	rBV5	4642	6759	0.23%	0.021%
86	17.633	2470	2473	2479	rVV8	7485	15227	0.51%	0.048%
87	17.798	2499	2501	2506	rVB6	5921	8117	0.27%	0.025%
88	18.110	2548	2554	2558	rBV2	106036	174717	5.85%	0.548%
89	18.186	2564	2567	2570	rVB	13814	17203	0.58%	0.054%
90	18.292	2581	2585	2590	rBV4	16227	27742	0.93%	0.087%
91	18.839	2674	2678	2683	rBV5	33863	47009	1.57%	0.147%
92	19.010	2704	2707	2711	rVB3	16133	22691	0.76%	0.071%
93	19.239	2744	2746	2747	rBV2	13050	11365	0.38%	0.036%
94	19.274	2748	2752	2757	rVB	91552	127744	4.28%	0.400%
95	19.386	2767	2771	2775	rBV5	24623	39484	1.32%	0.124%
96	19.604	2803	2808	2821	rBV2	1491406	2290608	76.67%	7.179%
97	21.092	3058	3061	3066	rBV3	153909	210723	7.05%	0.660%
98	21.380	3105	3110	3115	rBV	2356139	2987046	99.97%	9.362%
99	23.521	3469	3474	3488	rVB	1045038	2413201	80.77%	7.563%
100	23.674	3494	3500	3514	rVB2	1554305	2987810	100.00%	9.364%




Sum of corrected areas: 31906130

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052721\
Data File : BM030212.D
Acq On : 27 May 2021 22:16
Operator : CG/JU
Sample : M2491-02
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JLX81

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

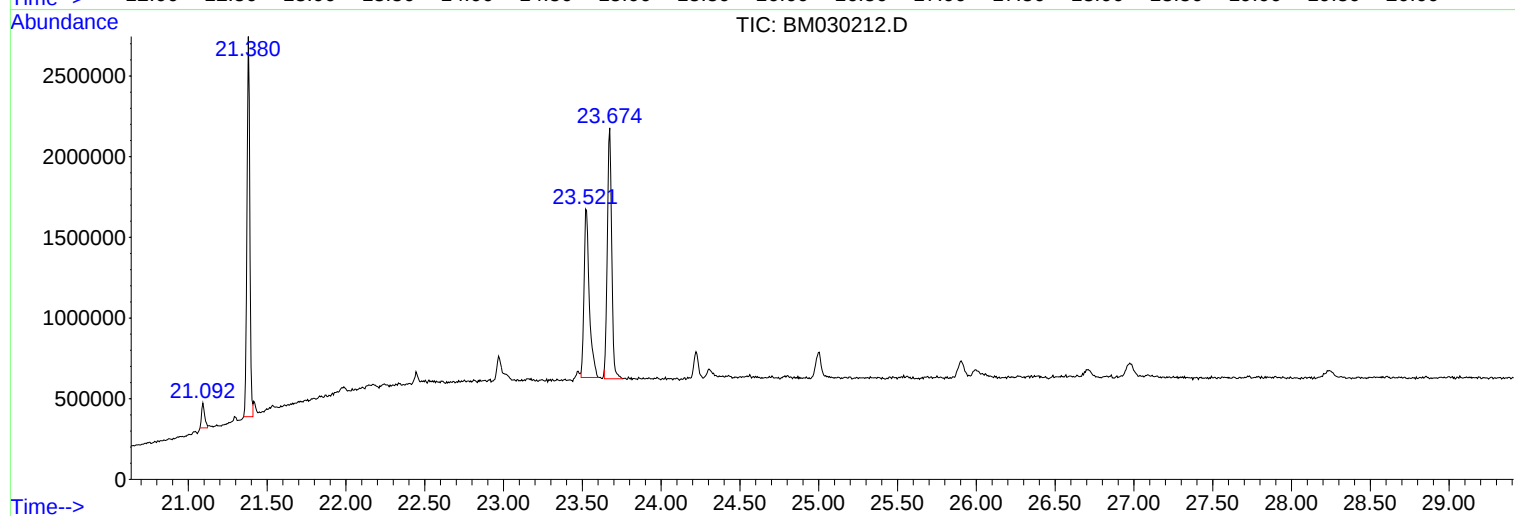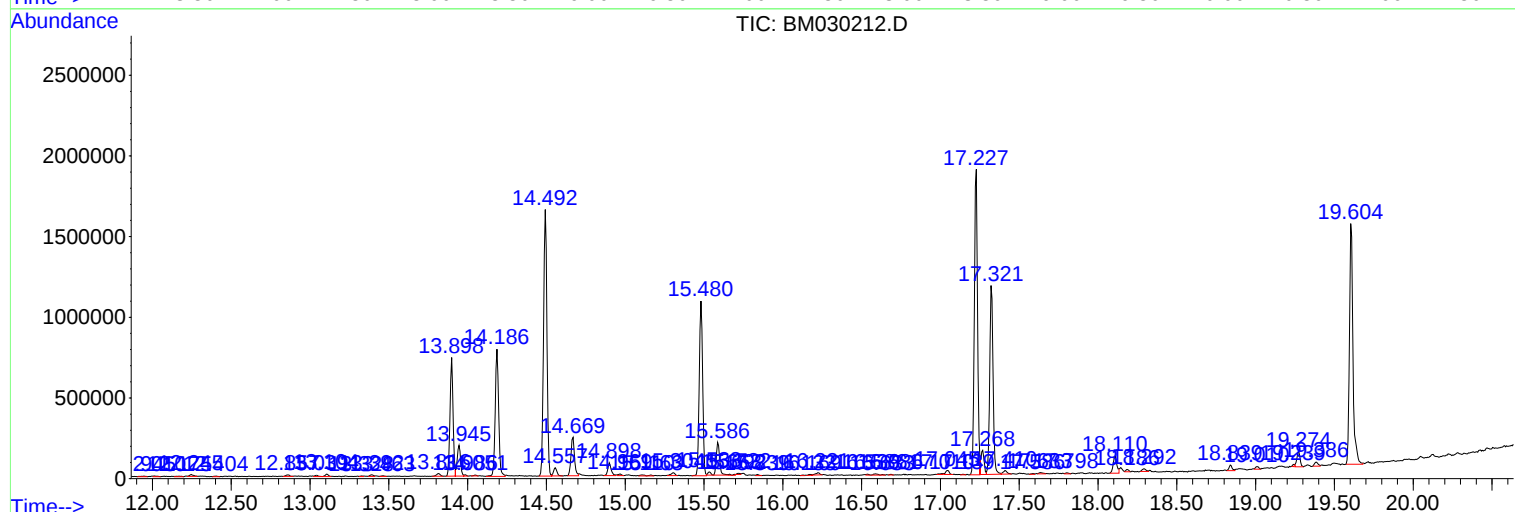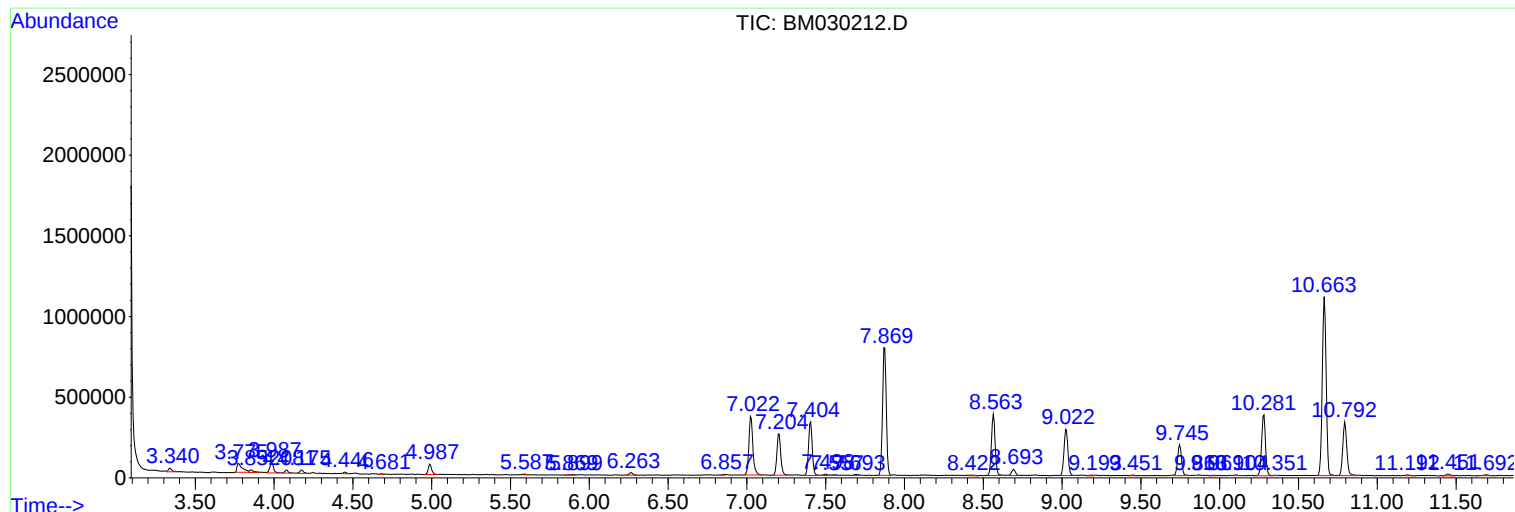

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052721\
Data File : BM030212.D
Acq On : 27 May 2021 22:16
Operator : CG/JU
Sample : M2491-02
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JLX81

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052721\
Data File : BM030212.D
Acq On : 27 May 2021 22:16
Operator : CG/JU
Sample : M2491-02
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JLX81

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
