

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052721\
 Data File : BM030221.D
 Acq On : 28 May 2021 04:53
 Operator : CG/JU
 Sample : PB136642BL
 Misc : GC/MS CONFIRMATION
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK642

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030221.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.169	11	14	17	rBV2	31648	30273	0.89%	0.169%
2	3.198	17	19	21	rVV	11924	10736	0.32%	0.060%
3	3.222	21	23	25	rVV2	18820	18333	0.54%	0.103%
4	3.257	25	29	41	rVB	1629842	1762823	51.87%	9.863%
5	3.598	83	87	93	rVB	44254	56664	1.67%	0.317%
6	4.069	163	167	172	rVB2	15902	23283	0.69%	0.130%
7	4.163	179	183	185	rVB5	3044	3602	0.11%	0.020%
8	4.998	323	325	327	rBV3	3318	3432	0.10%	0.019%
9	5.245	364	367	372	rVB7	2573	3870	0.11%	0.022%
10	7.869	806	813	821	rBV	963903	1506742	44.33%	8.430%
11	8.416	901	906	909	rBV7	2295	4097	0.12%	0.023%
12	9.639	1110	1114	1117	rVB5	2261	3753	0.11%	0.021%
13	10.663	1279	1288	1297	rVB	1176106	1993434	58.65%	11.153%
14	14.492	1932	1939	1948	rBV	1841619	2700817	79.46%	15.111%
15	15.474	2105	2106	2112	rVB6	2919	3447	0.10%	0.019%
16	17.009	2361	2367	2372	rBV2	9603	15404	0.45%	0.086%
17	17.227	2397	2404	2416	rVV	2339051	3398788	100.00%	19.016%
18	17.321	2417	2420	2424	rVB3	7412	8139	0.24%	0.046%
19	17.598	2463	2467	2468	rBV4	2724	3467	0.10%	0.019%
20	17.721	2486	2488	2491	rBV4	2638	3488	0.10%	0.020%
21	18.115	2552	2555	2556	rBV2	4606	5360	0.16%	0.030%
22	18.409	2603	2605	2608	rBV4	3782	4277	0.13%	0.024%
23	19.533	2793	2796	2800	rBV3	46104	50673	1.49%	0.284%
24	19.644	2813	2815	2819	rVB4	13536	14371	0.42%	0.080%
25	20.574	2970	2973	2975	rBV2	43275	38936	1.15%	0.218%
26	21.380	3105	3110	3115	rBV	2673190	3279291	96.48%	18.347%
27	23.668	3493	3499	3511	rVB	1544782	2925996	86.09%	16.371%

Sum of corrected areas: 17873496

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052721\
Data File : BM030221.D
Acq On : 28 May 2021 04:53
Operator : CG/JU
Sample : PB136642BL
Misc : GC/MS CONFIRMATION
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK642










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.260	23.40 ng/ul	1762820	1,4-Dichlorobenzene-d4	7.869

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Heptane			100	C7H16	000142-82-5	95
2	Heptane			100	C7H16	000142-82-5	94
3	Heptane			100	C7H16	000142-82-5	91
4	Heptane			100	C7H16	000142-82-5	80
5	Oxalic acid, isobutyl pentyl ester			216	C11H20O4	1000309-37-0	59

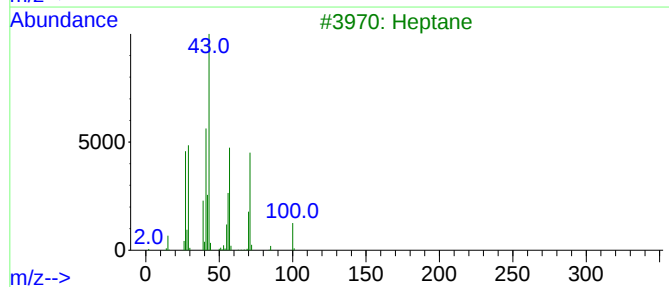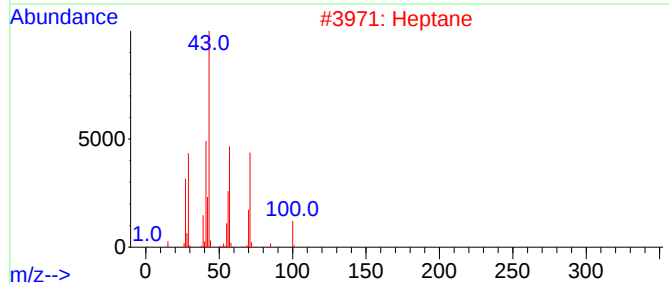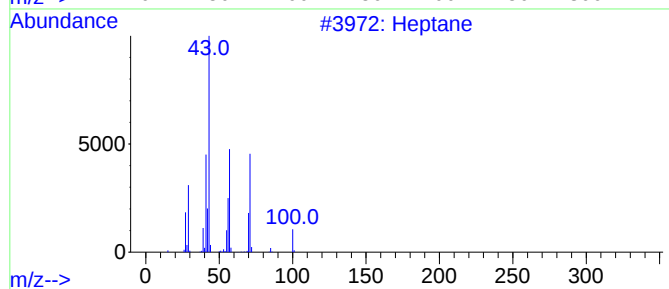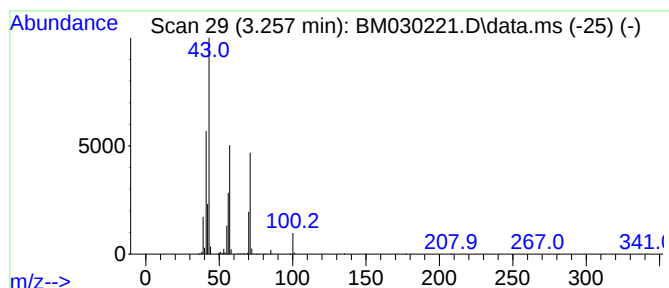

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052721\
Data File : BM030221.D
Acq On : 28 May 2021 04:53
Operator : CG/JU
Sample : PB136642BL
Misc : GC/MS CONFIRMATION
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK642

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	3.260	23.4	ng/ul	1762820	1	7.869	1506740	20.0