

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052721\
 Data File : BM030222.D
 Acq On : 28 May 2021 05:29
 Operator : CG/JU
 Sample : M2511-01
 Misc : GC/MS CONFIRMATION
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0CL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030222.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	11	15	17	rBV	59463	62608	1.47%	0.303%
2	3.205	17	20	21	rVV	25698	27650	0.65%	0.134%
3	3.228	21	24	26	rVV	41781	46050	1.08%	0.223%
4	3.263	26	30	39	rVB	4209783	4270805	100.00%	20.683%
5	3.575	79	83	84	rBV4	11651	15047	0.35%	0.073%
6	3.605	84	88	94	rVB	114160	141101	3.30%	0.683%
7	3.693	100	103	109	rVB4	8582	11115	0.26%	0.054%
8	3.940	140	145	147	rBV5	3263	4536	0.11%	0.022%
9	3.981	148	152	155	rVV6	4056	6269	0.15%	0.030%
10	4.075	164	168	171	rBV2	17796	21912	0.51%	0.106%
11	4.257	196	199	202	rVB5	4598	4546	0.11%	0.022%
12	4.516	239	243	249	rVB2	11902	18464	0.43%	0.089%
13	4.969	317	320	324	rBV6	2883	4802	0.11%	0.023%
14	7.869	806	813	822	rVB	944593	1482493	34.71%	7.179%
15	10.445	1246	1251	1256	rVB7	6120	11399	0.27%	0.055%
16	10.663	1275	1288	1296	rBV	1157188	2012781	47.13%	9.747%
17	10.804	1306	1312	1319	rVB9	7341	17753	0.42%	0.086%
18	10.922	1328	1332	1336	rVB5	4487	7626	0.18%	0.037%
19	11.016	1346	1348	1353	rVB4	3122	4473	0.10%	0.022%
20	11.086	1353	1360	1362	rBV5	3530	7114	0.17%	0.034%
21	11.139	1362	1369	1374	rBV9	6425	11901	0.28%	0.058%
22	14.492	1931	1939	1948	rBV	1782094	2644676	61.92%	12.808%
23	17.015	2363	2368	2371	rBV3	7567	10498	0.25%	0.051%
24	17.221	2397	2403	2413	rBV	2106168	3066042	71.79%	14.848%
25	17.321	2417	2420	2425	rVB3	7001	10204	0.24%	0.049%
26	18.109	2549	2554	2560	rBV9	14664	29149	0.68%	0.141%
27	18.292	2580	2585	2589	rVB	64023	86995	2.04%	0.421%
28	18.351	2591	2595	2600	rVB5	15325	19928	0.47%	0.097%
29	18.574	2629	2633	2638	rBV4	28628	34352	0.80%	0.166%
30	18.745	2660	2662	2667	rVB5	9219	9563	0.22%	0.046%
31	19.056	2712	2715	2718	rVB4	12085	15385	0.36%	0.075%
32	19.104	2718	2723	2724	rBV4	28954	36290	0.85%	0.176%
33	19.133	2725	2728	2734	rVB3	106258	139346	3.26%	0.675%
34	19.221	2739	2743	2746	rBV5	13833	18511	0.43%	0.090%
35	19.339	2760	2763	2767	rBV6	21951	28605	0.67%	0.139%
36	19.415	2771	2776	2781	rVV2	156172	215568	5.05%	1.044%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052721\
 Data File : BM030222.D
 Acq On : 28 May 2021 05:29
 Operator : CG/JU
 Sample : M2511-01
 Misc : GC/MS CONFIRMATION
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0CL2

Integration Parameters: LSCINT.P
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
 Title : SVOA CALIBRATION

37	19.480	2783	2787	2791	rBV5	52406	69773	1.63%	0.338%
38	19.674	2816	2820	2824	rBV4	42908	53075	1.24%	0.257%
39	19.751	2829	2833	2837	rVB2	67526	83277	1.95%	0.403%
40	19.803	2839	2842	2845	rVV3	20276	24359	0.57%	0.118%
41	19.856	2847	2851	2856	rVB	151093	190972	4.47%	0.925%
42	20.121	2892	2896	2900	rBV4	62760	83390	1.95%	0.404%
43	20.168	2900	2904	2911	rVV2	133420	155945	3.65%	0.755%
44	20.392	2939	2942	2948	rBV2	81185	96772	2.27%	0.469%
45	20.450	2949	2952	2953	rVV	37103	41203	0.96%	0.200%
46	20.474	2954	2956	2960	rVB2	53823	51091	1.20%	0.247%
47	20.686	2989	2992	2993	rBV2	40074	45719	1.07%	0.221%
48	20.709	2993	2996	3002	rVB3	89580	130443	3.05%	0.632%
49	21.380	3105	3110	3118	rBV	2110303	2659305	62.27%	12.878%
50	23.668	3493	3499	3508	rVB2	1265225	2408393	56.39%	11.663%

Sum of corrected areas: 20649274

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052721\
Data File : BM030222.D
Acq On : 28 May 2021 05:29
Operator : CG/JU
Sample : M2511-01
Misc : GC/MS CONFIRMATION
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0CL2










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.260	57.62 ng/ul	4270810	1,4-Dichlorobenzene-d4	7.869

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Heptane			100	C7H16	000142-82-5	95
2	Heptane			100	C7H16	000142-82-5	94
3	Heptane			100	C7H16	000142-82-5	91
4	Heptane			100	C7H16	000142-82-5	90
5	Hexane, 3-methyl-			100	C7H16	000589-34-4	45

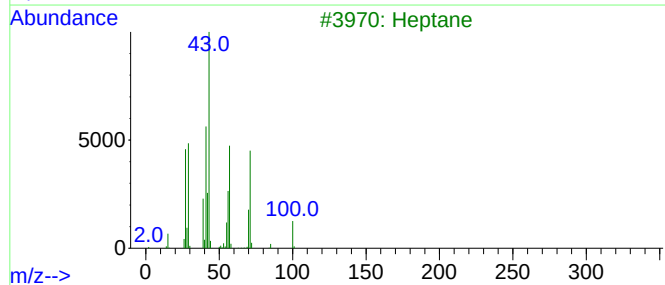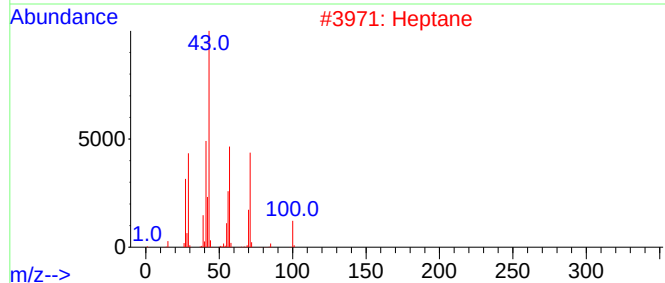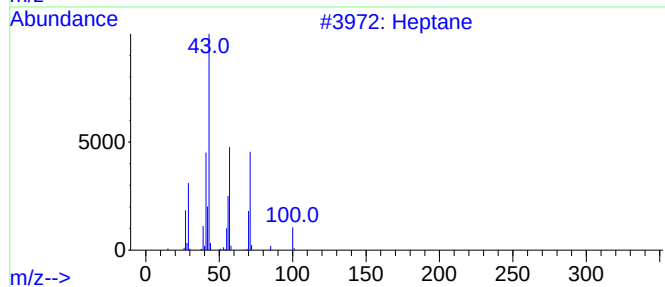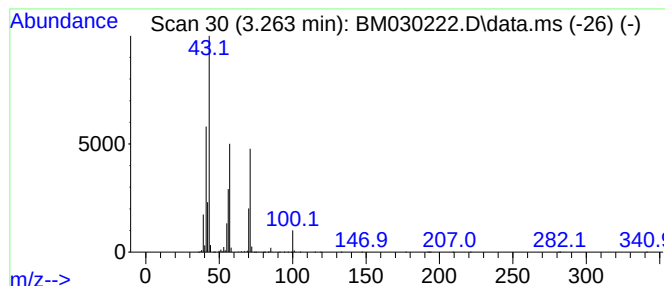

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052721\
Data File : BM030222.D
Acq On : 28 May 2021 05:29
Operator : CG/JU
Sample : M2511-01
Misc : GC/MS CONFIRMATION
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0CL2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	3.260	57.6	ng/ul	4270810	1	7.869	1482490	20.0