

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052721\
 Data File : BM030225.D
 Acq On : 28 May 2021 07:18
 Operator : CG/JU
 Sample : M2511-11
 Misc : GC/MS CONFIRMATION
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0CM0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
 Title : SVOA CALIBRATION

Signal : TIC: BM030225.D

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.175	11	15	18	rBV	70032	73715	1.52%	0.354%
2	3.204	18	20	22	rVV	28213	28977	0.60%	0.139%
3	3.228	22	24	26	rVV	43883	41133	0.85%	0.198%
4	3.263	26	30	35	rVB	4790527	4860528	100.00%	23.373%
5	3.575	79	83	84	rBV4	15113	18223	0.37%	0.088%
6	3.604	84	88	93	rVB	122977	149074	3.07%	0.717%
7	3.698	100	104	106	rVB4	7975	9204	0.19%	0.044%
8	4.075	164	168	173	rVB	18359	23889	0.49%	0.115%
9	4.516	237	243	252	rVB	50797	74278	1.53%	0.357%
10	7.010	663	667	671	rVB3	6918	11825	0.24%	0.057%
11	7.869	805	813	822	rVB	967565	1512484	31.12%	7.273%
12	10.439	1247	1250	1256	rVB7	3742	5993	0.12%	0.029%
13	10.663	1276	1288	1297	rVB	1133505	1976619	40.67%	9.505%
14	10.922	1327	1332	1335	rBV7	4537	7530	0.15%	0.036%
15	11.133	1363	1368	1375	rVB7	5283	10718	0.22%	0.052%
16	12.992	1681	1684	1688	rBV6	6546	9087	0.19%	0.044%
17	13.227	1717	1724	1726	rBV6	3909	5457	0.11%	0.026%
18	13.974	1846	1851	1854	rBV3	6706	9507	0.20%	0.046%
19	14.110	1870	1874	1879	rVB4	6264	9612	0.20%	0.046%
20	14.492	1932	1939	1946	rBV	1735600	2518956	51.82%	12.113%
21	14.809	1990	1993	2000	rVB6	3571	5701	0.12%	0.027%
22	16.198	2226	2229	2234	rVB6	3255	5211	0.11%	0.025%
23	17.009	2359	2367	2371	rBV5	8542	21676	0.45%	0.104%
24	17.221	2397	2403	2410	rBV	1891250	2744381	56.46%	13.197%
25	17.321	2417	2420	2425	rVB5	6075	9047	0.19%	0.044%
26	17.821	2503	2505	2509	rVB4	6147	7294	0.15%	0.035%
27	17.892	2514	2517	2522	rBV7	4617	5952	0.12%	0.029%
28	18.109	2551	2554	2561	rBV7	10414	17942	0.37%	0.086%
29	18.292	2581	2585	2589	rBV2	45214	61182	1.26%	0.294%
30	18.350	2591	2595	2598	rVV5	10721	12375	0.25%	0.060%
31	18.415	2601	2606	2614	rBV8	10221	24419	0.50%	0.117%
32	18.574	2629	2633	2638	rBV7	22706	29248	0.60%	0.141%
33	19.044	2711	2713	2717	rVB5	7962	10116	0.21%	0.049%
34	19.103	2720	2723	2725	rVV3	28227	38254	0.79%	0.184%
35	19.133	2725	2728	2734	rVB3	80485	112598	2.32%	0.541%
36	19.215	2740	2742	2745	rBV3	9428	9792	0.20%	0.047%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052721\
 Data File : BM030225.D
 Acq On : 28 May 2021 07:18
 Operator : CG/JU
 Sample : M2511-11
 Misc : GC/MS CONFIRMATION
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0CM0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
 Title : SVOA CALIBRATION

37	19.339	2760	2763	2766	rBV6	18788	26977	0.56%	0.130%
38	19.415	2772	2776	2781	rVB	130167	168392	3.46%	0.810%
39	19.480	2783	2787	2791	rVB3	46106	55795	1.15%	0.268%
40	19.533	2792	2796	2802	rBV	108586	129256	2.66%	0.622%
41	19.615	2807	2810	2813	rVV2	25658	31872	0.66%	0.153%
42	19.650	2813	2816	2818	rVV2	25168	30605	0.63%	0.147%
43	19.674	2818	2820	2825	rVB5	33961	40242	0.83%	0.194%
44	19.750	2829	2833	2838	rBV2	59364	77713	1.60%	0.374%
45	19.856	2847	2851	2857	rVB2	136376	169493	3.49%	0.815%
46	20.121	2892	2896	2899	rBV5	59349	84999	1.75%	0.409%
47	20.168	2901	2904	2909	rVB	122985	144265	2.97%	0.694%
48	20.397	2939	2943	2947	rBV2	66179	88253	1.82%	0.424%
49	20.450	2949	2952	2954	rBV3	37098	54745	1.13%	0.263%
50	20.574	2970	2973	2977	rVB	82109	83566	1.72%	0.402%
51	20.639	2981	2984	2988	rVB2	54605	61095	1.26%	0.294%
52	20.709	2993	2996	3002	rVB5	84706	119590	2.46%	0.575%
53	21.097	3059	3062	3065	rBV	63686	72106	1.48%	0.347%
54	21.380	3105	3110	3121	rBV	1997097	2511885	51.68%	12.079%
55	23.668	3493	3499	3509	rVB2	1257189	2372836	48.82%	11.410%




Sum of corrected areas: 20795682

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052721\
Data File : BM030225.D
Acq On : 28 May 2021 07:18
Operator : CG/JU
Sample : M2511-11
Misc : GC/MS CONFIRMATION
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0C00

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

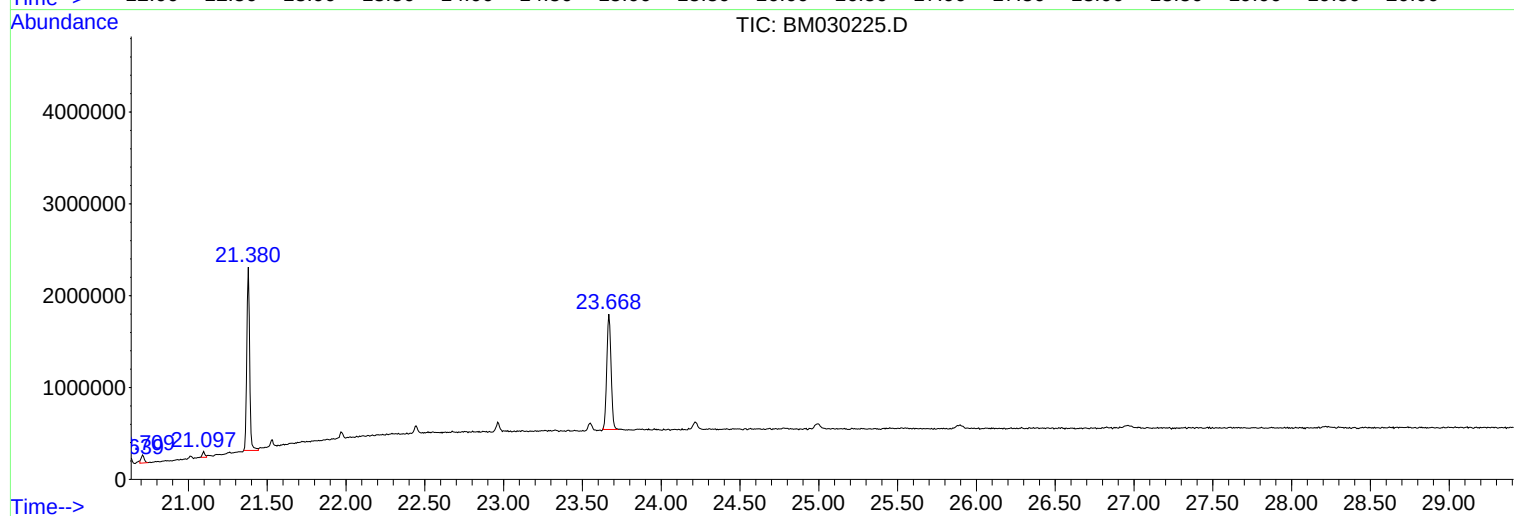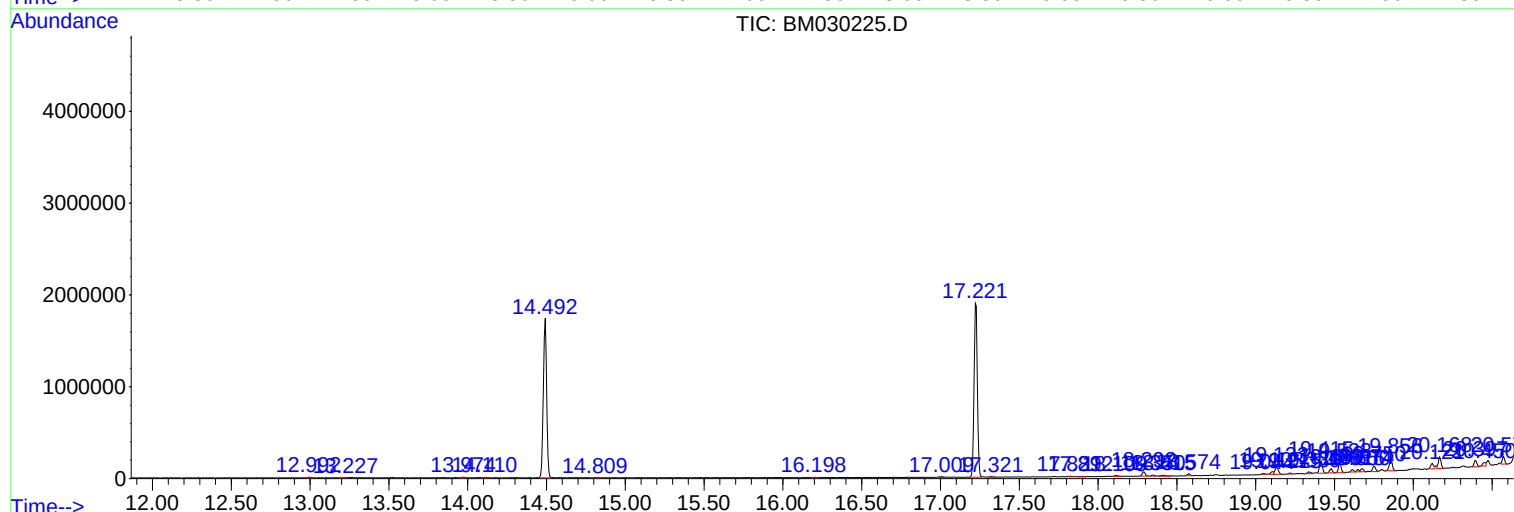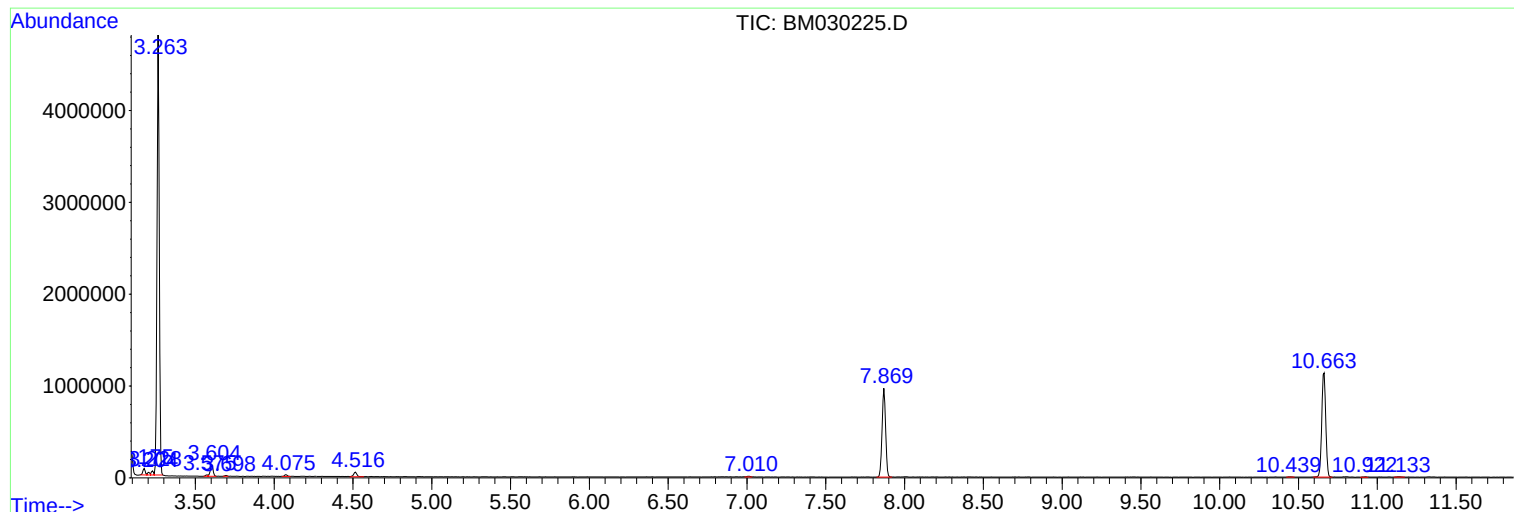

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052721\
Data File : BM030225.D
Acq On : 28 May 2021 07:18
Operator : CG/JU
Sample : M2511-11
Misc : GC/MS CONFIRMATION
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0CM0










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.260	64.27 ng/ul	4860530	1,4-Dichlorobenzene-d4	7.869

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Heptane			100	C7H16	000142-82-5	95
2	Heptane			100	C7H16	000142-82-5	94
3	Heptane			100	C7H16	000142-82-5	91
4	Heptane			100	C7H16	000142-82-5	90
5	Hexane, 3-methyl-			100	C7H16	000589-34-4	42

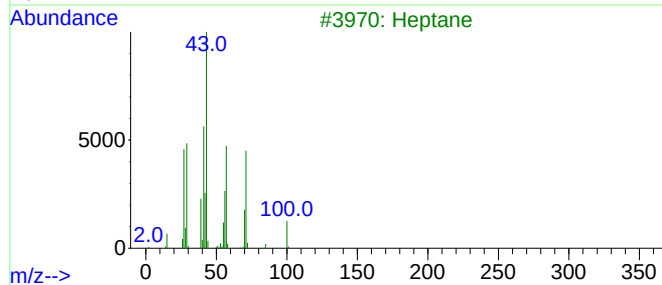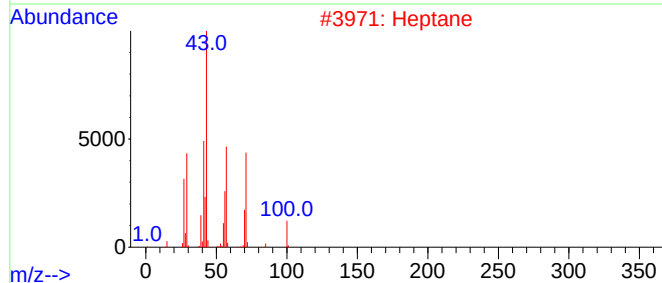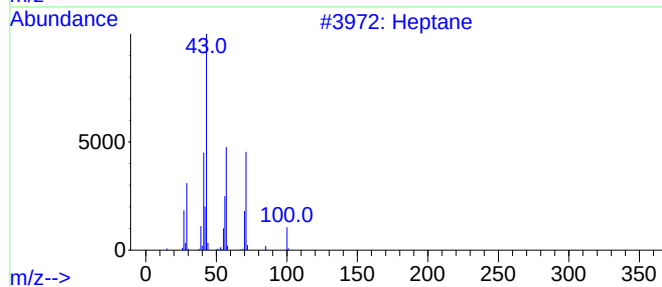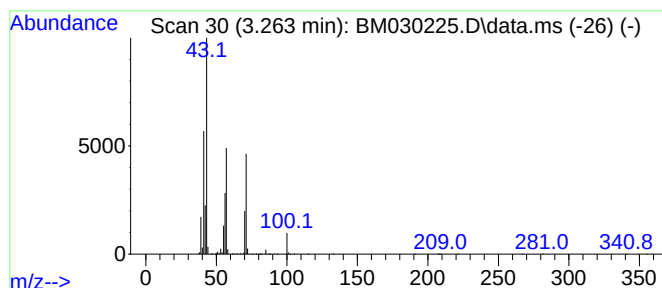

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM052721\
Data File : BM030225.D
Acq On : 28 May 2021 07:18
Operator : CG/JU
Sample : M2511-11
Misc : GC/MS CONFIRMATION
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0CM0

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM052621.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	3.260	64.3	ng/ul	4860530	1	7.869	1512480	20.0