

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060322\
 Data File : BM035388.D
 Acq On : 03 Jun 2022 10:41
 Operator : CG/JU
 Sample : PB145235BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB145235BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM035388.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.434	392	399	419	rBV	2850550	4184454	25.45%	7.048%
2	7.034	662	671	691	rBV	2727065	4447292	27.04%	7.491%
3	7.845	803	809	823	rVB	543316	878726	5.34%	1.480%
4	9.010	998	1007	1023	rBV	1729621	2942033	17.89%	4.955%
5	10.645	1278	1285	1306	rBV	763463	1342147	8.16%	2.261%
6	13.116	1697	1705	1722	rBV	6214112	9308708	56.61%	15.679%
7	14.486	1931	1938	1956	rBV	1484505	2262637	13.76%	3.811%
8	15.980	2185	2192	2218	rBV	5528808	8376149	50.94%	14.108%
9	17.233	2399	2405	2417	rBV	2012902	3028301	18.42%	5.101%
10	19.862	2846	2852	2857	rBV	12875051	16444655	100.00%	27.698%
11	21.415	3111	3116	3126	rBV	2410236	3340146	20.31%	5.626%
12	23.774	3511	3517	3530	rVB2	1357421	2815909	17.12%	4.743%




Sum of corrected areas: 59371157

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060322\
Data File : BM035388.D
Acq On : 03 Jun 2022 10:41
Operator : CG/JU
Sample : PB145235BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145235BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

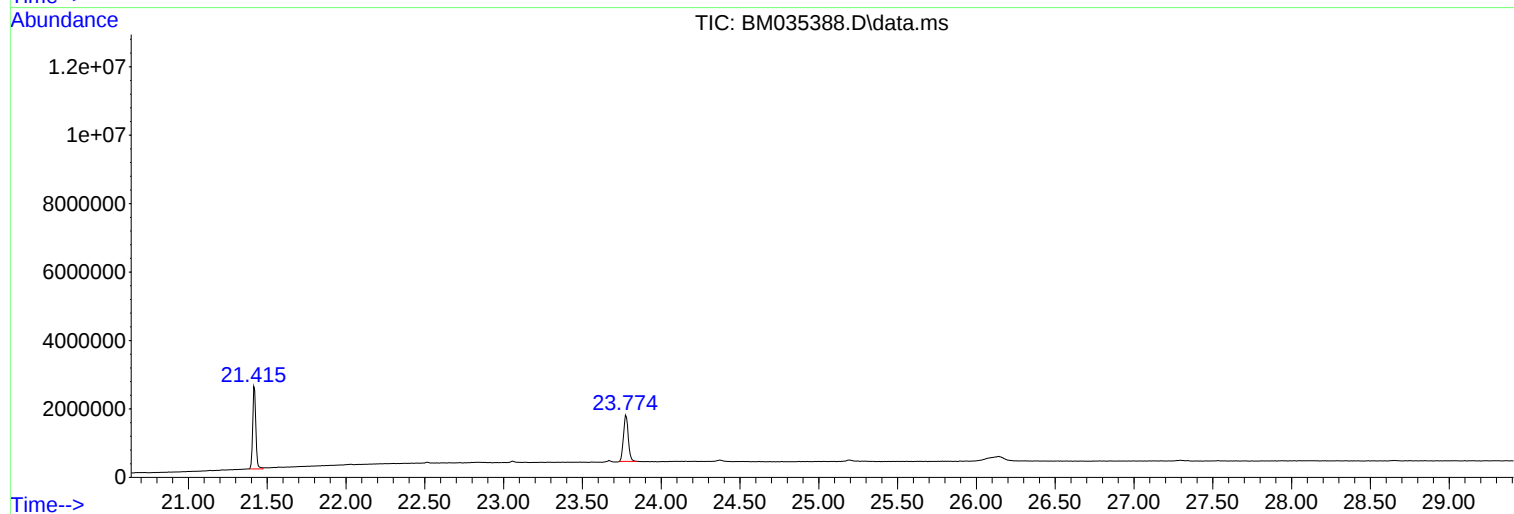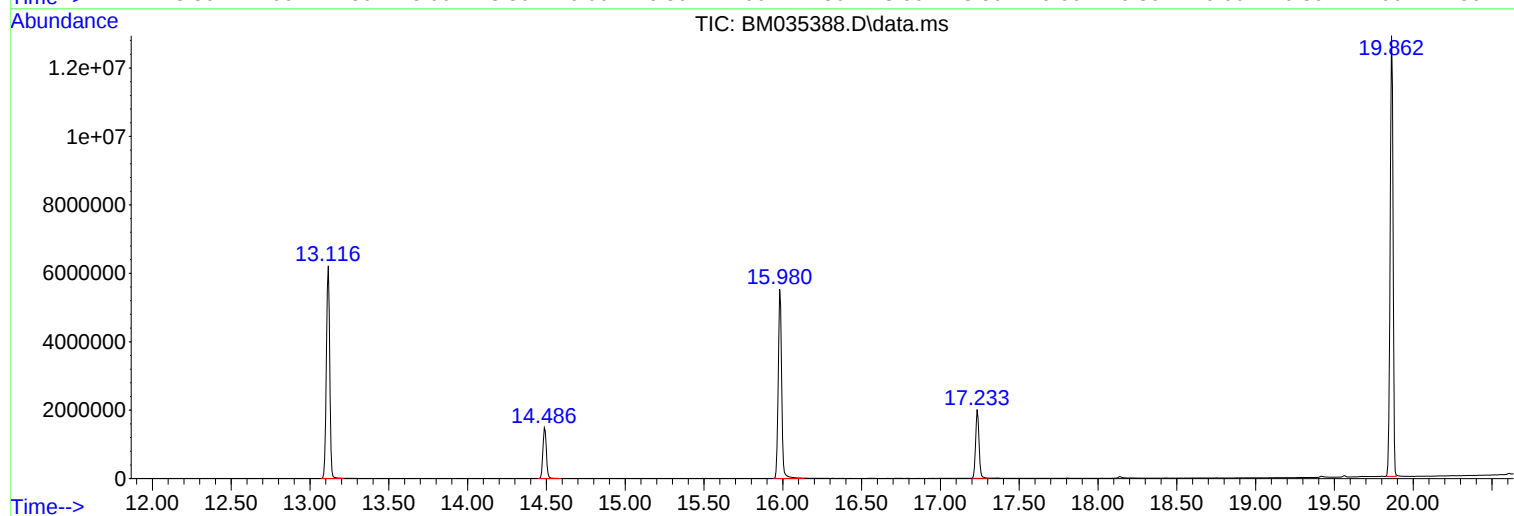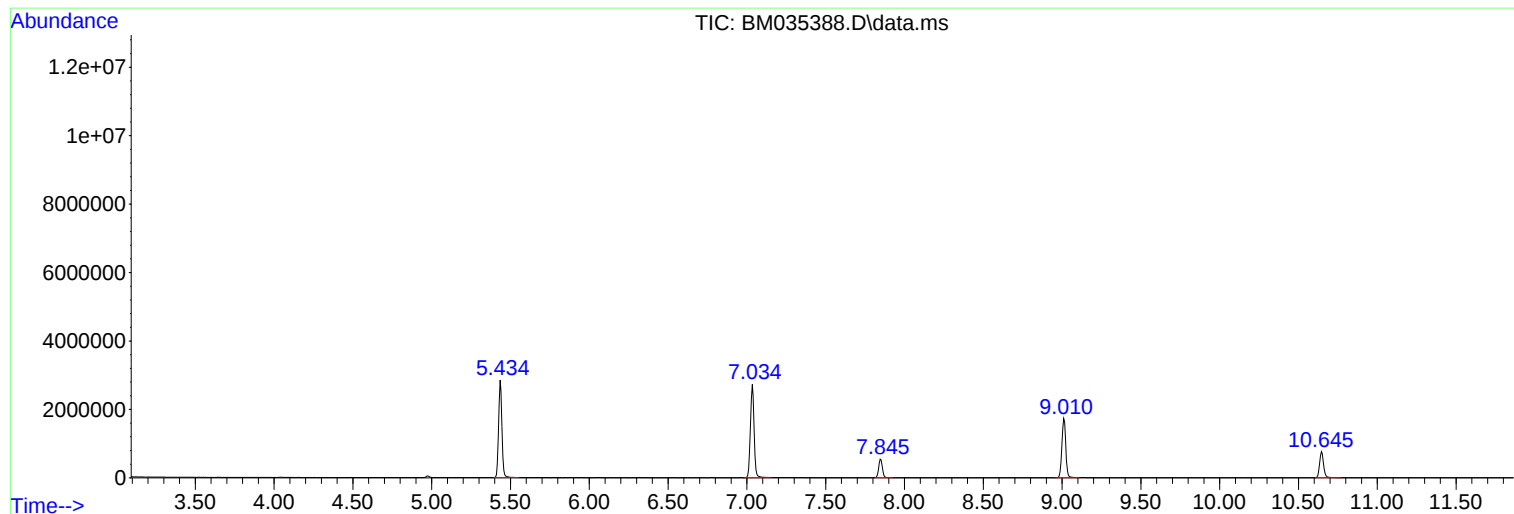

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060322\
Data File : BM035388.D
Acq On : 03 Jun 2022 10:41
Operator : CG/JU
Sample : PB145235BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145235BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060322\
Data File : BM035388.D
Acq On : 03 Jun 2022 10:41
Operator : CG/JU
Sample : PB145235BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145235BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------