

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060322\
 Data File : BM035405.D
 Acq On : 03 Jun 2022 21:14
 Operator : CG/JU
 Sample : N3179-01 10X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 TR-4-060222

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM035405.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.440	394	400	406	rBV	242700	394782	6.24%	1.594%
2	5.493	406	409	419	rVB	31000	66944	1.06%	0.270%
3	7.040	661	672	687	rBV	192947	419247	6.63%	1.692%
4	7.851	803	810	825	rBV	658262	1085104	17.16%	4.380%
5	9.016	1002	1008	1019	rBV	121970	240452	3.80%	0.971%
6	10.645	1275	1285	1303	rBV	805629	1469026	23.24%	5.930%
7	13.116	1696	1705	1715	rBV	455454	711084	11.25%	2.871%
8	14.216	1885	1892	1899	rBV	39677	76093	1.20%	0.307%
9	14.492	1928	1939	1946	rBV	1277782	1931728	30.55%	7.798%
10	15.986	2187	2193	2199	rBV	325722	504919	7.99%	2.038%
11	16.210	2226	2231	2240	rBV9	27065	67164	1.06%	0.271%
12	17.233	2399	2405	2410	rBV	1483889	2197574	34.76%	8.871%
13	17.280	2410	2413	2420	rVB	138716	196629	3.11%	0.794%
14	17.374	2425	2429	2433	rVB	59402	87496	1.38%	0.353%
15	17.915	2516	2521	2526	rBV	373232	466084	7.37%	1.882%
16	18.139	2556	2559	2562	rBV3	55863	79155	1.25%	0.320%
17	18.304	2584	2587	2592	rBV2	62713	115672	1.83%	0.467%
18	19.056	2708	2715	2718	rBV	1871516	2396501	37.90%	9.674%
19	19.086	2718	2720	2725	rVB2	1042076	1170709	18.52%	4.726%
20	19.221	2739	2743	2749	rVB2	267583	313563	4.96%	1.266%
21	19.298	2752	2756	2764	rVB	268139	381365	6.03%	1.540%
22	19.656	2813	2817	2827	rVB	321668	536960	8.49%	2.168%
23	19.862	2847	2852	2856	rBV	766955	1015450	16.06%	4.099%
24	21.421	3113	3117	3120	rBV	1977437	2525234	39.94%	10.194%
25	23.780	3514	3518	3542	rVB3	1988150	6322454	100.00%	25.523%




Sum of corrected areas: 24771389

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060322\
Data File : BM035405.D
Acq On : 03 Jun 2022 21:14
Operator : CG/JU
Sample : N3179-01 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TR-4-060222

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

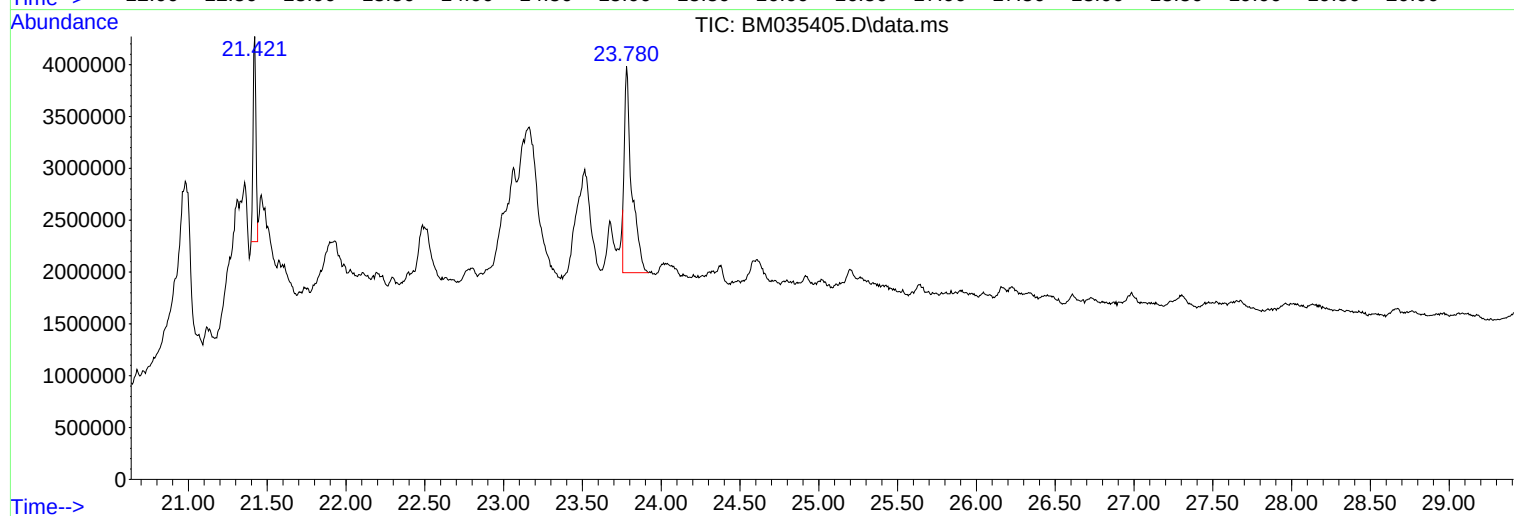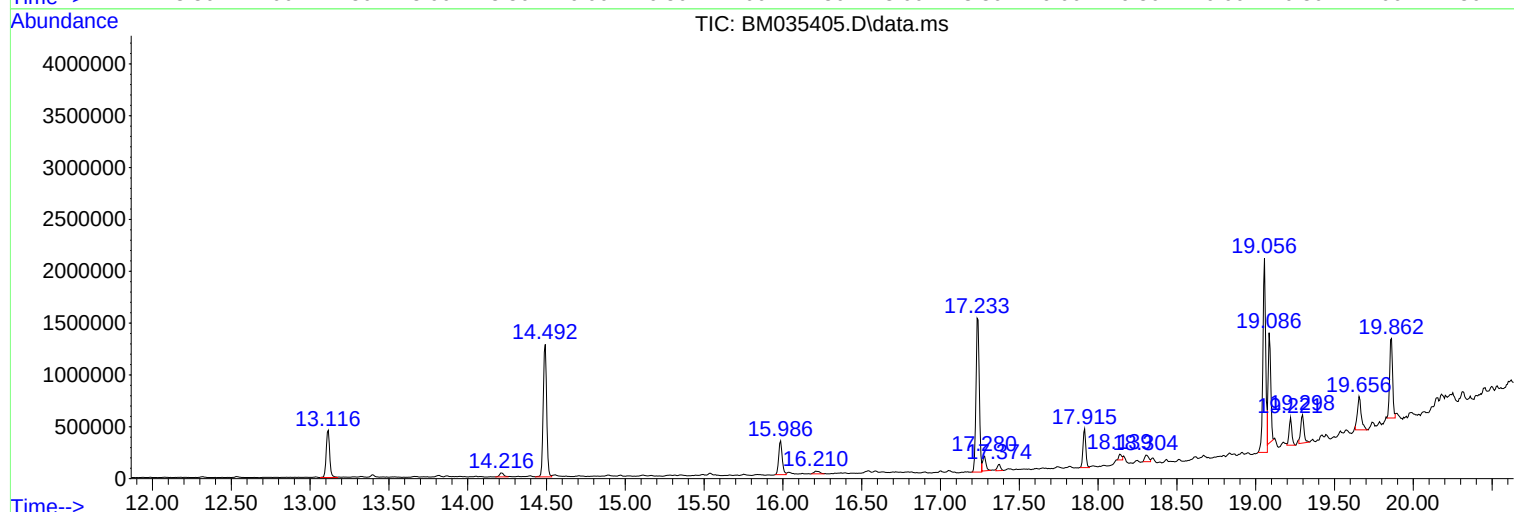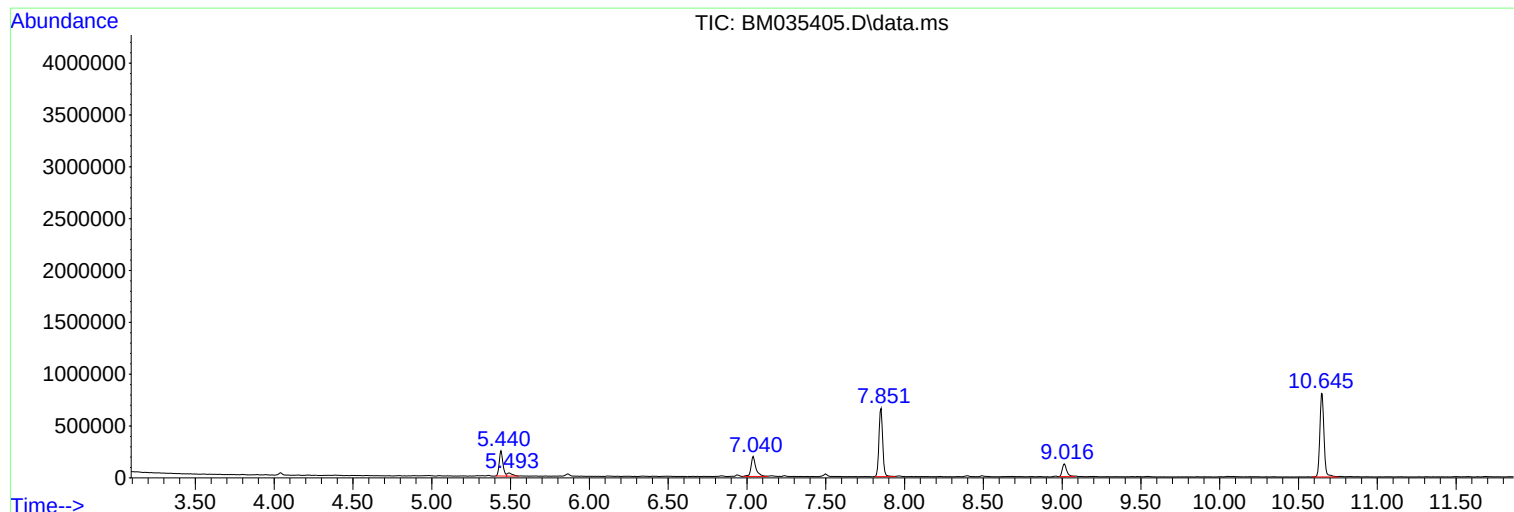

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060322\
Data File : BM035405.D
Acq On : 03 Jun 2022 21:14
Operator : CG/JU
Sample : N3179-01 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TR-4-060222

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060322\
Data File : BM035405.D
Acq On : 03 Jun 2022 21:14
Operator : CG/JU
Sample : N3179-01 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
TR-4-060222

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------