
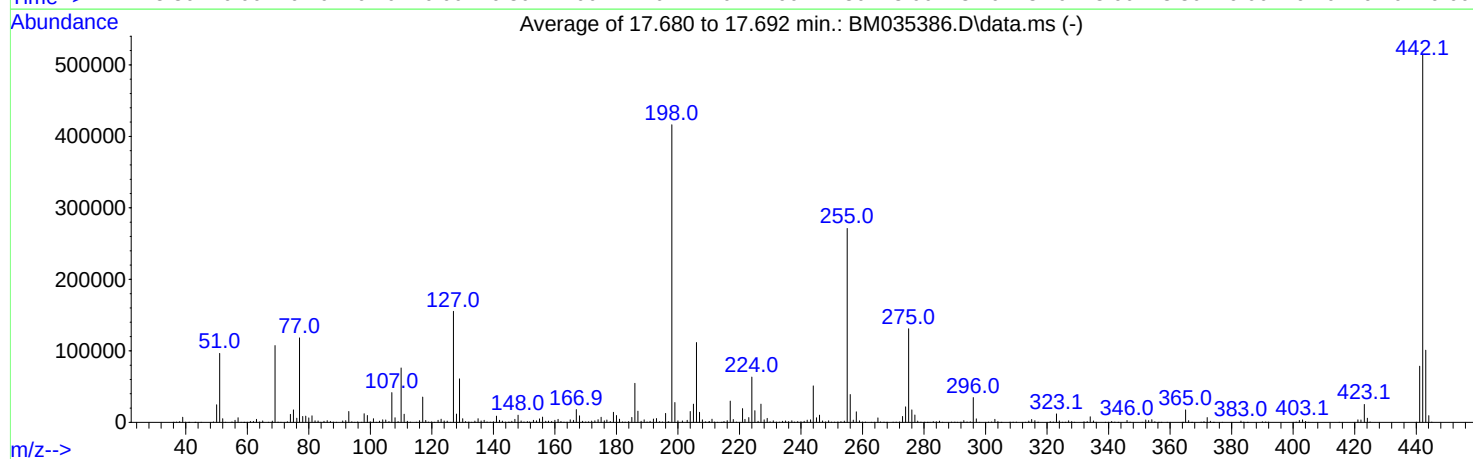


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060322\
 Data File : BM035386.D
 Acq On : 03 Jun 2022 09:28
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jun 02 16:16:23 2022

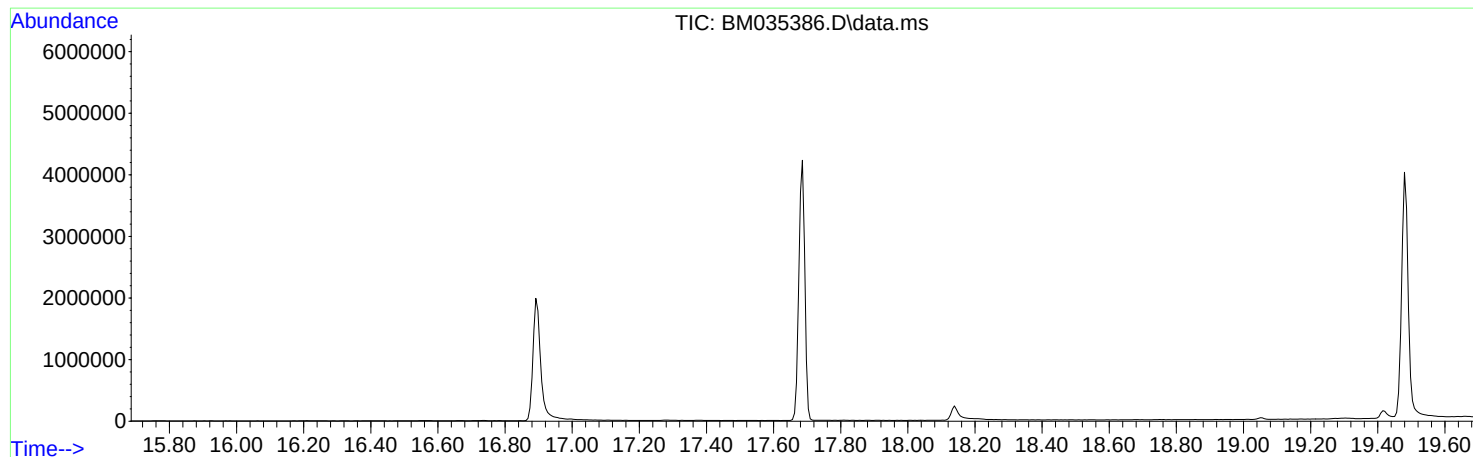




AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2474

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	23.2	96560	PASS
68	69	0.00	2	1.7	1837	PASS
69	198	0.00	100	25.8	107347	PASS
70	69	0.00	2	0.5	556	PASS
127	198	10	80	37.3	155280	PASS
197	198	0.00	2	0.2	836	PASS
198	198	100	100	100.0	416299	PASS
199	198	5	9	6.7	27728	PASS
275	198	10	60	31.4	130893	PASS
365	198	1	100	4.2	17392	PASS
441	198	0.01	100	18.9	78515	PASS
442	442	50	100	100.0	514517	PASS
443	442	15	24	19.6	100987	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060322\
 Data File : BM035386.D
 Acq On : 03 Jun 2022 09:28
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Jun 04 05:00:54 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jun 02 16:16:23 2022
 Response via : Initial Calibration

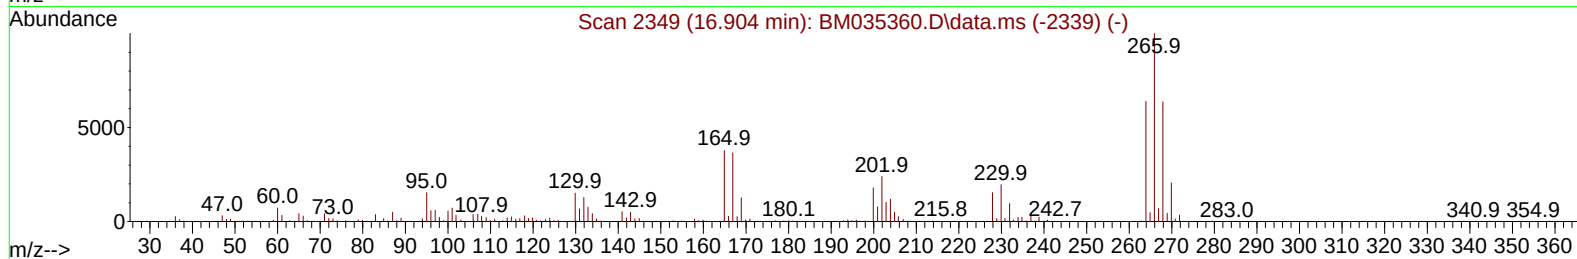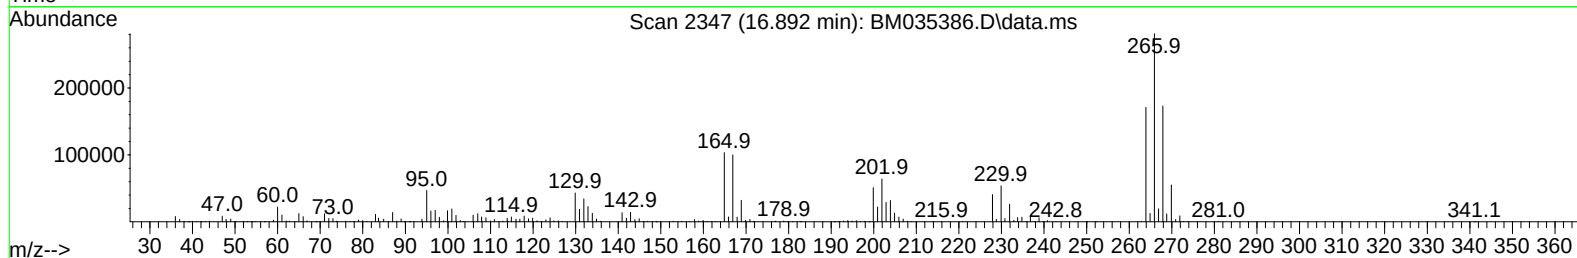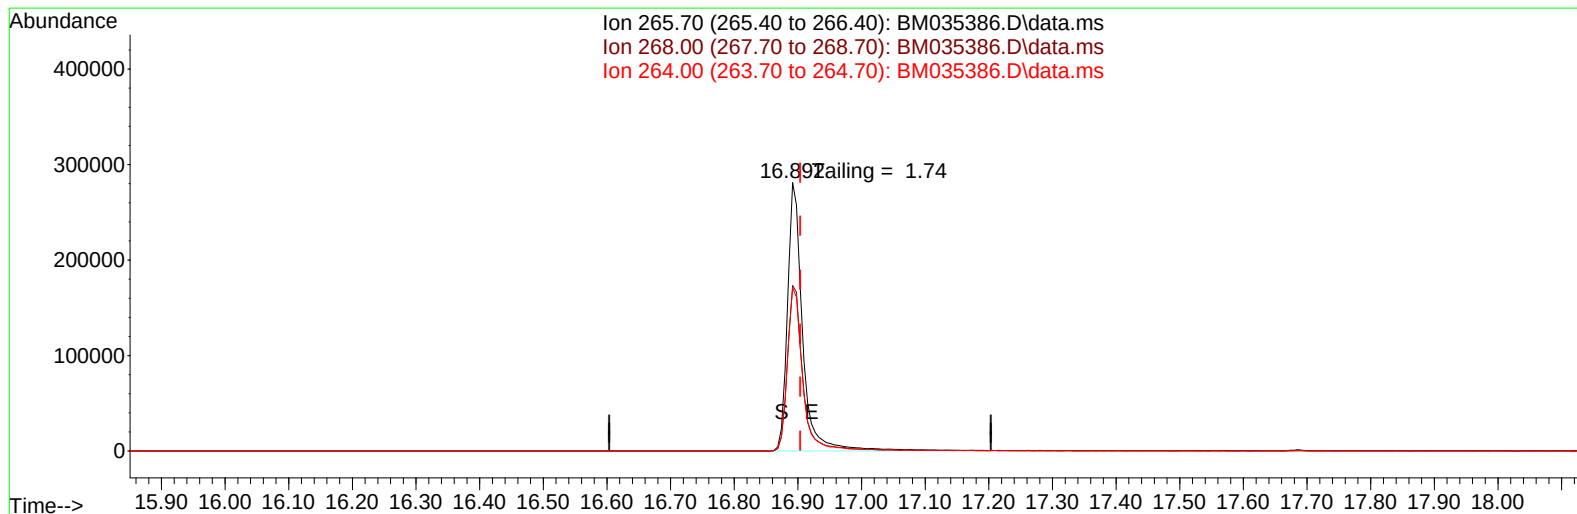

TIC: BM035386.D\data.ms

(70) Pentachlorophenol (C)

16.892min (-0.012) 0.00 ng




response 468074

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	61.68
264.00	63.30	60.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060322\
Data File : BM035386.D
Acq On : 03 Jun 2022 09:28
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jun 04 05:00:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jun 02 16:16:23 2022
Response via : Initial Calibration

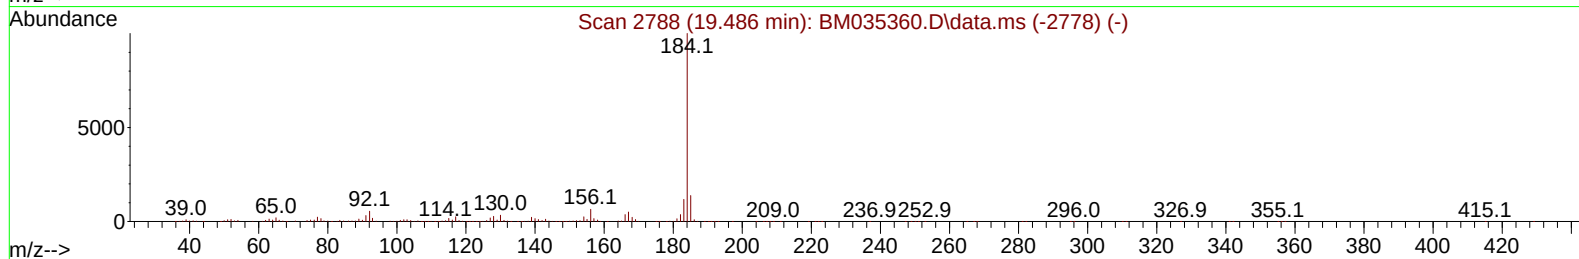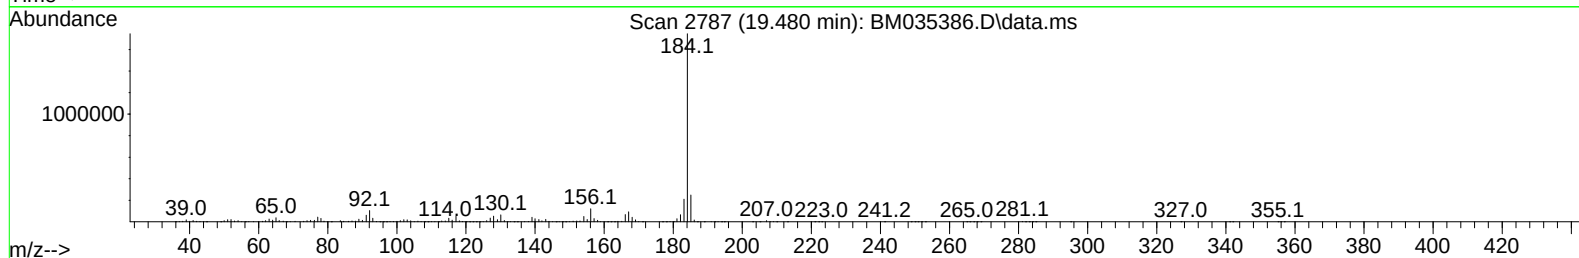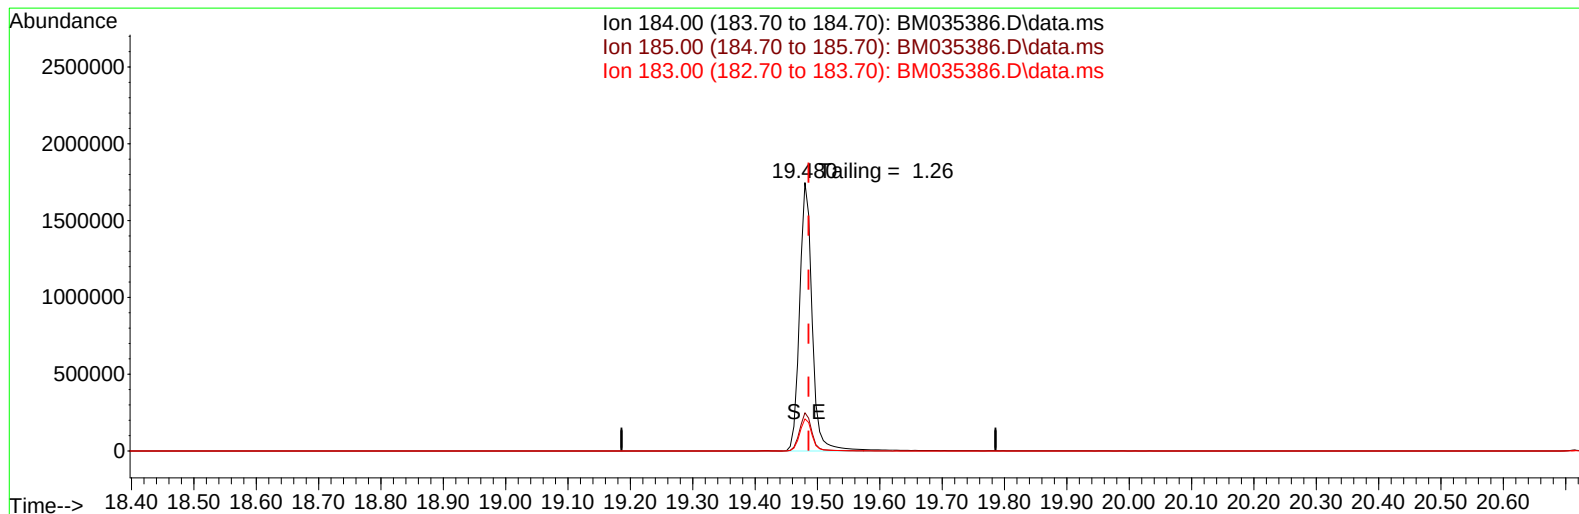

TIC: BM035386.D\data.ms

(77) Benzidine

19.480min (-0.006) 135674.63 ng

response 2472283

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.25
183.00	11.90	12.03
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/3/2022	BNA_M	<u>BM035386.D</u>
Compound Name	Response	Retention Time
DDT	1538932	20.715
DDD	13757	20.327
DDE	2320	19.768
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16077	1555009	1.03

Instrument :
BNA_M
ClientSampleId :
DFTPP