

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060722\
 Data File : BM035408.D
 Acq On : 07 Jun 2022 11:43
 Operator : CG/JU
 Sample : PB145347BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB145347BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM035408.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.428	392	398	419	rBV	2705450	4078473	32.45%	8.051%
2	7.028	663	670	697	rBV	2519739	4161842	33.11%	8.215%
3	7.839	802	808	822	rBV	596073	968547	7.71%	1.912%
4	9.004	998	1006	1022	rBV	1558561	2684439	21.36%	5.299%
5	10.639	1276	1284	1304	rBV	744374	1365691	10.87%	2.696%
6	13.110	1696	1704	1722	rBV	5481634	8203622	65.27%	16.193%
7	14.486	1931	1938	1953	rBV	1326453	2096295	16.68%	4.138%
8	15.974	2185	2191	2217	rBV	4177223	6427614	51.14%	12.688%
9	17.227	2398	2404	2422	rBV	1684255	2635596	20.97%	5.202%
10	19.856	2845	2851	2863	rBV	9983626	12568966	100.00%	24.810%
11	21.415	3111	3116	3124	rBV	2047396	2844326	22.63%	5.614%
12	23.774	3511	3517	3533	rVB2	1268230	2625534	20.89%	5.183%




Sum of corrected areas: 50660945

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060722\
Data File : BM035408.D
Acq On : 07 Jun 2022 11:43
Operator : CG/JU
Sample : PB145347BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145347BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

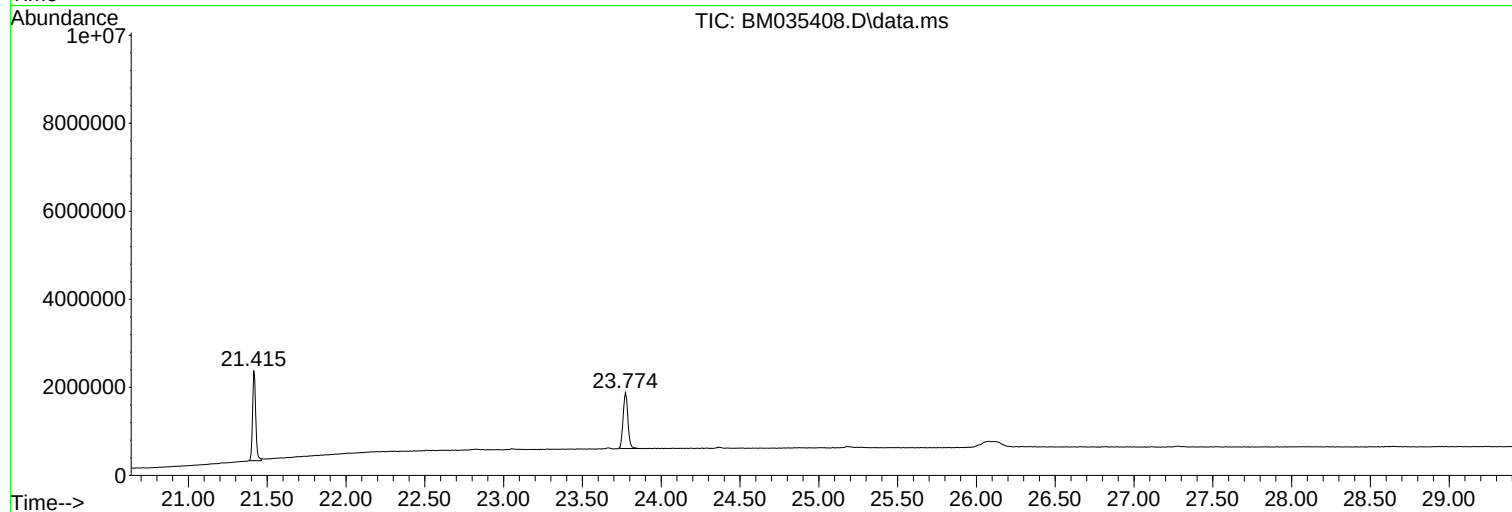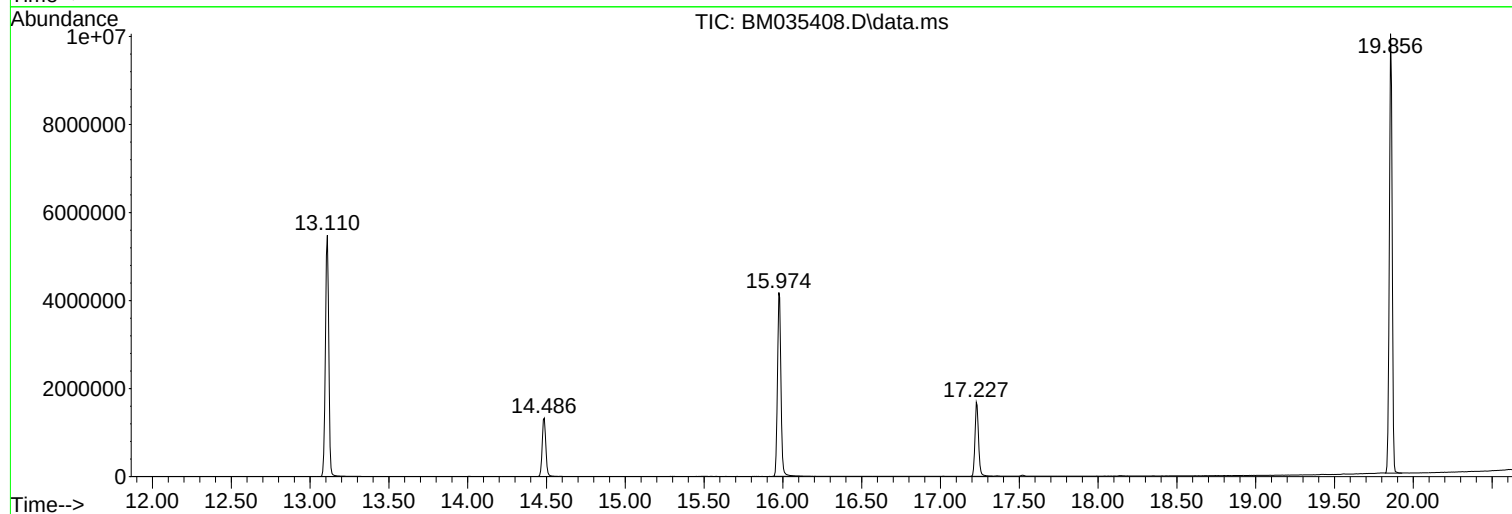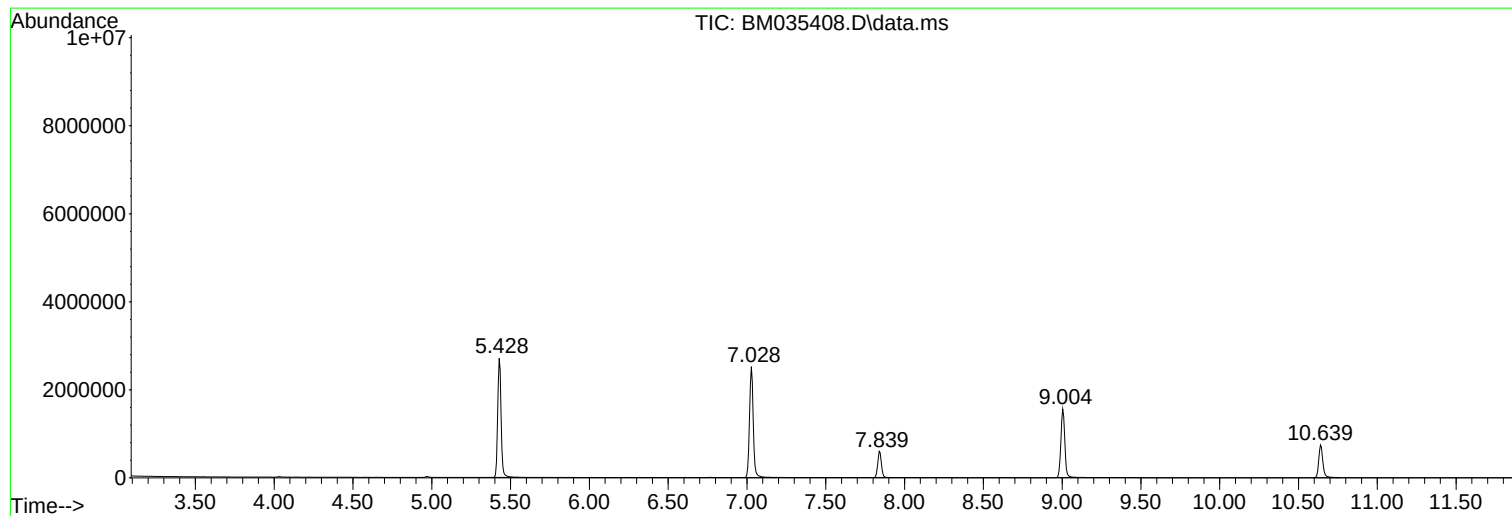

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060722\
Data File : BM035408.D
Acq On : 07 Jun 2022 11:43
Operator : CG/JU
Sample : PB145347BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145347BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060722\
Data File : BM035408.D
Acq On : 07 Jun 2022 11:43
Operator : CG/JU
Sample : PB145347BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB145347BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------