


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060722\
 Data File : BM035406.D
 Acq On : 07 Jun 2022 10:27
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 07 14:28:07 2022

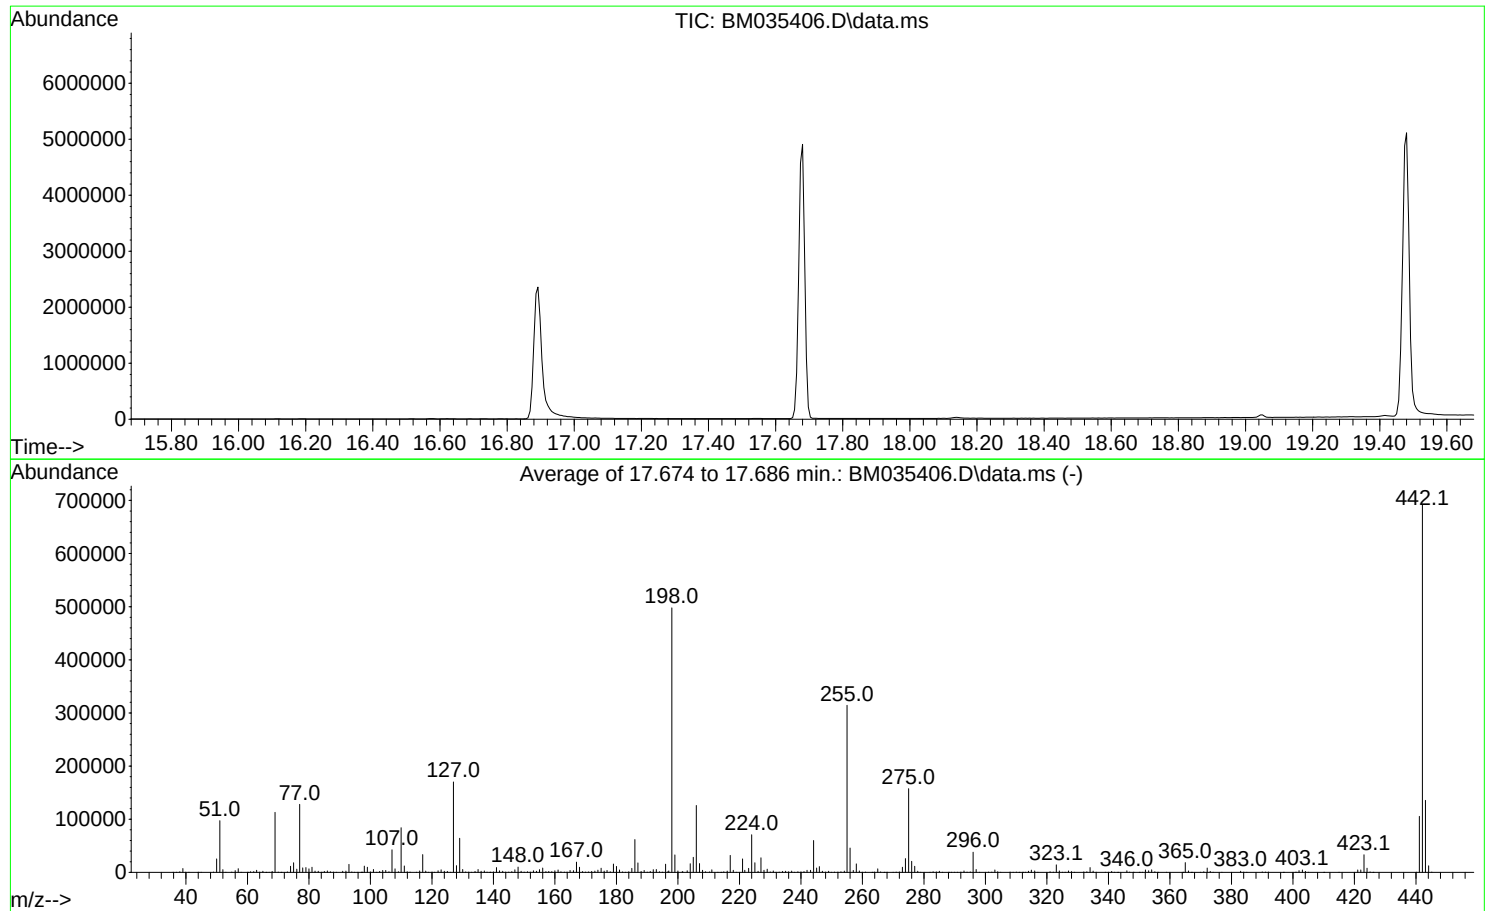




AutoFind: Scans 2480, 2481, 2482; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	19.5	97131	PASS
68	69	0.00	2	1.7	1978	PASS
69	198	0.00	100	22.7	113077	PASS
70	69	0.00	2	0.5	615	PASS
127	198	10	80	34.2	170160	PASS
197	198	0.00	2	0.5	2615	PASS
198	198	100	100	100.0	497621	PASS
199	198	5	9	6.6	32827	PASS
275	198	10	60	31.6	157483	PASS
365	198	1	100	3.7	18331	PASS
441	198	0.01	100	21.2	105384	PASS
442	442	50	100	100.0	692267	PASS
443	442	15	24	19.6	135512	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060722\
Data File : BM035406.D
Acq On : 07 Jun 2022 10:27
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jun 07 15:30:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jun 07 14:28:07 2022
Response via : Initial Calibration

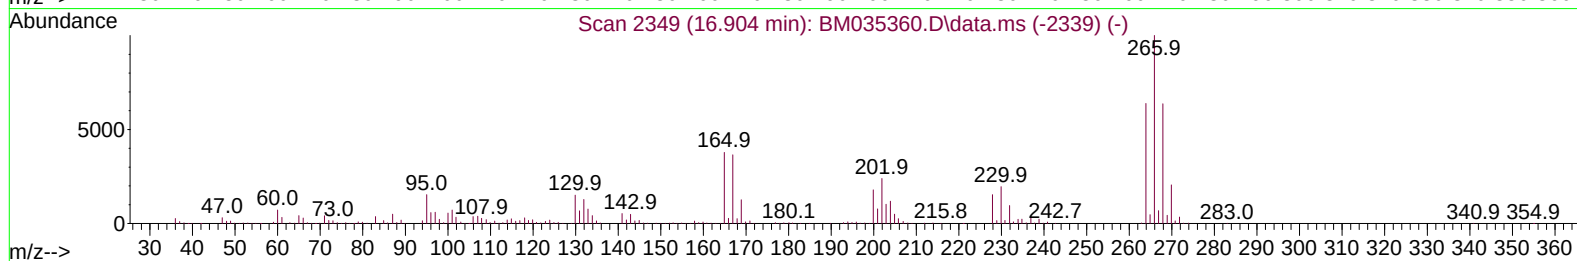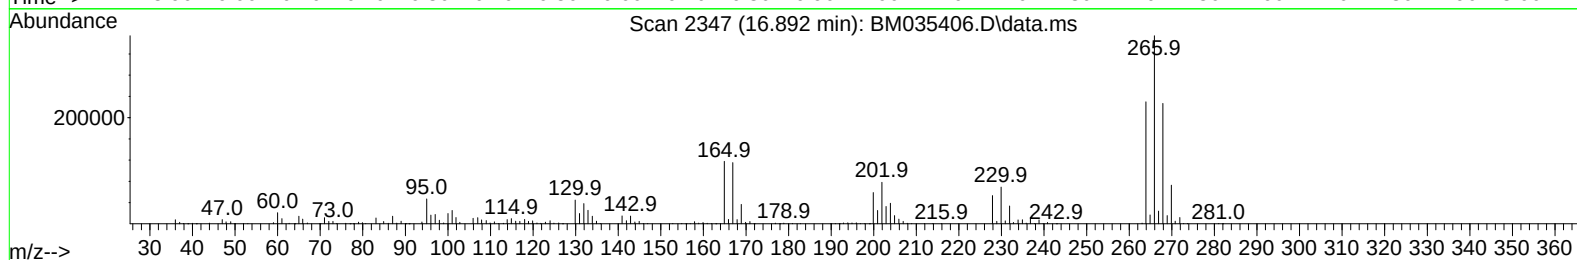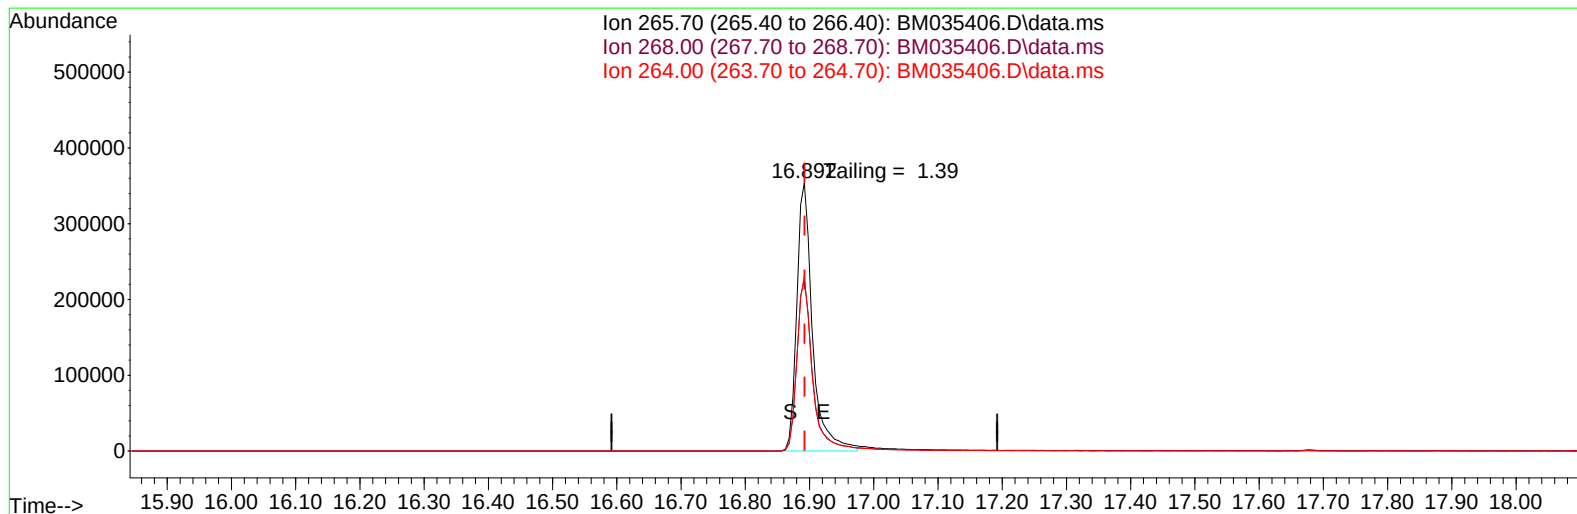

TIC: BM035406.D\data.ms

(70) Pentachlorophenol (C)

16.892min (-0.000) 0.00 ng




response 624838

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	64.05
264.00	63.30	64.90
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM060722\
 Data File : BM035406.D
 Acq On : 07 Jun 2022 10:27
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Jun 07 15:30:54 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM060222.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jun 07 14:28:07 2022
 Response via : Initial Calibration

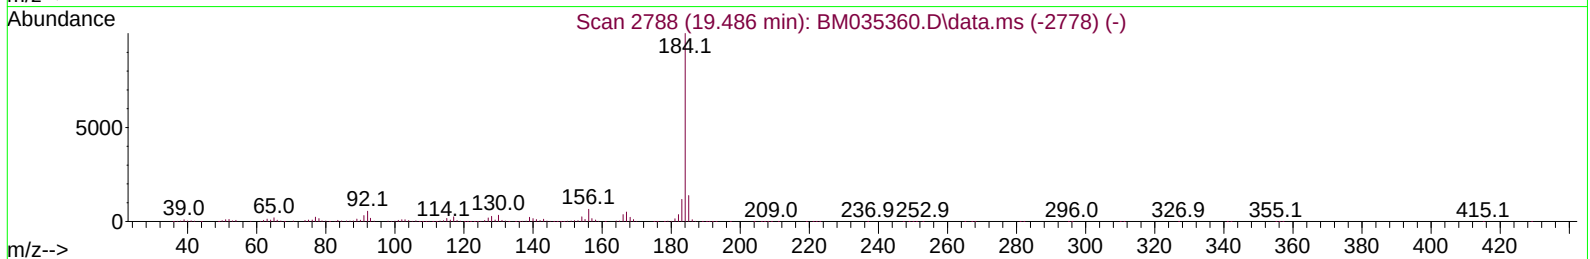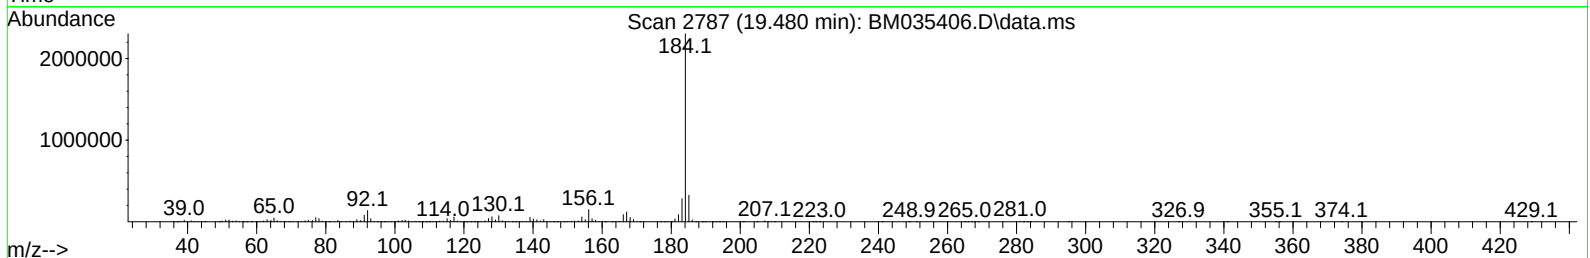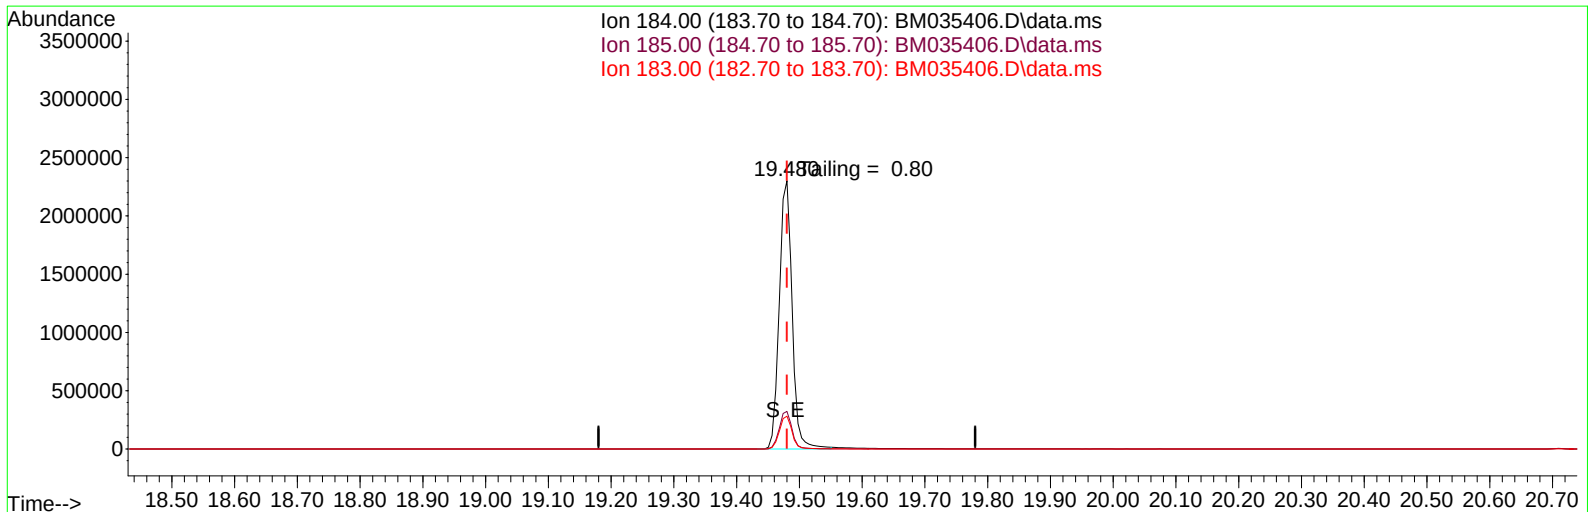

TIC: BM035406.D\data.ms

(77) Benzidine

19.480min (-0.000) 745573.95 ng

response 3312279

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.03
183.00	11.90	12.22
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
6/7/2022	BNA_M	BM035406.D
Compound Name	Response	Retention Time
DDT	1791331	20.7
DDD	8291	20.27
DDE	4231	19.76
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12522	1803853	0.69

Instrument :
BNA_M
ClientSampleId :
DFTPP