

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
 Data File : BM035490.D
 Acq On : 17 Jun 2022 12:07
 Operator : CG/JU
 Sample : N3226-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4L2

Quant Time: Jun 17 23:01:03 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 17 01:58:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.816	152	202530	20.000	ng/ul	0.00
20) Naphthalene-d8	10.610	136	856363	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.457	164	497768	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.204	188	996647	20.000	ng/ul	0.00
79) Chrysene-d12	21.391	240	1010647	20.000	ng/ul	0.00
88) Perylene-d12	23.727	264	1109797	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.269	96	35764	7.049	ng/uL	0.00
4) Pyridine-d5	3.687	84	435080	34.818	ng/ul	0.00
7) Phenol-d5	6.998	99	555661	35.799	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.145	67	369413	38.271	ng/ul	0.00
11) 2-Chlorophenol-d4	7.351	132	516915	38.449	ng/ul	0.00
15) 4-Methylphenol-d8	8.539	113	456672	35.145	ng/ul	0.00
21) Nitrobenzene-d5	8.975	128	238271	37.378	ng/ul	0.00
24) 2-Nitrophenol-d4	9.704	143	263883	38.390	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.251	165	408190	34.976	ng/ul	0.00
31) 4-Chloroaniline-d4	10.757	131	636188	34.645	ng/ul	0.00
46) Dimethylphthalate-d6	13.874	166	1367824	40.398	ng/ul	0.00
49) Acenaphthylene-d8	14.151	160	1669556	39.790	ng/ul	0.00
54) 4-Nitrophenol-d4	14.721	143	158873	30.545	ng/ul	0.02
60) Fluorene-d10	15.451	176	1203955	41.066	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.592	200	177441	29.863	ng/ul	0.00
73) Anthracene-d10	17.304	188	1847290	41.236	ng/ul	0.00
81) Pyrene-d10	19.597	212	2122264	42.713	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.580	264	2284427	42.677	ng/ul	0.00
Target Compounds						
48) 2,6-Dinitrotoluene	13.874	165	7992	1.184	ng/ul#	Qvalue 40


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
Data File : BM035490.D
Acq On : 17 Jun 2022 12:07
Operator : CG/JU
Sample : N3226-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4L2


Quant Time: Jun 17 23:01:03 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 17 01:58:49 2022
Response via : Initial Calibration

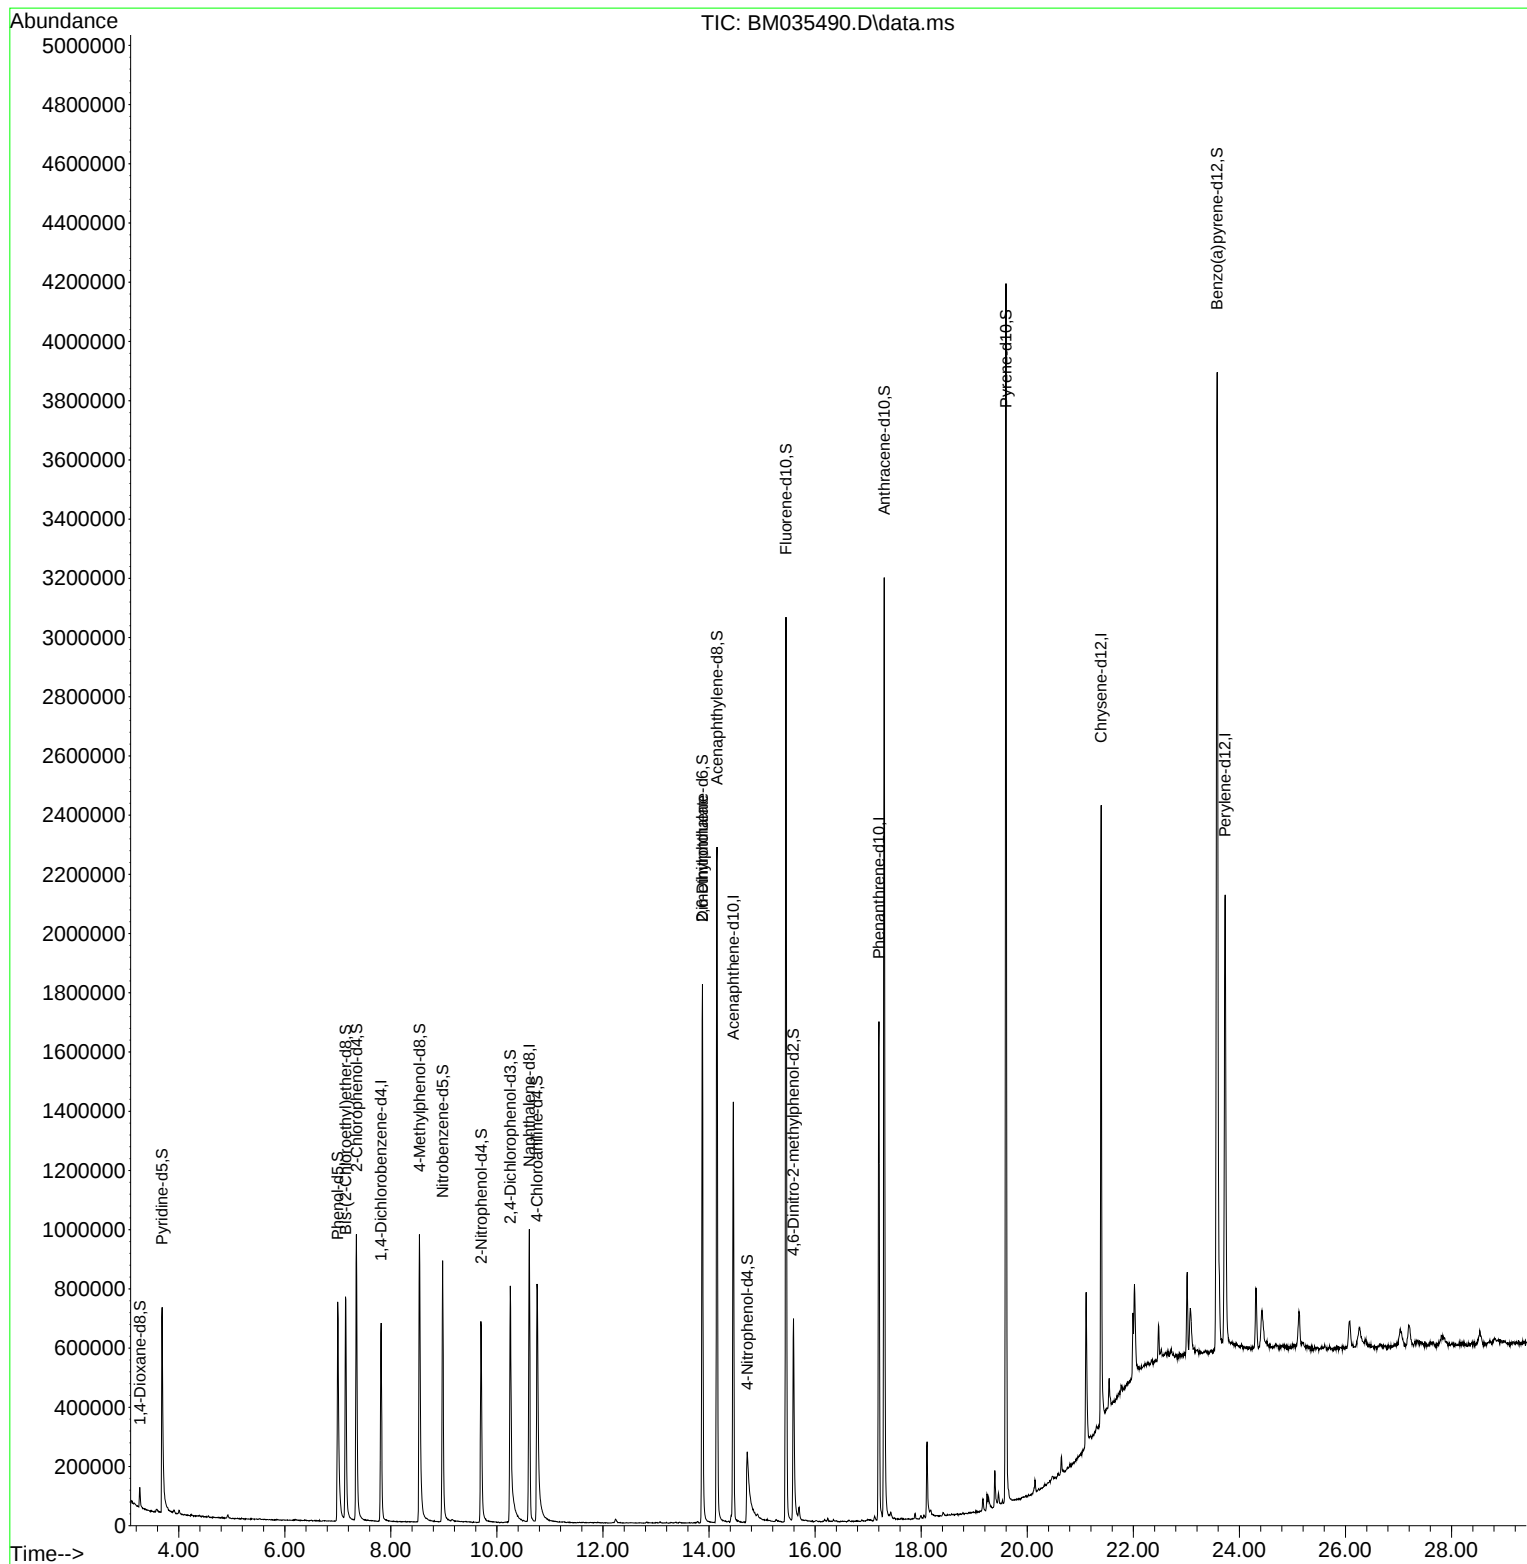

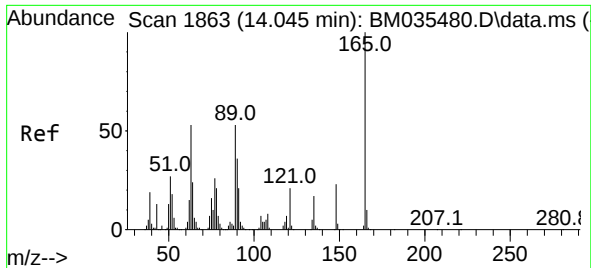

#48
 2,6-Dinitrotoluene
 Concen: 1.184 ng/ul
 RT: 13.874 min Scan# 11
 Delta R.T. -0.171 min
 Lab File: BM035490.D
 Acq: 17 Jun 2022 12:07

Instrument :
 BNA_M
 ClientSampleId :
 EW4L2

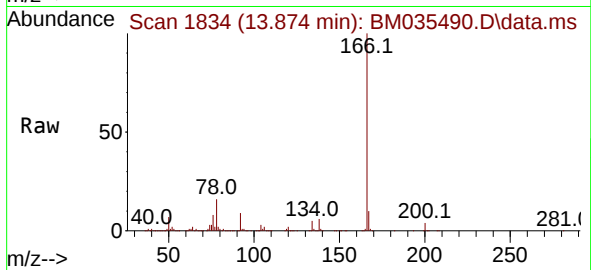

Tgt Ion:165 Resp: 7992
 Ion Ratio Lower Upper
 165 100
 89 0.0 42.5 63.7#
 121 33.0 17.2 25.8#

