

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
 Data File : BM035500.D
 Acq On : 17 Jun 2022 18:17
 Operator : CG/JU
 Sample : N3226-03
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4L4

Quant Time: Jun 17 23:02:42 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 17 01:58:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.816	152	193109	20.000	ng/ul	0.00
20) Naphthalene-d8	10.610	136	826553	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.457	164	493147	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.204	188	1001516	20.000	ng/ul	0.00
79) Chrysene-d12	21.392	240	1028666	20.000	ng/ul	0.00
88) Perylene-d12	23.733	264	1100751	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.269	96	7863	1.625	ng/uL	0.00
4) Pyridine-d5	3.693	84	317	0.027	ng/ul	0.00
7) Phenol-d5	7.016	99	109346	7.388	ng/ul	0.02
9) Bis-(2-Chloroethyl)eth...	7.151	67	77891	8.463	ng/ul	0.00
11) 2-Chlorophenol-d4	7.357	132	111111	8.668	ng/ul	0.00
15) 4-Methylphenol-d8	8.557	113	86613	6.991	ng/ul	0.02
21) Nitrobenzene-d5	8.986	128	50492	8.207	ng/ul	0.01
24) 2-Nitrophenol-d4	9.710	143	51368	7.743	ng/ul	0.01
28) 2,4-Dichlorophenol-d3	10.286	165	59699	5.300	ng/ul	0.04
31) 4-Chloroaniline-d4	10.781	131	96564	5.448	ng/ul	0.02
46) Dimethylphthalate-d6	13.880	166	313828	9.356	ng/ul	0.00
49) Acenaphthylene-d8	14.151	160	373335	8.981	ng/ul	0.00
54) 4-Nitrophenol-d4	14.698	143	60	0.012	ng/ul	0.00
60) Fluorene-d10	15.457	176	292113	10.057	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.615	200	13543	2.268	ng/ul	0.02
73) Anthracene-d10	17.304	188	476920	10.594	ng/ul	0.00
81) Pyrene-d10	19.598	212	660535	13.061	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.580	264	662303	12.475	ng/ul	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.303	149	46384	1.129	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
Data File : BM035500.D
Acq On : 17 Jun 2022 18:17
Operator : CG/JU
Sample : N3226-03
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4L4

Quant Time: Jun 17 23:02:42 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 17 01:58:49 2022
Response via : Initial Calibration

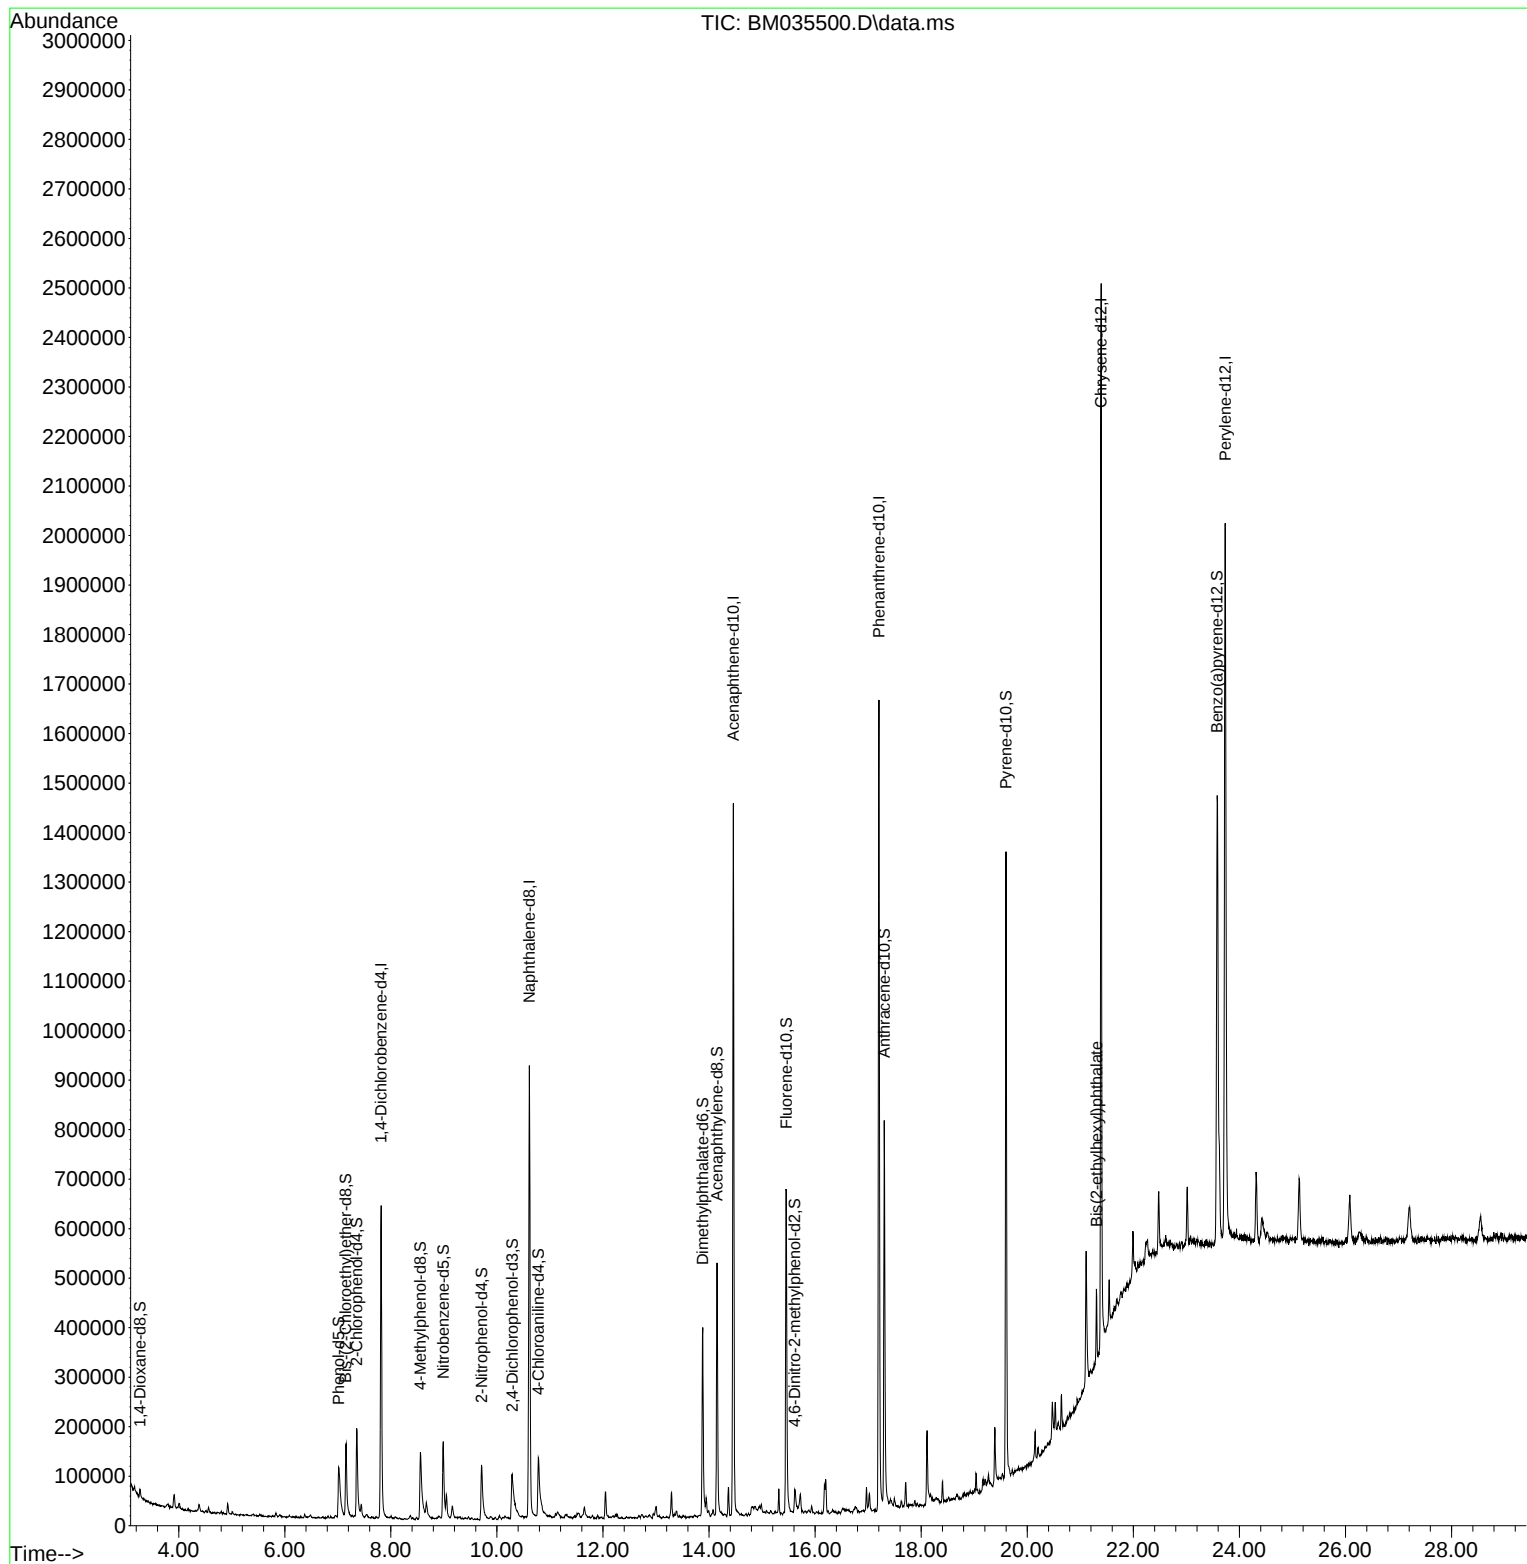

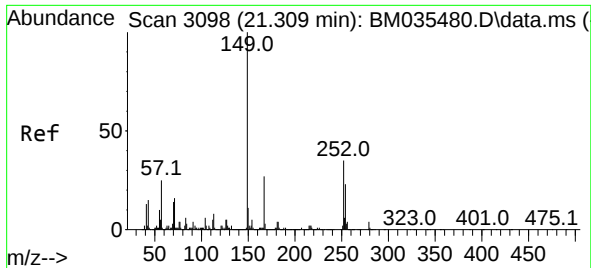

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.129 ng/ul
 RT: 21.303 min Scan# 30
 Delta R.T. -0.006 min
 Lab File: BM035500.D
 Acq: 17 Jun 2022 18:17

Instrument :
 BNA_M
 ClientSampleId :
 EW4L4

Tgt Ion:149 Resp: 46384
 Ion Ratio Lower Upper
 149 100
 167 25.4 21.5 32.3
 279 3.8 3.4 5.2

