




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
Data File : BM035497.D
Acq On : 17 Jun 2022 16:26
Operator : CG/JU
Sample : N3226-20
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4P0

Manual IntegrationsAPPROVED

Quant Time: Jun 17 23:02:06 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 17 01:58:49 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/18/2022
Supervised By :Yogesh Patel 06/22/2022

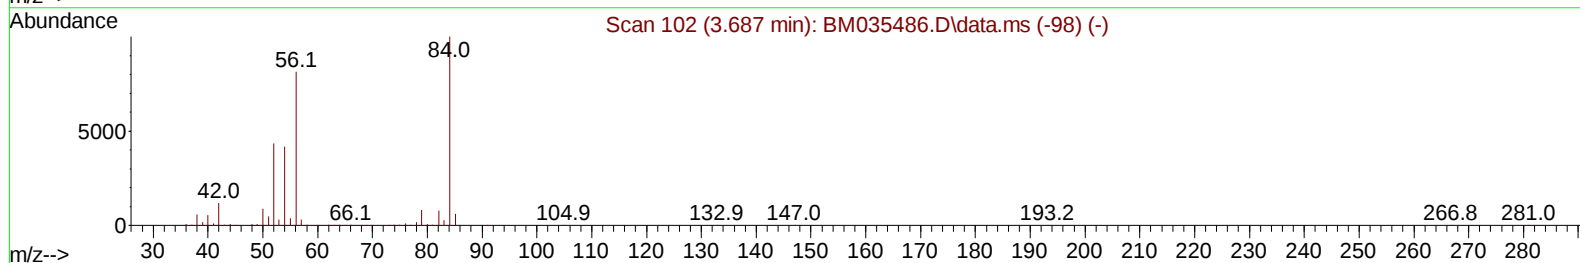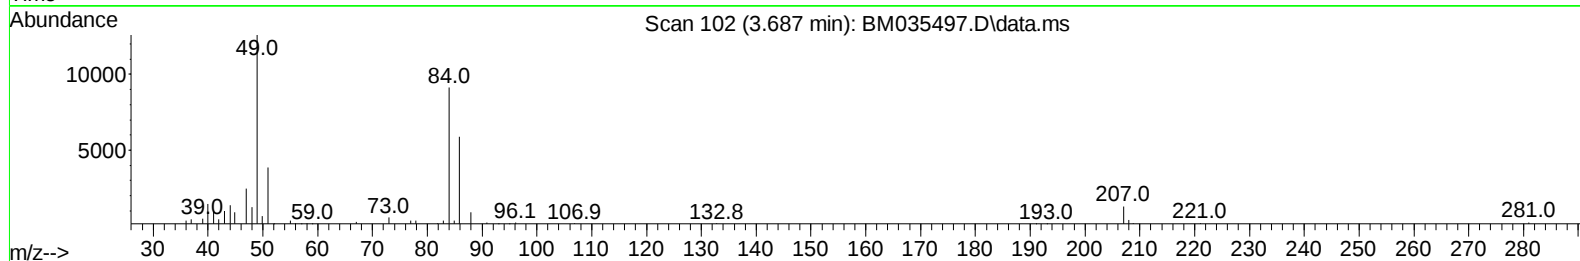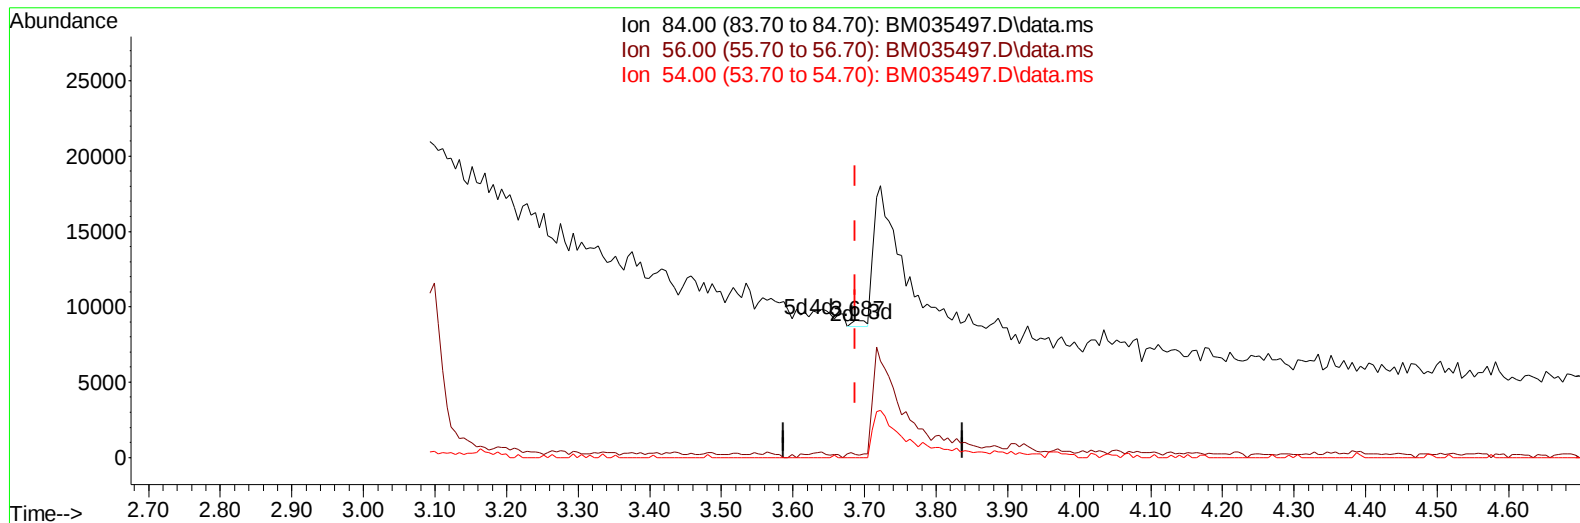

TIC: BM035497.D\data.ms

(4) Pyridine-d5 (S)

3.687min (+ 0.000) 0.04 ng/u1

response 527

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	70.90	2.01#
54.00	32.70	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
 Data File : BM035497.D
 Acq On : 17 Jun 2022 16:26
 Operator : CG/JU
 Sample : N3226-20
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4P0

Manual IntegrationsAPPROVED

Quant Time: Jun 17 23:02:06 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 17 01:58:49 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/18/2022
 Supervised By :Yogesh Patel 06/22/2022

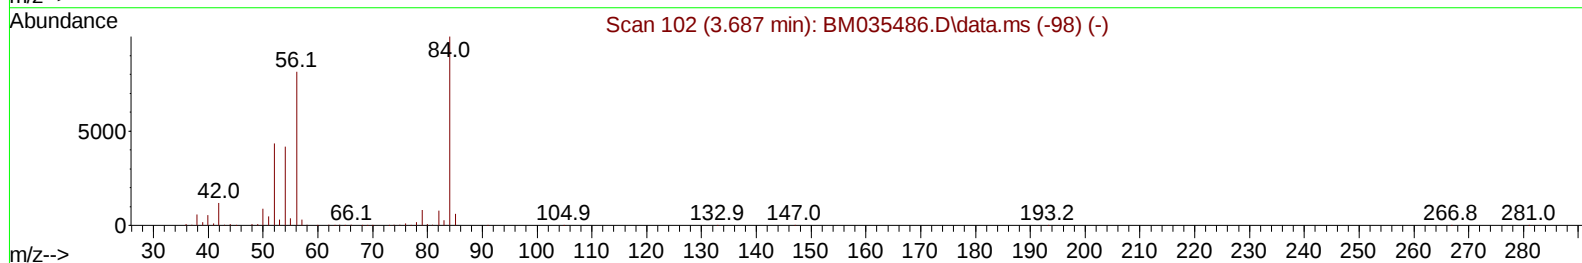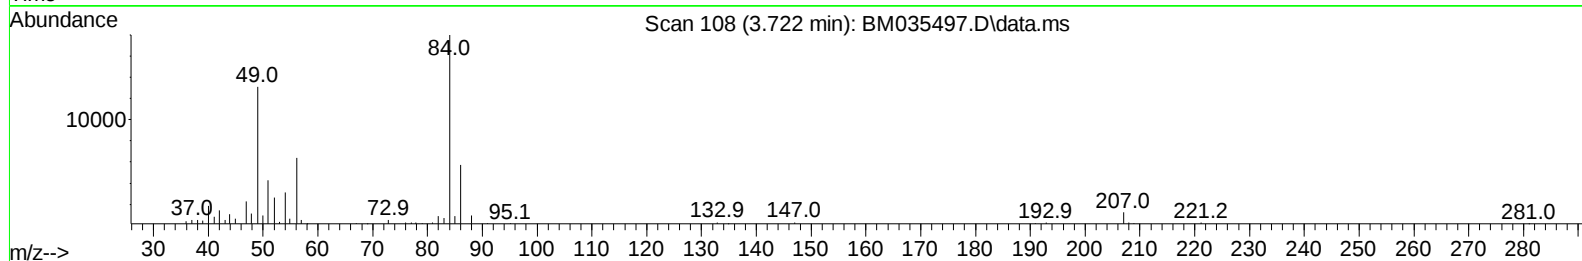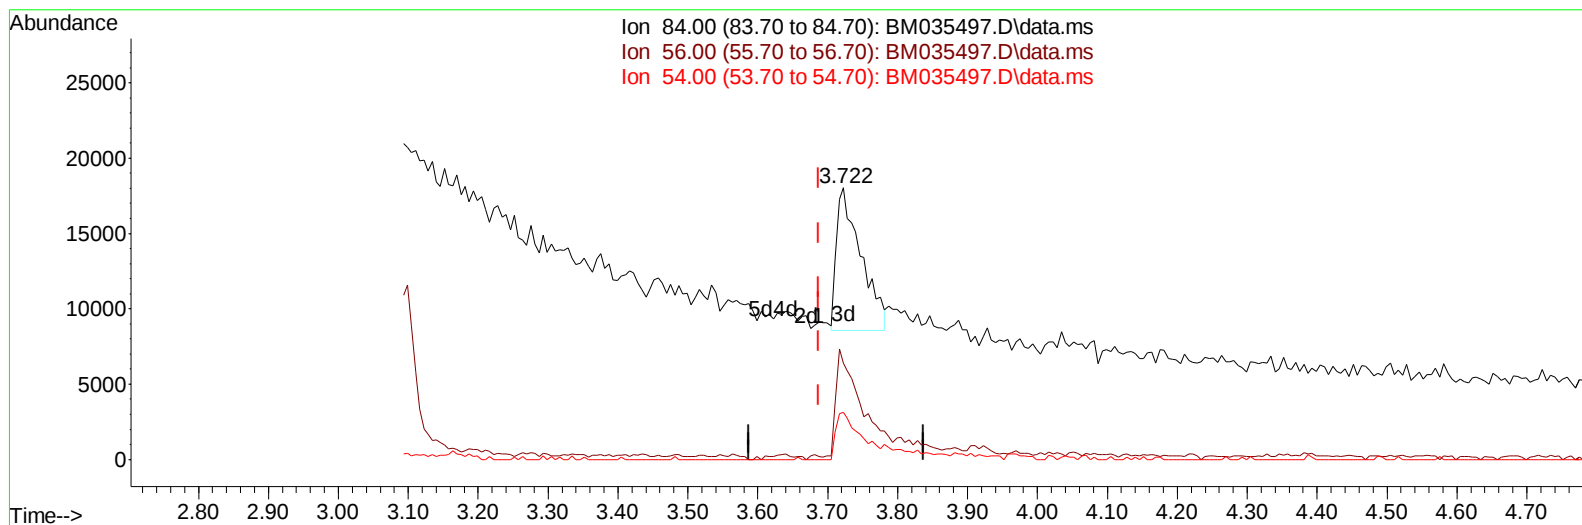

TIC: BM035497.D\data.ms

(4) Pyridine-d5 (S)

3.722min (+ 0.035) 1.85 ng/u1 m

response 23222

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	70.90	35.41#
54.00	32.70	17.39#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
Data File : BM035497.D
Acq On : 17 Jun 2022 16:26
Operator : CG/JU
Sample : N3226-20
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4P0

Manual IntegrationsAPPROVED

Quant Time: Jun 17 23:02:06 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 17 01:58:49 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/18/2022
Supervised By :Yogesh Patel 06/22/2022

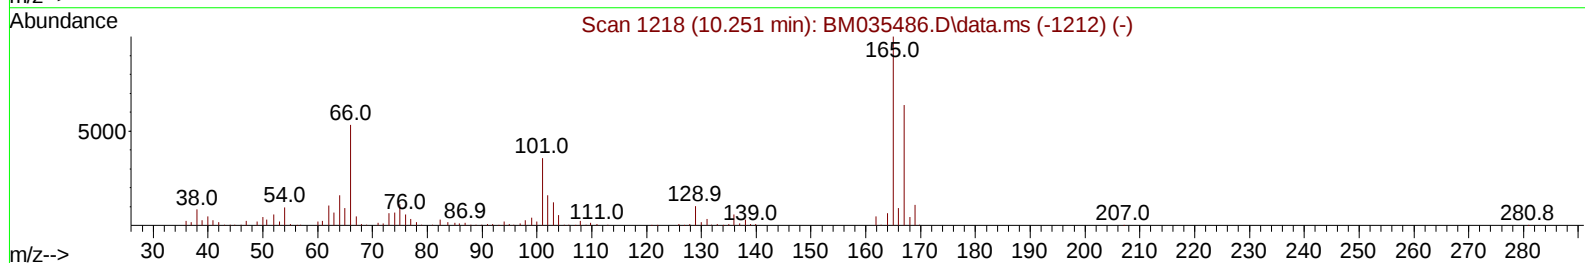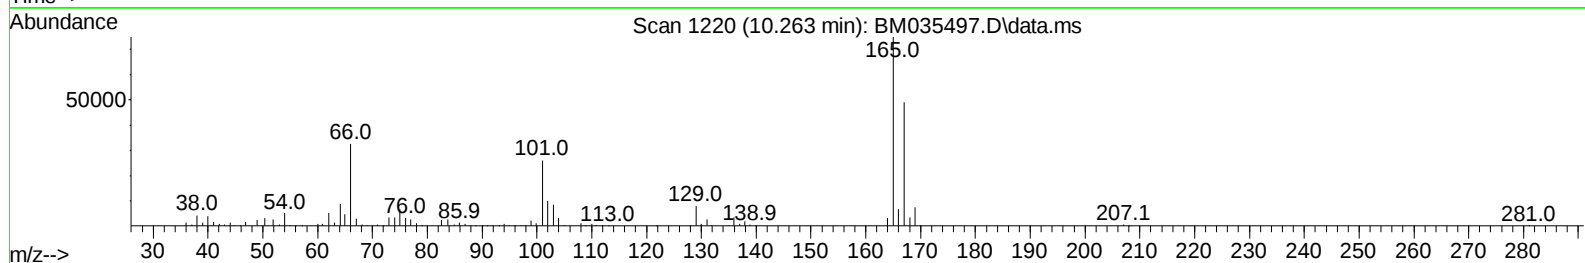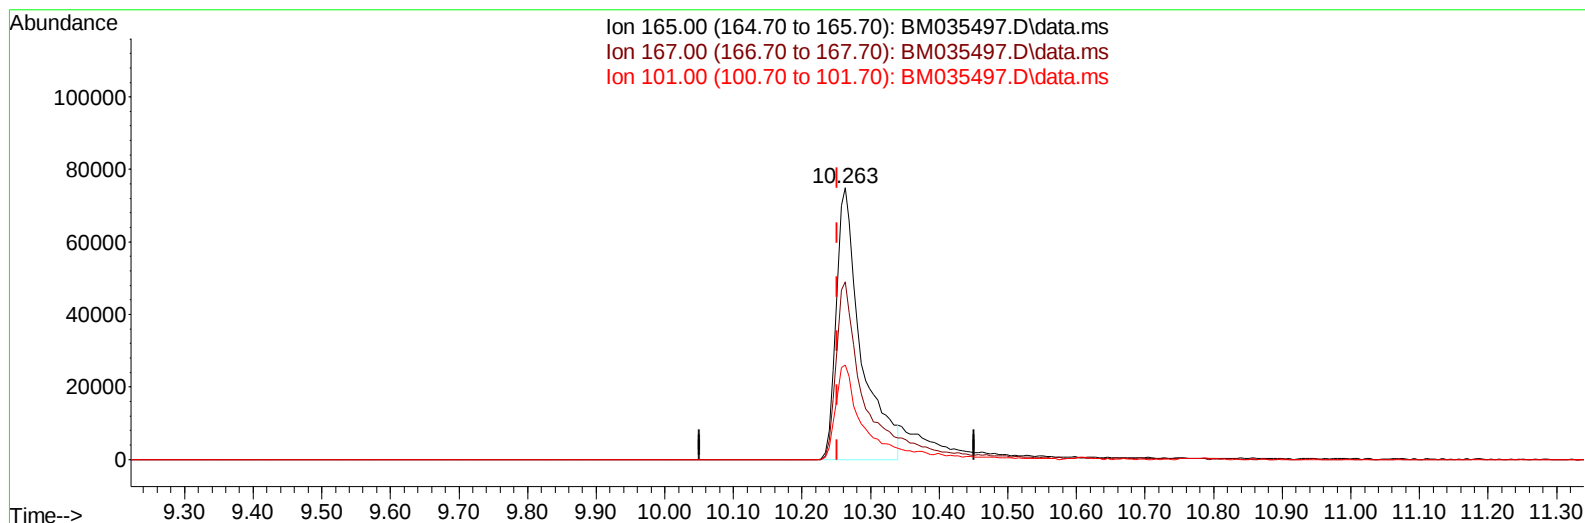

TIC: BM035497.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.263min (+ 0.012) 15.47 ng/u1

response 189522

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	65.20	65.51
101.00	35.30	34.89
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
 Data File : BM035497.D
 Acq On : 17 Jun 2022 16:26
 Operator : CG/JU
 Sample : N3226-20
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4P0

Manual IntegrationsAPPROVED

Quant Time: Jun 17 23:02:06 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 17 01:58:49 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/18/2022
 Supervised By :Yogesh Patel 06/22/2022

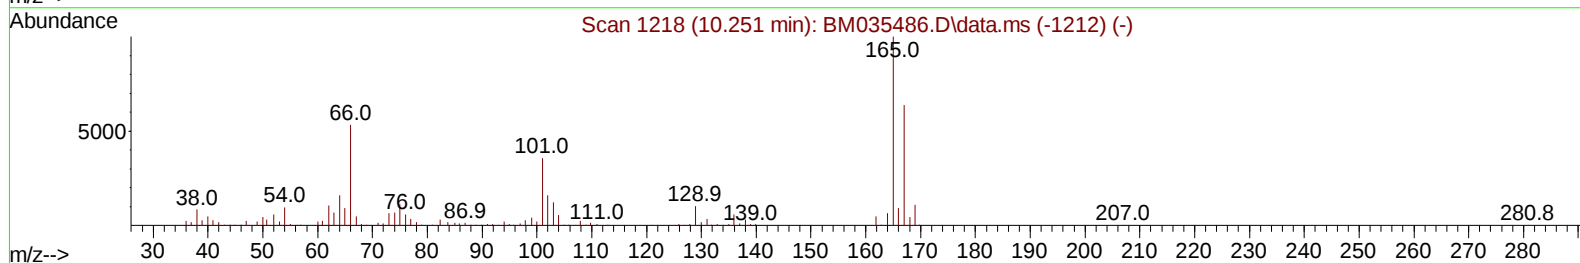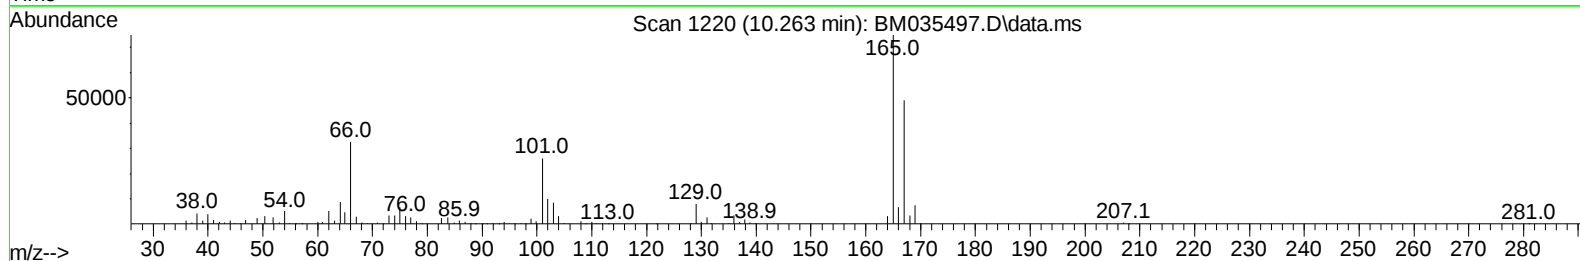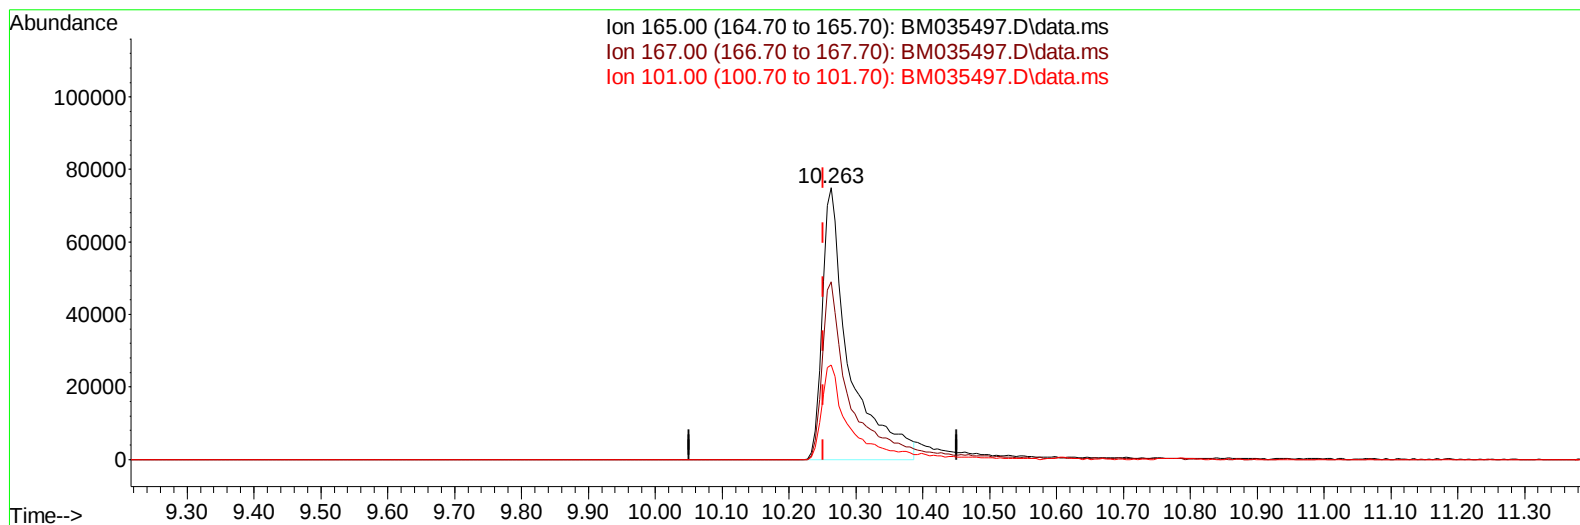

TIC: BM035497.D\data.ms

(28) 2,4-Dichlorophenol-d3 (S)

10.263min (+ 0.012) 17.02 ng/ul m

response 208506

Ion	Exp%	Act%
165.00	100.00	100.00
167.00	65.20	65.51
101.00	35.30	34.89
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
Data File : BM035497.D
Acq On : 17 Jun 2022 16:26
Operator : CG/JU
Sample : N3226-20
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4P0

Manual IntegrationsAPPROVED

Quant Time: Jun 17 23:02:06 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 17 01:58:49 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/18/2022
Supervised By :Yogesh Patel 06/22/2022

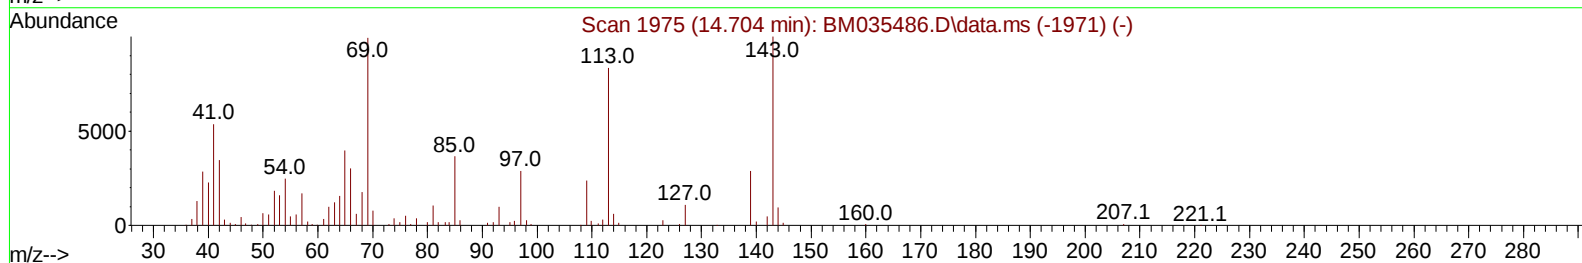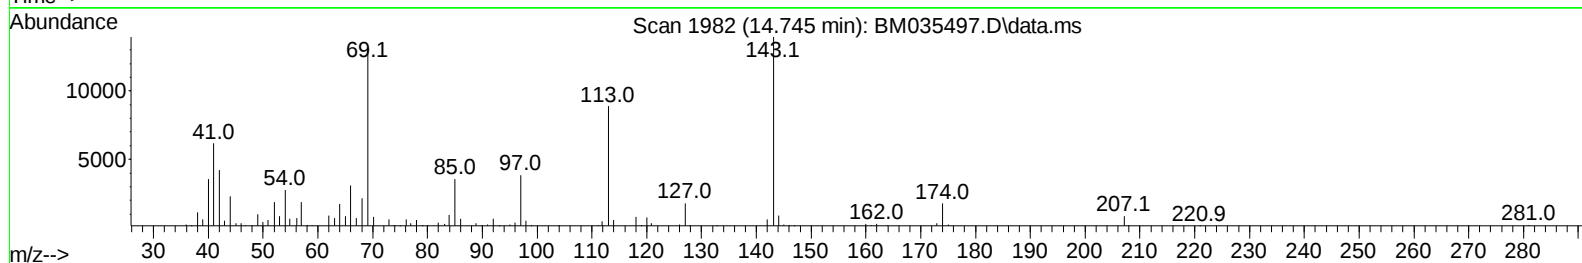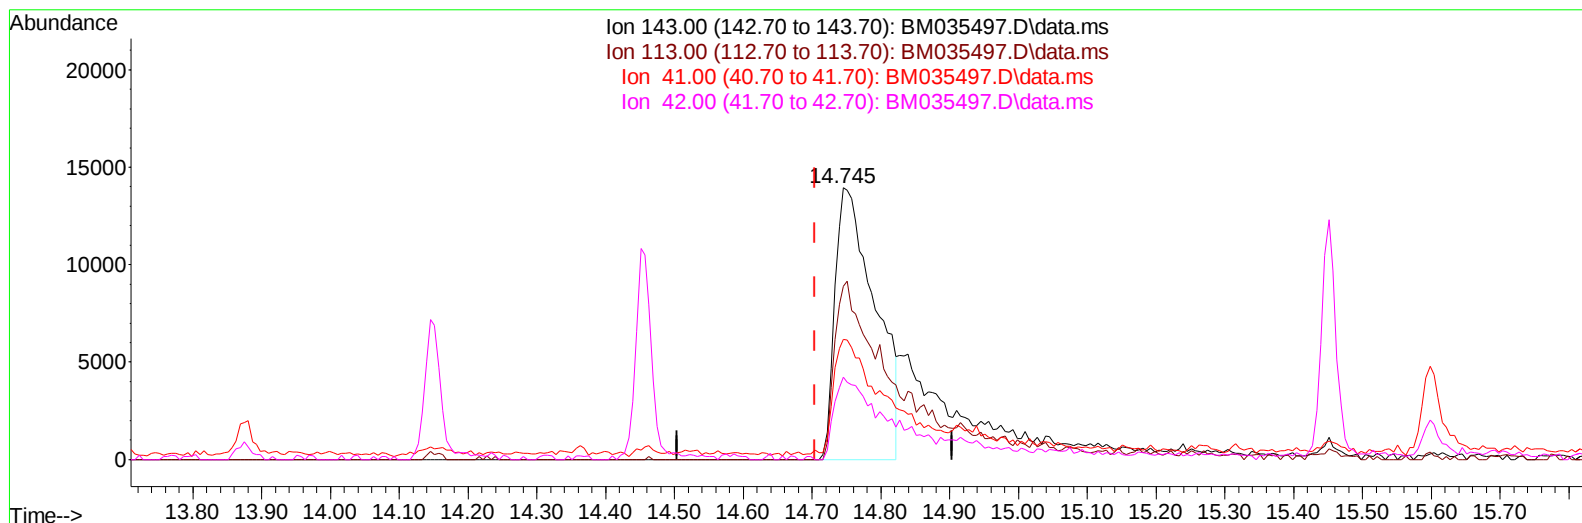

TIC: BM035497.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.745min (+ 0.041) 9.71 ng/ul

response 56350

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	61.40	63.75
41.00	41.00	44.29
42.00	29.30	30.24




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
Data File : BM035497.D
Acq On : 17 Jun 2022 16:26
Operator : CG/JU
Sample : N3226-20
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4P0

Manual IntegrationsAPPROVED

Quant Time: Jun 17 23:02:06 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 17 01:58:49 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/18/2022
Supervised By :Yogesh Patel 06/22/2022

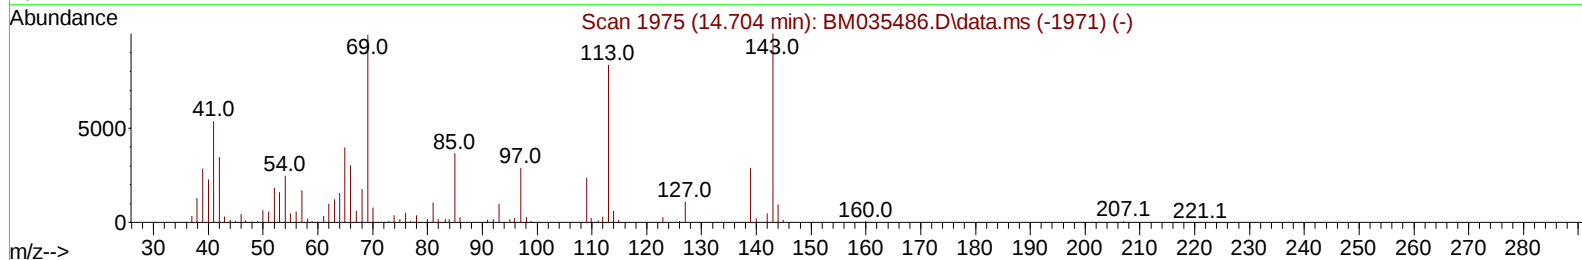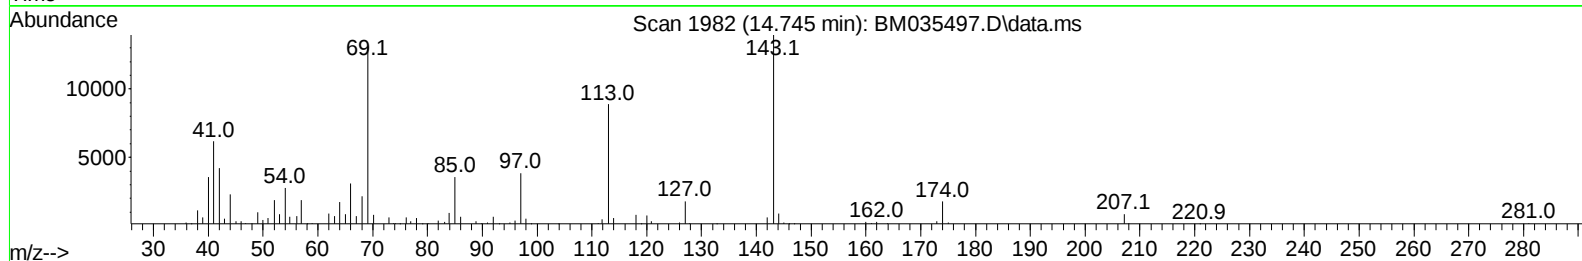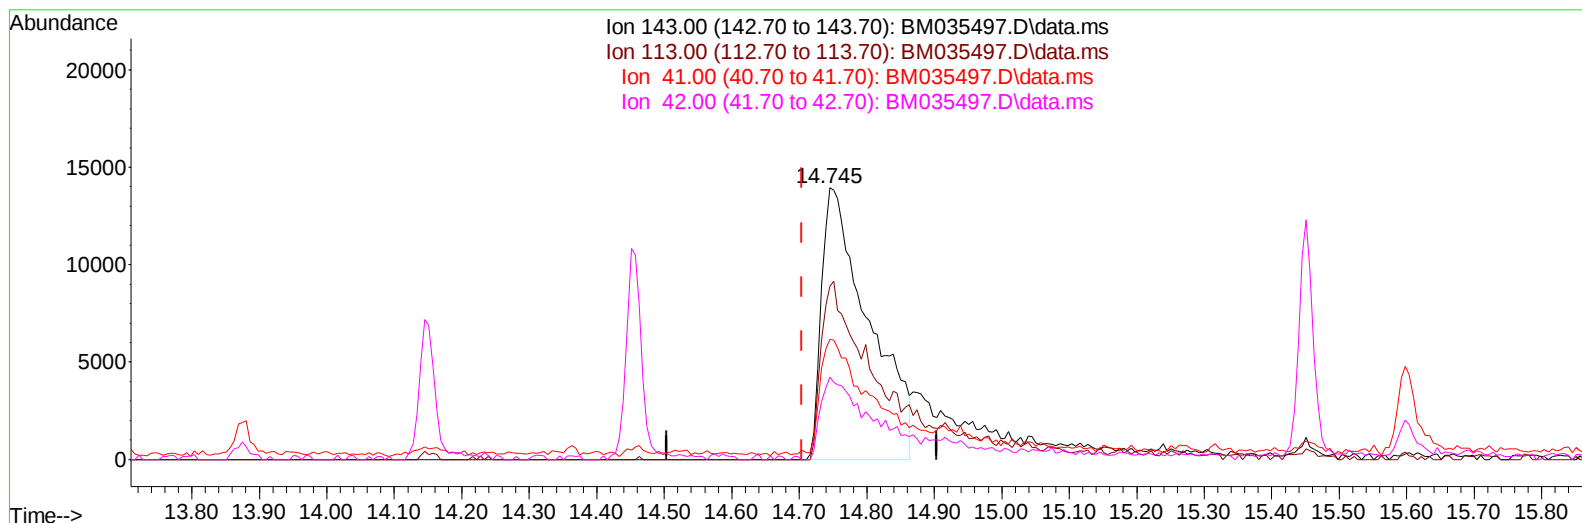

TIC: BM035497.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.745min (+ 0.041) 11.66 ng/ul m

response 67654

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	61.40	63.75
41.00	41.00	44.29
42.00	29.30	30.24

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
 Data File : BM035497.D
 Acq On : 17 Jun 2022 16:26
 Operator : CG/JU
 Sample : N3226-20
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4P0

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/18/2022
 Supervised By :Yogesh Patel 06/22/2022

Quant Time: Jun 17 23:02:06 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 17 01:58:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.816	152	203380	20.000	ng/ul	0.00
20) Naphthalene-d8	10.610	136	898913	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.457	164	555430	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.204	188	1141763	20.000	ng/ul	0.00
79) Chrysene-d12	21.392	240	960526	20.000	ng/ul	0.00
88) Perylene-d12	23.733	264	992826	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.269	96	17955	3.524	ng/uL	0.00
4) Pyridine-d5	3.722	84	23222m	1.851	ng/ul	0.04
7) Phenol-d5	7.004	99	288651	18.519	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.152	67	199441	20.576	ng/ul	0.00
11) 2-Chlorophenol-d4	7.352	132	277172	20.530	ng/ul	0.00
15) 4-Methylphenol-d8	8.546	113	250713	19.214	ng/ul	0.00
21) Nitrobenzene-d5	8.981	128	128148	19.151	ng/ul	0.00
24) 2-Nitrophenol-d4	9.704	143	138067	19.135	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.263	165	208506m	17.020	ng/ul	0.01
31) 4-Chloroaniline-d4	10.769	131	284652	14.767	ng/ul	0.01
46) Dimethylphthalate-d6	13.875	166	825252	21.843	ng/ul	0.00
49) Acenaphthylene-d8	14.151	160	968353	20.683	ng/ul	0.00
54) 4-Nitrophenol-d4	14.745	143	67654m	11.657	ng/ul	0.04
60) Fluorene-d10	15.451	176	728991	22.284	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.598	200	85380	12.543	ng/ul	0.00
73) Anthracene-d10	17.304	188	1054183	20.541	ng/ul	0.00
81) Pyrene-d10	19.598	212	1158936	24.542	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.586	264	1112083	23.223	ng/ul	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.663	105	24722	1.250	ng/ul#	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
Data File : BM035497.D
Acq On : 17 Jun 2022 16:26
Operator : CG/JU
Sample : N3226-20
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4P0

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/18/2022
Supervised By :Yogesh Patel 06/22/2022

Quant Time: Jun 17 23:02:06 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 17 01:58:49 2022
Response via : Initial Calibration

