




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
 Data File : BM035512.D
 Acq On : 18 Jun 2022 02:14
 Operator : CG/JU
 Sample : N3226-11
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4N1

Manual IntegrationsAPPROVED

Quant Time: Jun 18 04:05:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 17 01:58:49 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/18/2022
 Supervised By :Yogesh Patel 06/22/2022

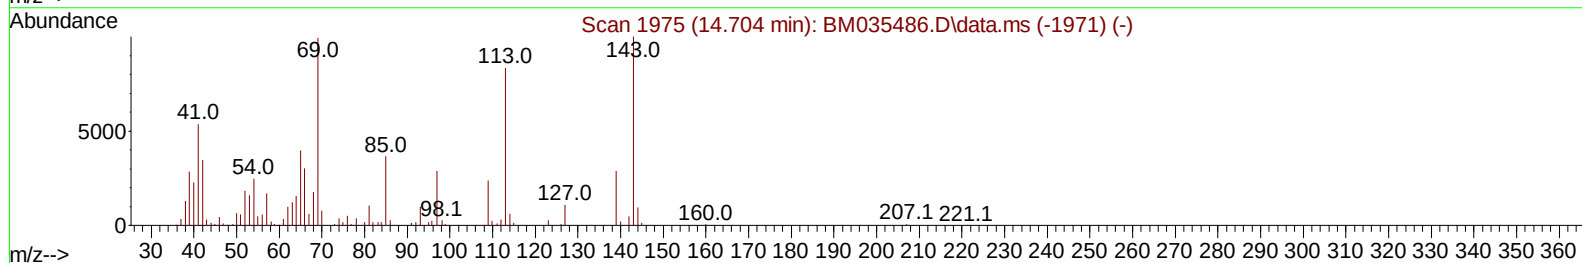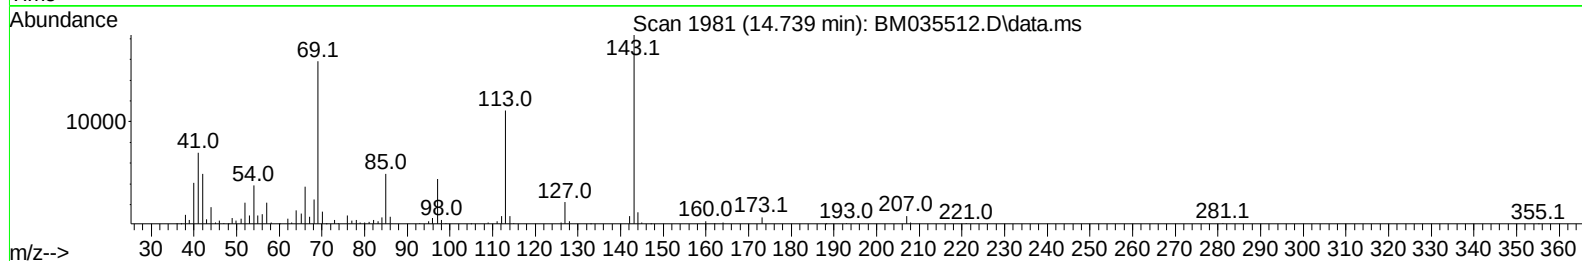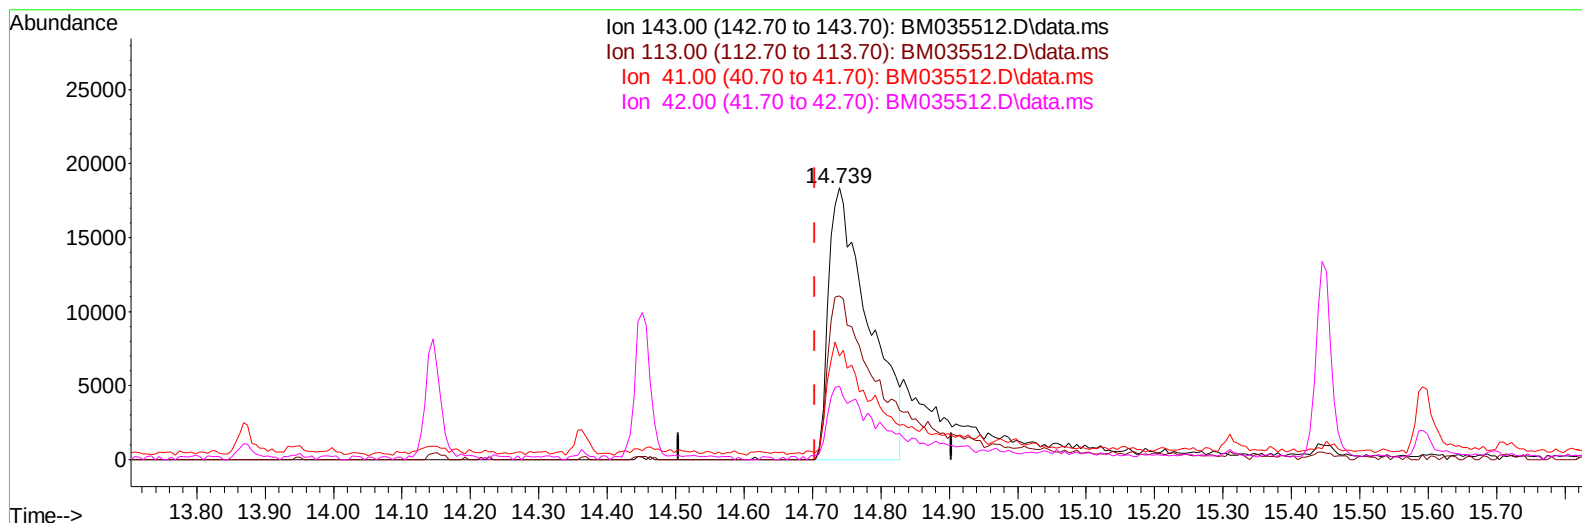

TIC: BM035512.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.739min (+ 0.035) 13.19 ng/ul

response 74645

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	61.40	60.27
41.00	41.00	38.11
42.00	29.30	26.97




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
 Data File : BM035512.D
 Acq On : 18 Jun 2022 02:14
 Operator : CG/JU
 Sample : N3226-11
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4N1

Manual IntegrationsAPPROVED

Quant Time: Jun 18 04:05:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 17 01:58:49 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 06/18/2022
 Supervised By :Yogesh Patel 06/22/2022

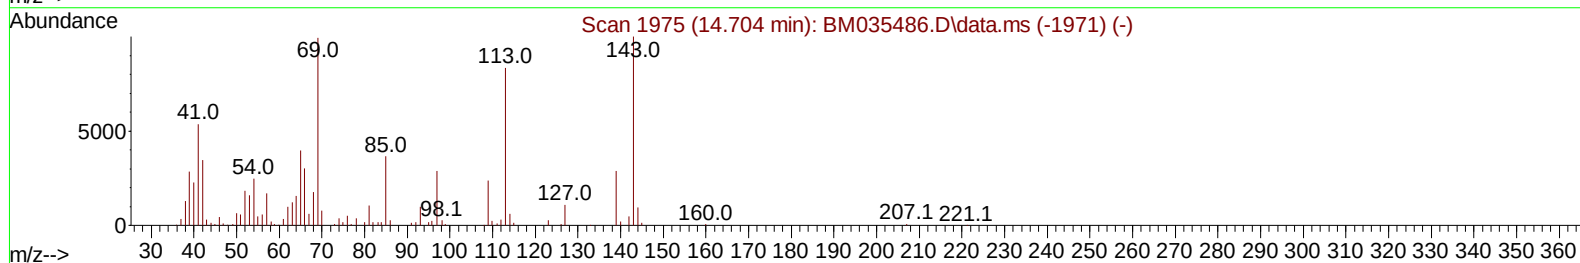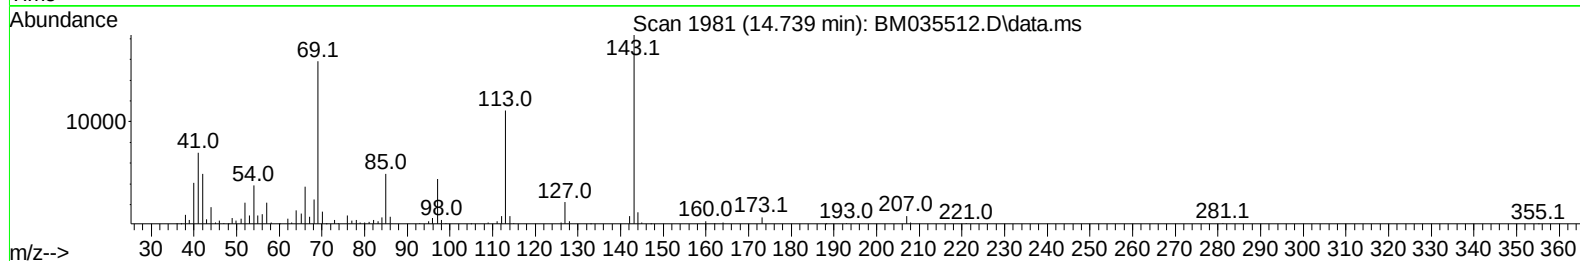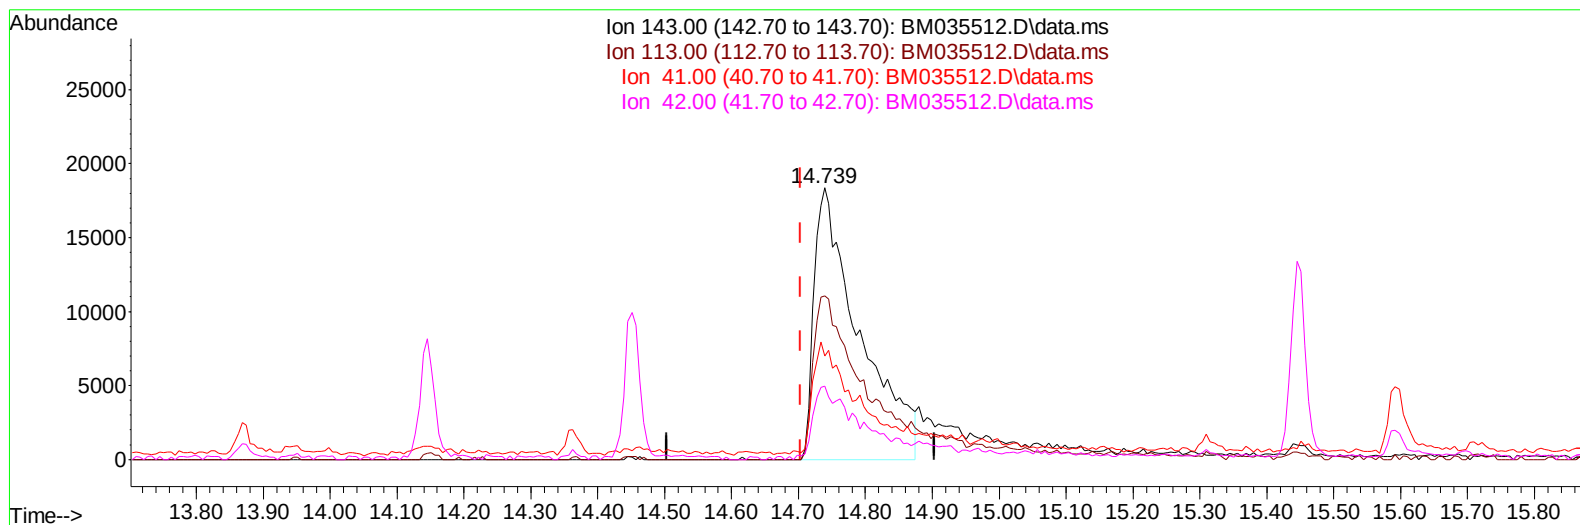

TIC: BM035512.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.739min (+ 0.035) 15.20 ng/ul m

response 86073

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	61.40	60.27
41.00	41.00	38.11
42.00	29.30	26.97

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
 Data File : BM035512.D
 Acq On : 18 Jun 2022 02:14
 Operator : CG/JU
 Sample : N3226-11
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4N1

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/18/2022
 Supervised By :Yogesh Patel 06/22/2022

Quant Time: Jun 18 04:05:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 17 01:58:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.810	152	210182	20.000	ng/ul	0.00
20) Naphthalene-d8	10.604	136	894618	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.451	164	541788	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.198	188	1119515	20.000	ng/ul	0.00
79) Chrysene-d12	21.386	240	1141958	20.000	ng/ul	0.00
88) Perylene-d12	23.727	264	1214354	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.269	96	25102	4.767	ng/uL	0.00
4) Pyridine-d5	3.687	84	274985	21.205	ng/ul	0.00
7) Phenol-d5	6.998	99	361372	22.434	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.145	67	239805	23.939	ng/ul	0.00
11) 2-Chlorophenol-d4	7.351	132	341152	24.451	ng/ul	0.00
15) 4-Methylphenol-d8	8.540	113	317098	23.515	ng/ul	0.00
21) Nitrobenzene-d5	8.975	128	159652	23.974	ng/ul	0.00
24) 2-Nitrophenol-d4	9.698	143	172560	24.031	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.257	165	272853	22.380	ng/ul	0.00
31) 4-Chloroaniline-d4	10.763	131	431262	22.481	ng/ul	0.00
46) Dimethylphthalate-d6	13.869	166	976848	26.506	ng/ul	0.00
49) Acenaphthylene-d8	14.145	160	1164699	25.503	ng/ul	0.00
54) 4-Nitrophenol-d4	14.739	143	86073m	15.204	ng/ul	0.04
60) Fluorene-d10	15.445	176	859149	26.924	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.592	200	90331	13.534	ng/ul	0.00
73) Anthracene-d10	17.298	188	1328016	26.391	ng/ul	0.00
81) Pyrene-d10	19.592	212	1547902	27.571	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.574	264	1599630	27.311	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
Data File : BM035512.D
Acq On : 18 Jun 2022 02:14
Operator : CG/JU
Sample : N3226-11
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4N1

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 06/18/2022
Supervised By :Yogesh Patel 06/22/2022

Quant Time: Jun 18 04:05:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 17 01:58:49 2022
Response via : Initial Calibration

