

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
 Data File : BM035495.D
 Acq On : 17 Jun 2022 15:12
 Operator : CG/JU
 Sample : N3226-14
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4N4

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 06/18/2022
 Supervised By :Yogesh Patel 06/22/2022

Quant Time: Jun 17 23:01:52 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 17 01:58:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.816	152	193744	20.000	ng/u1	0.00
20) Naphthalene-d8	10.610	136	818511	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.457	164	494944	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.204	188	1016536	20.000	ng/u1	0.00
79) Chrysene-d12	21.392	240	1023780	20.000	ng/u1	0.00
88) Perylene-d12	23.733	264	1080773	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.269	96	17255m	3.555	ng/uL	0.00
4) Pyridine-d5	3.699	84	97204	8.132	ng/u1	0.01
7) Phenol-d5	7.010	99	236327	15.916	ng/u1	0.01
9) Bis-(2-Chloroethyl)eth...	7.151	67	159534	17.277	ng/u1	0.00
11) 2-Chlorophenol-d4	7.357	132	231313	17.986	ng/u1	0.00
15) 4-Methylphenol-d8	8.545	113	200645	16.142	ng/u1	0.00
21) Nitrobenzene-d5	8.981	128	104907	17.218	ng/u1	0.00
24) 2-Nitrophenol-d4	9.710	143	110128	16.762	ng/u1	0.01
28) 2,4-Dichlorophenol-d3	10.263	165	165918	14.874	ng/u1	0.01
31) 4-Chloroaniline-d4	10.769	131	246349	14.036	ng/u1	0.01
46) Dimethylphthalate-d6	13.874	166	639864	19.006	ng/u1	0.00
49) Acenaphthylene-d8	14.151	160	756609	18.135	ng/u1	0.00
54) 4-Nitrophenol-d4	14.763	143	57478m	11.114	ng/u1	0.06
60) Fluorene-d10	15.451	176	573433	19.671	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.604	200	60814	10.035	ng/u1	0.01
73) Anthracene-d10	17.304	188	908502	19.883	ng/u1	0.00
81) Pyrene-d10	19.598	212	1129204	22.435	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.580	264	1168112	22.408	ng/u1	0.00
Target Compounds						
					Qvalue	
16) Acetophenone	8.657	105	39180	2.079	ng/u1	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
Data File : BM035495.D
Acq On : 17 Jun 2022 15:12
Operator : CG/JU
Sample : N3226-14
Misc :
ALS Vial : 11 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
EW4N4

Quant Time: Jun 17 23:01:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 17 01:58:49 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 06/18/2022
Supervised By :Yogesh Patel 06/22/2022

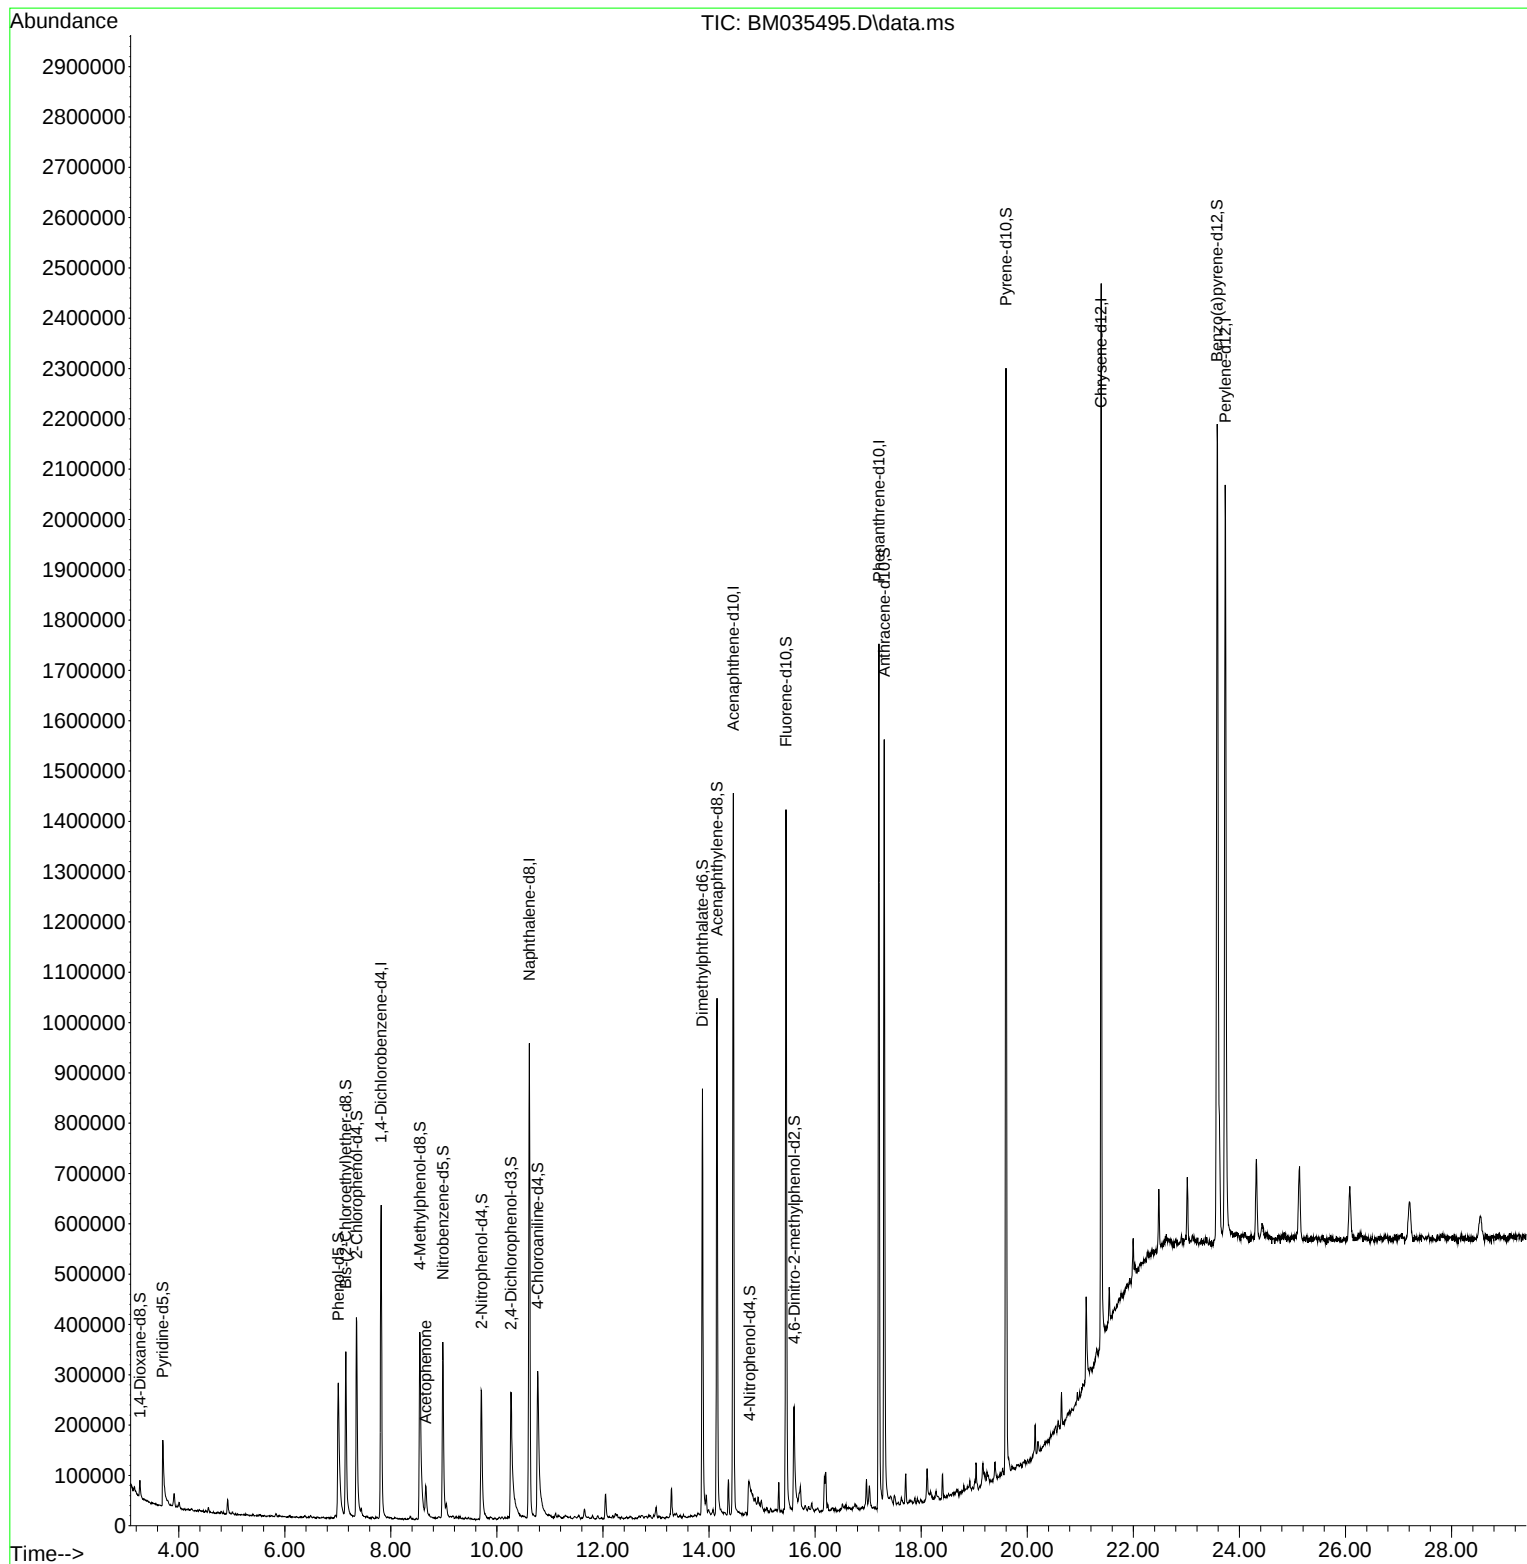

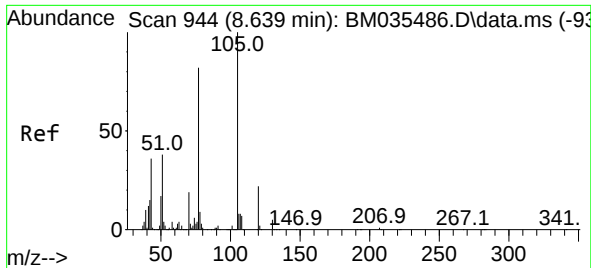

#16
Acetophenone
Concen: 2.079 ng/ul
RT: 8.657 min Scan# 94
Delta R.T. 0.012 min
Lab File: BM035495.D
Acq: 17 Jun 2022 15:12

Instrument :
BNA_M
ClientSampleId :
EW4N4

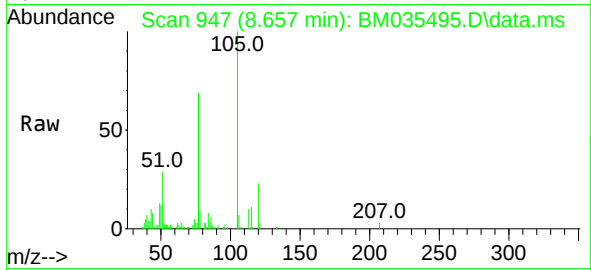

Tgt Ion:105 Resp: 39180
Ion Ratio Lower Upper
105 100
77 69.2 59.8 89.6
51 29.4 22.1 33.1

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 06/18/2022
Supervised By :Yogesh Patel 06/22/2022

