

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
 Data File : BM035500.D
 Acq On : 17 Jun 2022 18:17
 Operator : CG/JU
 Sample : N3226-03
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4L4

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 06/18/2022
 Supervised By :Yogesh Patel 06/22/2022

Quant Time: Jun 17 23:02:42 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jun 17 01:58:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.816	152	193109	20.000	ng/u1	0.00
20) Naphthalene-d8	10.610	136	826553	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.457	164	493147	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.204	188	1001516	20.000	ng/u1	0.00
79) Chrysene-d12	21.392	240	1028666	20.000	ng/u1	0.00
88) Perylene-d12	23.733	264	1100751	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.269	96	8550m	1.767	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/u1	
7) Phenol-d5	7.016	99	109346	7.388	ng/u1	0.02
9) Bis-(2-Chloroethyl)eth...	7.151	67	77891	8.463	ng/u1	0.00
11) 2-Chlorophenol-d4	7.357	132	111111	8.668	ng/u1	0.00
15) 4-Methylphenol-d8	8.557	113	86613	6.991	ng/u1	0.02
21) Nitrobenzene-d5	8.986	128	50492	8.207	ng/u1	0.01
24) 2-Nitrophenol-d4	9.710	143	51368	7.743	ng/u1	0.01
28) 2,4-Dichlorophenol-d3	10.286	165	73272m	6.505	ng/u1	0.04
31) 4-Chloroaniline-d4	10.781	131	96564	5.448	ng/u1	0.02
46) Dimethylphthalate-d6	13.880	166	313828	9.356	ng/u1	0.00
49) Acenaphthylene-d8	14.151	160	373335	8.981	ng/u1	0.00
54) 4-Nitrophenol-d4	14.827	143	20603m	3.998	ng/u1	0.12
60) Fluorene-d10	15.457	176	292113	10.057	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.615	200	16621m	2.784	ng/u1	0.02
73) Anthracene-d10	17.304	188	476920	10.594	ng/u1	0.00
81) Pyrene-d10	19.598	212	660535	13.061	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.580	264	662303	12.475	ng/u1	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.303	149	46384	1.129	ng/u1	Qvalue 97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
Data File : BM035500.D
Acq On : 17 Jun 2022 18:17
Operator : CG/JU
Sample : N3226-03
Misc :
ALS Vial : 16 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
EW4L4

Quant Time: Jun 17 23:02:42 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jun 17 01:58:49 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 06/18/2022
Supervised By :Yogesh Patel 06/22/2022

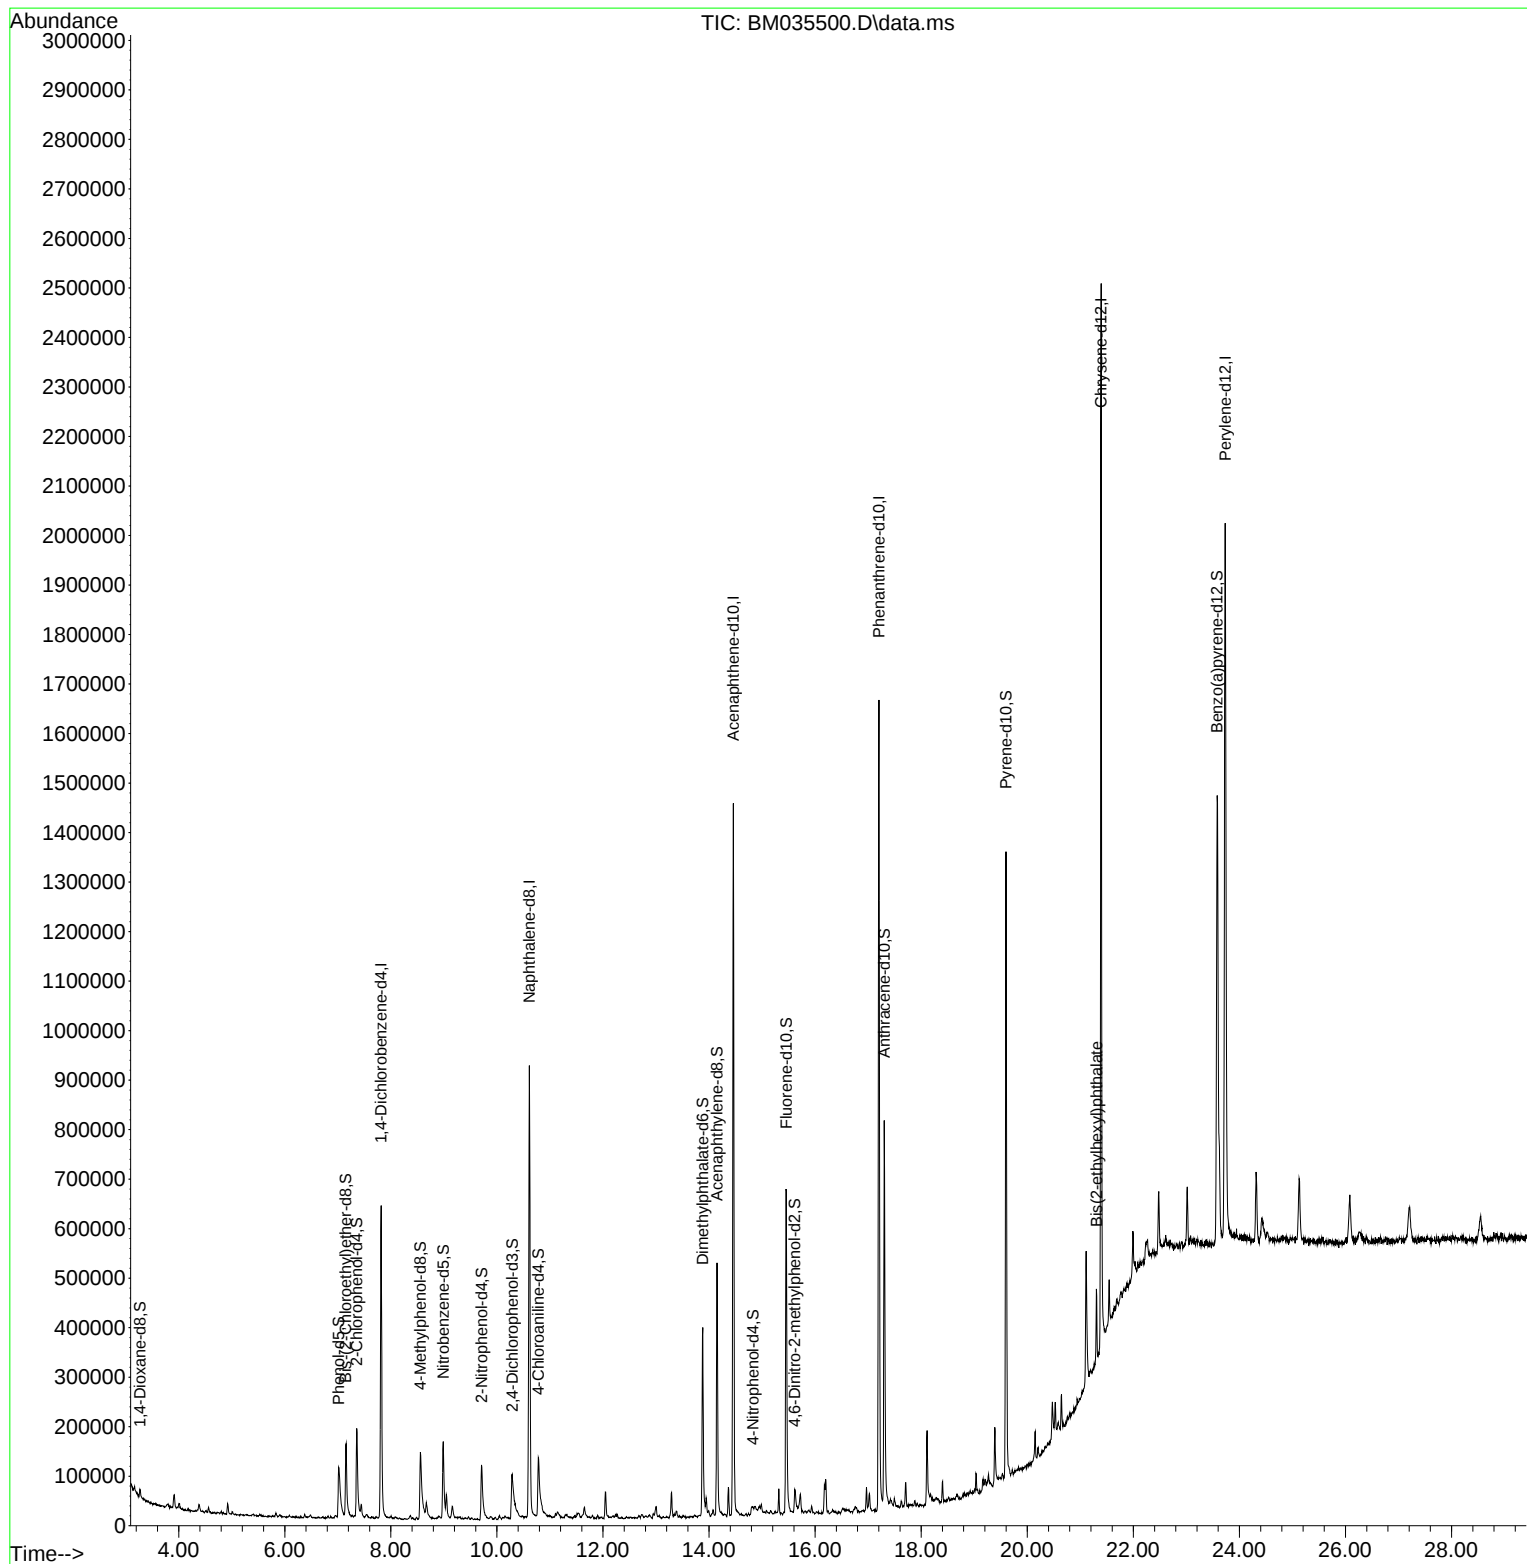

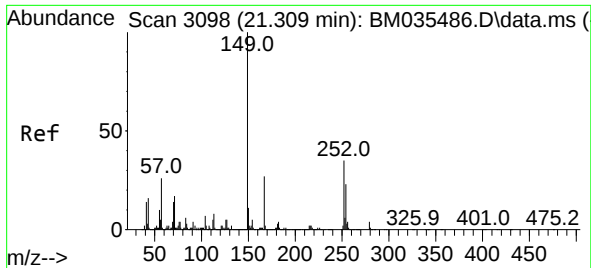

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.129 ng/ul
 RT: 21.303 min Scan# 3097
 Delta R.T. -0.006 min
 Lab File: BM035500.D
 Acq: 17 Jun 2022 18:17

Instrument :
 BNA_M
 ClientSampleId :
 EW4L4

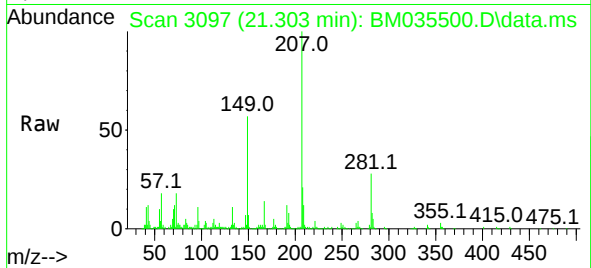

Tgt Ion:149 Resp: 46384

Ion	Ratio	Lower	Upper
149	100		
167	25.4	21.5	32.3
279	3.8	3.4	5.2

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 06/18/2022
 Supervised By :Yogesh Patel 06/22/2022

