

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
 Data File : BM035487.D
 Acq On : 17 Jun 2022 10:15
 Operator : CG/JU
 Sample : PB145488BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK488

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
 Title : SVOA CALIBRATION

Signal : TIC: BM035487.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	27	31	38	rVB	50837	71199	1.46%	0.153%
2	3.687	99	102	122	rBV	451081	840881	17.20%	1.803%
3	4.005	153	156	163	rVB2	14336	22665	0.46%	0.049%
4	7.004	660	666	684	rBV	457638	1043969	21.36%	2.239%
5	7.146	685	690	712	rVB	495143	902887	18.47%	1.936%
6	7.351	719	725	742	rBV	654316	1171039	23.95%	2.511%
7	7.810	797	803	818	rBV	656953	1162681	23.78%	2.493%
8	8.540	921	927	947	rBV	625063	1364763	27.92%	2.927%
9	8.975	994	1001	1015	rBV	562020	1049183	21.46%	2.250%
10	9.704	1118	1125	1143	rBV	435324	863637	17.67%	1.852%
11	10.257	1212	1219	1253	rBV	481510	1252755	25.63%	2.686%
12	10.492	1258	1259	1265	rVB6	3766	5185	0.11%	0.011%
13	10.610	1271	1279	1295	rBV	1004279	1735420	35.50%	3.721%
14	10.757	1296	1304	1343	rBV	826683	2077189	42.49%	4.454%
15	12.251	1551	1558	1564	rBV5	8258	19577	0.40%	0.042%
16	13.875	1827	1834	1853	rBV	1246731	2016964	41.26%	4.325%
17	14.151	1874	1881	1898	rBV	1550878	2432379	49.76%	5.216%
18	14.457	1926	1933	1951	rVV	1483816	2258757	46.20%	4.844%
19	14.733	1974	1980	2011	rBV2	131587	718212	14.69%	1.540%
20	15.051	2030	2034	2041	rVB8	3175	5826	0.12%	0.012%
21	15.451	2095	2102	2119	rBV	2026129	3162528	64.69%	6.782%
22	15.592	2121	2126	2138	rVV	413410	840258	17.19%	1.802%
23	15.698	2141	2144	2157	rVB2	34583	74441	1.52%	0.160%
24	16.239	2231	2236	2240	rVB4	8438	11384	0.23%	0.024%
25	17.004	2363	2366	2373	rVB7	4502	5645	0.12%	0.012%
26	17.204	2393	2400	2410	rBV	1751232	2565576	52.48%	5.502%
27	17.304	2410	2417	2441	rVB	2280964	3546980	72.56%	7.606%
28	17.874	2511	2514	2521	rVB8	6969	9898	0.20%	0.021%
29	18.004	2533	2536	2540	rBV6	2800	5251	0.11%	0.011%
30	18.133	2553	2558	2564	rBV9	11458	24797	0.51%	0.053%
31	19.168	2730	2734	2739	rBV4	27761	37494	0.77%	0.080%
32	19.245	2743	2747	2751	rBV	21465	32007	0.65%	0.069%
33	19.398	2770	2773	2777	rBV6	17211	29815	0.61%	0.064%
34	19.598	2801	2807	2823	rBV	2847436	4126759	84.42%	8.849%
35	21.392	3107	3112	3126	rBV	2089011	3095416	63.32%	6.638%
36	23.580	3477	3484	3501	rBV2	2391785	4888612	100.00%	10.483%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
Data File : BM035487.D
Acq On : 17 Jun 2022 10:15
Operator : CG/JU
Sample : PB145488BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK488

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
Title : SVOA CALIBRATION

37 23.733 3504 3510 3521 rVB2 1477544 3161029 64.66% 6.779%




Sum of corrected areas: 46633058

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
Data File : BM035487.D
Acq On : 17 Jun 2022 10:15
Operator : CG/JU
Sample : PB145488BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK488

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

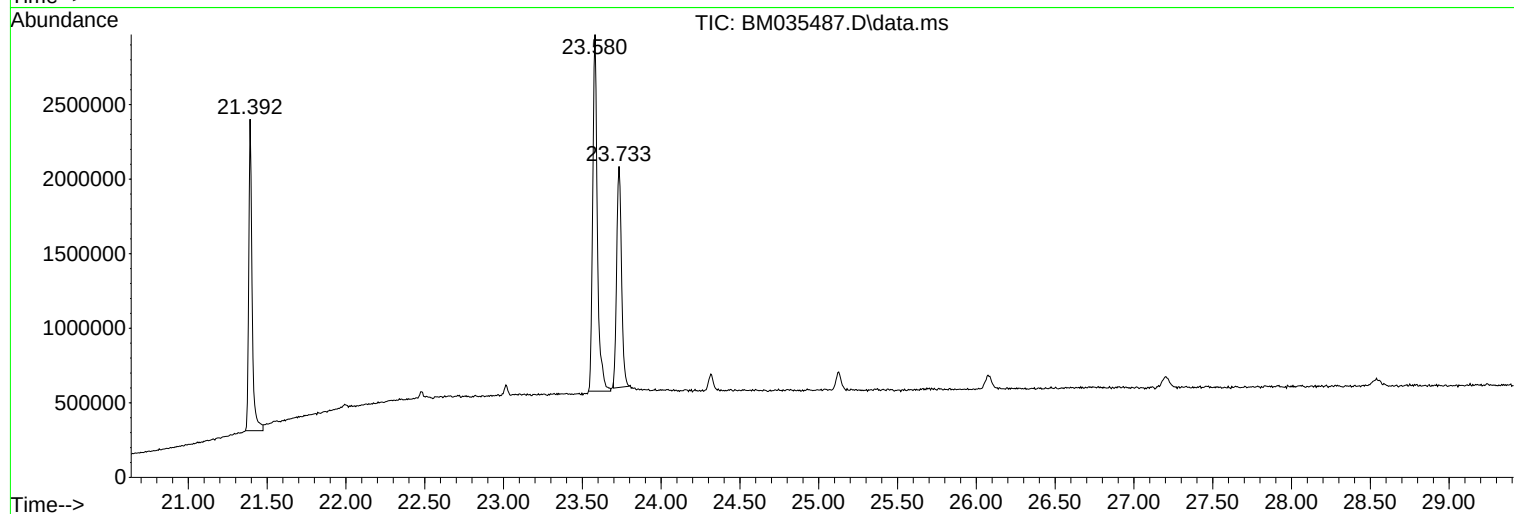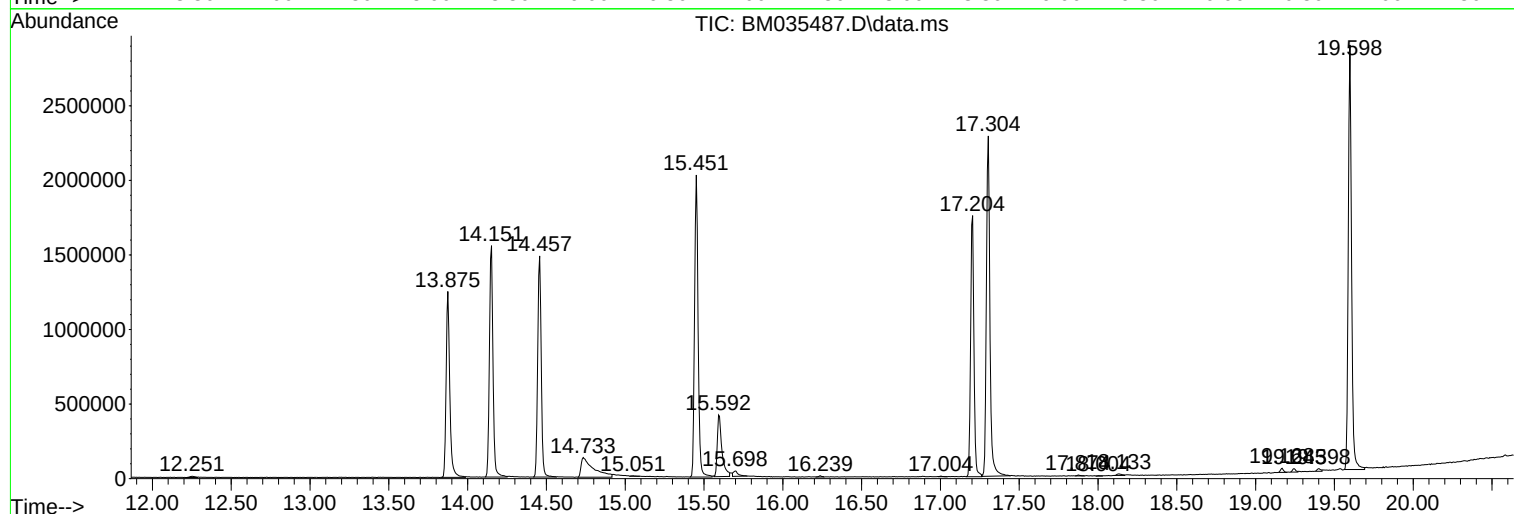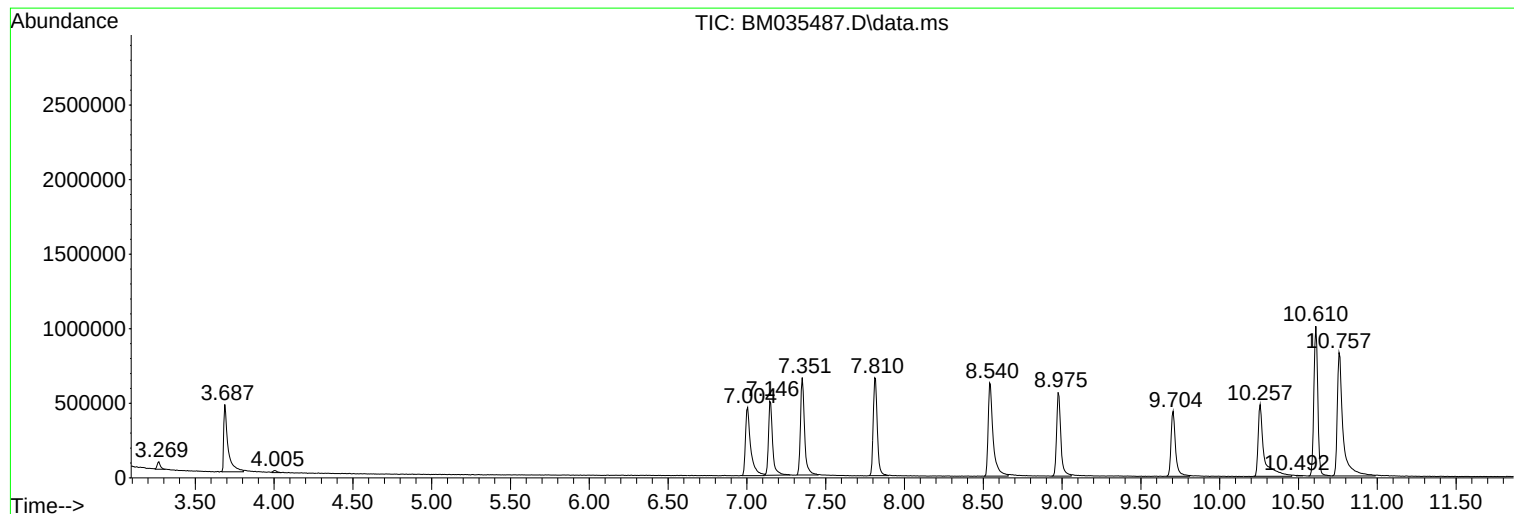

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
Data File : BM035487.D
Acq On : 17 Jun 2022 10:15
Operator : CG/JU
Sample : PB145488BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK488

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
Data File : BM035487.D
Acq On : 17 Jun 2022 10:15
Operator : CG/JU
Sample : PB145488BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK488

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------