

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
 Data File : BM035488.D
 Acq On : 17 Jun 2022 10:54
 Operator : CG/JU
 Sample : N3226-04
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4L5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
 Title : SVOA CALIBRATION

Signal : TIC: BM035488.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	29	31	36	rVB3	24709	29313	0.80%	0.089%
2	3.757	109	114	118	rBV7	8386	21417	0.58%	0.065%
3	3.910	135	140	145	rVB	36410	60610	1.65%	0.183%
4	4.004	153	156	161	rVB2	16163	22100	0.60%	0.067%
5	4.381	216	220	224	rBV5	15460	21961	0.60%	0.066%
6	4.563	247	251	256	rVB	14158	20500	0.56%	0.062%
7	4.798	288	291	296	rVB5	7484	10367	0.28%	0.031%
8	4.922	307	312	322	rVV	42742	65041	1.77%	0.197%
9	5.010	324	327	332	rVB6	8057	11656	0.32%	0.035%
10	5.834	460	467	471	rVV4	14119	23822	0.65%	0.072%
11	6.375	554	559	563	rBV5	10118	18874	0.51%	0.057%
12	6.487	574	578	584	rVB2	10954	13929	0.38%	0.042%
13	6.945	652	656	662	rBV7	9608	20089	0.55%	0.061%
14	7.016	662	668	686	rBV	143687	395327	10.74%	1.195%
15	7.151	686	691	703	rVB	207539	358883	9.75%	1.085%
16	7.357	720	726	737	rVV	244271	474013	12.88%	1.433%
17	7.440	737	740	749	rVV	40384	65668	1.78%	0.199%
18	7.539	753	757	766	rVB10	8843	21082	0.57%	0.064%
19	7.816	795	804	822	rBV	747296	1339458	36.39%	4.050%
20	8.369	891	898	902	rBV8	11964	22304	0.61%	0.067%
21	8.481	911	917	921	rBV6	7768	12303	0.33%	0.037%
22	8.557	924	930	945	rBV	186542	516440	14.03%	1.562%
23	8.669	945	949	958	rVB2	34510	75586	2.05%	0.229%
24	8.916	989	991	996	rVV5	7321	10849	0.29%	0.033%
25	8.981	996	1002	1010	rVV	208368	421191	11.44%	1.274%
26	9.045	1010	1013	1024	rVB	74308	123333	3.35%	0.373%
27	9.163	1024	1033	1038	rBV7	20105	44044	1.20%	0.133%
28	9.463	1079	1084	1089	rVB7	8783	14836	0.40%	0.045%
29	9.522	1089	1094	1100	rBV10	4973	11113	0.30%	0.034%
30	9.710	1119	1126	1136	rBV	152333	347074	9.43%	1.049%
31	9.875	1149	1154	1156	rBV3	8748	11011	0.30%	0.033%
32	9.963	1166	1169	1174	rVB5	8560	13388	0.36%	0.040%
33	10.045	1174	1183	1188	rBV7	13404	29810	0.81%	0.090%
34	10.151	1197	1201	1205	rVB7	8312	10631	0.29%	0.032%
35	10.280	1215	1223	1240	rBV	133947	449879	12.22%	1.360%
36	10.610	1271	1279	1290	rBV	1151477	2097239	56.97%	6.341%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
 Data File : BM035488.D
 Acq On : 17 Jun 2022 10:54
 Operator : CG/JU
 Sample : N3226-04
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4L5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
 Title : SVOA CALIBRATION

37	10.780	1302	1308	1328	rBV	175317	464507	12.62%	1.405%
38	11.104	1359	1363	1365	rBV2	14330	19875	0.54%	0.060%
39	11.127	1365	1367	1377	rVB7	17284	39581	1.08%	0.120%
40	11.292	1390	1395	1397	rBV6	10124	16803	0.46%	0.051%
41	11.316	1397	1399	1404	rVB5	9137	12688	0.34%	0.038%
42	11.522	1429	1434	1436	rBV6	10233	19524	0.53%	0.059%
43	11.645	1449	1455	1464	rVV3	31685	66211	1.80%	0.200%
44	11.804	1476	1482	1486	rVB7	11132	20473	0.56%	0.062%
45	11.898	1492	1498	1503	rBV7	11865	21207	0.58%	0.064%
46	11.975	1508	1511	1517	rVB7	7063	11733	0.32%	0.035%
47	12.045	1517	1523	1534	rBV	97544	176968	4.81%	0.535%
48	12.239	1551	1556	1558	rBV6	8355	17029	0.46%	0.051%
49	12.686	1623	1632	1635	rBV10	9333	23264	0.63%	0.070%
50	12.733	1636	1640	1647	rVB7	13952	30564	0.83%	0.092%
51	12.951	1672	1677	1678	rBV5	12227	15901	0.43%	0.048%
52	12.998	1679	1685	1691	rVB2	37898	75139	2.04%	0.227%
53	13.286	1726	1734	1742	rBV	94162	159657	4.34%	0.483%
54	13.386	1746	1751	1757	rVV3	21450	39978	1.09%	0.121%
55	13.439	1758	1760	1765	rVB6	6554	10514	0.29%	0.032%
56	13.810	1817	1823	1824	rBV6	7589	13123	0.36%	0.040%
57	13.874	1829	1834	1843	rVV	501951	841171	22.85%	2.543%
58	13.945	1843	1846	1850	rVV2	55339	82200	2.23%	0.249%
59	13.992	1850	1854	1860	rVB6	17291	27140	0.74%	0.082%
60	14.068	1864	1867	1873	rVB2	16825	24426	0.66%	0.074%
61	14.151	1874	1881	1893	rBV	637192	1006630	27.35%	3.044%
62	14.363	1912	1917	1923	rBV	105426	144667	3.93%	0.437%
63	14.457	1923	1933	1947	rBV	1700599	2633531	71.54%	7.963%
64	14.804	1985	1992	1994	rBV5	26711	56579	1.54%	0.171%
65	14.868	2000	2003	2009	rVB8	14670	19936	0.54%	0.060%
66	14.980	2020	2022	2031	rVB6	27927	46262	1.26%	0.140%
67	15.163	2049	2053	2056	rBV4	11852	17138	0.47%	0.052%
68	15.315	2075	2079	2083	rVB	87129	104504	2.84%	0.316%
69	15.451	2096	2102	2118	rVV	840696	1353808	36.78%	4.094%
70	15.615	2125	2130	2138	rBV4	55786	120074	3.26%	0.363%
71	15.721	2143	2148	2157	rVB	62822	121718	3.31%	0.368%
72	15.810	2161	2163	2168	rVB6	11787	16093	0.44%	0.049%
73	15.880	2171	2175	2180	rBV8	11766	19420	0.53%	0.059%
74	15.933	2180	2184	2188	rBV4	22011	29257	0.79%	0.088%
75	16.174	2221	2225	2227	rBV	99036	131760	3.58%	0.398%
76	16.198	2227	2229	2234	rVB	107870	134668	3.66%	0.407%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
 Data File : BM035488.D
 Acq On : 17 Jun 2022 10:54
 Operator : CG/JU
 Sample : N3226-04
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4L5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
 Title : SVOA CALIBRATION

77	16.515	2278	2283	2286	rBV3	14507	23871	0.65%	0.072%
78	16.968	2356	2360	2364	rBV	68973	84280	2.29%	0.255%
79	17.021	2365	2369	2382	rVB2	59524	98197	2.67%	0.297%
80	17.204	2394	2400	2411	rBV	2029123	3002673	81.57%	9.079%
81	17.304	2411	2417	2430	rVB	903995	1468103	39.88%	4.439%
82	17.492	2445	2449	2455	rVB5	17769	33226	0.90%	0.100%
83	17.621	2468	2471	2479	rVB8	16592	27872	0.76%	0.084%
84	17.709	2479	2486	2492	rVB	77033	108889	2.96%	0.329%
85	17.874	2511	2514	2519	rVB7	16992	24828	0.67%	0.075%
86	18.109	2548	2554	2564	rBV2	112241	227382	6.18%	0.688%
87	18.398	2600	2603	2608	rBV	64331	78334	2.13%	0.237%
88	19.039	2708	2712	2719	rVB	59375	82666	2.25%	0.250%
89	19.162	2729	2733	2736	rBV4	26109	42799	1.16%	0.129%
90	19.386	2767	2771	2780	rBV	88685	151470	4.11%	0.458%
91	19.598	2802	2807	2821	rBV	1307896	1920800	52.18%	5.808%
92	20.150	2897	2901	2905	rVB	79609	87073	2.37%	0.263%
93	20.527	2962	2965	2970	rVB	91410	102146	2.77%	0.309%
94	20.645	2982	2985	2990	rVB	104732	111740	3.04%	0.338%
95	21.109	3060	3064	3069	rBV2	197406	275348	7.48%	0.833%
96	21.392	3107	3112	3123	rBV	2571730	3503645	95.18%	10.594%
97	21.544	3135	3138	3141	rBV	128834	142476	3.87%	0.431%
98	22.480	3294	3297	3305	rVB3	185939	255652	6.95%	0.773%
99	23.580	3479	3484	3498	rVB2	952014	2146625	58.32%	6.491%
100	23.733	3503	3510	3524	rVB2	1763188	3681062	100.00%	11.130%




Sum of corrected areas: 33072019

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
Data File : BM035488.D
Acq On : 17 Jun 2022 10:54
Operator : CG/JU
Sample : N3226-04
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4L5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

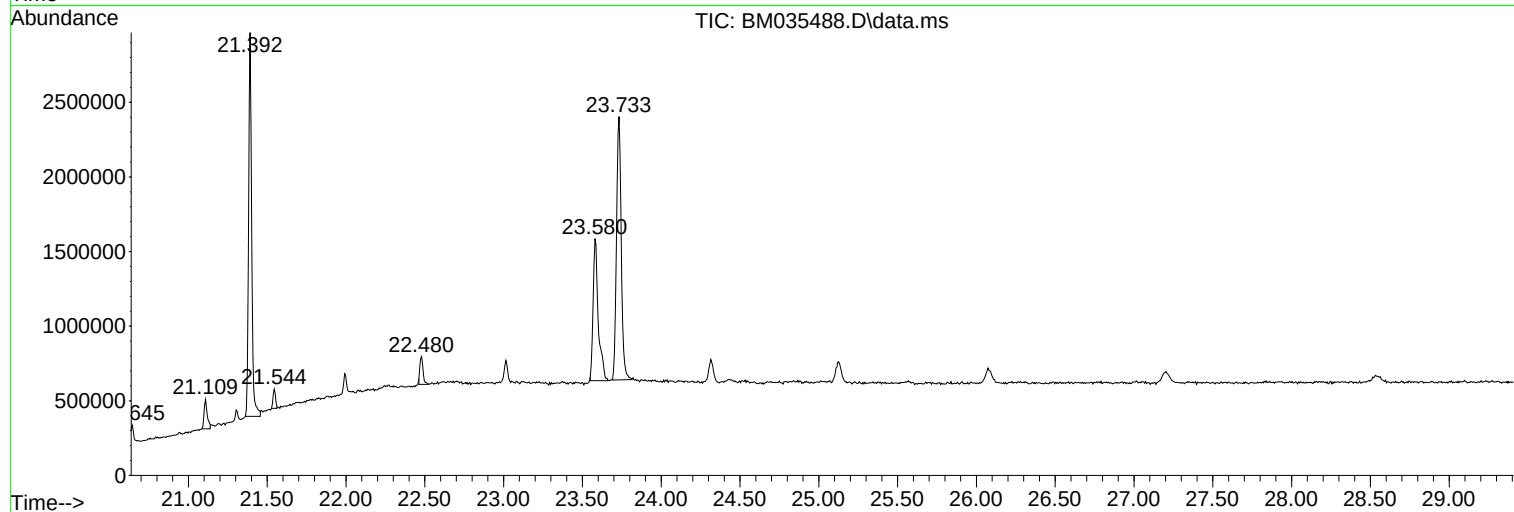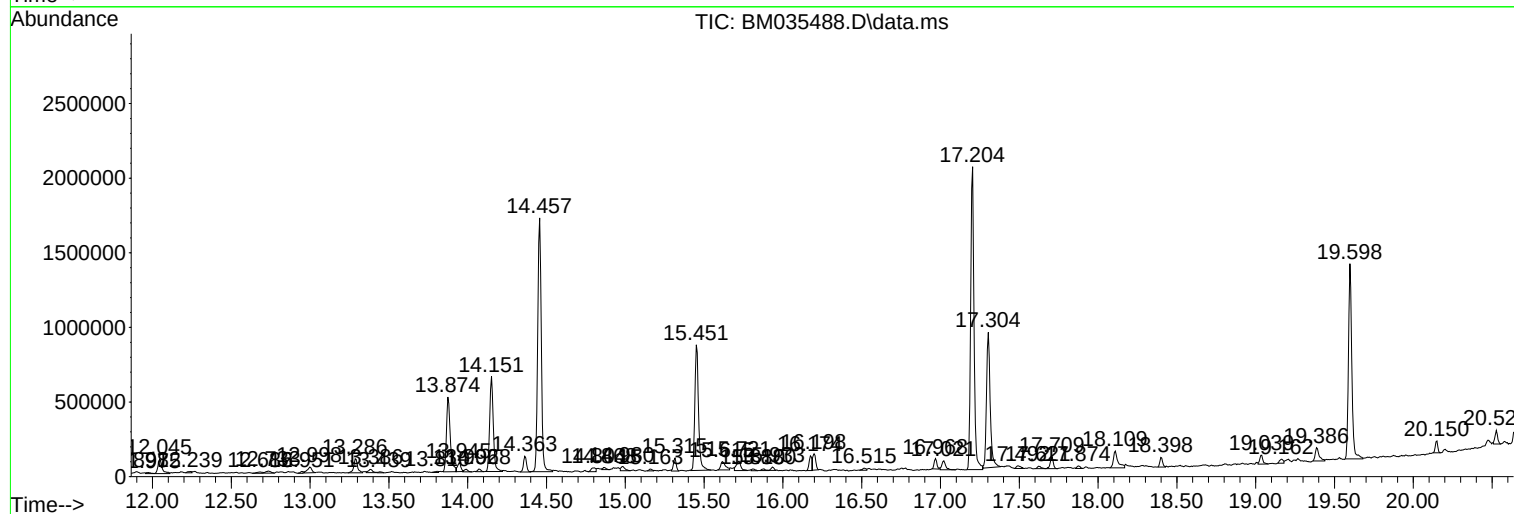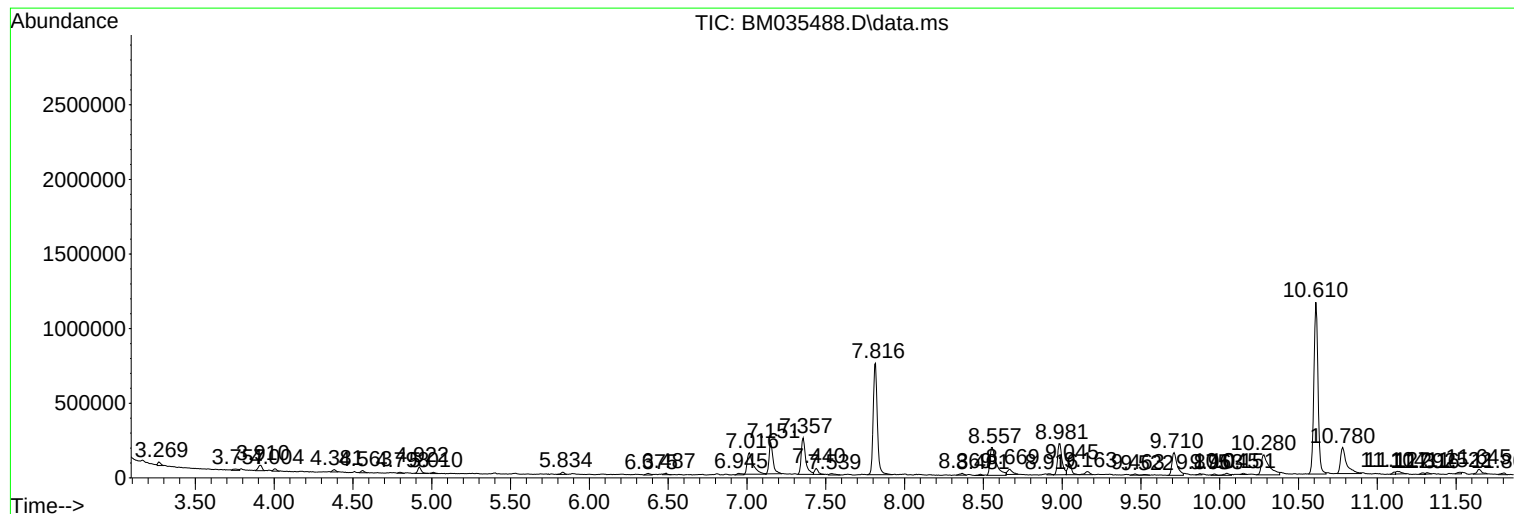

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
Data File : BM035488.D
Acq On : 17 Jun 2022 10:54
Operator : CG/JU
Sample : N3226-04
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4L5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
Data File : BM035488.D
Acq On : 17 Jun 2022 10:54
Operator : CG/JU
Sample : N3226-04
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4L5

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc