

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
 Data File : BM035494.D
 Acq On : 17 Jun 2022 14:35
 Operator : CG/JU
 Sample : N3226-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4M4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
 Title : SVOA CALIBRATION

Signal : TIC: BM035494.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	29	31	39	rVB2	21174	34178	1.14%	0.131%
2	3.910	136	140	146	rVB2	25328	43666	1.45%	0.168%
3	4.004	154	156	161	rVB3	13298	18866	0.63%	0.073%
4	4.387	217	221	226	rBV8	4996	9553	0.32%	0.037%
5	4.563	248	251	256	rVB2	9202	11945	0.40%	0.046%
6	4.810	287	293	294	rBV5	6446	9510	0.32%	0.037%
7	4.922	308	312	320	rVB	27835	39324	1.31%	0.151%
8	6.375	554	559	564	rBV9	4206	8593	0.29%	0.033%
9	6.875	640	644	647	rVB6	3738	5932	0.20%	0.023%
10	6.951	653	657	663	rBV8	5426	11614	0.39%	0.045%
11	7.022	663	669	686	rBV	106500	315945	10.50%	1.215%
12	7.157	686	692	705	rVV	145277	272843	9.07%	1.050%
13	7.357	721	726	738	rBV	177715	364624	12.12%	1.403%
14	7.439	738	740	749	rVB4	14797	25241	0.84%	0.097%
15	7.816	795	804	822	rBV	613818	1096382	36.45%	4.218%
16	8.369	895	898	904	rVB8	5071	8714	0.29%	0.034%
17	8.563	924	931	946	rBV	134929	395148	13.14%	1.520%
18	8.675	946	950	958	rVB	21271	45428	1.51%	0.175%
19	8.986	997	1003	1011	rBV	161464	325126	10.81%	1.251%
20	9.051	1011	1014	1023	rVV2	32453	60205	2.00%	0.232%
21	9.122	1023	1026	1029	rVV4	4030	6614	0.22%	0.025%
22	9.163	1030	1033	1040	rVB8	4402	8735	0.29%	0.034%
23	9.469	1080	1085	1089	rVB7	4522	7176	0.24%	0.028%
24	9.710	1119	1126	1144	rBV	114316	284654	9.46%	1.095%
25	9.963	1165	1169	1175	rVB6	4804	9561	0.32%	0.037%
26	10.045	1178	1183	1191	rBV10	6437	17079	0.57%	0.066%
27	10.151	1196	1201	1208	rBV7	4847	11118	0.37%	0.043%
28	10.286	1218	1224	1241	rBV2	86556	331703	11.03%	1.276%
29	10.610	1271	1279	1298	rBV	903993	1646900	54.75%	6.336%
30	10.780	1302	1308	1320	rBV	119640	332959	11.07%	1.281%
31	11.104	1358	1363	1366	rBV6	7063	12090	0.40%	0.047%
32	11.145	1366	1370	1383	rVB10	13181	31414	1.04%	0.121%
33	11.292	1389	1395	1397	rBV6	6394	10198	0.34%	0.039%
34	11.463	1419	1424	1427	rBV7	3013	5751	0.19%	0.022%
35	11.651	1449	1456	1465	rBV4	16029	36215	1.20%	0.139%
36	11.798	1476	1481	1489	rVB10	7432	16220	0.54%	0.062%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
 Data File : BM035494.D
 Acq On : 17 Jun 2022 14:35
 Operator : CG/JU
 Sample : N3226-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4M4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
 Title : SVOA CALIBRATION

37	11.898	1496	1498	1504	rVB6	5994	7374	0.25%	0.028%
38	11.974	1509	1511	1517	rVB7	3906	6291	0.21%	0.024%
39	12.045	1517	1523	1532	rBV	42687	83395	2.77%	0.321%
40	12.239	1551	1556	1557	rBV5	5581	6578	0.22%	0.025%
41	12.339	1569	1573	1579	rBV7	4755	10171	0.34%	0.039%
42	12.451	1583	1592	1594	rBV10	4973	9280	0.31%	0.036%
43	12.680	1628	1631	1635	rVV5	4312	7529	0.25%	0.029%
44	12.745	1635	1642	1648	rVV7	6764	15282	0.51%	0.059%
45	12.816	1648	1654	1656	rVV6	4646	8981	0.30%	0.035%
46	12.863	1659	1662	1665	rBV5	4831	6558	0.22%	0.025%
47	13.004	1679	1686	1691	rVB6	18960	33155	1.10%	0.128%
48	13.292	1726	1735	1742	rBV	45474	81683	2.72%	0.314%
49	13.351	1742	1745	1746	rVV3	6277	8025	0.27%	0.031%
50	13.386	1749	1751	1757	rVV5	10591	14436	0.48%	0.056%
51	13.451	1760	1762	1767	rVB6	4396	6405	0.21%	0.025%
52	13.727	1804	1809	1812	rBV7	4502	7541	0.25%	0.029%
53	13.880	1827	1835	1843	rBV	390451	675965	22.47%	2.601%
54	13.945	1844	1846	1851	rVV2	30057	41860	1.39%	0.161%
55	13.986	1851	1853	1858	rVB6	8731	11906	0.40%	0.046%
56	14.074	1860	1868	1873	rBV8	8605	21124	0.70%	0.081%
57	14.151	1873	1881	1892	rBV	506845	816022	27.13%	3.139%
58	14.363	1913	1917	1925	rVB	47914	65580	2.18%	0.252%
59	14.457	1925	1933	1942	rBV	1374517	2082731	69.24%	8.013%
60	14.692	1971	1973	1977	rVB5	4108	5885	0.20%	0.023%
61	14.815	1987	1994	1998	rBV9	17331	43703	1.45%	0.168%
62	14.863	2000	2002	2008	rVB6	7365	13261	0.44%	0.051%
63	14.986	2021	2023	2027	rVB5	13091	13440	0.45%	0.052%
64	15.157	2050	2052	2055	rBV4	5298	6061	0.20%	0.023%
65	15.251	2065	2068	2072	rVB6	5059	8170	0.27%	0.031%
66	15.315	2075	2079	2083	rVB	41035	49884	1.66%	0.192%
67	15.457	2097	2103	2114	rVV	652931	1114538	37.05%	4.288%
68	15.627	2126	2132	2138	rBV3	37080	80378	2.67%	0.309%
69	15.721	2142	2148	2153	rVB3	29320	60382	2.01%	0.232%
70	15.880	2171	2175	2179	rVV7	7353	9816	0.33%	0.038%
71	15.939	2181	2185	2190	rVB4	12344	17641	0.59%	0.068%
72	16.174	2221	2225	2227	rVV2	47178	62060	2.06%	0.239%
73	16.198	2227	2229	2234	rVB2	55470	67218	2.23%	0.259%
74	16.327	2242	2251	2254	rBV10	7883	19663	0.65%	0.076%
75	16.515	2281	2283	2287	rBV4	6773	10981	0.37%	0.042%
76	16.574	2292	2293	2298	rVB5	5839	6375	0.21%	0.025%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
 Data File : BM035494.D
 Acq On : 17 Jun 2022 14:35
 Operator : CG/JU
 Sample : N3226-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4M4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
 Title : SVOA CALIBRATION

77	16.733	2317	2320	2322	rBV4	3815	5694	0.19%	0.022%
78	16.968	2355	2360	2365	rBV	39716	54057	1.80%	0.208%
79	17.021	2365	2369	2373	rVB4	25379	41556	1.38%	0.160%
80	17.204	2394	2400	2411	rBV	1607266	2377551	79.04%	9.147%
81	17.304	2411	2417	2434	rVV2	743334	1314951	43.71%	5.059%
82	17.421	2435	2437	2445	rVV8	18394	39610	1.32%	0.152%
83	17.498	2446	2450	2455	rVB6	13402	24817	0.83%	0.095%
84	17.615	2468	2470	2471	rBV2	8036	6782	0.23%	0.026%
85	17.709	2482	2486	2491	rVB	38555	50992	1.70%	0.196%
86	17.886	2511	2516	2520	rVB7	10673	16011	0.53%	0.062%
87	17.927	2520	2523	2527	rVB6	6514	8813	0.29%	0.034%
88	18.109	2549	2554	2562	rBV	106459	195692	6.51%	0.753%
89	18.403	2600	2604	2607	rBV2	33791	38201	1.27%	0.147%
90	19.033	2708	2711	2718	rVB	34067	46873	1.56%	0.180%
91	19.168	2729	2734	2736	rBV6	24541	39449	1.31%	0.152%
92	19.392	2768	2772	2780	rBV3	54756	98881	3.29%	0.380%
93	19.597	2802	2807	2821	rBV	1114963	1697580	56.43%	6.531%
94	20.145	2898	2900	2905	rVB	58498	67486	2.24%	0.260%
95	20.644	2982	2985	2989	rBV2	75427	82181	2.73%	0.316%
96	21.109	3060	3064	3073	rBV	250865	426153	14.17%	1.639%
97	21.391	3107	3112	3125	rBV	2147758	2892890	96.17%	11.129%
98	21.544	3135	3138	3142	rBV	112238	124625	4.14%	0.479%
99	23.580	3479	3484	3498	rVB2	799496	1845627	61.35%	7.100%
100	23.733	3504	3510	3524	rVB2	1404877	3008114	100.00%	11.573%




Sum of corrected areas: 25993138

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
Data File : BM035494.D
Acq On : 17 Jun 2022 14:35
Operator : CG/JU
Sample : N3226-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4M4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

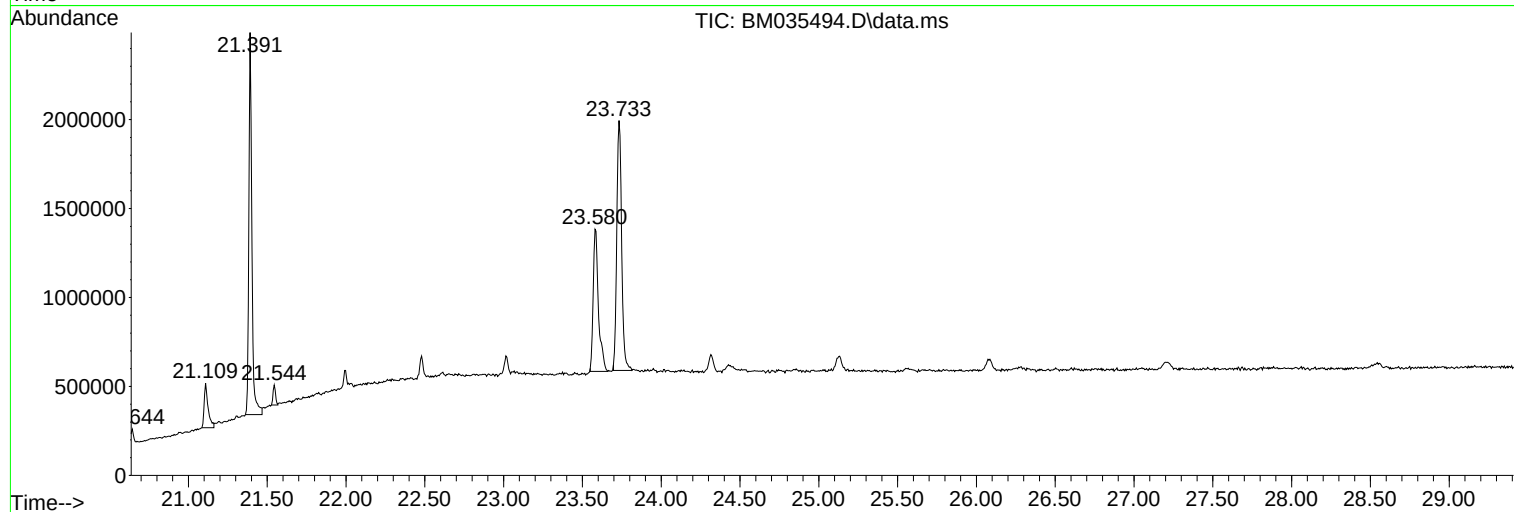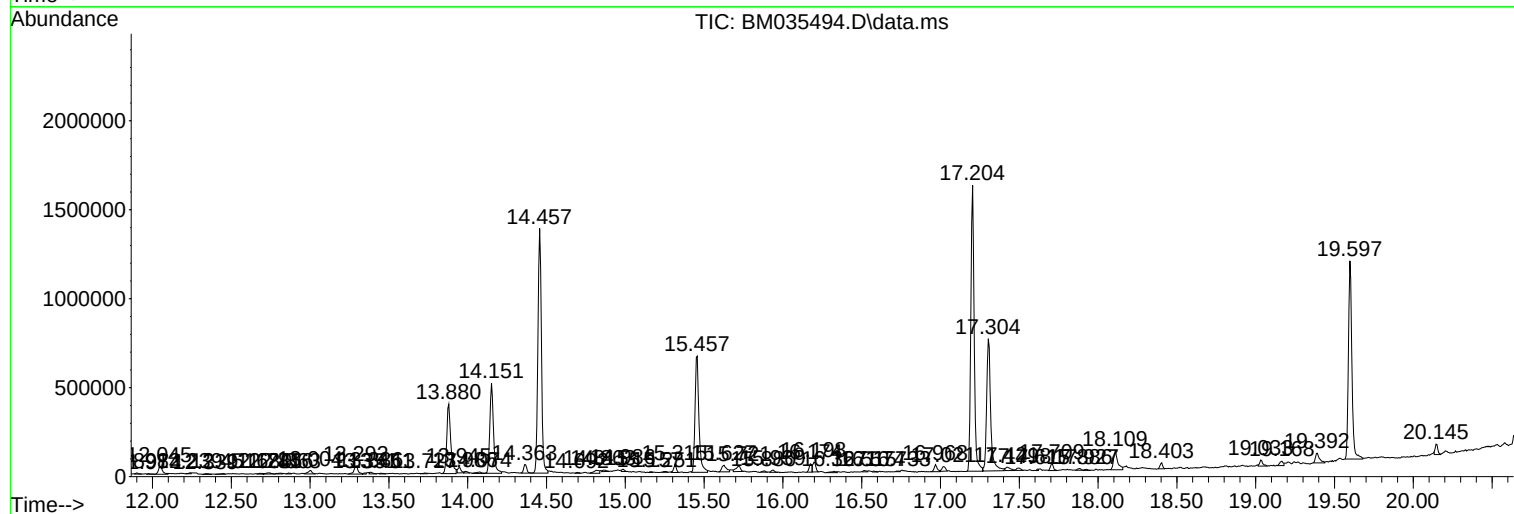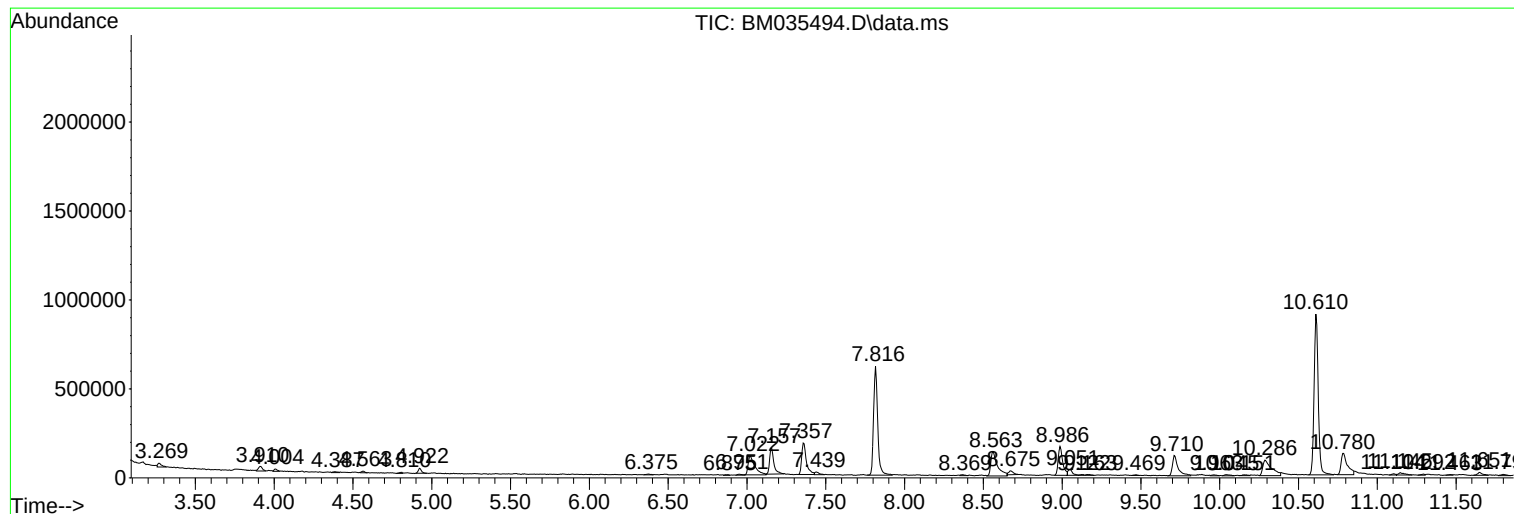

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
Data File : BM035494.D
Acq On : 17 Jun 2022 14:35
Operator : CG/JU
Sample : N3226-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4M4










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetratriacontyl trifluoroac... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.109	2.95 ng/ul	426153	Chrysene-d12	21.392

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetratriacontyl trifluoroacetate	591	C36H69F3O2	1000351-75-3	91
2			Octacosyl trifluoroacetate	506	C30H57F3O2	1000351-74-9	91
3			Dotriacontyl heptafluorobutyrate	662	C36H65F7O2	1000351-84-2	91
4			Hexatriacontyl pentafluoropropio...	669	C39H73F5O2	1000351-89-0	91
5			1-Dodecanol, 2-octyl-	298	C20H42O	005333-42-6	91

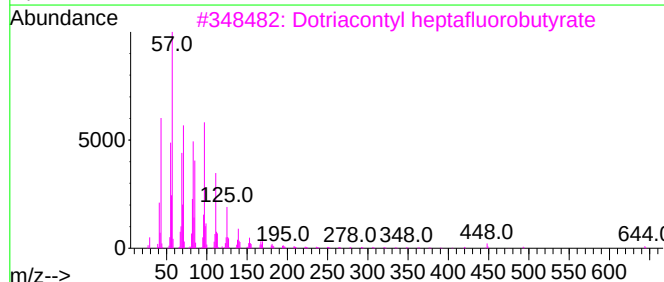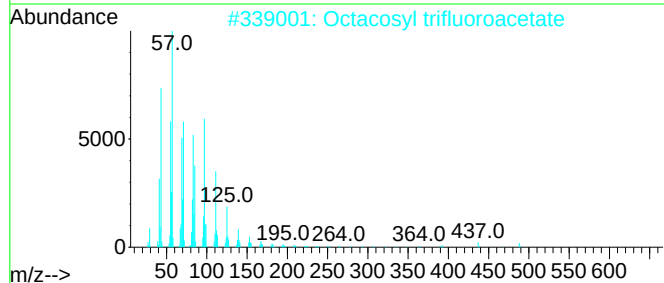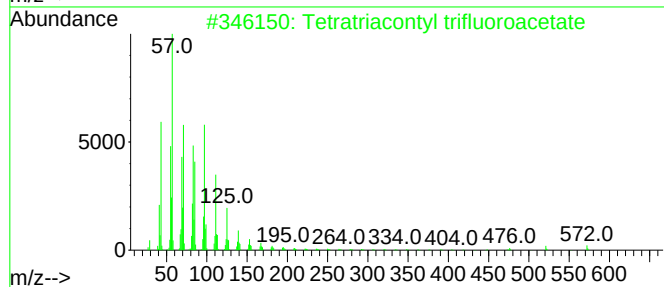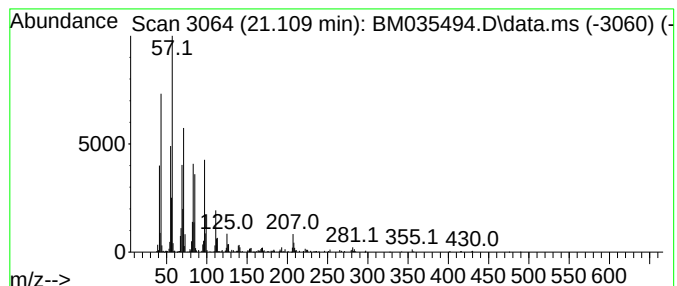

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
Data File : BM035494.D
Acq On : 17 Jun 2022 14:35
Operator : CG/JU
Sample : N3226-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4M4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetratriacontyl...	21.109	3.0	ng/u1	426153	5	21.392	2892890	20.0