

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
 Data File : BM035495.D
 Acq On : 17 Jun 2022 15:12
 Operator : CG/JU
 Sample : N3226-14
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4N4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
 Title : SVOA CALIBRATION

Signal : TIC: BM035495.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.269	28	31	42	rVB	38631	60934	1.71%	0.164%
2	3.699	101	104	118	rBV	130411	270976	7.61%	0.731%
3	3.916	136	141	146	rVB	26881	44565	1.25%	0.120%
4	4.005	154	156	162	rVB	12764	17884	0.50%	0.048%
5	4.387	218	221	226	rBV6	3969	5992	0.17%	0.016%
6	4.557	247	250	255	rVB	9581	13609	0.38%	0.037%
7	4.799	288	291	295	rVV5	4786	6944	0.19%	0.019%
8	4.922	308	312	318	rBV	29020	44755	1.26%	0.121%
9	5.834	462	467	471	rBV8	5993	9183	0.26%	0.025%
10	6.381	553	560	565	rVB10	4338	8330	0.23%	0.022%
11	6.487	575	578	583	rVB6	4960	7599	0.21%	0.020%
12	6.951	653	657	661	rBV6	5951	10596	0.30%	0.029%
13	7.010	661	667	685	rVV	267488	676785	19.00%	1.826%
14	7.151	685	691	705	rVB	323993	550918	15.47%	1.486%
15	7.351	719	725	738	rBV	394597	735188	20.64%	1.983%
16	7.440	738	740	745	rVB3	14325	18198	0.51%	0.049%
17	7.816	795	804	816	rBV	622666	1087957	30.55%	2.935%
18	8.363	893	897	902	rVB7	5305	8423	0.24%	0.023%
19	8.545	922	928	942	rBV	372391	834227	23.42%	2.250%
20	8.657	943	947	957	rVB	58649	120408	3.38%	0.325%
21	8.904	984	989	994	rBV7	3013	6187	0.17%	0.017%
22	8.981	996	1002	1010	rVV	348848	649189	18.23%	1.751%
23	9.045	1010	1013	1022	rVB3	26793	51580	1.45%	0.139%
24	9.704	1119	1125	1145	rBV	257418	552742	15.52%	1.491%
25	10.045	1176	1183	1187	rBV7	4205	8579	0.24%	0.023%
26	10.098	1187	1192	1196	rVB7	3969	7186	0.20%	0.019%
27	10.263	1214	1220	1250	rBV	250362	784850	22.04%	2.117%
28	10.610	1271	1279	1290	rBV	943543	1678354	47.12%	4.528%
29	10.769	1299	1306	1334	rBV	288616	815546	22.90%	2.200%
30	11.110	1358	1364	1368	rBV8	9275	16426	0.46%	0.044%
31	11.286	1390	1394	1397	rBV5	4399	6509	0.18%	0.018%
32	11.539	1431	1437	1443	rVB9	7789	17526	0.49%	0.047%
33	11.651	1447	1456	1465	rBV3	18457	41657	1.17%	0.112%
34	11.804	1478	1482	1490	rVB8	7817	14414	0.40%	0.039%
35	11.898	1494	1498	1504	rVV6	6229	11101	0.31%	0.030%
36	12.051	1516	1524	1532	rBV	49228	91047	2.56%	0.246%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
 Data File : BM035495.D
 Acq On : 17 Jun 2022 15:12
 Operator : CG/JU
 Sample : N3226-14
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4N4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
 Title : SVOA CALIBRATION

37	12.186	1544	1547	1550	rBV5	4719	6076	0.17%	0.016%
38	12.233	1550	1555	1558	rBV7	8004	14355	0.40%	0.039%
39	12.528	1603	1605	1609	rVB5	4457	6234	0.18%	0.017%
40	12.680	1626	1631	1636	rBV6	5492	11002	0.31%	0.030%
41	12.792	1647	1650	1653	rBV5	3708	6258	0.18%	0.017%
42	12.863	1659	1662	1665	rVV5	6096	8864	0.25%	0.024%
43	12.892	1665	1667	1673	rVB7	5919	7923	0.22%	0.021%
44	12.951	1673	1677	1679	rBV5	6860	7840	0.22%	0.021%
45	13.004	1679	1686	1690	rVB2	20966	36249	1.02%	0.098%
46	13.292	1724	1735	1741	rBV	57743	101155	2.84%	0.273%
47	13.351	1741	1745	1747	rVV5	6675	10307	0.29%	0.028%
48	13.380	1747	1750	1755	rVB6	7502	12888	0.36%	0.035%
49	13.457	1760	1763	1767	rVB5	5201	6337	0.18%	0.017%
50	13.516	1769	1773	1777	rBV7	6650	10012	0.28%	0.027%
51	13.792	1815	1820	1821	rBV5	6987	9383	0.26%	0.025%
52	13.875	1828	1834	1843	rBV	847160	1334509	37.47%	3.600%
53	13.945	1843	1846	1850	rVV	35864	52718	1.48%	0.142%
54	13.992	1850	1854	1861	rVB9	9682	19607	0.55%	0.053%
55	14.074	1862	1868	1873	rVB5	11905	20163	0.57%	0.054%
56	14.151	1874	1881	1891	rBV	1026154	1605720	45.08%	4.332%
57	14.363	1912	1917	1924	rBV	70534	94654	2.66%	0.255%
58	14.457	1925	1933	1948	rBV	1433466	2181706	61.26%	5.885%
59	14.751	1978	1983	1994	rBV4	65755	264549	7.43%	0.714%
60	14.921	2009	2012	2016	rVV6	14196	17051	0.48%	0.046%
61	14.986	2020	2023	2032	rVB9	21429	41730	1.17%	0.113%
62	15.045	2032	2033	2037	rBV4	4921	5863	0.16%	0.016%
63	15.086	2037	2040	2045	rVB7	9453	15793	0.44%	0.043%
64	15.157	2049	2052	2058	rBV6	7908	13713	0.39%	0.037%
65	15.316	2075	2079	2083	rVB	59665	71556	2.01%	0.193%
66	15.410	2091	2095	2096	rBV4	8100	8840	0.25%	0.024%
67	15.451	2096	2102	2115	rVV	1393473	2154356	60.49%	5.812%
68	15.604	2122	2128	2140	rBV	205787	449497	12.62%	1.213%
69	15.721	2141	2148	2156	rVV3	47701	122156	3.43%	0.330%
70	15.810	2160	2163	2170	rVB8	10629	20183	0.57%	0.054%
71	15.874	2170	2174	2179	rBV8	8733	15389	0.43%	0.042%
72	15.939	2181	2185	2193	rVB5	17913	33001	0.93%	0.089%
73	16.174	2221	2225	2227	rBV2	66876	90644	2.55%	0.245%
74	16.198	2227	2229	2233	rVV	75515	91788	2.58%	0.248%
75	16.239	2233	2236	2242	rVB8	13233	16345	0.46%	0.044%
76	16.386	2259	2261	2265	rVB5	8000	8896	0.25%	0.024%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
 Data File : BM035495.D
 Acq On : 17 Jun 2022 15:12
 Operator : CG/JU
 Sample : N3226-14
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EW4N4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
 Title : SVOA CALIBRATION

77	16.427	2265	2268	2271	rBV5	4224	5874	0.16%	0.016%
78	16.515	2280	2283	2287	rVV6	10250	14945	0.42%	0.040%
79	16.968	2352	2360	2364	rBV2	57616	89336	2.51%	0.241%
80	17.021	2365	2369	2379	rVB2	45009	80103	2.25%	0.216%
81	17.204	2394	2400	2411	rBV	1719977	2524248	70.87%	6.810%
82	17.304	2411	2417	2431	rVV	1513498	2355528	66.14%	6.354%
83	17.492	2446	2449	2455	rVB5	17031	31862	0.89%	0.086%
84	17.627	2468	2472	2478	rBV7	14379	26403	0.74%	0.071%
85	17.710	2481	2486	2490	rBV	59426	78393	2.20%	0.211%
86	18.110	2549	2554	2562	rBV6	61441	113081	3.17%	0.305%
87	18.280	2579	2583	2587	rBV5	14567	21234	0.60%	0.057%
88	18.404	2600	2604	2607	rBV	48968	59320	1.67%	0.160%
89	18.804	2670	2672	2675	rVB3	12070	11992	0.34%	0.032%
90	19.033	2708	2711	2719	rVB	53901	77088	2.16%	0.208%
91	19.162	2729	2733	2738	rBV6	33509	59567	1.67%	0.161%
92	19.239	2744	2746	2749	rBV	16534	17973	0.50%	0.048%
93	19.392	2769	2772	2778	rVB5	31321	44995	1.26%	0.121%
94	19.598	2801	2807	2815	rBV	2200135	3074947	86.34%	8.295%
95	20.151	2898	2901	2904	rVB2	57525	60515	1.70%	0.163%
96	20.645	2982	2985	2989	rVB2	63690	68438	1.92%	0.185%
97	21.109	3060	3064	3075	rBV2	170920	322245	9.05%	0.869%
98	21.392	3107	3112	3123	rBV	2118737	2964294	83.23%	7.997%
99	23.580	3478	3484	3499	rBV2	1611831	3561634	100.00%	9.608%
100	23.733	3504	3510	3527	rVB2	1489892	3113552	87.42%	8.399%




Sum of corrected areas: 37069241

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
Data File : BM035495.D
Acq On : 17 Jun 2022 15:12
Operator : CG/JU
Sample : N3226-14
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4N4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

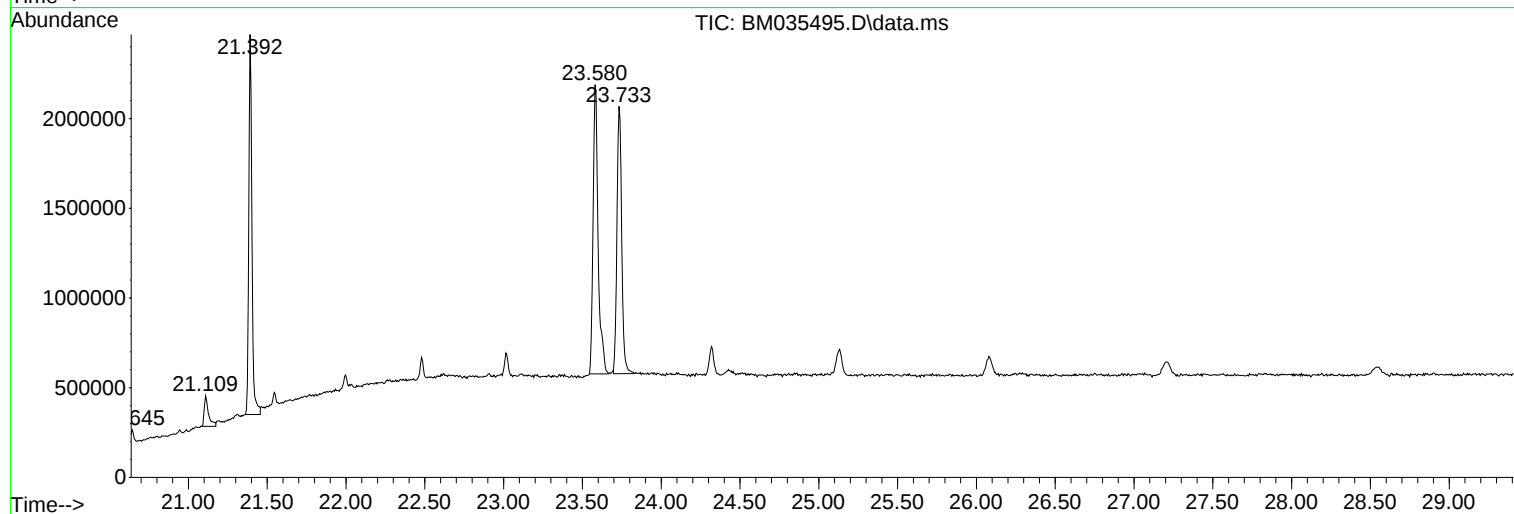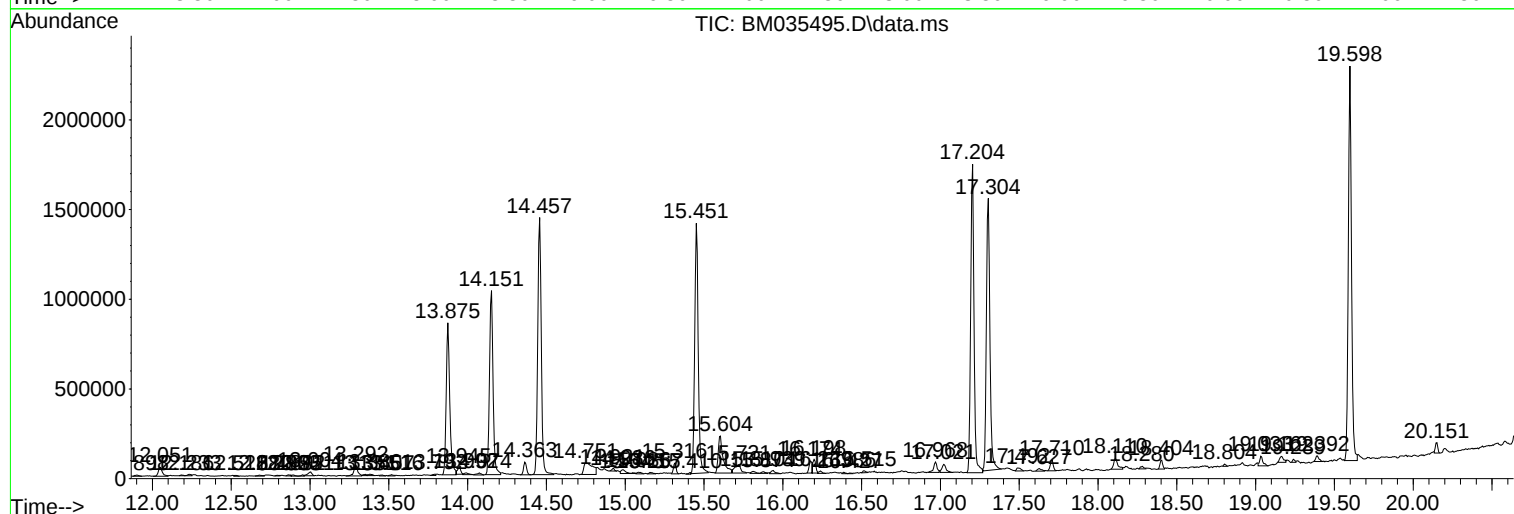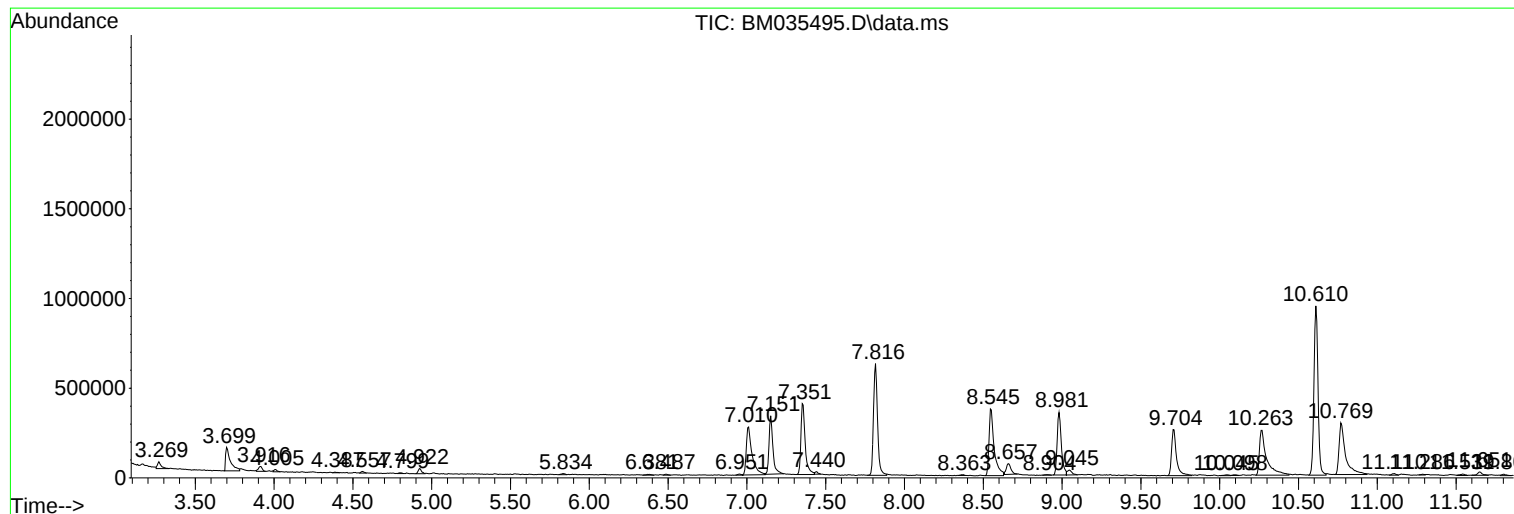

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
Data File : BM035495.D
Acq On : 17 Jun 2022 15:12
Operator : CG/JU
Sample : N3226-14
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4N4










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 1-Dodecanol, 2-octyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.109	2.17 ng/ul	322245	Chrysene-d12	21.392

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	1-Dodecanol, 2-octyl-			298	C20H42O	005333-42-6	90
2	Oxalic acid, isobutyl hexadecyl ...			370	C22H42O4	1000309-38-1	87
3	Carbonic acid, decyl heptadecyl ...			440	C28H56O3	1000383-16-6	87
4	Ethanol, 2-(hexadecyloxy)-			286	C18H38O2	002136-71-2	87
5	Oxalic acid, pentadecyl propyl e...			342	C20H38O4	1000309-26-8	83

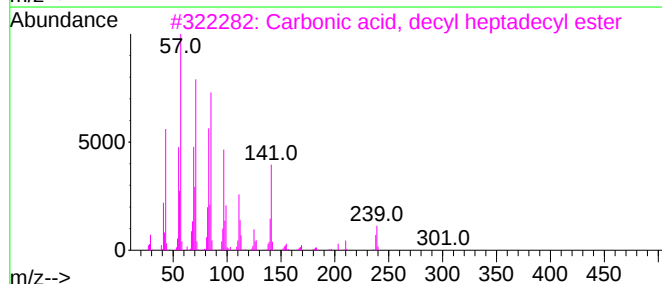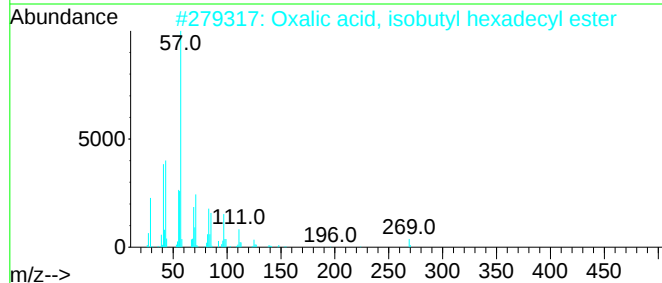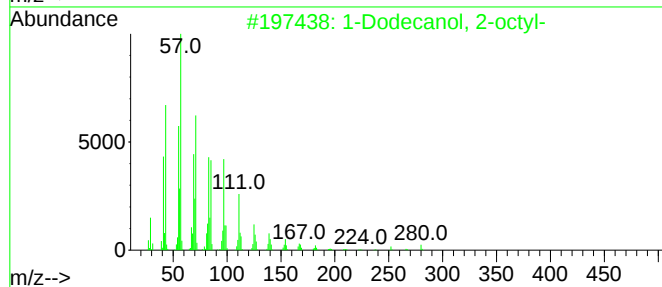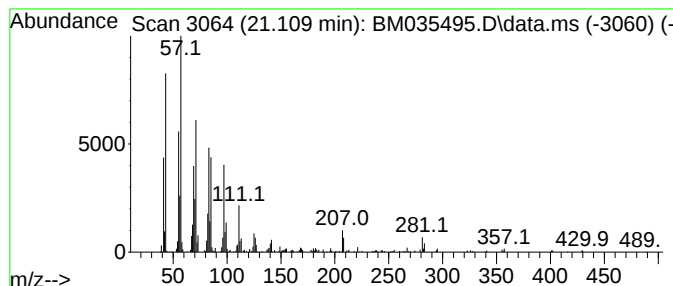

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM061722\
Data File : BM035495.D
Acq On : 17 Jun 2022 15:12
Operator : CG/JU
Sample : N3226-14
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EW4N4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM061622.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1-Dodecanol, 2-...	21.109	2.2	ng/u1	322245	5	21.392	2964290	20.0